

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083022\
 Data File : PL077388.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Aug 2022 17:04
 Operator : AR\AJ
 Sample : N4430-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CRUSHED-MASONARY-PILE-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 30 18:00:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082222.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 23 05:36:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.416	2.630	10489581	24002444	7.709	7.810
28)	SA Decachlor...	8.907	7.733	11902927	24315598	10.157	8.714
Target Compounds							
12)	B 4,4'-DDE	6.077	5.060	4185101	9487425	3.224	2.937



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083022\
Data File : PL077388.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Aug 2022 17:04
Operator : AR\AJ
Sample : N4430-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
CRUSHED-MASONARY-PILE-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 30 18:00:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082222.M
Quant Title : GC Extractables
QLast Update : Tue Aug 23 05:36:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

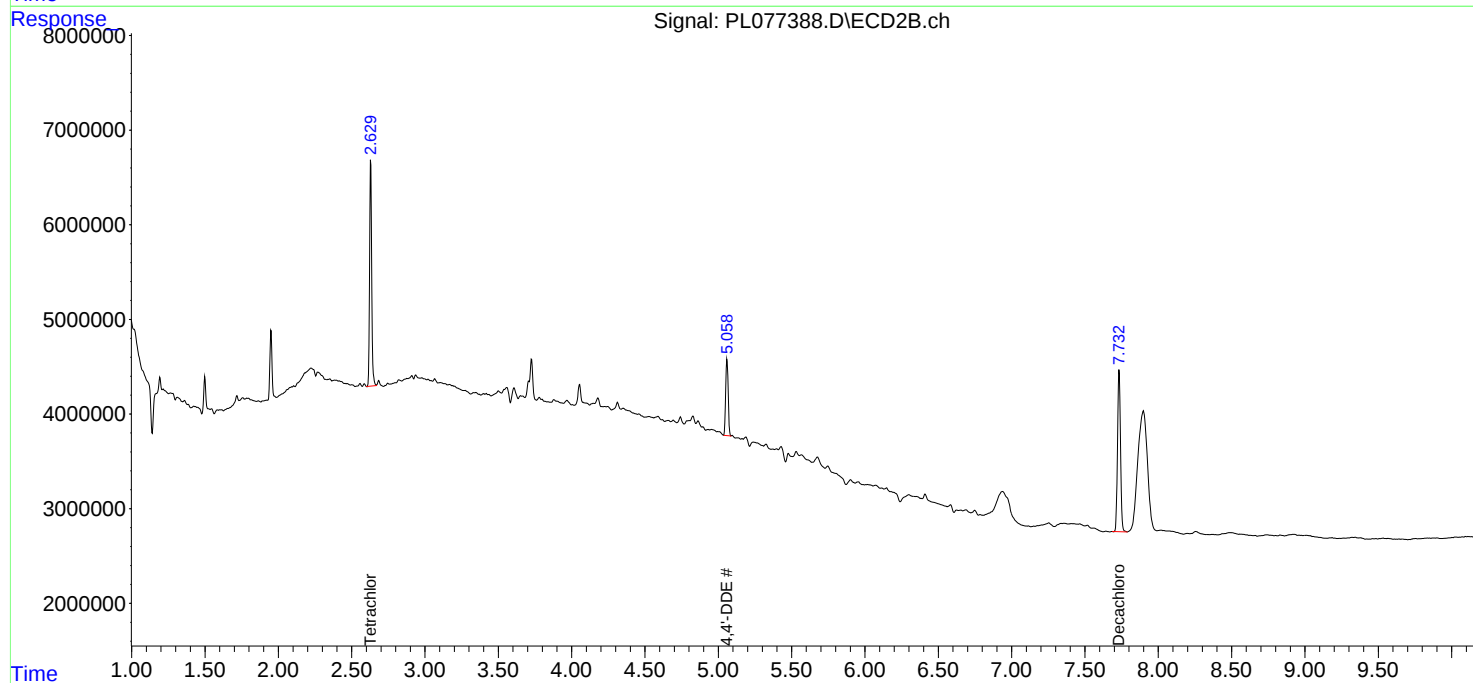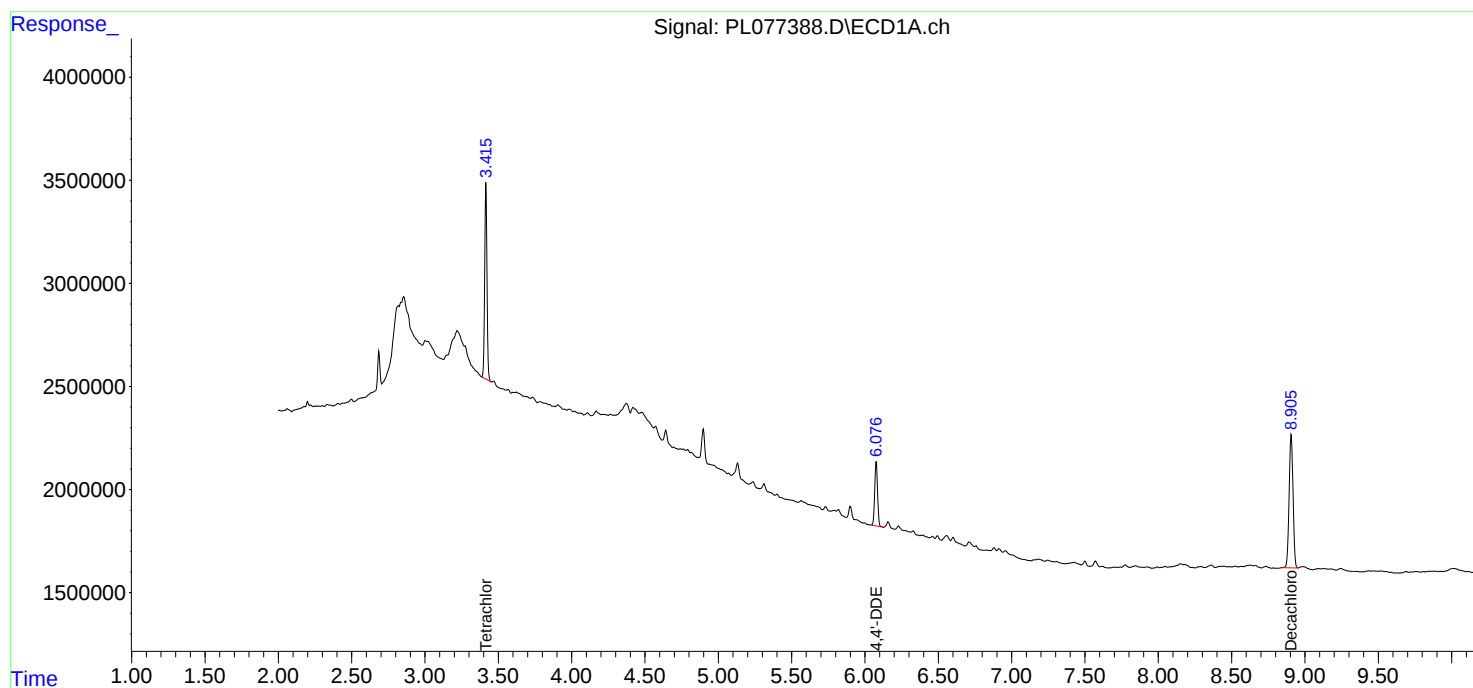


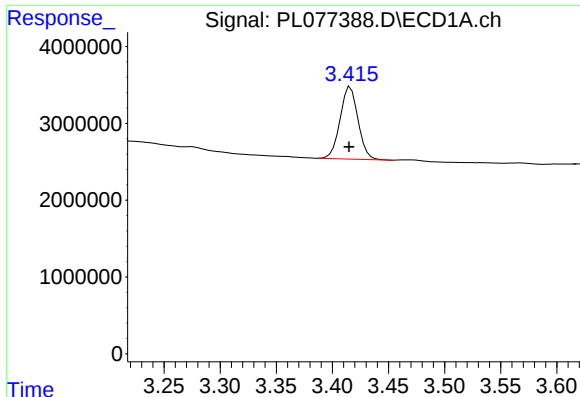

#1 Tetrachloro-m-xylene


R.T.: 3.416 min
Delta R.T.: 0.001 min
Response: 10489581
Conc: 7.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
CRUSHED-MASONARY-PILE-3

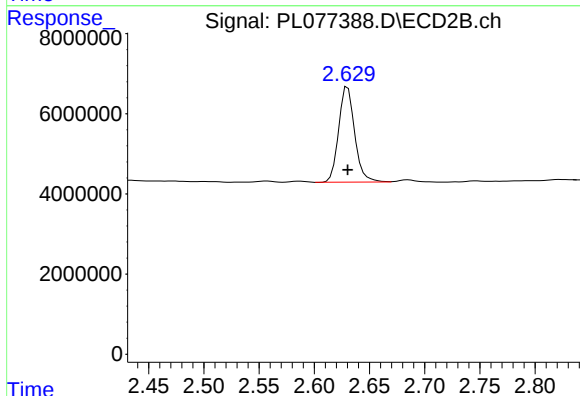


#1 Tetrachloro-m-xylene

R.T.: 2.630 min
Delta R.T.: 0.000 min
Response: 24002444
Conc: 7.81 ng/ml

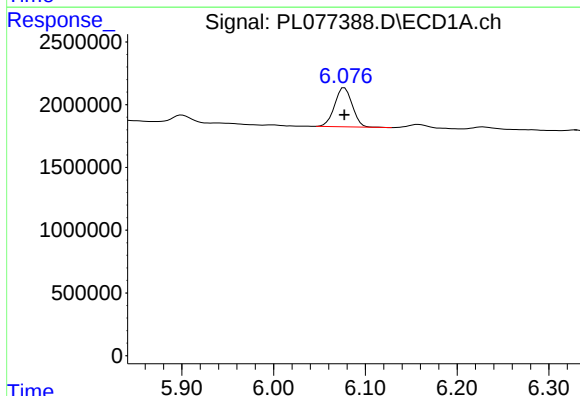


#12 4,4'-DDE

R.T.: 6.077 min
Delta R.T.: 0.000 min
Response: 4185101
Conc: 3.22 ng/ml

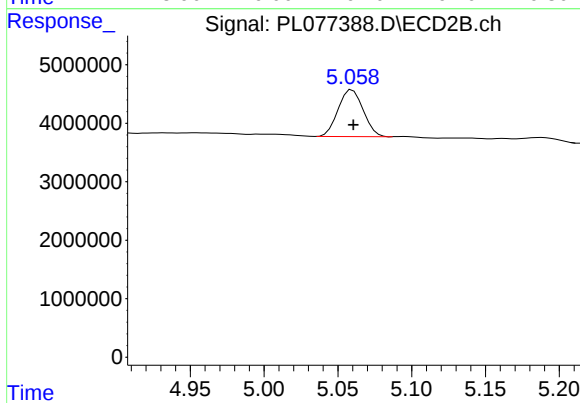

#12 4,4'-DDE


R.T.: 5.060 min
Delta R.T.: 0.000 min
Response: 9487425
Conc: 2.94 ng/ml

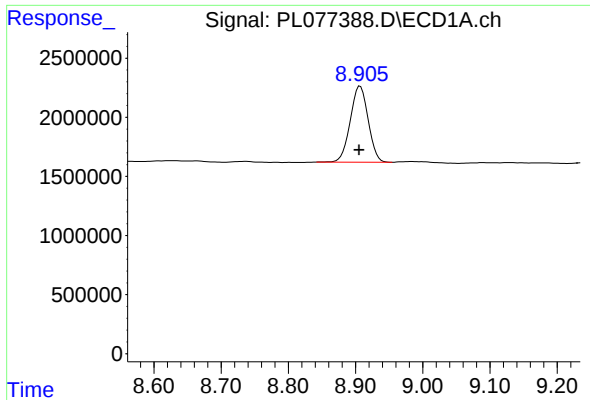

#28 Decachlorobiphenyl

R.T.: 8.907 min
Delta R.T.: 0.001 min
Response: 11902927
Conc: 10.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
CRUSHED-MASONARY-PILE-3

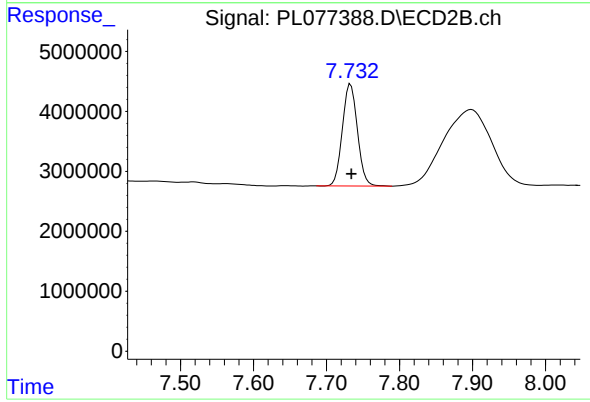

#28 Decachlorobiphenyl

R.T.: 7.733 min
Delta R.T.: -0.001 min
Response: 24315598
Conc: 8.71 ng/ml