

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083118\
 Data File : PL039641.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Aug 2018 12:03
 Operator : AJ\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 23:26:51 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

4) MA	Heptachlor	4.225f	0.000	10273187	0	0.976	N.D.	#
6) B	beta-BHC	4.225f	0.000	10273187	0	2.211	N.D.	#
8) B	Heptachlo...	4.914f	0.000	69532386	0	7.281	N.D.	#
14) MA	Endrin	5.725f	0.000	4680499	0	0.523	N.D.	#
17) MA	4,4'-DDT	6.176	0.000	1997298	0	0.263	N.D.	#
18) B	Endrin al...	6.217	0.000	7730678	0	1.141	N.D.	#
20) A	Methoxychlor	6.689	0.000	17284522	0	4.224	N.D.	#
27)	Chlordane-5	6.133	0.000	26709758	0	82.354	N.D.	#


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083118\
Data File : PL039641.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Aug 2018 12:03
Operator : AJ\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 23:26:51 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

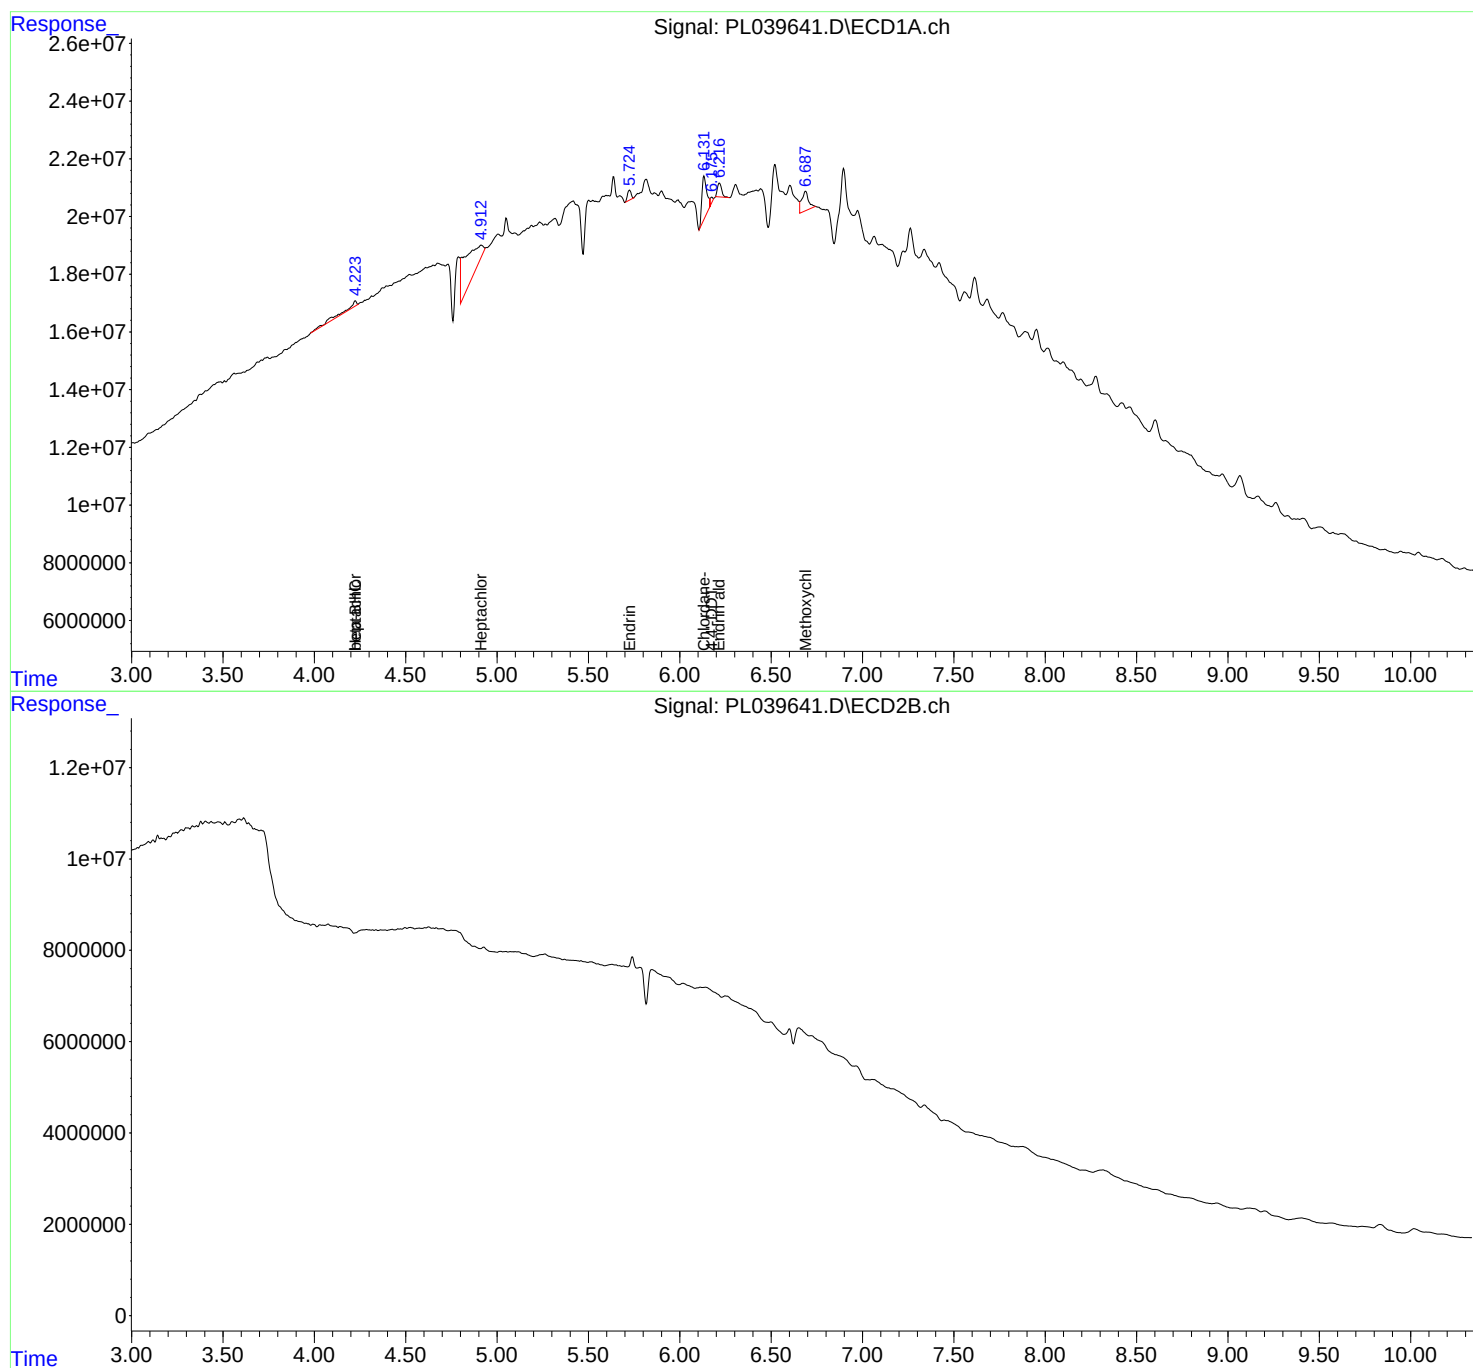


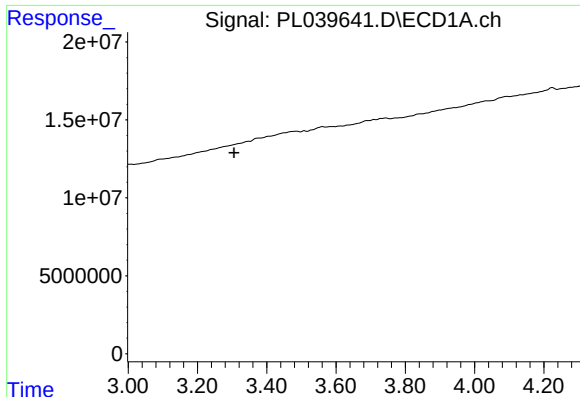

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.306 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

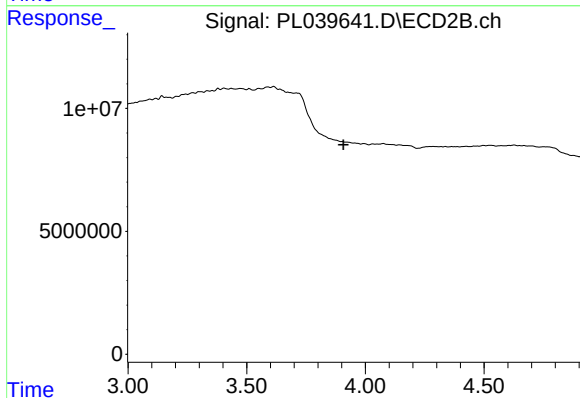


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.907 min
Response: 0
Conc: N.D.

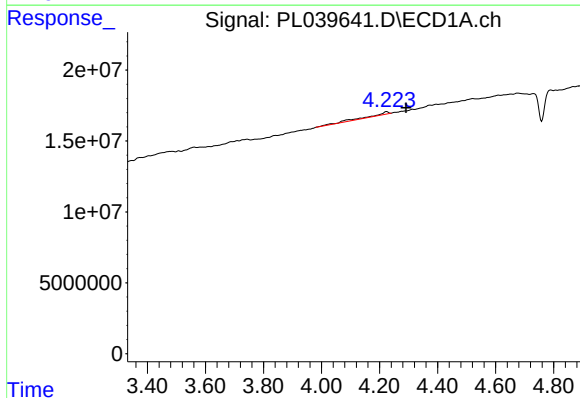


#4 Heptachlor

R.T.: 4.225 min
Delta R.T.: -0.067 min
Response: 10273187
Conc: 0.98 ng/ml

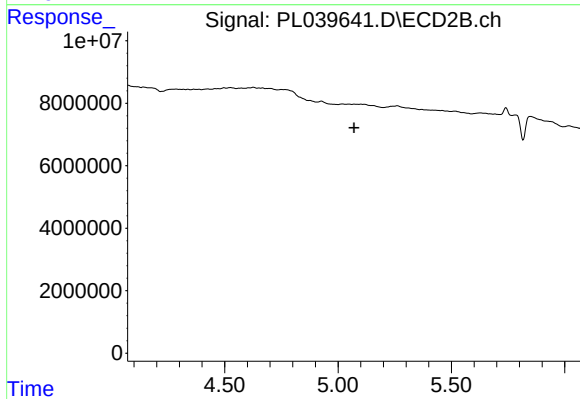

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 5.071 min
Response: 0
Conc: N.D.

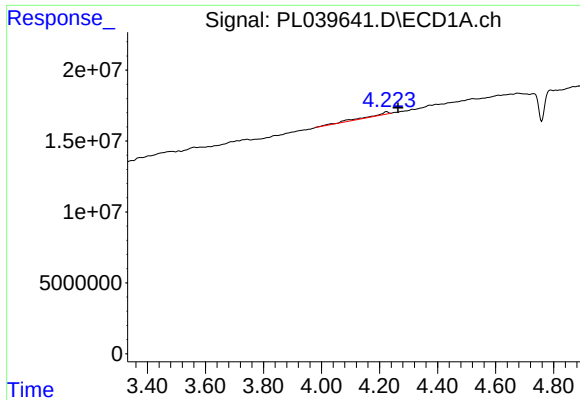

#6 beta-BHC


R.T.: 4.225 min
Delta R.T.: -0.040 min
Response: 10273187
Conc: 2.21 ng/ml

Instrument :
ECD_L
ClientSampleId :

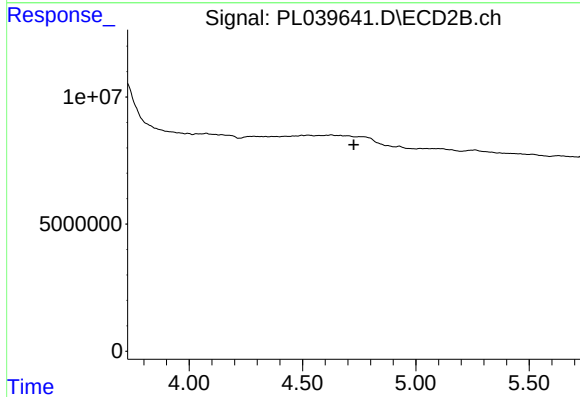


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.726 min
Response: 0
Conc: N.D.

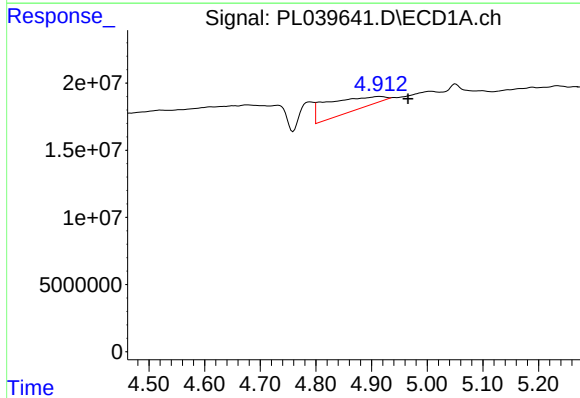


#8 Heptachlor epoxide

R.T.: 4.914 min
Delta R.T.: -0.052 min
Response: 69532386
Conc: 7.28 ng/ml

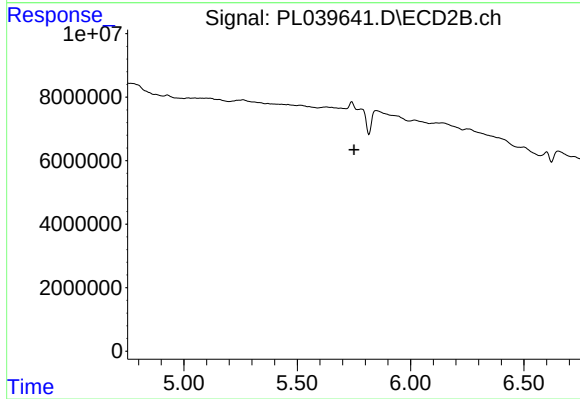

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.751 min
Response: 0
Conc: N.D.

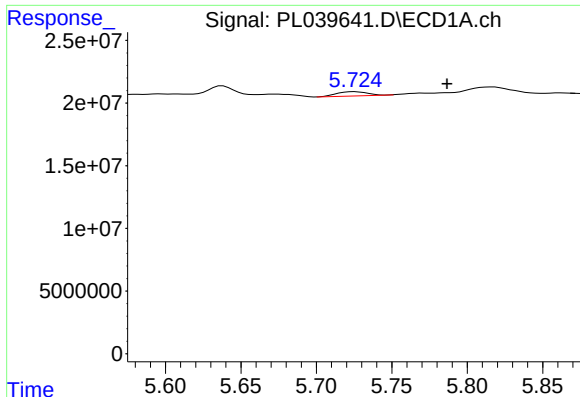

#14 Endrin


R.T.: 5.725 min
Delta R.T.: -0.061 min
Response: 4680499
Conc: 0.52 ng/ml

Instrument :
ECD_L
ClientSampleId :

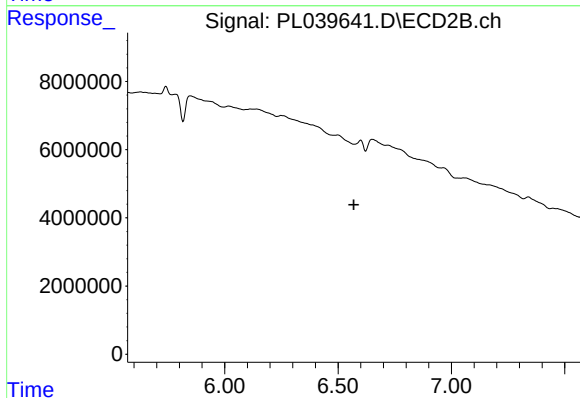


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.570 min
Response: 0
Conc: N.D.

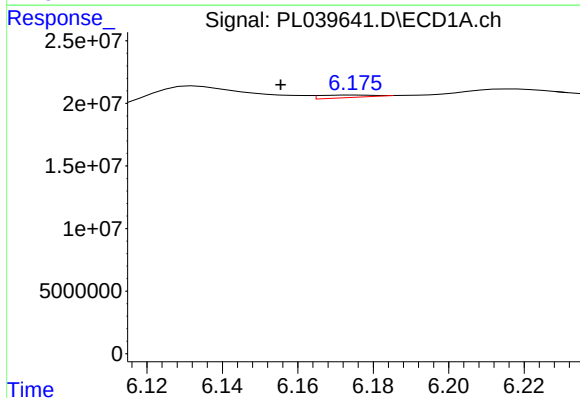


#17 4,4'-DDT

R.T.: 6.176 min
Delta R.T.: 0.020 min
Response: 1997298
Conc: 0.26 ng/ml

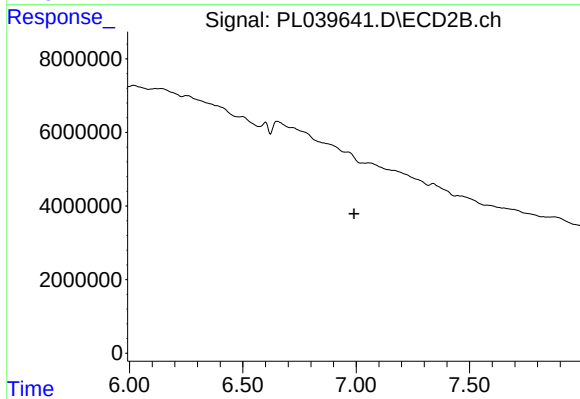

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 6.991 min
Response: 0
Conc: N.D.

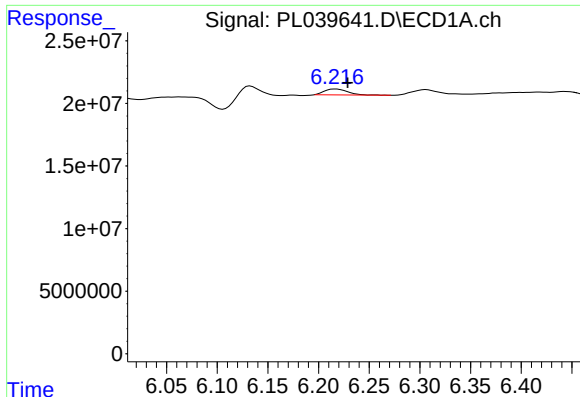

#18 Endrin aldehyde


R.T.: 6.217 min
Delta R.T.: -0.012 min
Response: 7730678
Conc: 1.14 ng/ml

Instrument :
ECD_L
ClientSampleId :

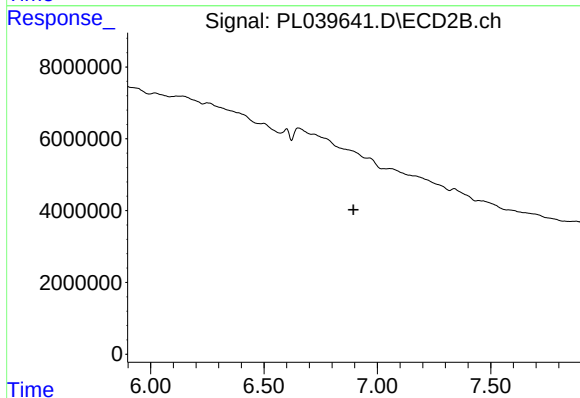


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.895 min
Response: 0
Conc: N.D.

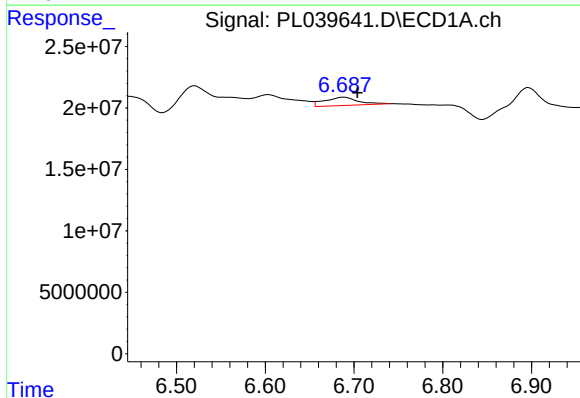


#20 Methoxychlor

R.T.: 6.689 min
Delta R.T.: -0.015 min
Response: 17284522
Conc: 4.22 ng/ml

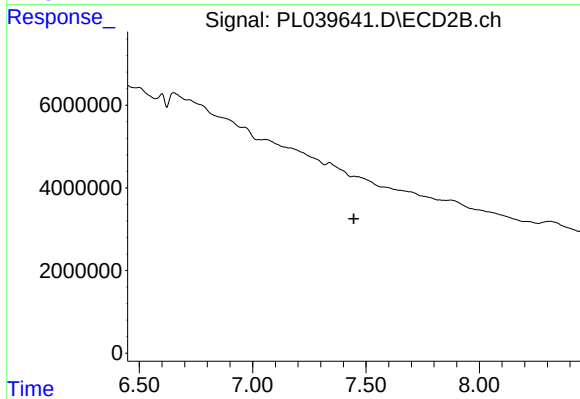

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.446 min
Response: 0
Conc: N.D.

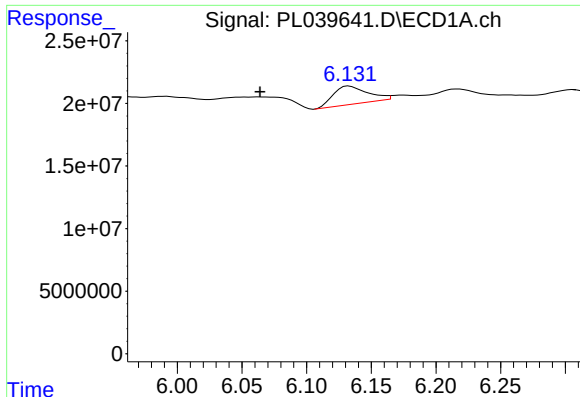

#27 Chlordane-5


R.T.: 6.133 min
Delta R.T.: 0.069 min
Response: 26709758
Conc: 82.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

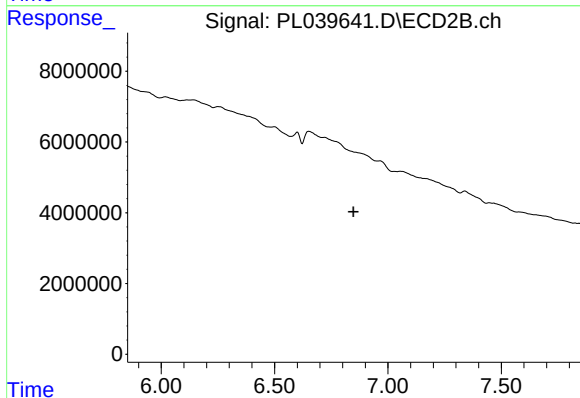


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.848 min
Response: 0
Conc: N.D.

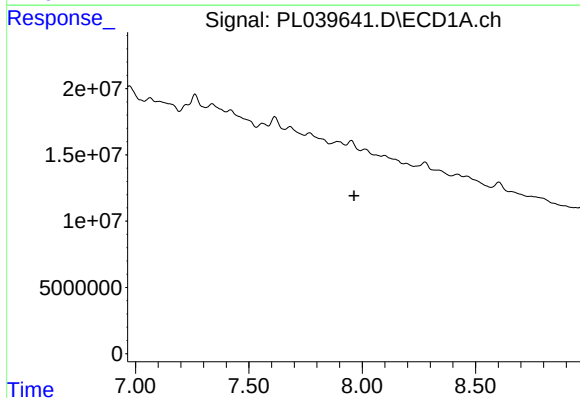

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.964 min
Response: 0
Conc: N.D.

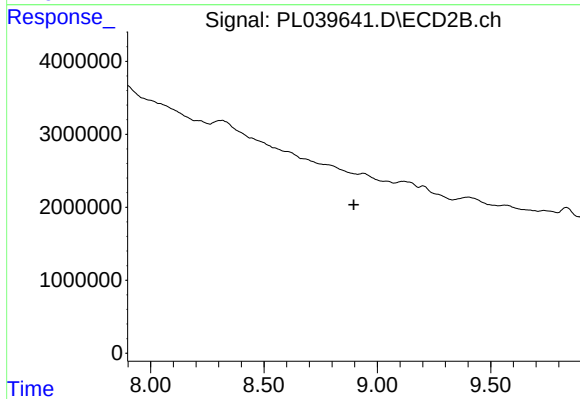

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.896 min
Response: 0
Conc: N.D.