

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083118\
 Data File : PL039645.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Aug 2018 15:10
 Operator : AJ\SJ
 Sample : PB112525BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 23:28:22 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.312	3.903	137.8E6	58507251	19.708	21.824
28)	SA Decachlor...	7.967	8.893	141.7E6	53982548	20.172	23.262
Target Compounds							
3)	MA gamma-BHC...	3.968f	4.523f	950714	57377	0.090	0.014 #
8)	B Heptachlo...	4.912f	0.000	11494222	0	1.204	N.D. #
9)	A Endosulfan I	5.324	0.000	2638240	0	0.301	N.D. #
17)	MA 4,4'-DDT	6.138	0.000	5956175	0	0.786	N.D. #
20)	A Methoxychlor	6.644f	0.000	10389823	0	2.539	N.D. #
23)	Chlordane-1	4.089	0.000	8033180	0	25.374	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083118\
Data File : PL039645.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Aug 2018 15:10
Operator : AJ\SJ
Sample : PB112525BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 23:28:22 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

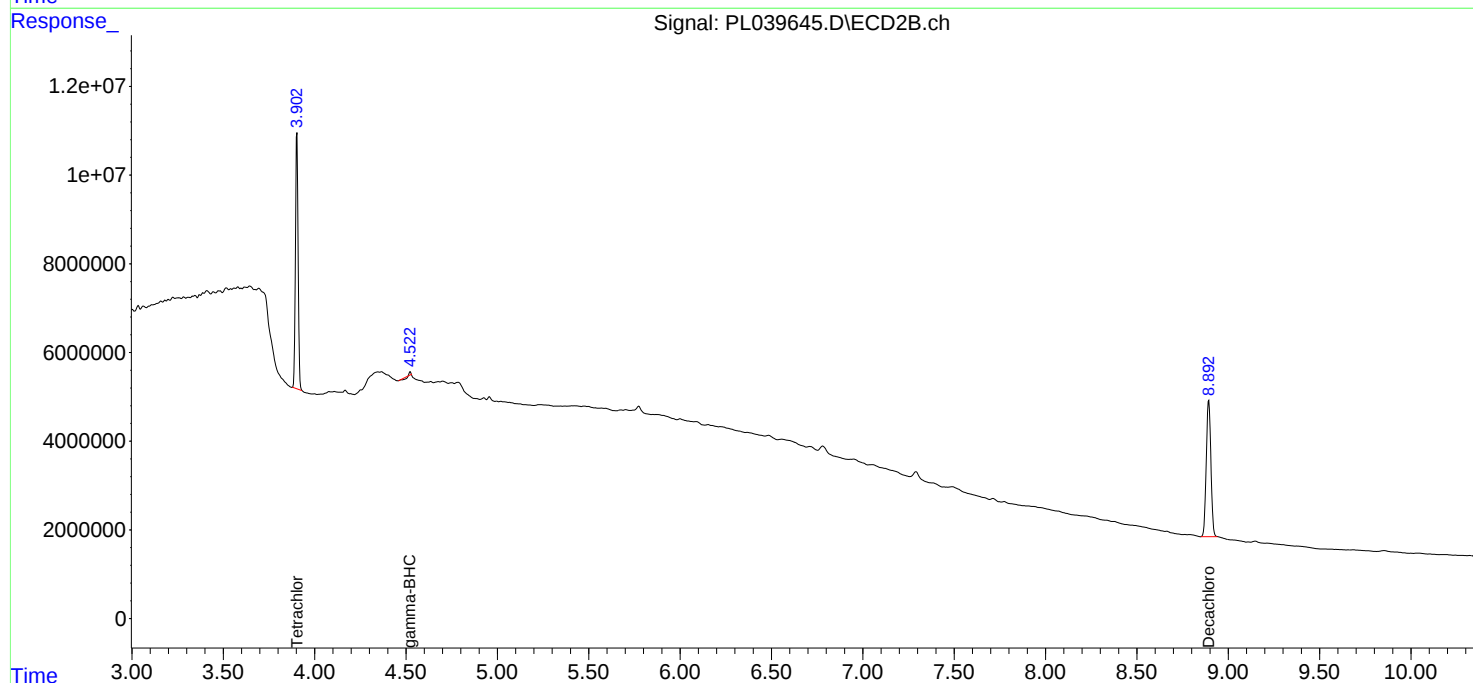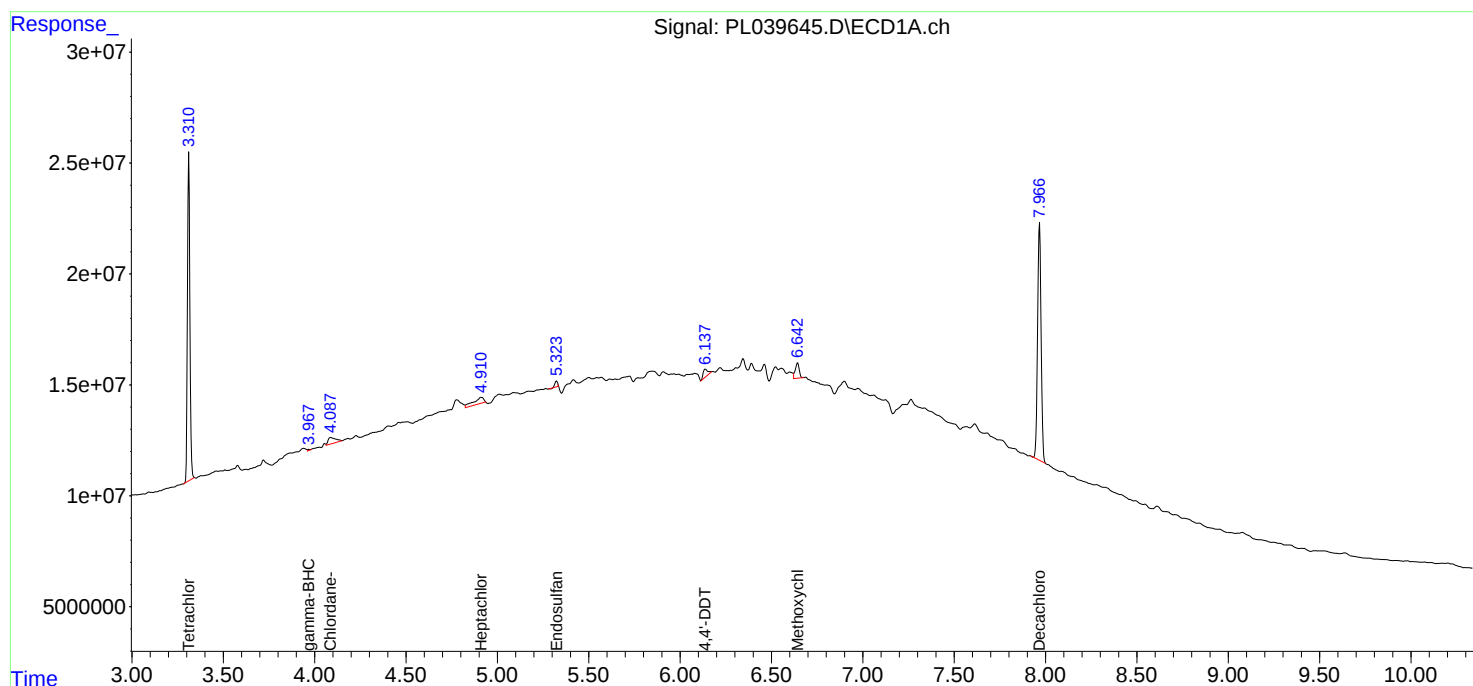


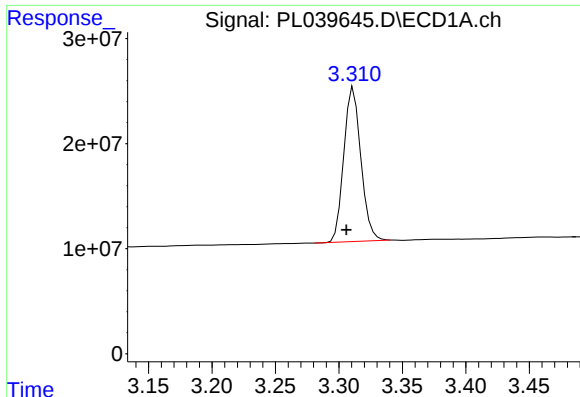

#1 Tetrachloro-m-xylene


R.T.: 3.312 min
Delta R.T.: 0.006 min
Response: 137765082
Conc: 19.71 ng/ml

Instrument :
ECD_L
ClientSampleId :

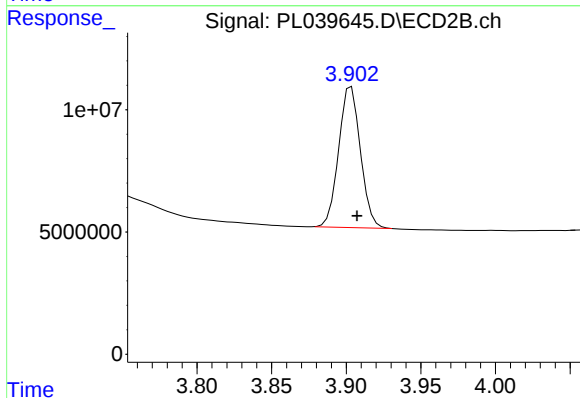


#1 Tetrachloro-m-xylene

R.T.: 3.903 min
Delta R.T.: -0.004 min
Response: 58507251
Conc: 21.82 ng/ml

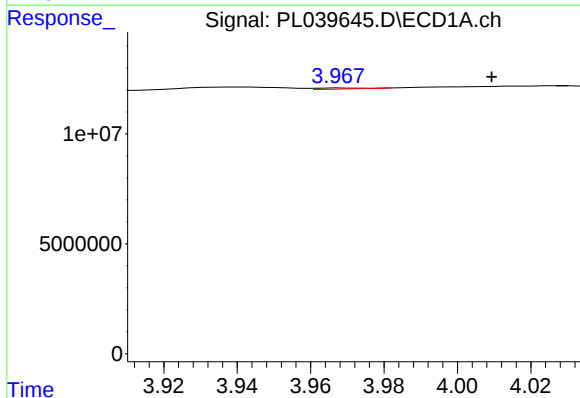


#3 gamma-BHC (Lindane)

R.T.: 3.968 min
Delta R.T.: -0.041 min
Response: 950714
Conc: 0.09 ng/ml

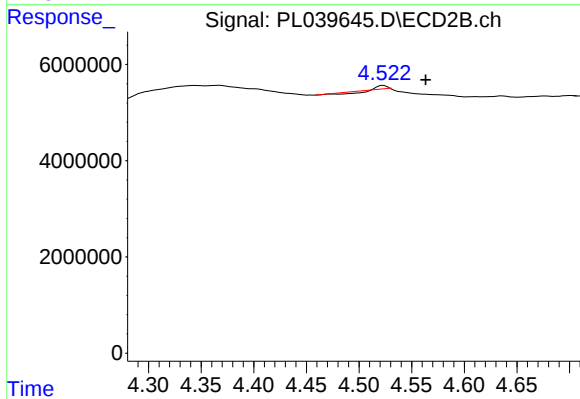

#3 gamma-BHC (Lindane)


R.T.: 4.523 min
Delta R.T.: -0.040 min
Response: 57377
Conc: 0.01 ng/ml

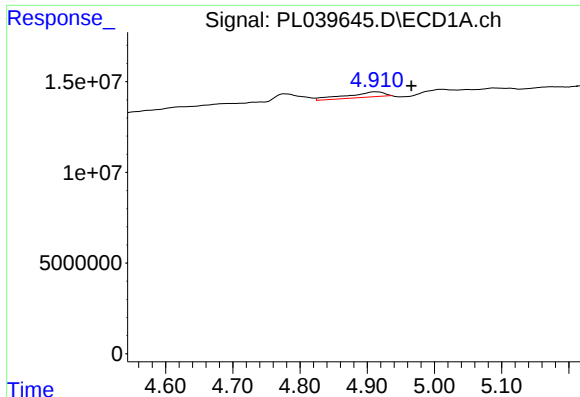

#8 Heptachlor epoxide


R.T.: 4.912 min
Delta R.T.: -0.054 min
Response: 11494222
Conc: 1.20 ng/ml

Instrument :
ECD_L
ClientSampleId :

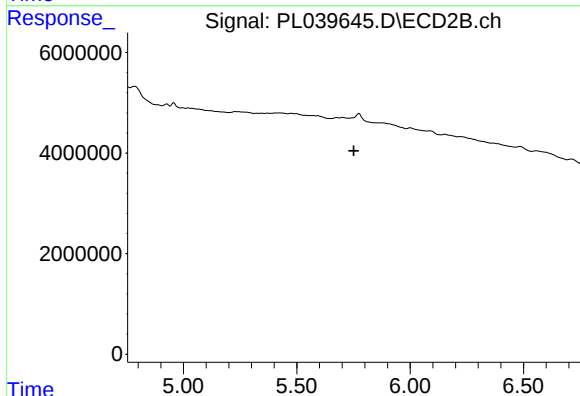


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.751 min
Response: 0
Conc: N.D.

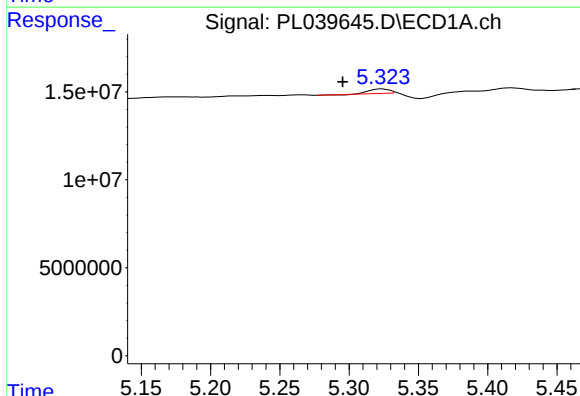


#9 Endosulfan I

R.T.: 5.324 min
Delta R.T.: 0.029 min
Response: 2638240
Conc: 0.30 ng/ml

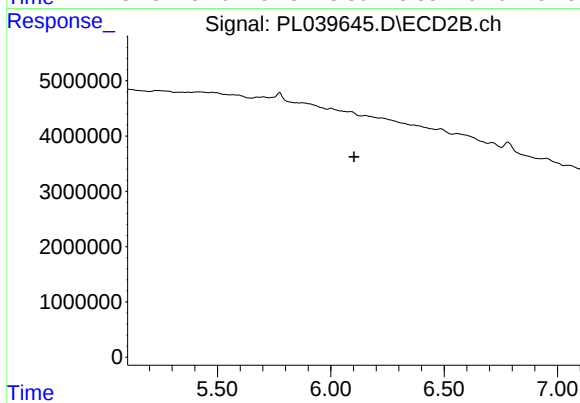

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.102 min
Response: 0
Conc: N.D.

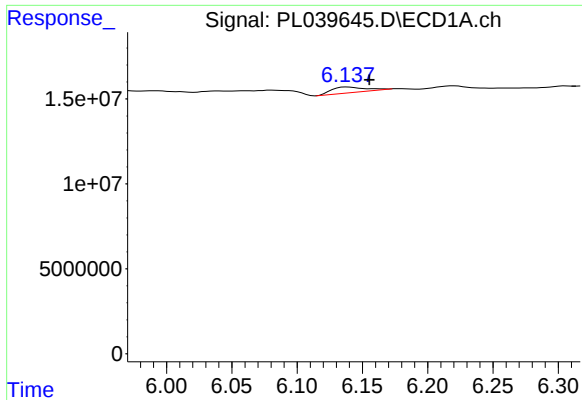

#17 4,4'-DDT


R.T.: 6.138 min
Delta R.T.: -0.017 min
Response: 5956175
Conc: 0.79 ng/ml

Instrument :
ECD_L
ClientSampleId :

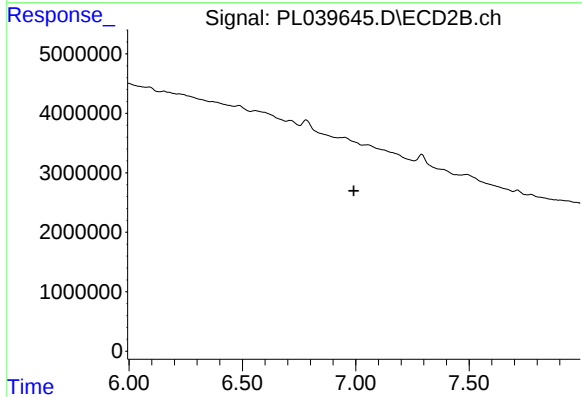


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.991 min
Response: 0
Conc: N.D.

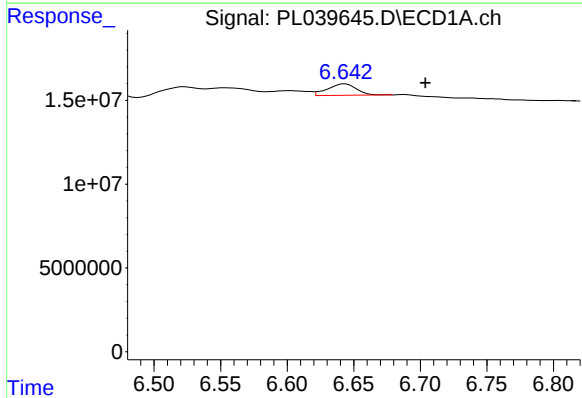


#20 Methoxychlor

R.T.: 6.644 min
Delta R.T.: -0.060 min
Response: 10389823
Conc: 2.54 ng/ml

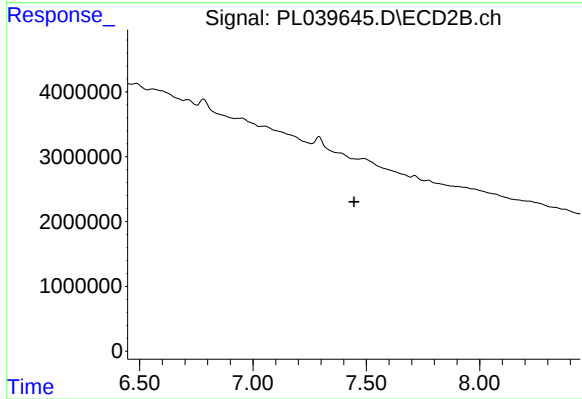

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.446 min
Response: 0
Conc: N.D.

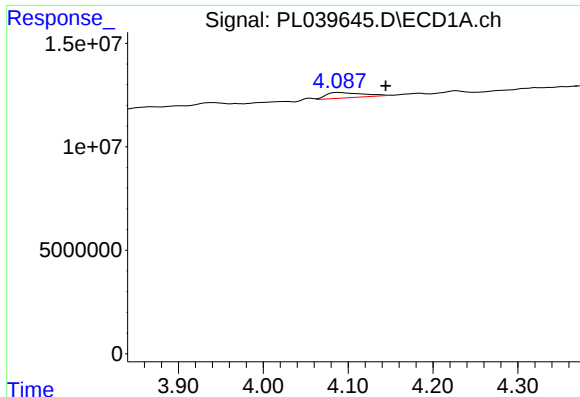

#23 Chlordane-1


R.T.: 4.089 min
Delta R.T.: -0.056 min
Response: 8033180
Conc: 25.37 ng/ml

Instrument :
ECD_L
ClientSampleId :

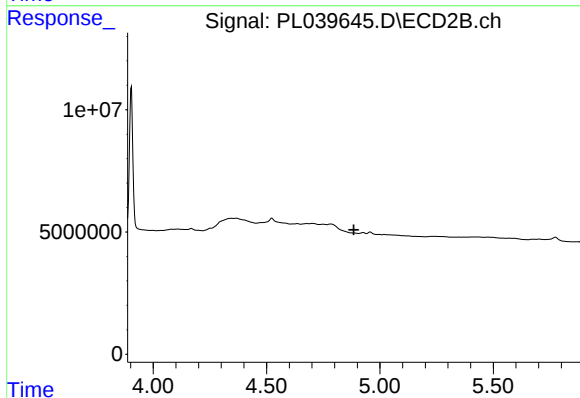


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.885 min
Response: 0
Conc: N.D.

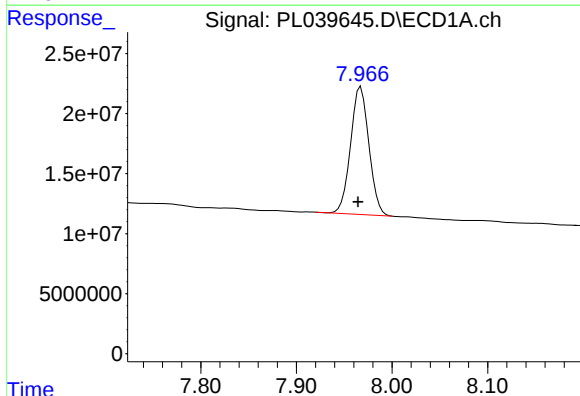

#28 Decachlorobiphenyl

R.T.: 7.967 min
Delta R.T.: 0.003 min
Response: 141678254
Conc: 20.17 ng/ml

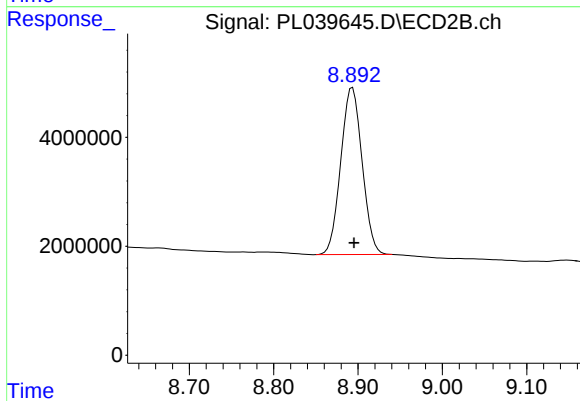

#28 Decachlorobiphenyl

R.T.: 8.893 min
Delta R.T.: -0.002 min
Response: 53982548
Conc: 23.26 ng/ml