

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083118\
 Data File : PL039666.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Aug 2018 20:11
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 23:36:14 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.303	3.905	120.2E6	50878573	17.198	18.978
28)	SA Decachlor...	7.956	8.891	111.0E6	42828047	15.799	18.456
Target Compounds							
8) B	Heptachlo...	4.914f	0.000	1959280	0	0.205	N.D. #
23)	Chlordane-1	4.212	0.000	9022053	0	28.498	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083118\
Data File : PL039666.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Aug 2018 20:11
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 23:36:14 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

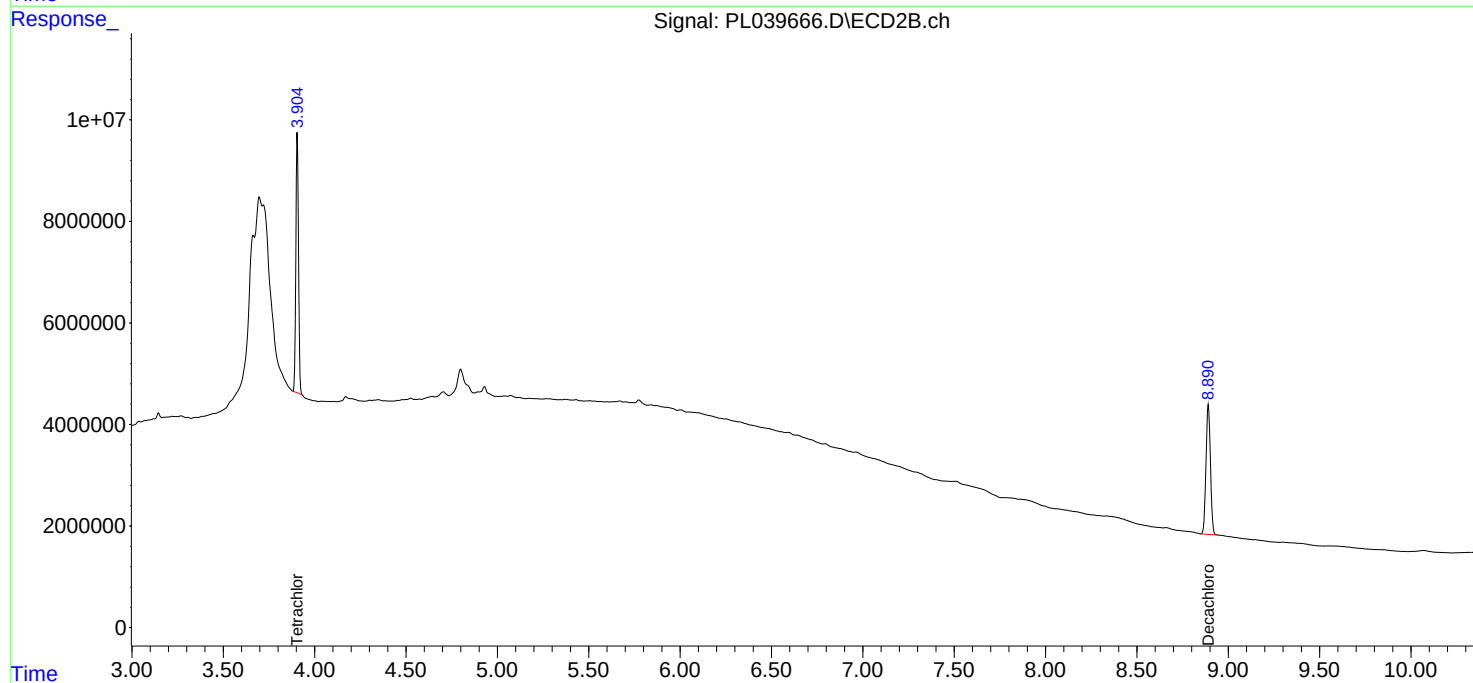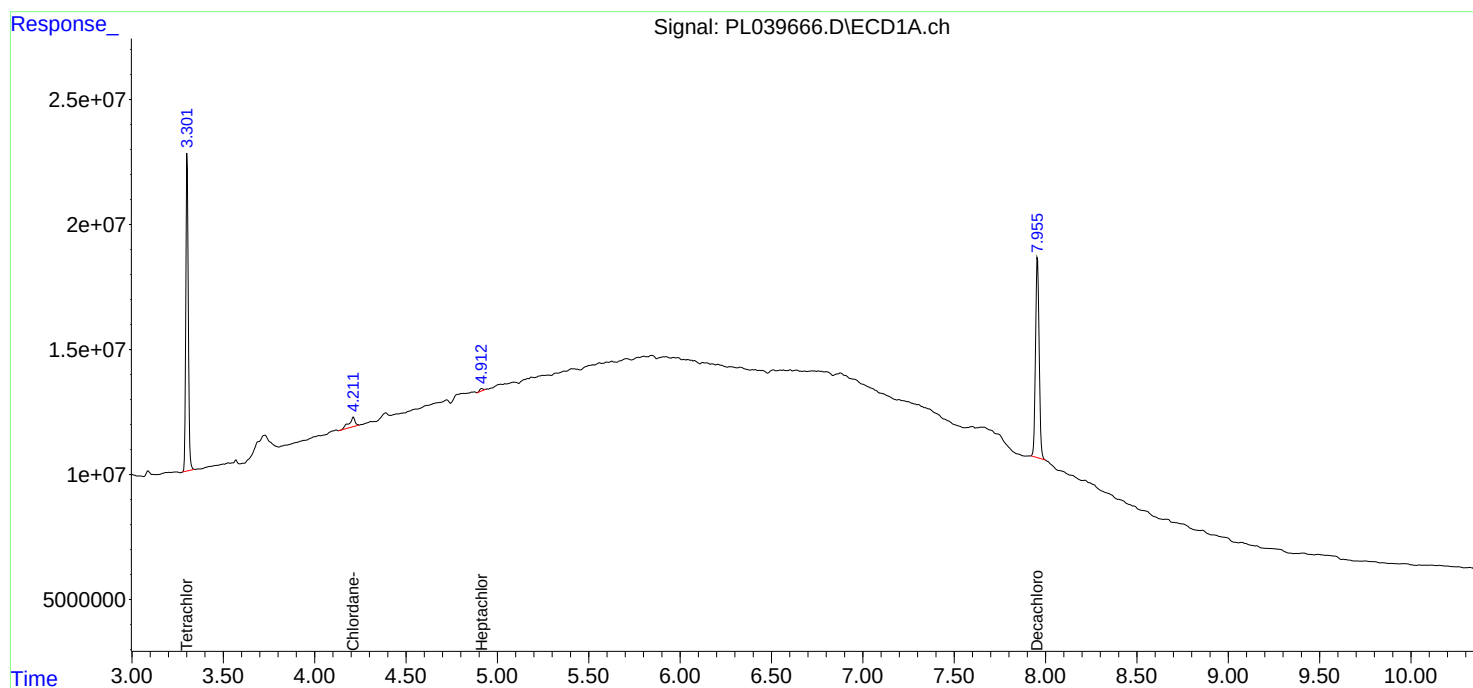


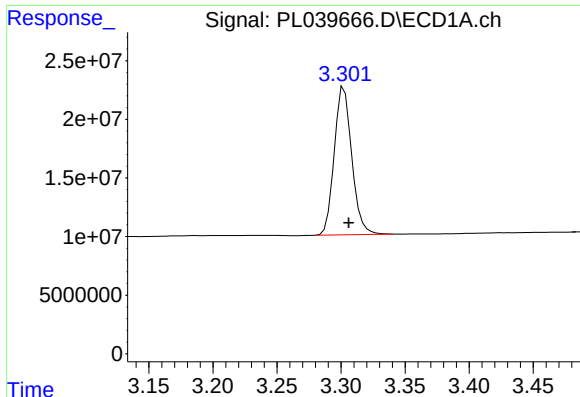

#1 Tetrachloro-m-xylene


R.T.: 3.303 min
Delta R.T.: -0.003 min
Response: 120221897
Conc: 17.20 ng/ml

Instrument :
ECD_L
ClientSampleId :

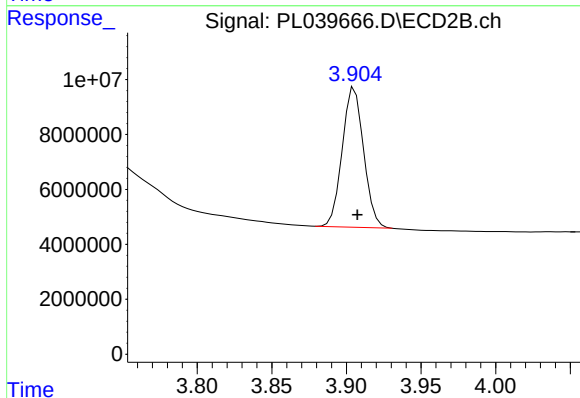


#1 Tetrachloro-m-xylene

R.T.: 3.905 min
Delta R.T.: -0.002 min
Response: 50878573
Conc: 18.98 ng/ml

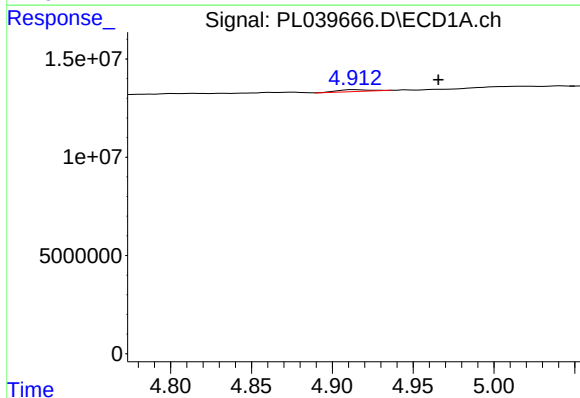


#8 Heptachlor epoxide

R.T.: 4.914 min
Delta R.T.: -0.052 min
Response: 1959280
Conc: 0.21 ng/ml

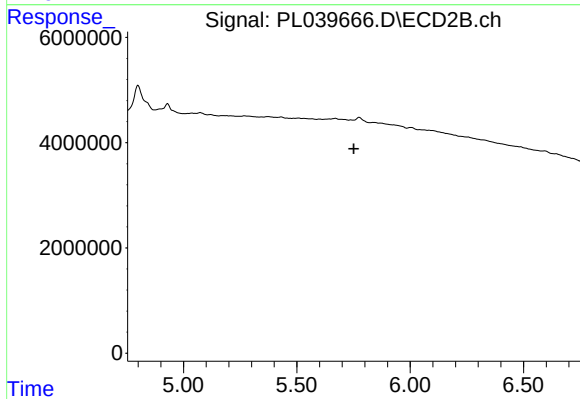

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.751 min
Response: 0
Conc: N.D.

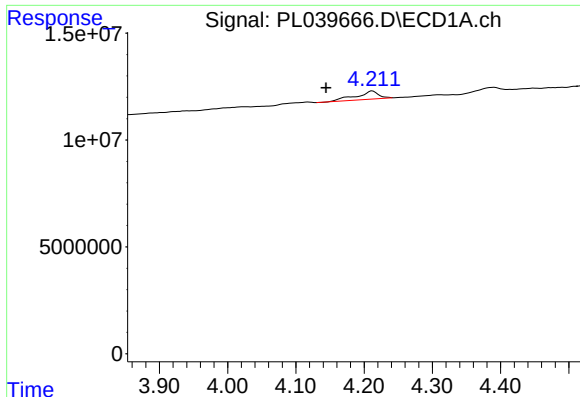

#23 Chlordane-1


R.T.: 4.212 min
Delta R.T.: 0.068 min
Response: 9022053
Conc: 28.50 ng/ml

Instrument :
ECD_L
ClientSampleId :

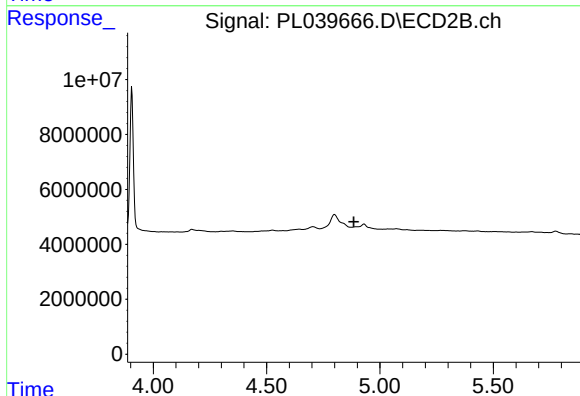


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.885 min
Response: 0
Conc: N.D.

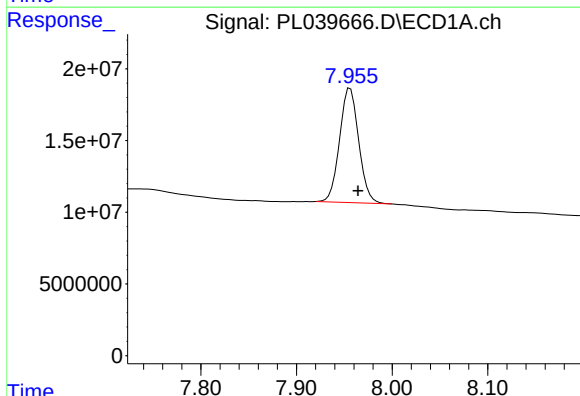

#28 Decachlorobiphenyl

R.T.: 7.956 min
Delta R.T.: -0.008 min
Response: 110960198
Conc: 15.80 ng/ml

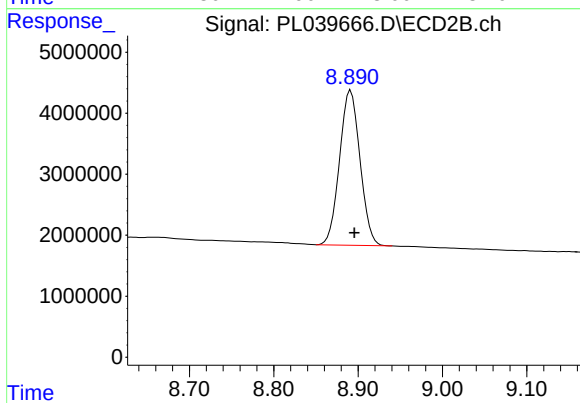

#28 Decachlorobiphenyl

R.T.: 8.891 min
Delta R.T.: -0.004 min
Response: 42828047
Conc: 18.46 ng/ml