

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083119\
 Data File : PL052108.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Aug 2019 12:35
 Operator : SG\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 22:38:48 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	3.314	3.923	245.8E6	60612611	28.722	27.743
28)	SA Decachlor...	7.972	8.947	319.4E6	73070344	26.316	24.006
Target Compounds							
6)	B beta-BHC	0.000	4.801f	0	533310	N.D.	0.366 #
8)	B Heptachlo...	0.000	5.782	0	11720028	N.D.	3.473 #
9)	A Endosulfan I	5.327f	0.000	14558689	0	1.083	N.D. #
14)	MA Endrin	5.810	6.617	4232783	826592	0.290	0.273
15)	B Endosulfa...	0.000	6.844f	0	259769	N.D.	0.079 #
18)	B Endrin al...	0.000	6.974f	0	1462180	N.D.	0.517 #
20)	A Methoxychlor	0.000	7.501	0	196632	N.D.	0.117 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083119\
Data File : PL052108.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Aug 2019 12:35
Operator : SG\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 22:38:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

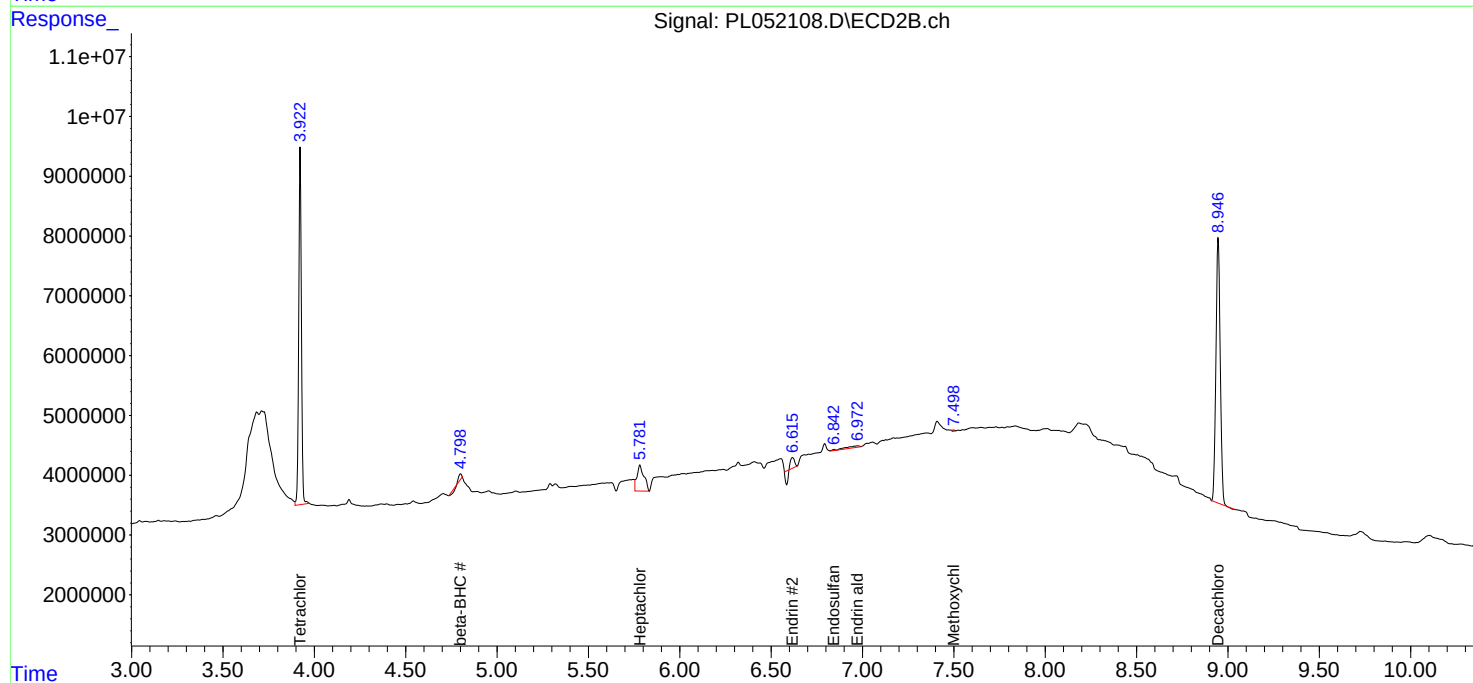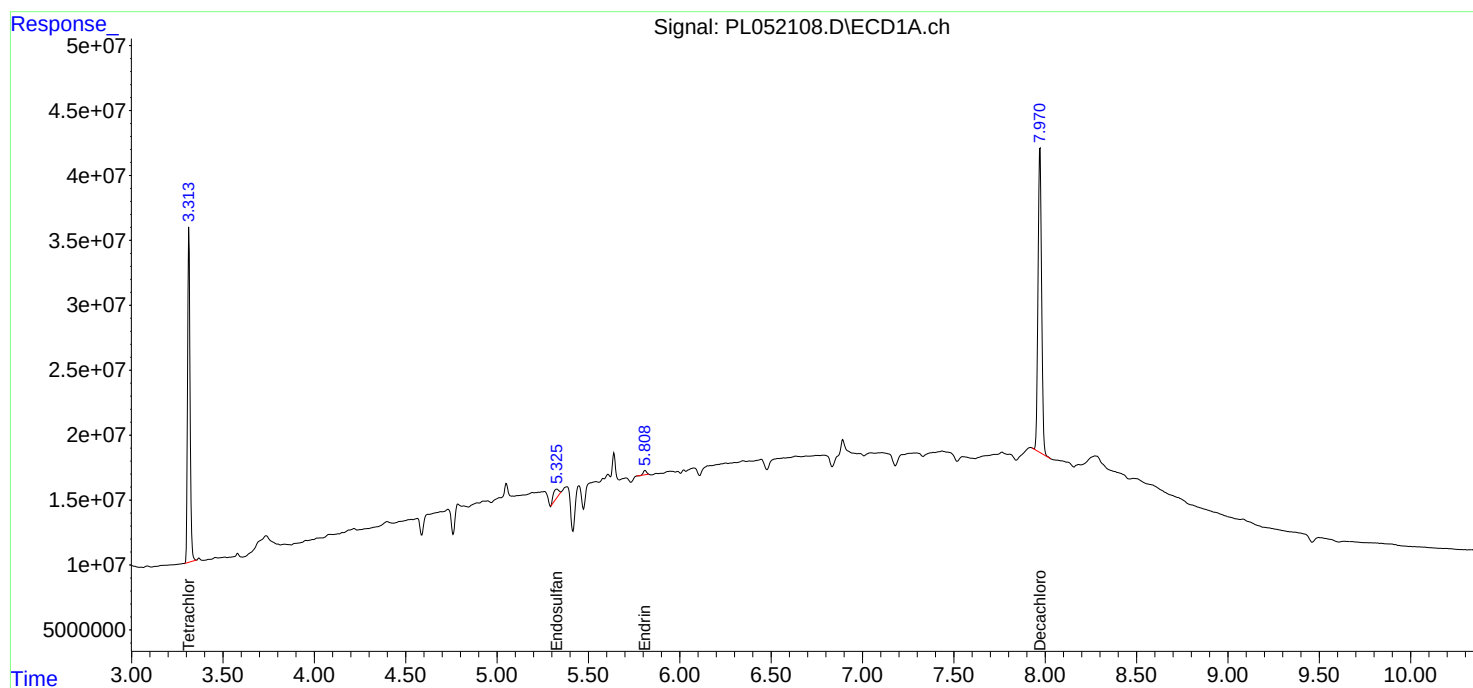

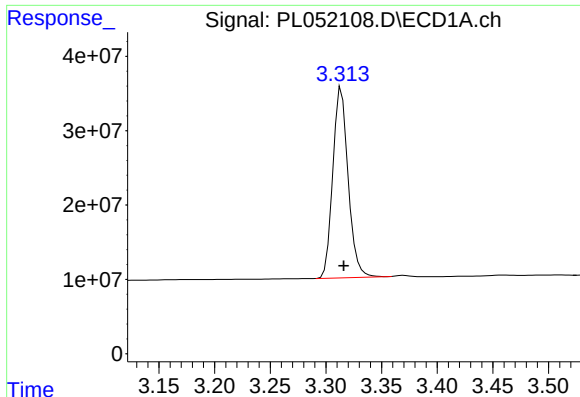


#1 Tetrachloro-m-xylene

R.T.: 3.314 min
Delta R.T.: -0.002 min
Response: 245817723
Conc: 28.72 ng/ml

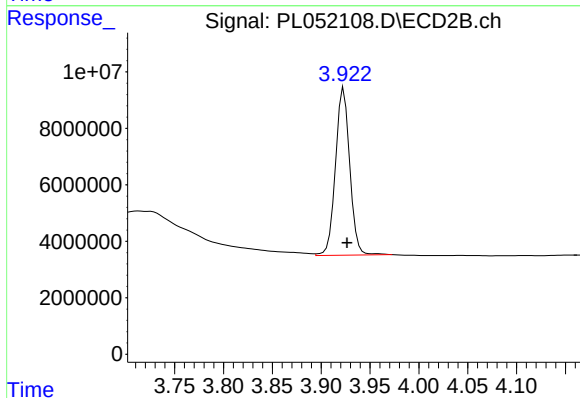


#1 Tetrachloro-m-xylene

R.T.: 3.923 min
Delta R.T.: -0.003 min
Response: 60612611
Conc: 27.74 ng/ml

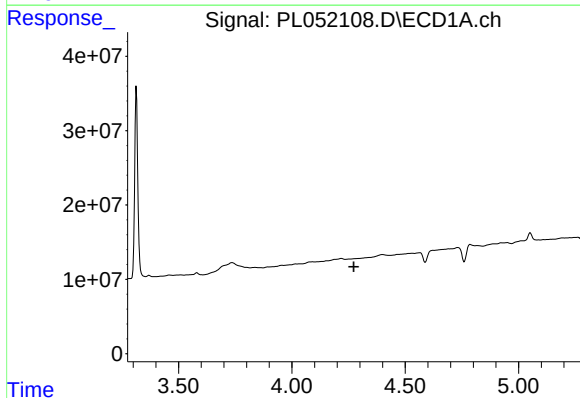


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.273 min
Response: 0
Conc: N.D.

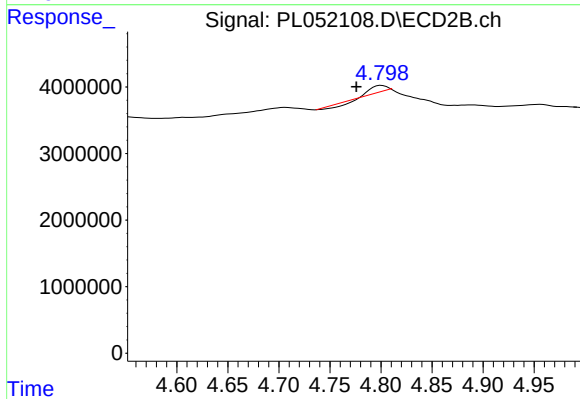


#6 beta-BHC

R.T.: 4.801 min
Delta R.T.: 0.025 min
Response: 533310
Conc: 0.37 ng/ml

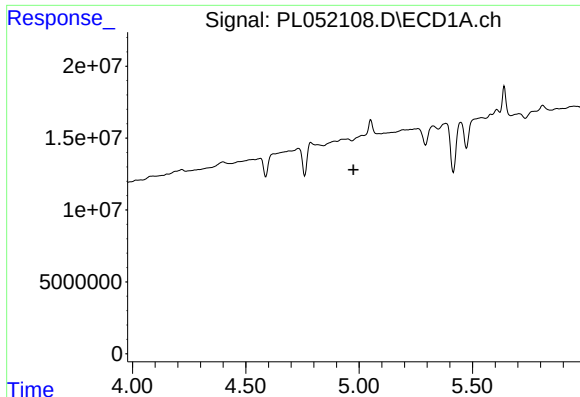


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.975 min
Response: 0
Conc: N.D.

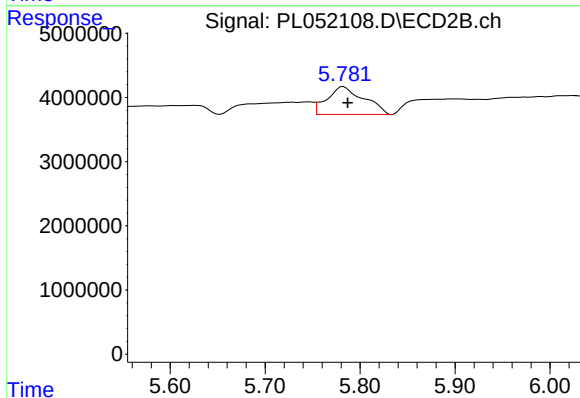


#8 Heptachlor epoxide

R.T.: 5.782 min
Delta R.T.: -0.005 min
Response: 11720028
Conc: 3.47 ng/ml

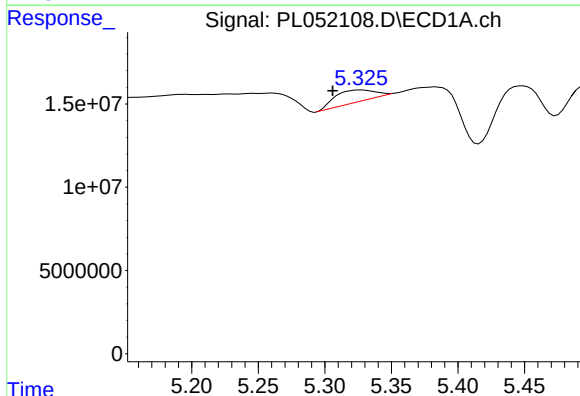


#9 Endosulfan I

R.T.: 5.327 min
Delta R.T.: 0.021 min
Response: 14558689
Conc: 1.08 ng/ml

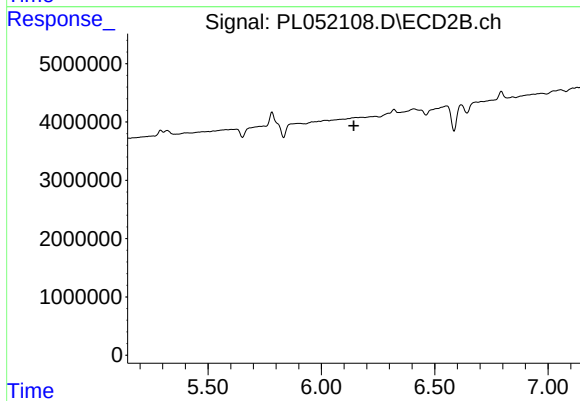


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.143 min
Response: 0
Conc: N.D.

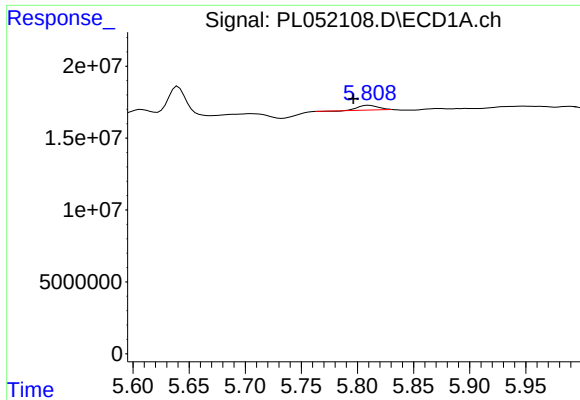


#14 Endrin

R.T.: 5.810 min
Delta R.T.: 0.014 min
Response: 4232783
Conc: 0.29 ng/ml

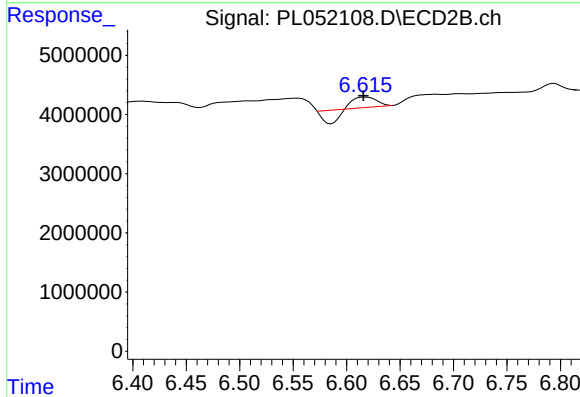


#14 Endrin

R.T.: 6.617 min
Delta R.T.: 0.002 min
Response: 826592
Conc: 0.27 ng/ml

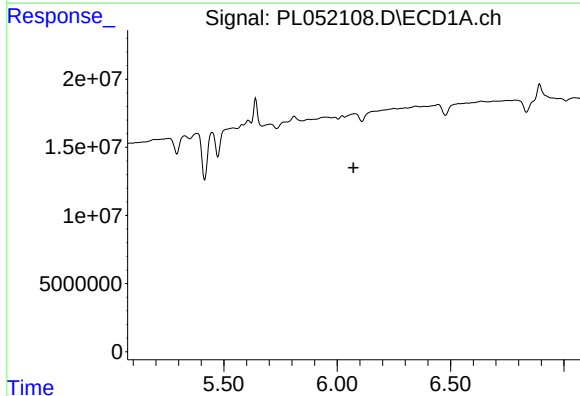


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.072 min
Response: 0
Conc: N.D.

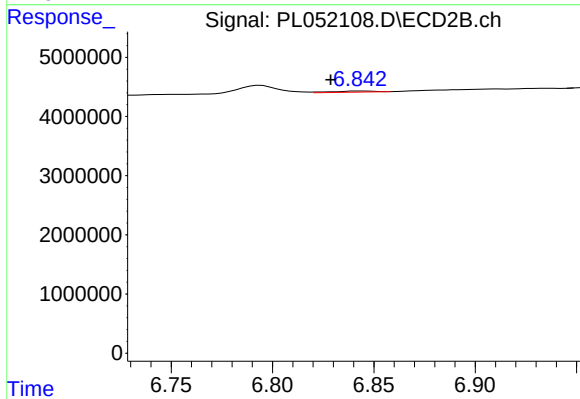


#15 Endosulfan II

R.T.: 6.844 min
Delta R.T.: 0.015 min
Response: 259769
Conc: 0.08 ng/ml

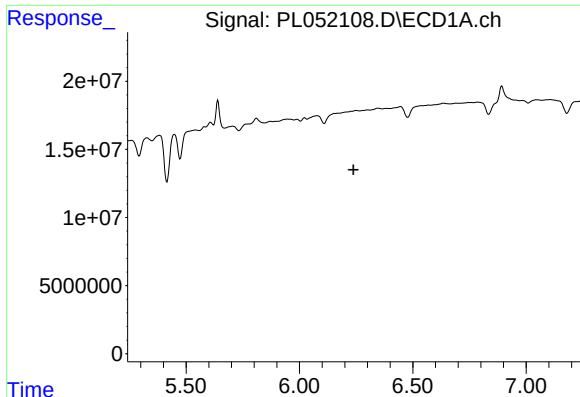


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.239 min
Response: 0
Conc: N.D.

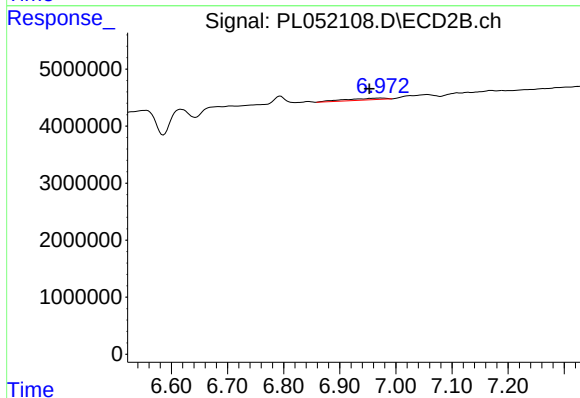


#18 Endrin aldehyde

R.T.: 6.974 min
Delta R.T.: 0.021 min
Response: 1462180
Conc: 0.52 ng/ml

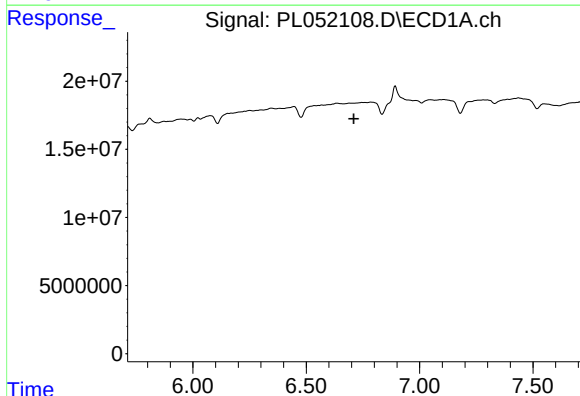


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.710 min
Response: 0
Conc: N.D.

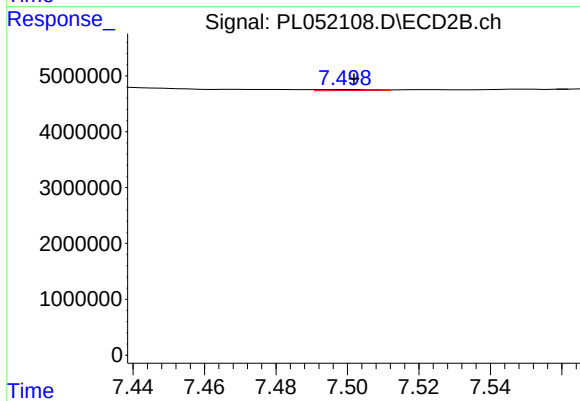


#20 Methoxychlor

R.T.: 7.501 min
Delta R.T.: -0.001 min
Response: 196632
Conc: 0.12 ng/ml

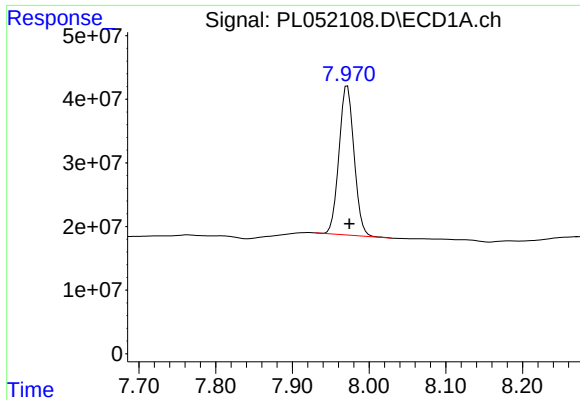

#28 Decachlorobiphenyl

R.T.: 7.972 min
Delta R.T.: -0.003 min
Response: 319413337
Conc: 26.32 ng/ml

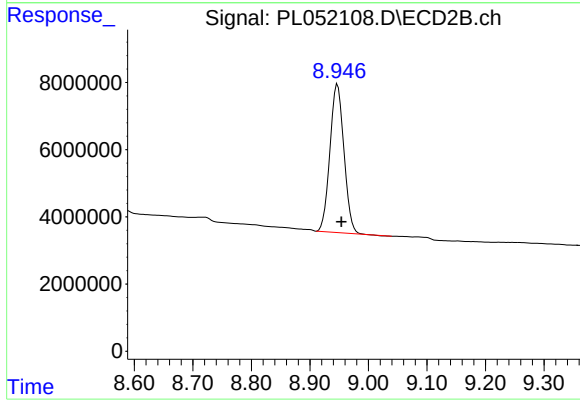

#28 Decachlorobiphenyl

R.T.: 8.947 min
Delta R.T.: -0.007 min
Response: 73070344
Conc: 24.01 ng/ml