

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083119\
 Data File : PL052123.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Aug 2019 16:34
 Operator : SG\AJ
 Sample : K4554-19
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 22:41:44 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	3.312	3.923	106.3E6	28699036	12.422	13.136
28)	SA Decachlor...	7.969	8.947	166.6E6	40256040	13.722	13.225
Target Compounds							
6)	B beta-BHC	0.000	4.801f	0	854970	N.D.	0.587 #
8)	B Heptachlo...	0.000	5.800	0	944723	N.D.	0.280 #
9)	A Endosulfan I	0.000	6.142	0	102992	N.D.	0.032 #
11)	B alpha-Chl...	0.000	6.088	0	633748	N.D.	0.184 #
18)	B Endrin al...	0.000	6.972f	0	3230519	N.D.	1.143 #
26)	Chlordane-4	0.000	6.088	0	633748	N.D.	1.167 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083119\
Data File : PL052123.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Aug 2019 16:34
Operator : SG\AJ
Sample : K4554-19
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 22:41:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

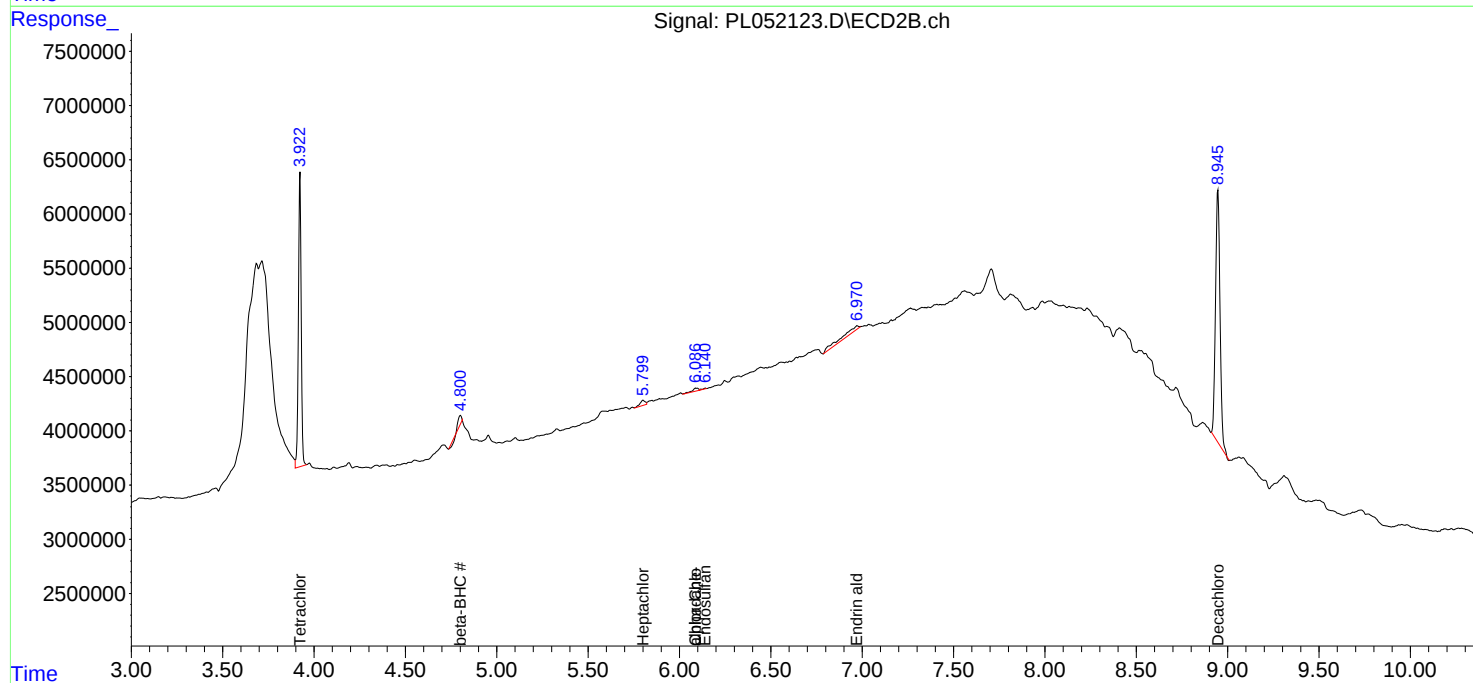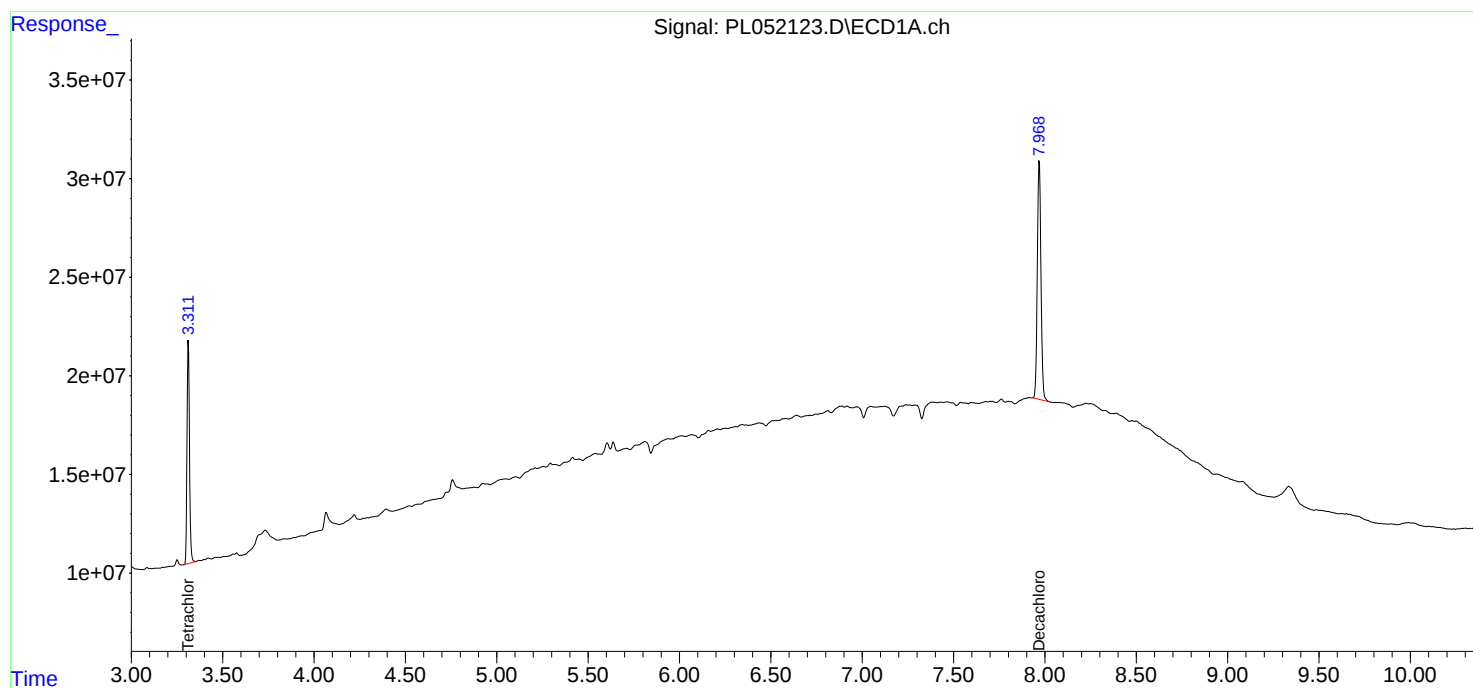

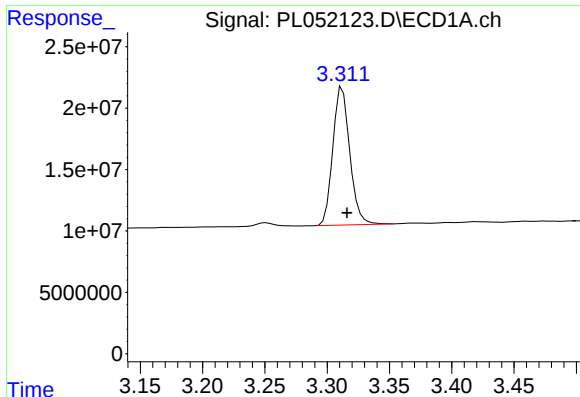


#1 Tetrachloro-m-xylene

R.T.: 3.312 min
Delta R.T.: -0.004 min
Response: 106313782
Conc: 12.42 ng/ml

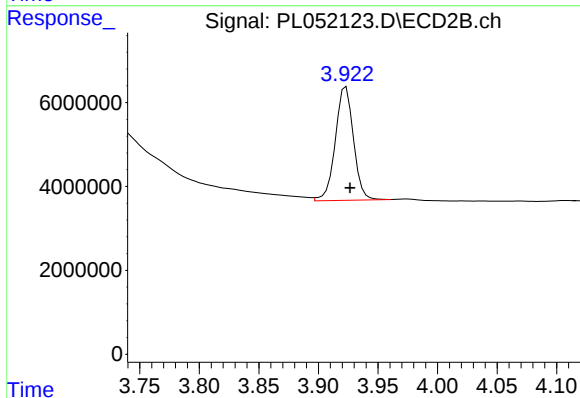


#1 Tetrachloro-m-xylene

R.T.: 3.923 min
Delta R.T.: -0.003 min
Response: 28699036
Conc: 13.14 ng/ml

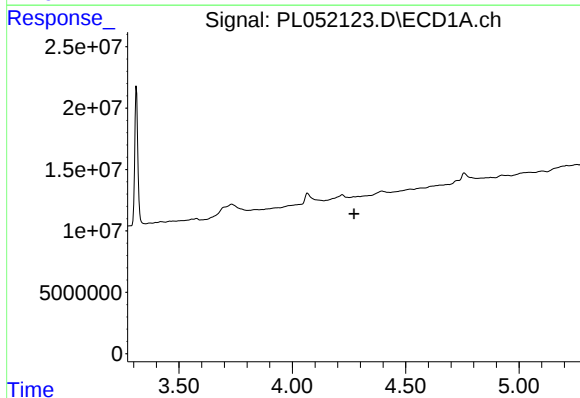


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.273 min
Response: 0
Conc: N.D.

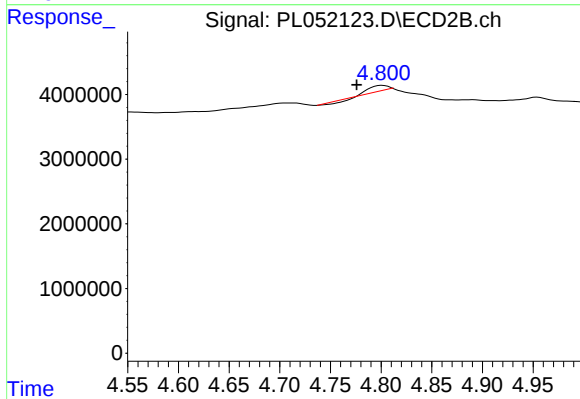


#6 beta-BHC

R.T.: 4.801 min
Delta R.T.: 0.025 min
Response: 854970
Conc: 0.59 ng/ml

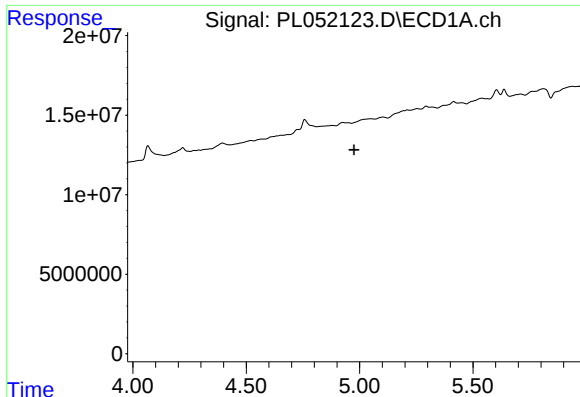


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.975 min
Response: 0
Conc: N.D.

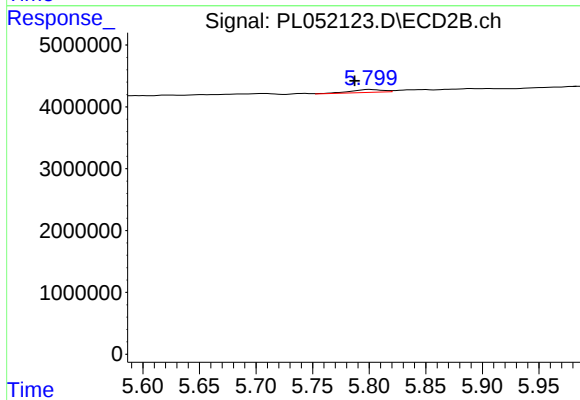


#8 Heptachlor epoxide

R.T.: 5.800 min
Delta R.T.: 0.013 min
Response: 944723
Conc: 0.28 ng/ml

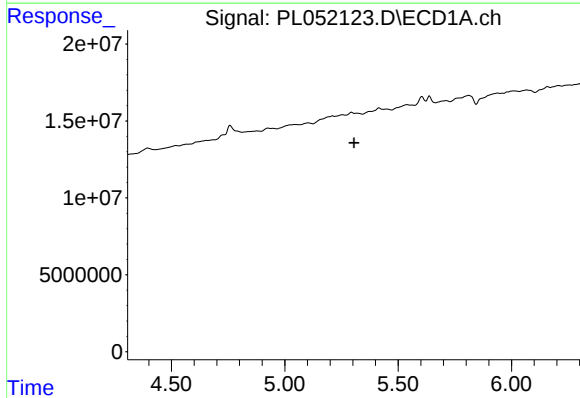


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.306 min
Response: 0
Conc: N.D.

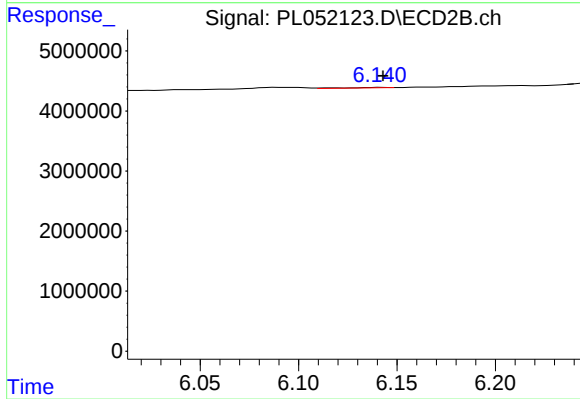


#9 Endosulfan I

R.T.: 6.142 min
Delta R.T.: -0.001 min
Response: 102992
Conc: 0.03 ng/ml

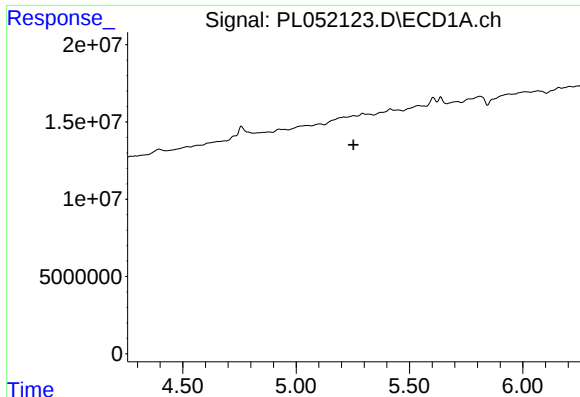


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.253 min
Response: 0
Conc: N.D.

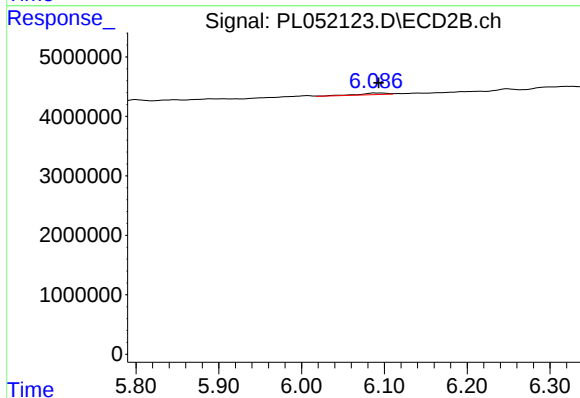


#11 alpha-Chlordane

R.T.: 6.088 min
Delta R.T.: -0.005 min
Response: 633748
Conc: 0.18 ng/ml

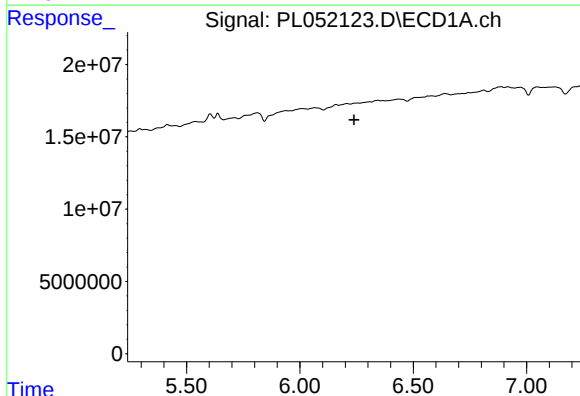


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.239 min
Response: 0
Conc: N.D.

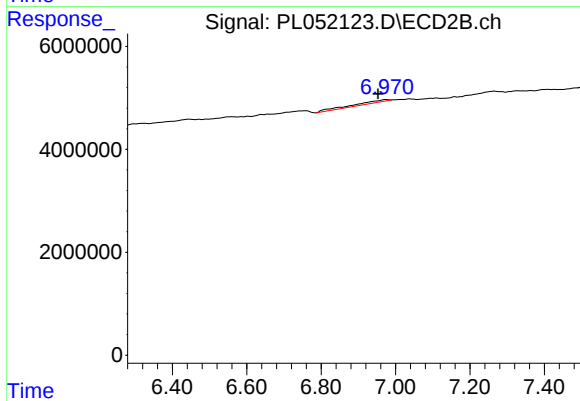


#18 Endrin aldehyde

R.T.: 6.972 min
Delta R.T.: 0.019 min
Response: 3230519
Conc: 1.14 ng/ml

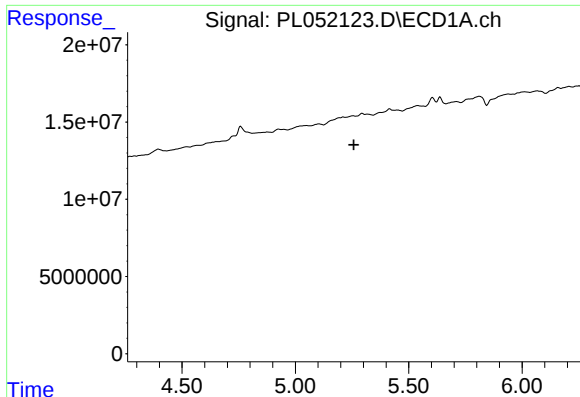


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.258 min
Response: 0
Conc: N.D.

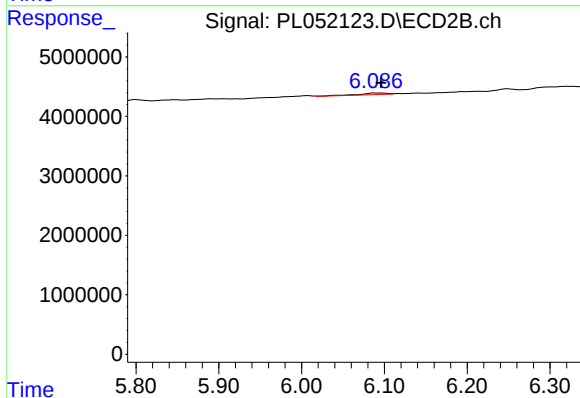


#26 Chlordane-4

R.T.: 6.088 min
Delta R.T.: -0.008 min
Response: 633748
Conc: 1.17 ng/ml

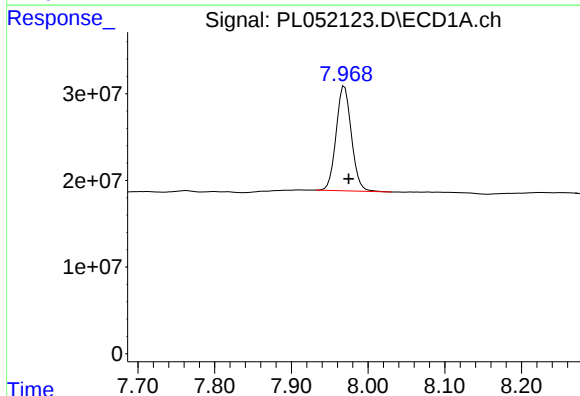

#28 Decachlorobiphenyl

R.T.: 7.969 min
Delta R.T.: -0.005 min
Response: 166556918
Conc: 13.72 ng/ml

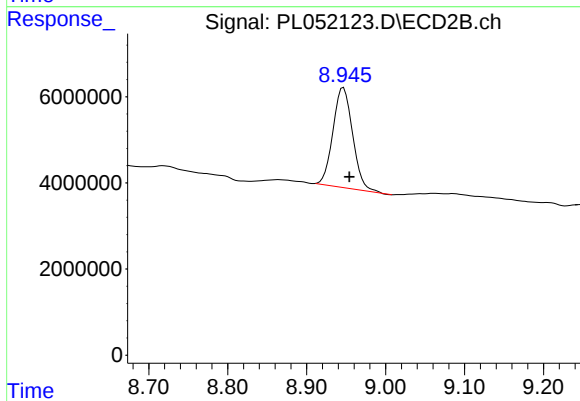

#28 Decachlorobiphenyl

R.T.: 8.947 min
Delta R.T.: -0.008 min
Response: 40256040
Conc: 13.23 ng/ml