

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083119\
 Data File : PL052127.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Aug 2019 17:31
 Operator : SG\AJ
 Sample : PB122728BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 22:42:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	3.313	3.923	165.1E6	43432261	19.286	19.879
28)	SA Decachlor...	7.969	8.946	233.7E6	55681744	19.254	18.293
Target Compounds							
6)	B beta-BHC	0.000	4.800f	0	747683	N.D.	0.513 #
8)	B Heptachlo...	0.000	5.799	0	1434879	N.D.	0.425 #
9)	A Endosulfan I	5.323f	6.152	7326966	154666	0.545	0.048 #
11)	B alpha-Chl...	0.000	6.113f	0	623577	N.D.	0.181 #
15)	B Endosulfa...	0.000	6.843	0	4339604	N.D.	1.317 #
18)	B Endrin al...	0.000	6.980f	0	4252248	N.D.	1.505 #
20)	A Methoxychlor	0.000	7.479f	0	82800	N.D.	0.049 #
21)	B Endrin ke...	0.000	7.641	0	2195921	N.D.	0.686 #
22)	Mirex	0.000	8.084	0	4384061	N.D.	1.802 #
26)	Chlordane-4	0.000	6.113f	0	623577	N.D.	1.148 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083119\
Data File : PL052127.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Aug 2019 17:31
Operator : SG\AJ
Sample : PB122728BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 22:42:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

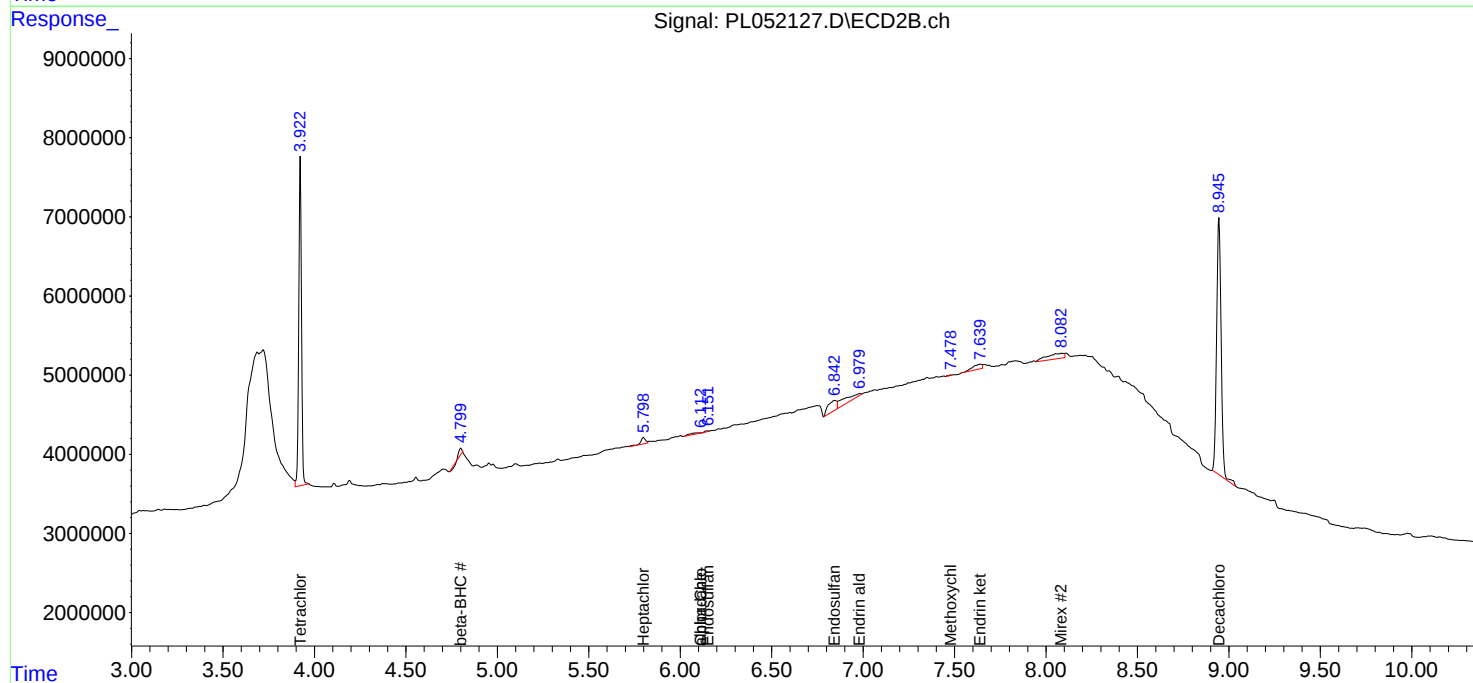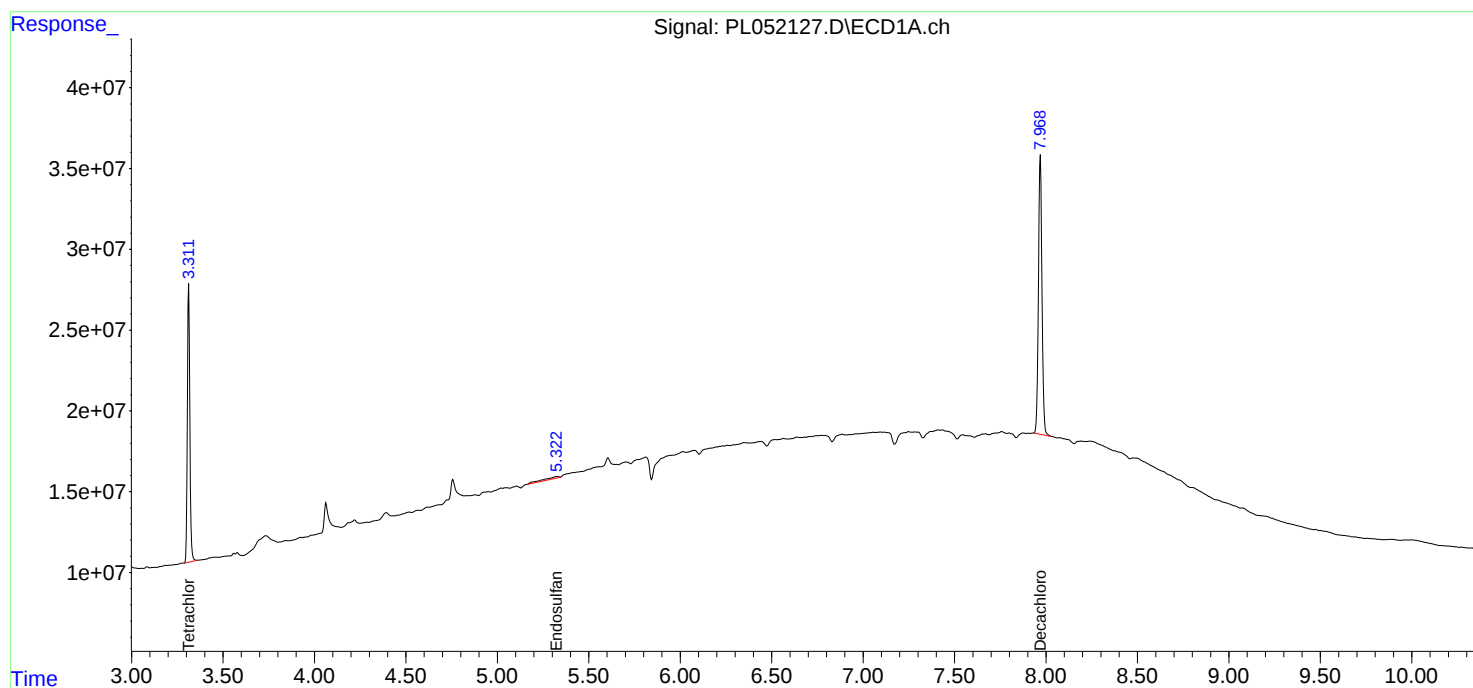

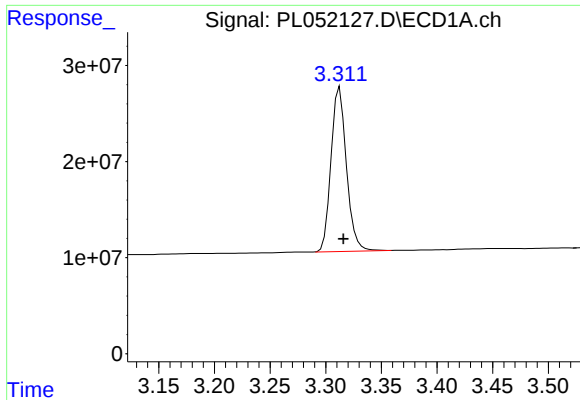


#1 Tetrachloro-m-xylene

R.T.: 3.313 min
Delta R.T.: -0.003 min
Response: 165064055
Conc: 19.29 ng/ml

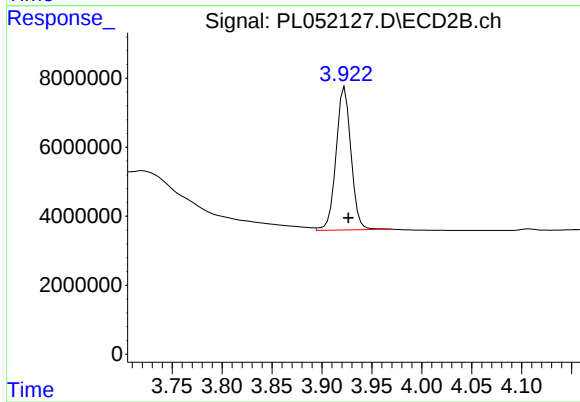


#1 Tetrachloro-m-xylene

R.T.: 3.923 min
Delta R.T.: -0.004 min
Response: 43432261
Conc: 19.88 ng/ml

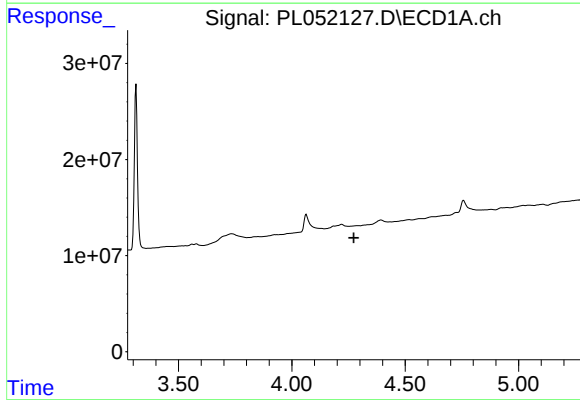


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.273 min
Response: 0
Conc: N.D.

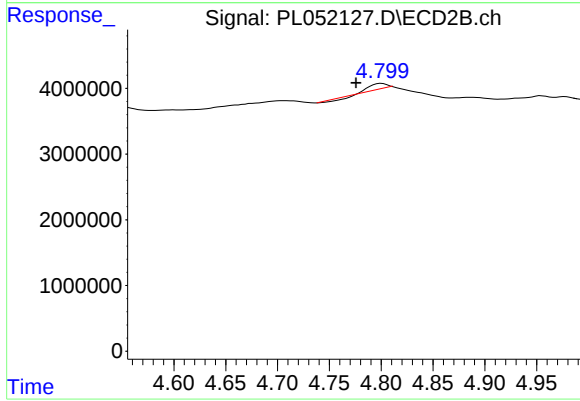


#6 beta-BHC

R.T.: 4.800 min
Delta R.T.: 0.025 min
Response: 747683
Conc: 0.51 ng/ml

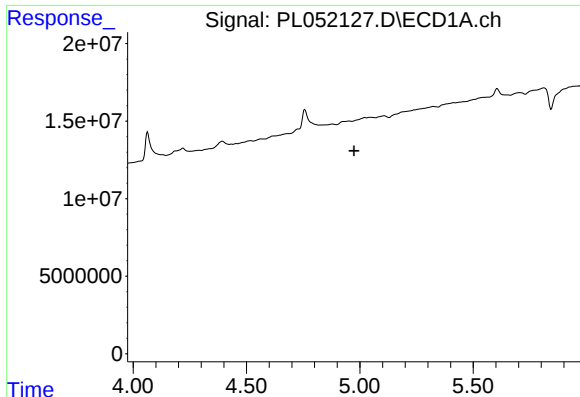


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 4.975 min
Response: 0
Conc: N.D.

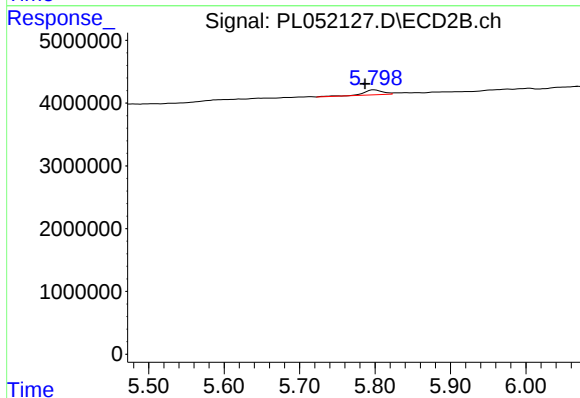


#8 Heptachlor epoxide

R.T.: 5.799 min
Delta R.T.: 0.012 min
Response: 1434879
Conc: 0.43 ng/ml

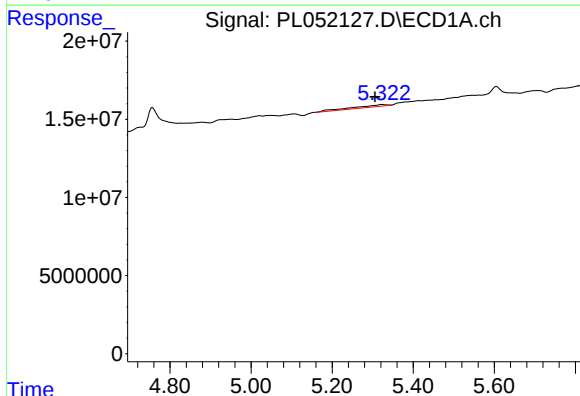


#9 Endosulfan I

R.T.: 5.323 min
Delta R.T.: 0.017 min
Response: 7326966
Conc: 0.55 ng/ml

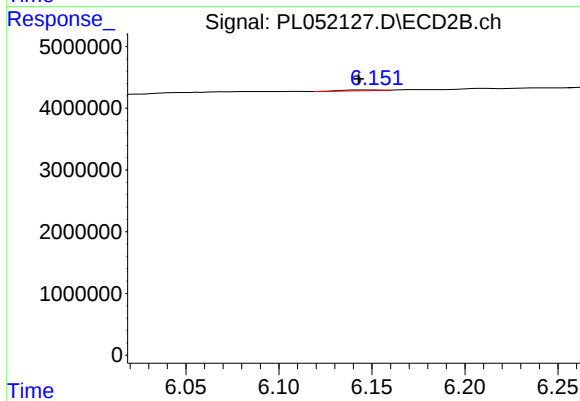


#9 Endosulfan I

R.T.: 6.152 min
Delta R.T.: 0.009 min
Response: 154666
Conc: 0.05 ng/ml

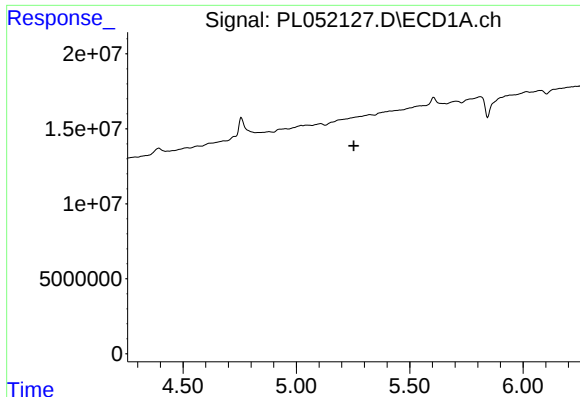


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.253 min
Response: 0
Conc: N.D.

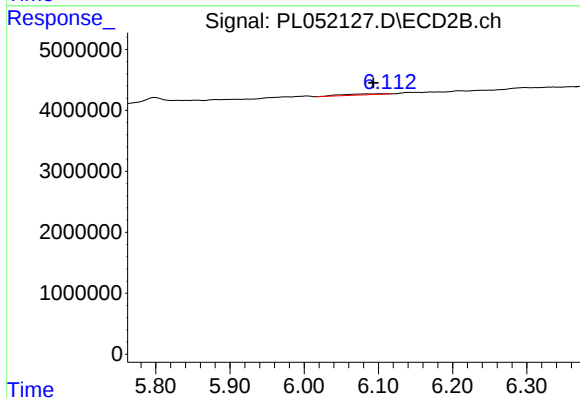


#11 alpha-Chlordane

R.T.: 6.113 min
Delta R.T.: 0.020 min
Response: 623577
Conc: 0.18 ng/ml

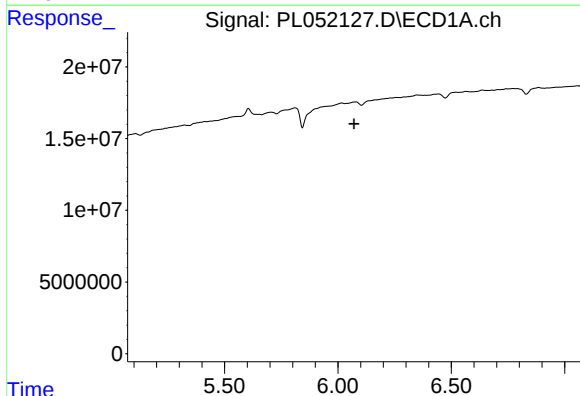


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.072 min
Response: 0
Conc: N.D.

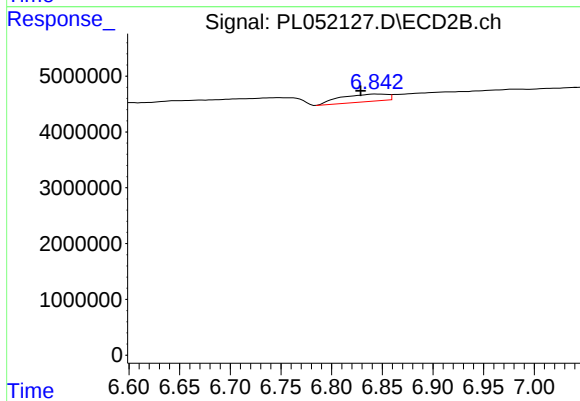


#15 Endosulfan II

R.T.: 6.843 min
Delta R.T.: 0.015 min
Response: 4339604
Conc: 1.32 ng/ml

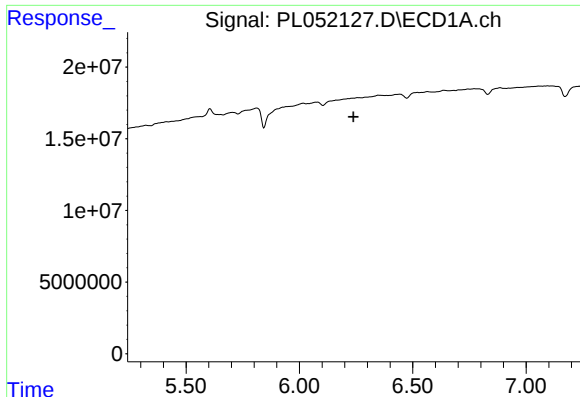


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.239 min
Response: 0
Conc: N.D.

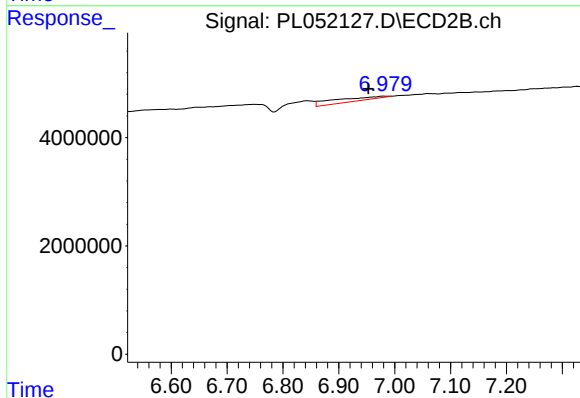


#18 Endrin aldehyde

R.T.: 6.980 min
Delta R.T.: 0.027 min
Response: 4252248
Conc: 1.50 ng/ml

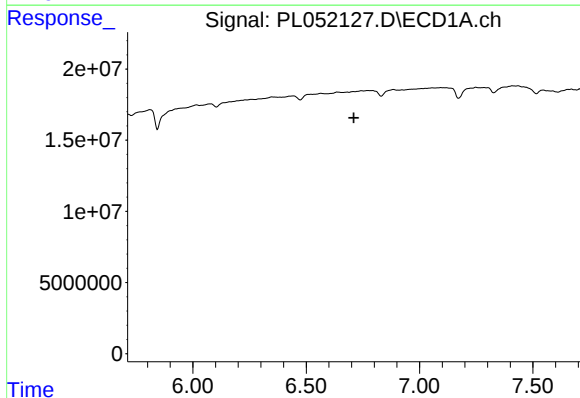


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.710 min
Response: 0
Conc: N.D.

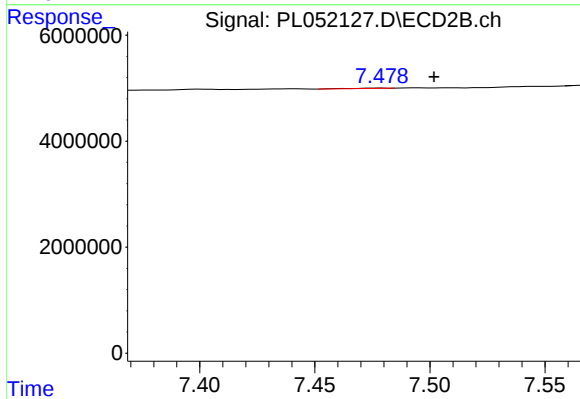


#20 Methoxychlor

R.T.: 7.479 min
Delta R.T.: -0.023 min
Response: 82800
Conc: 0.05 ng/ml

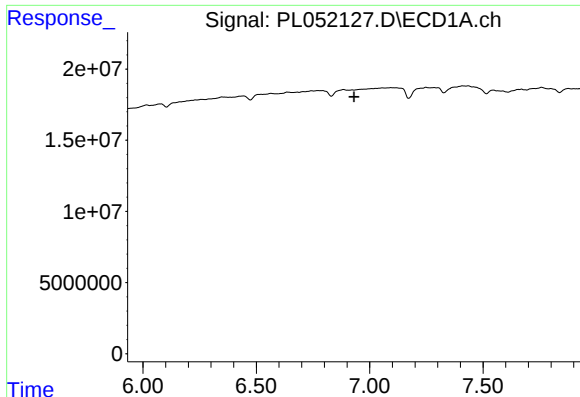


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.931 min
Response: 0
Conc: N.D.

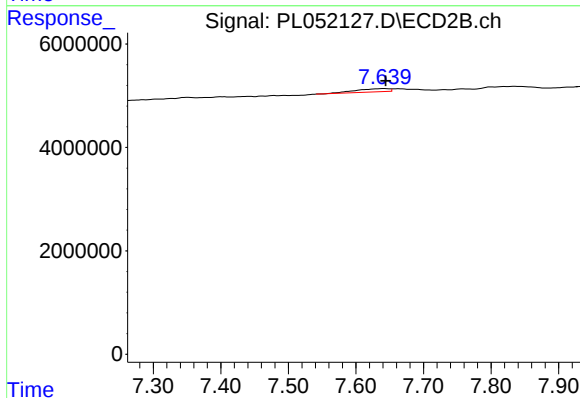


#21 Endrin ketone

R.T.: 7.641 min
Delta R.T.: -0.003 min
Response: 2195921
Conc: 0.69 ng/ml

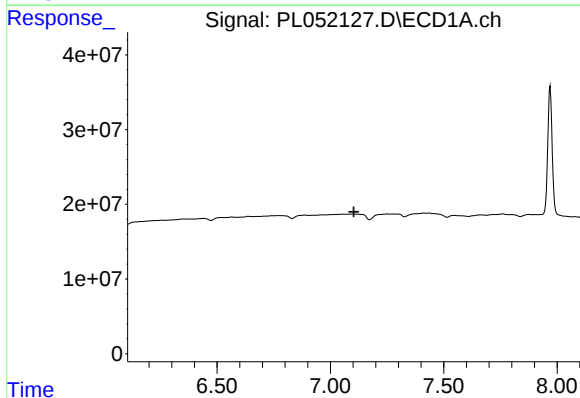


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 7.104 min
Response: 0
Conc: N.D.

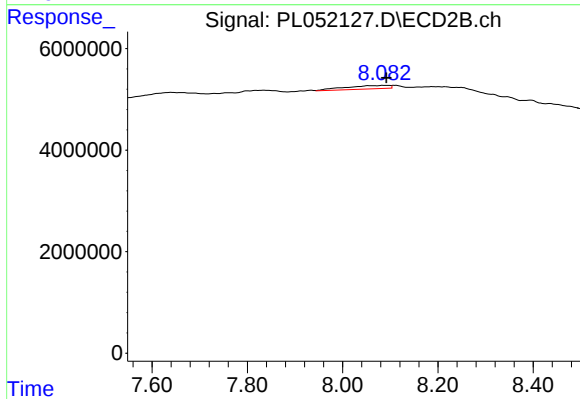


#22 Mirex

R.T.: 8.084 min
Delta R.T.: -0.008 min
Response: 4384061
Conc: 1.80 ng/ml

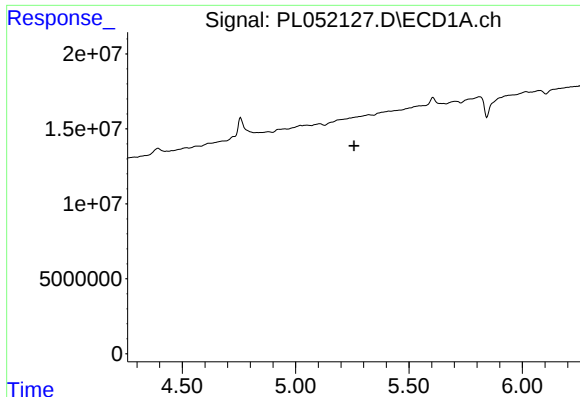


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.258 min
Response: 0
Conc: N.D.

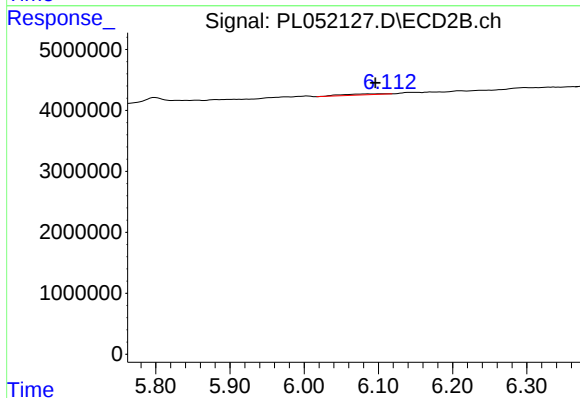


#26 Chlordane-4

R.T.: 6.113 min
Delta R.T.: 0.017 min
Response: 623577
Conc: 1.15 ng/ml

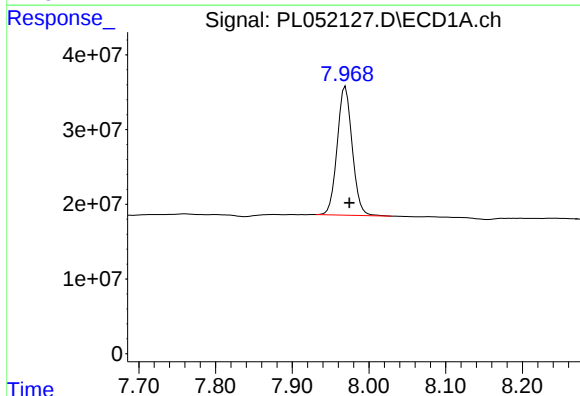

#28 Decachlorobiphenyl

R.T.: 7.969 min
Delta R.T.: -0.005 min
Response: 233703753
Conc: 19.25 ng/ml

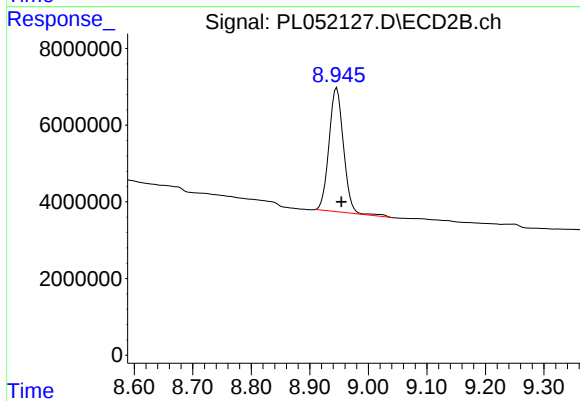

#28 Decachlorobiphenyl

R.T.: 8.946 min
Delta R.T.: -0.008 min
Response: 55681744
Conc: 18.29 ng/ml