

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083119\
 Data File : PL052137.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Aug 2019 19:52
 Operator : SG\AJ
 Sample : K4554-23
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 22:44:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	3.312	3.922	97798753	26638067	11.427	12.192
28)	SA Decachlor...	7.968	8.946	144.2E6	32737366	11.880	10.755
Target Compounds							
6)	B beta-BHC	0.000	4.799f	0	1107006	N.D.	0.760 #
8)	B Heptachlo...	0.000	5.798	0	865915	N.D.	0.257 #
9)	A Endosulfan I	5.294	0.000	3845038	0	0.286	N.D. #
11)	B alpha-Chl...	0.000	6.072f	0	517830	N.D.	0.150 #
15)	B Endosulfa...	0.000	6.844f	0	2667312	N.D.	0.809 #
18)	B Endrin al...	0.000	6.973f	0	2857433	N.D.	1.011 #
26)	Chlordane-4	0.000	6.072f	0	517830	N.D.	0.953 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083119\
Data File : PL052137.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Aug 2019 19:52
Operator : SG\AJ
Sample : K4554-23
Misc :
ALS Vial : 28 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 22:44:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

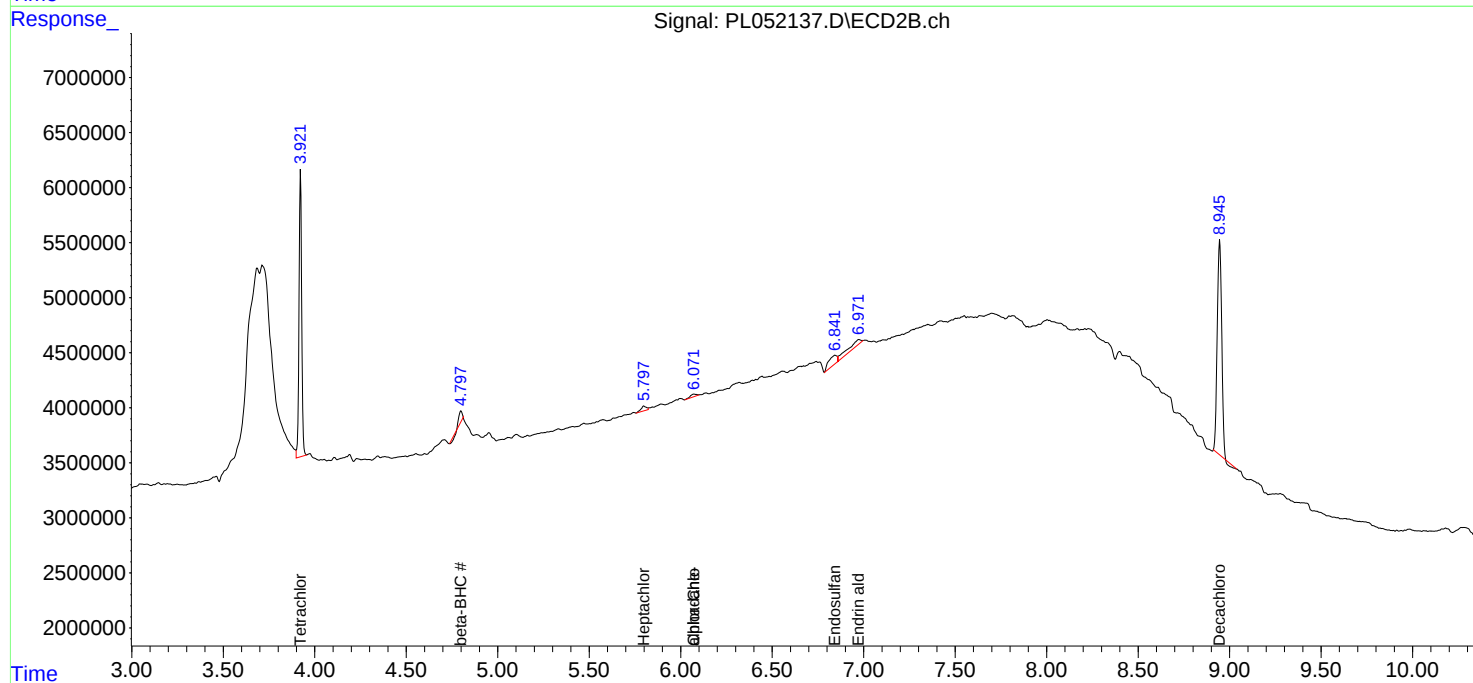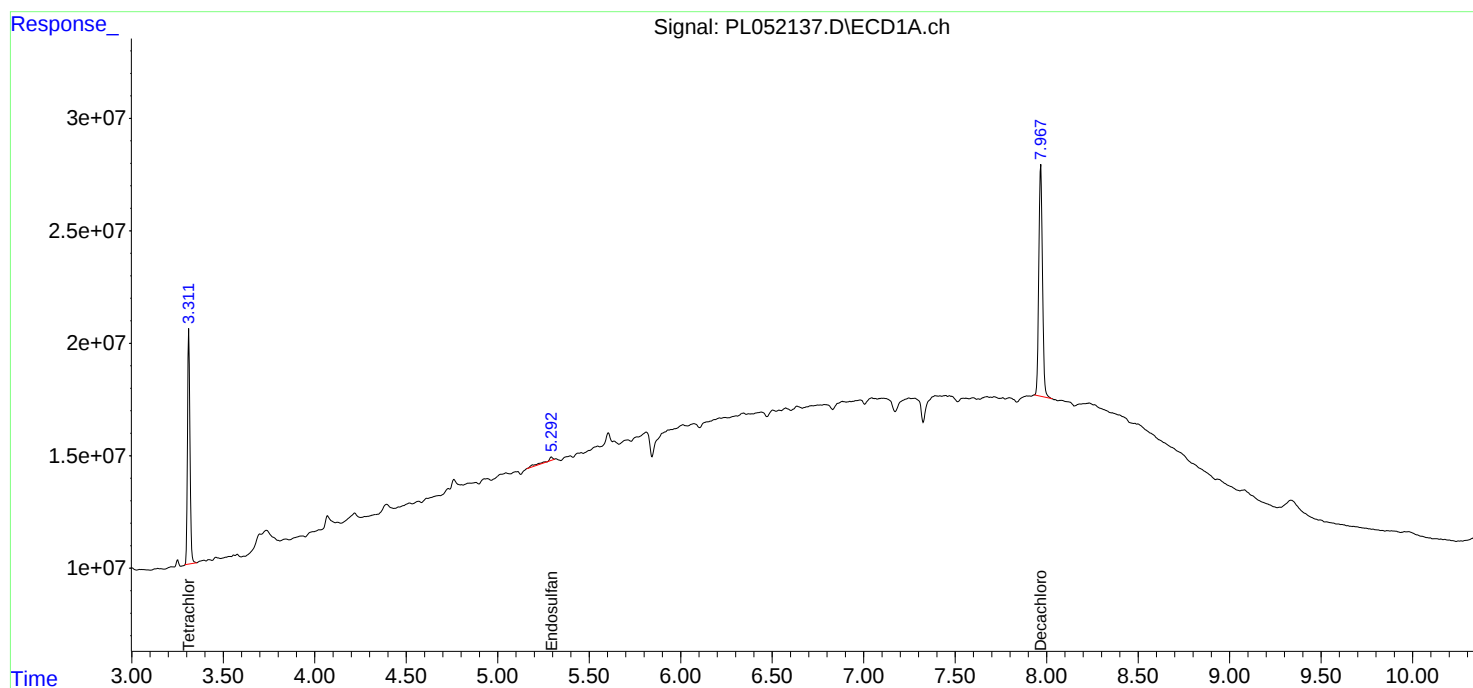

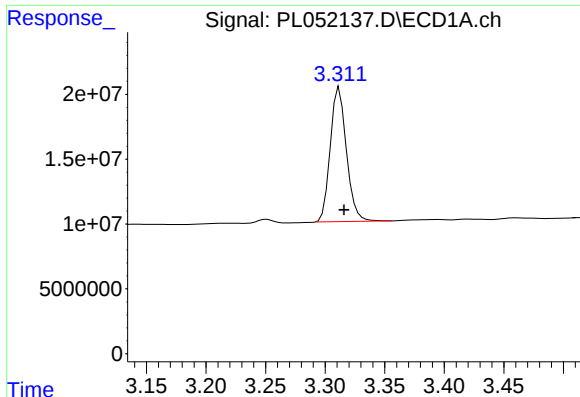


#1 Tetrachloro-m-xylene

R.T.: 3.312 min
Delta R.T.: -0.004 min
Response: 97798753
Conc: 11.43 ng/ml

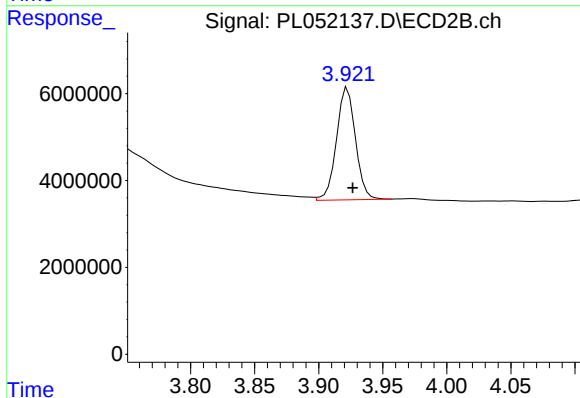


#1 Tetrachloro-m-xylene

R.T.: 3.922 min
Delta R.T.: -0.004 min
Response: 26638067
Conc: 12.19 ng/ml

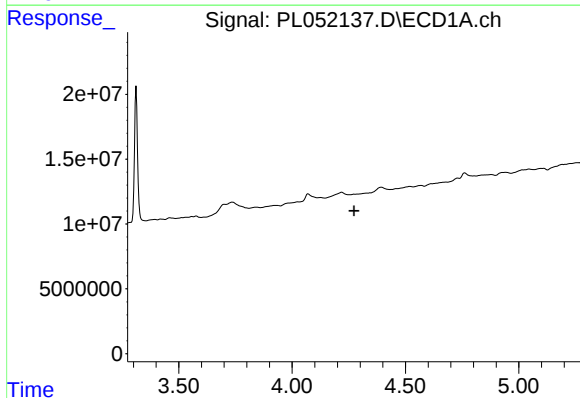


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.273 min
Response: 0
Conc: N.D.

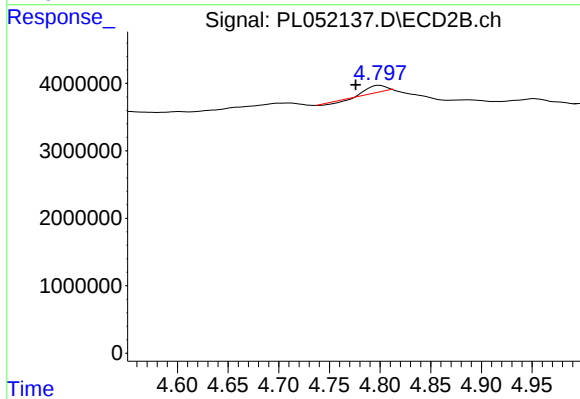


#6 beta-BHC

R.T.: 4.799 min
Delta R.T.: 0.024 min
Response: 1107006
Conc: 0.76 ng/ml

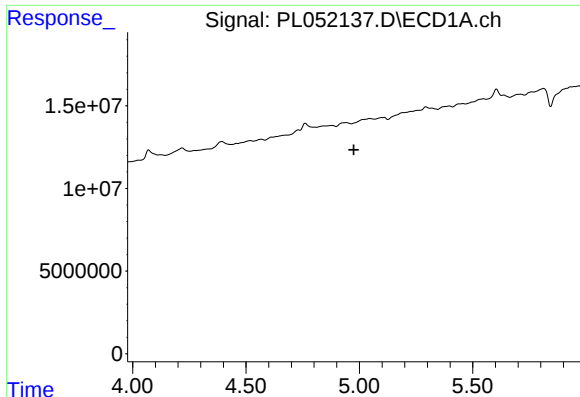


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.975 min
Response: 0
Conc: N.D.

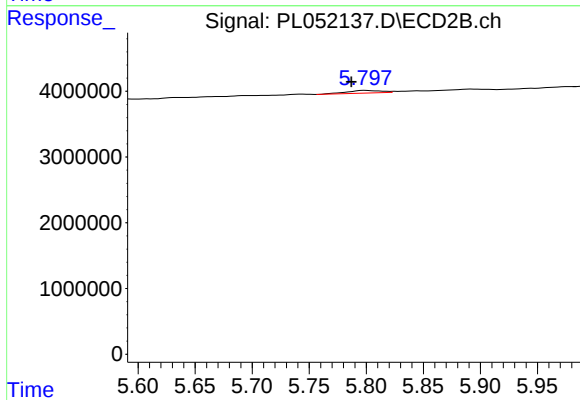


#8 Heptachlor epoxide

R.T.: 5.798 min
Delta R.T.: 0.011 min
Response: 865915
Conc: 0.26 ng/ml

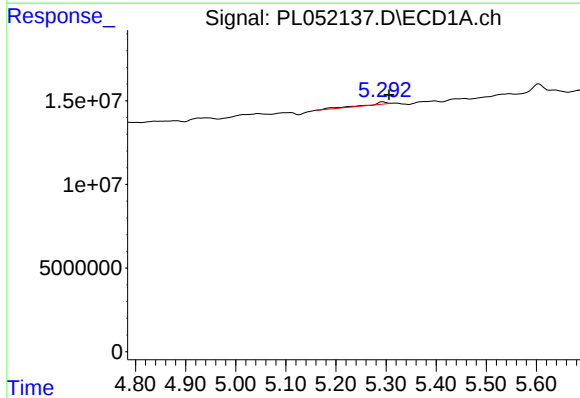


#9 Endosulfan I

R.T.: 5.294 min
Delta R.T.: -0.012 min
Response: 3845038
Conc: 0.29 ng/ml

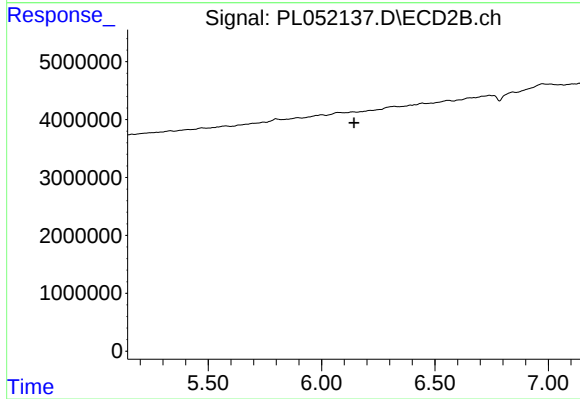


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.143 min
Response: 0
Conc: N.D.

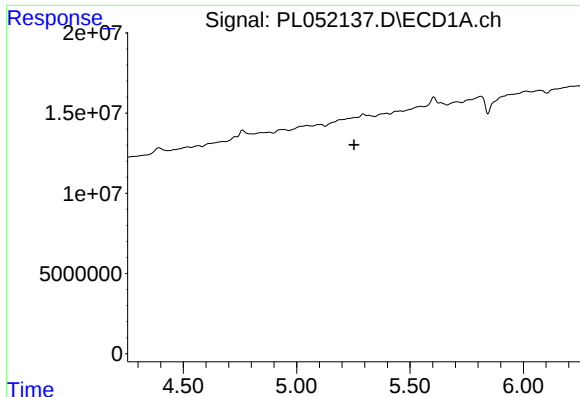


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.253 min
Response: 0
Conc: N.D.

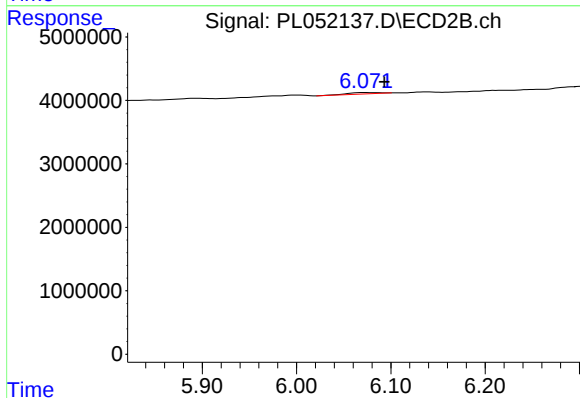


#11 alpha-Chlordane

R.T.: 6.072 min
Delta R.T.: -0.021 min
Response: 517830
Conc: 0.15 ng/ml

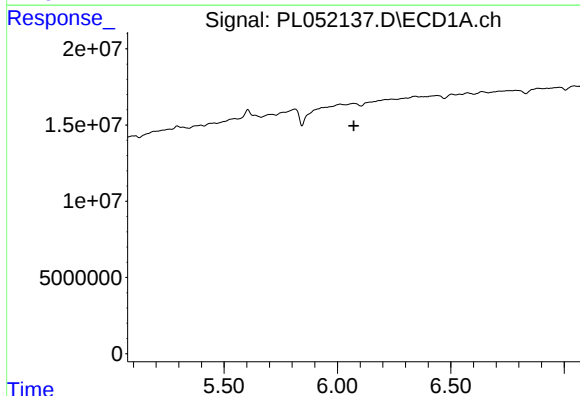


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.072 min
Response: 0
Conc: N.D.

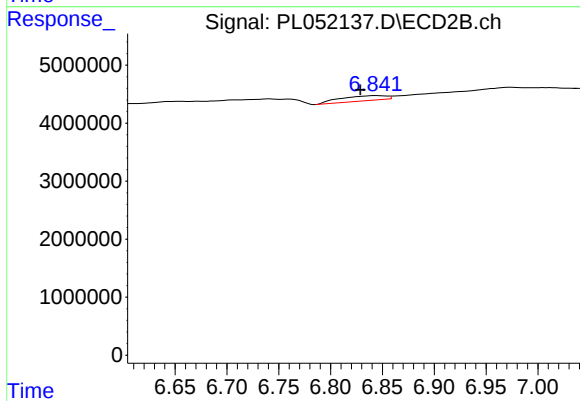


#15 Endosulfan II

R.T.: 6.844 min
Delta R.T.: 0.015 min
Response: 2667312
Conc: 0.81 ng/ml

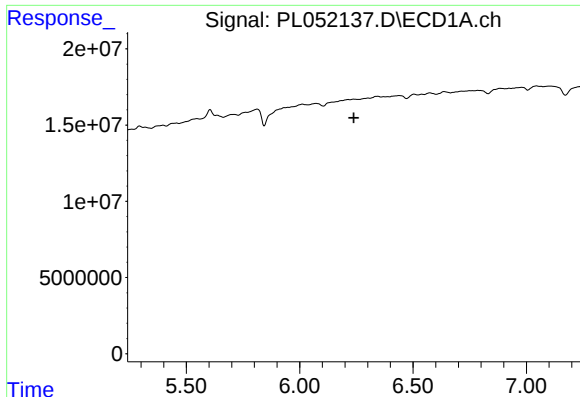


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.239 min
Response: 0
Conc: N.D.

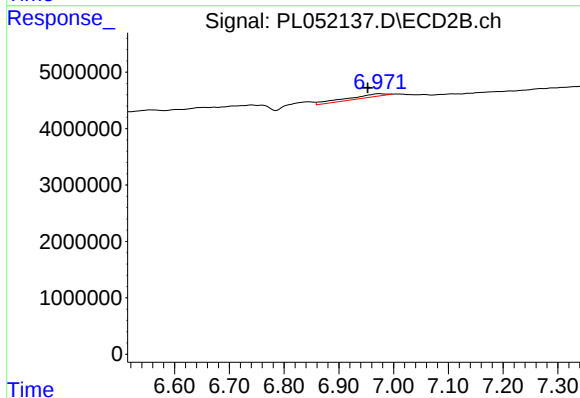


#18 Endrin aldehyde

R.T.: 6.973 min
Delta R.T.: 0.020 min
Response: 2857433
Conc: 1.01 ng/ml

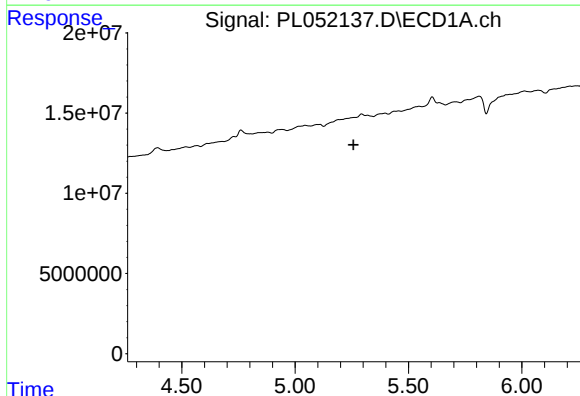


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.258 min
Response: 0
Conc: N.D.

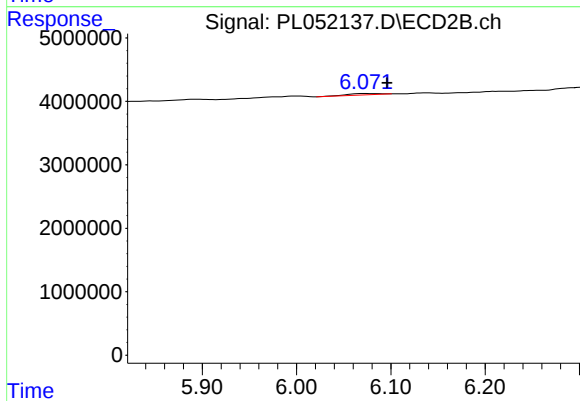


#26 Chlordane-4

R.T.: 6.072 min
Delta R.T.: -0.024 min
Response: 517830
Conc: 0.95 ng/ml

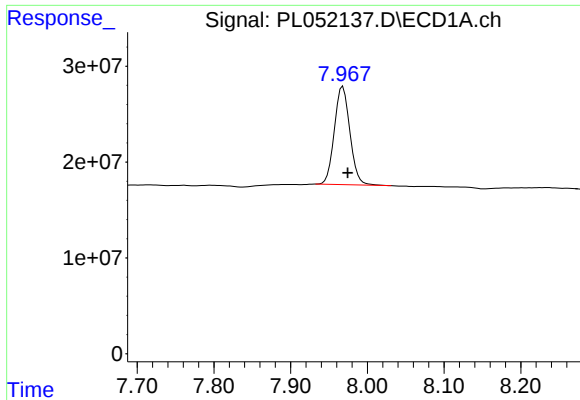

#28 Decachlorobiphenyl

R.T.: 7.968 min
Delta R.T.: -0.007 min
Response: 144193067
Conc: 11.88 ng/ml

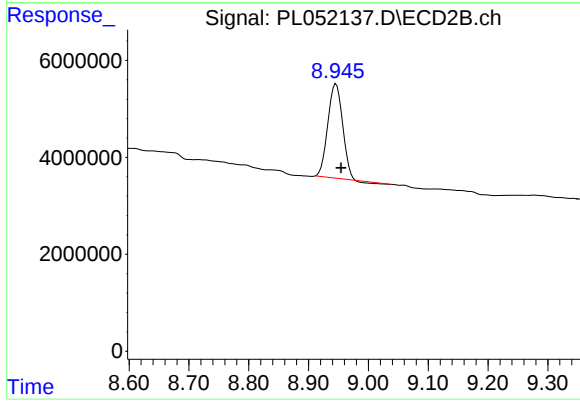

#28 Decachlorobiphenyl

R.T.: 8.946 min
Delta R.T.: -0.008 min
Response: 32737366
Conc: 10.76 ng/ml