

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083119\
 Data File : PL052164.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Sep 2019 02:14
 Operator : SG\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 03:45:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	3.312	3.923	228.4E6	61682967	26.687	28.233
28)	SA Decachlor...	7.968	8.945	216.2E6	56619715	17.809	18.601
Target Compounds							
6)	B beta-BHC	0.000	4.800f	0	545496	N.D.	0.374 #
8)	B Heptachlo...	0.000	5.782	0	6625966	N.D.	1.963 #
14)	MA Endrin	0.000	6.615	0	554860	N.D.	0.183 #
18)	B Endrin al...	0.000	6.951	0	643712	N.D.	0.228 #
20)	A Methoxychlor	0.000	7.522f	0	295718	N.D.	0.176 #
22)	Mirex	0.000	8.119f	0	1406713	N.D.	0.578 #
27)	Chlordane-5	0.000	6.917f	0	1495844	N.D.	15.173 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083119\
Data File : PL052164.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Sep 2019 02:14
Operator : SG\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 03:45:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

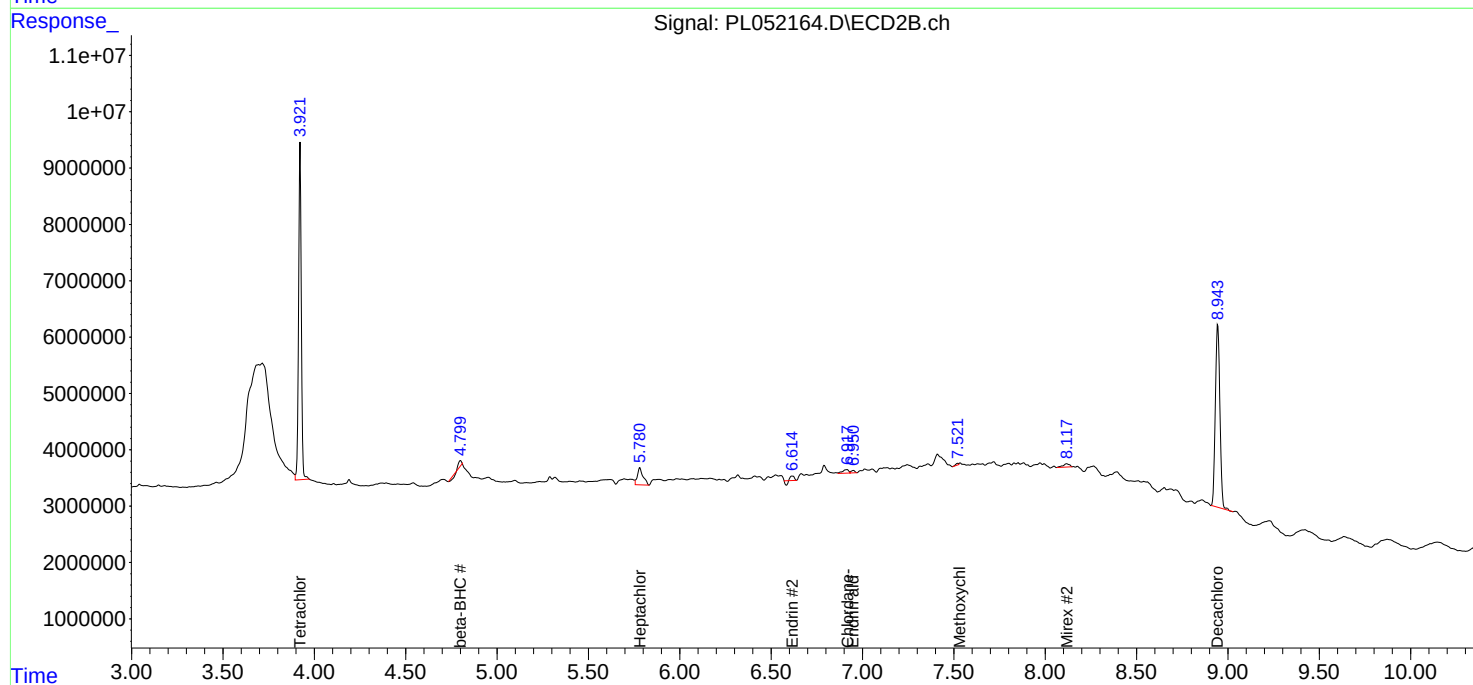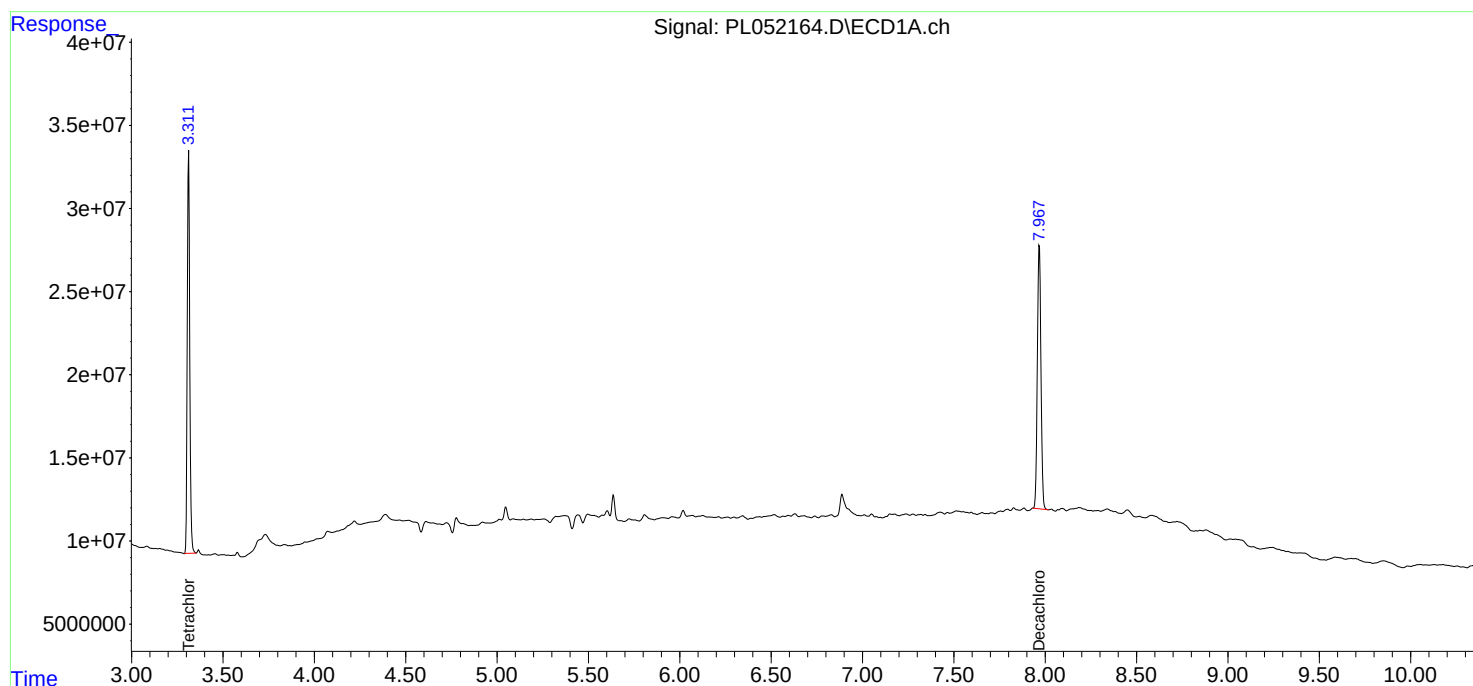

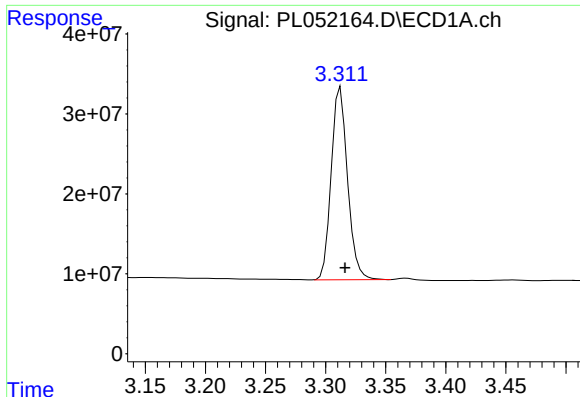


#1 Tetrachloro-m-xylene

R.T.: 3.312 min
Delta R.T.: -0.004 min
Response: 228406135
Conc: 26.69 ng/ml

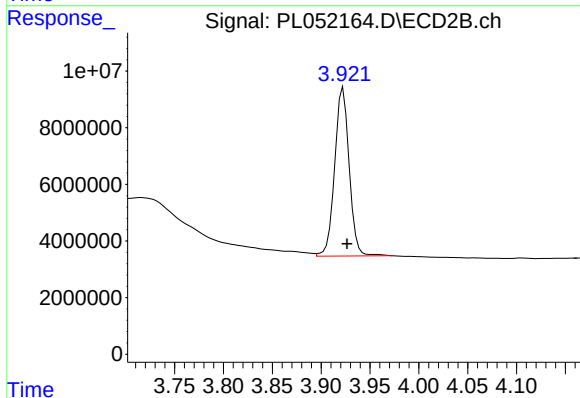


#1 Tetrachloro-m-xylene

R.T.: 3.923 min
Delta R.T.: -0.004 min
Response: 61682967
Conc: 28.23 ng/ml

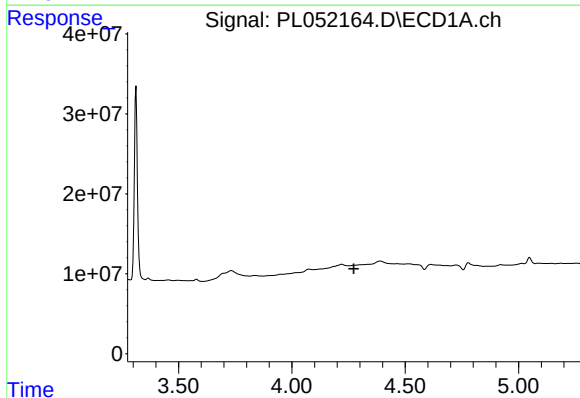


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.273 min
Response: 0
Conc: N.D.

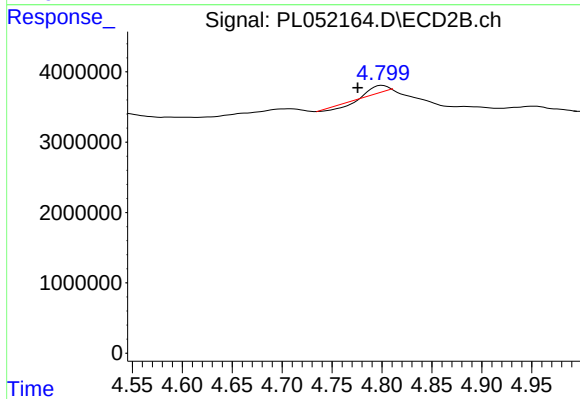


#6 beta-BHC

R.T.: 4.800 min
Delta R.T.: 0.025 min
Response: 545496
Conc: 0.37 ng/ml

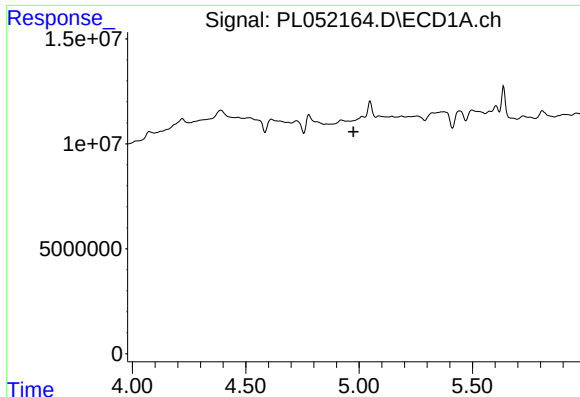


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.975 min
Response: 0
Conc: N.D.

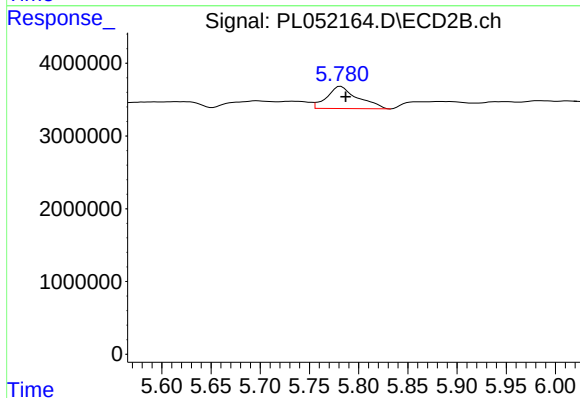


#8 Heptachlor epoxide

R.T.: 5.782 min
Delta R.T.: -0.005 min
Response: 6625966
Conc: 1.96 ng/ml

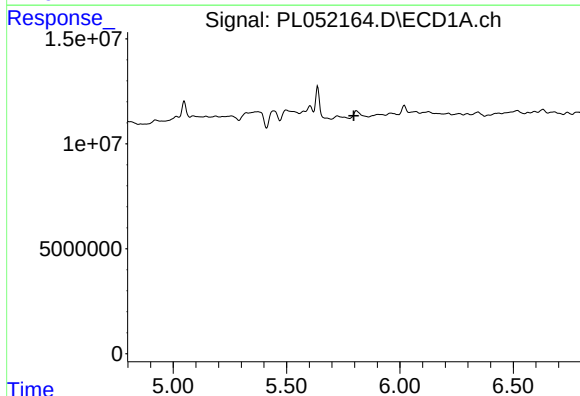


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 5.796 min
Response: 0
Conc: N.D.

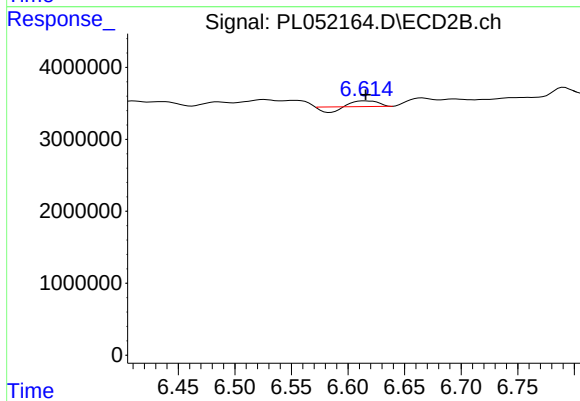


#14 Endrin

R.T.: 6.615 min
Delta R.T.: 0.000 min
Response: 554860
Conc: 0.18 ng/ml

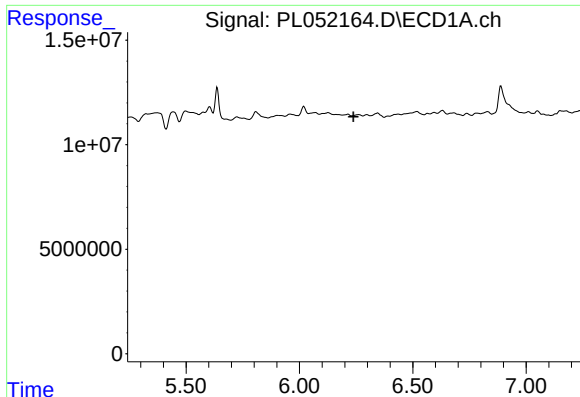


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.239 min
Response: 0
Conc: N.D.

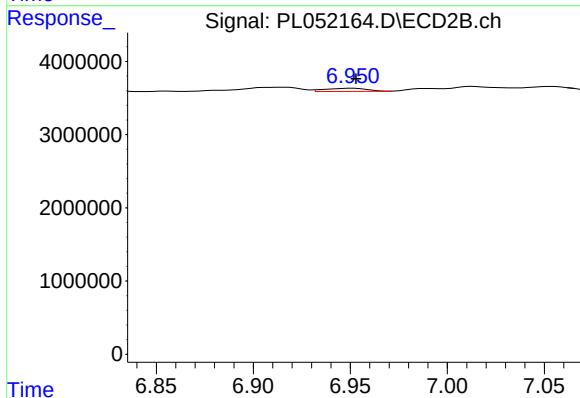


#18 Endrin aldehyde

R.T.: 6.951 min
Delta R.T.: -0.002 min
Response: 643712
Conc: 0.23 ng/ml

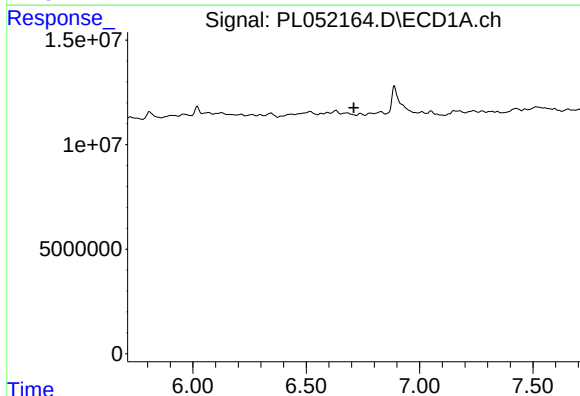


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 6.710 min
Response: 0
Conc: N.D.

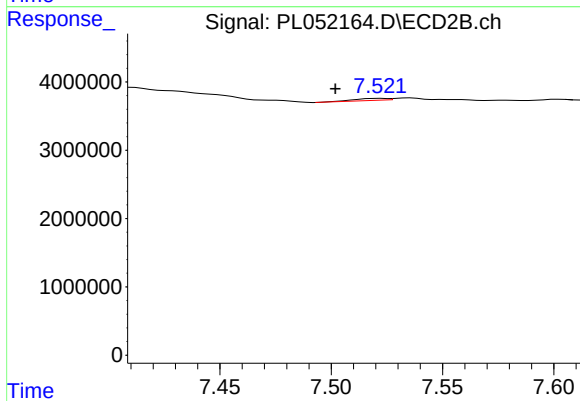

#20 Methoxychlor

R.T.: 7.522 min
Delta R.T.: 0.020 min
Response: 295718
Conc: 0.18 ng/ml

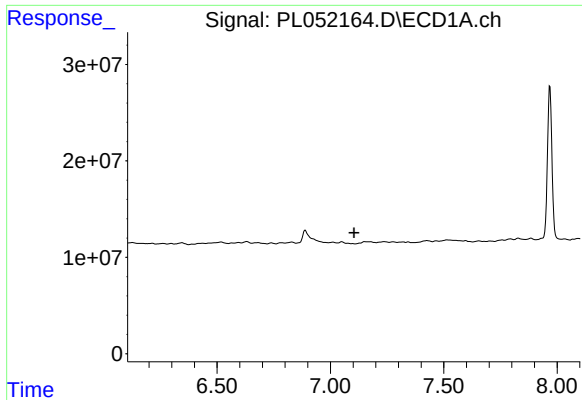


#22 Mirex

R.T.: 0.000 min

Exp R.T. : 7.104 min

Response: 0

Conc: N.D.

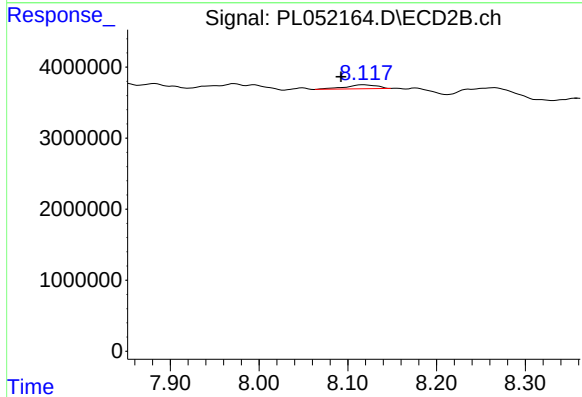


#22 Mirex

R.T.: 8.119 min

Delta R.T.: 0.026 min

Response: 1406713

Conc: 0.58 ng/ml

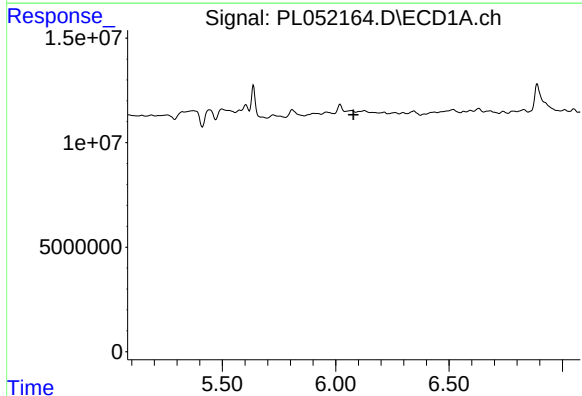


#27 Chlordane-5

R.T.: 0.000 min

Exp R.T. : 6.079 min

Response: 0

Conc: N.D.

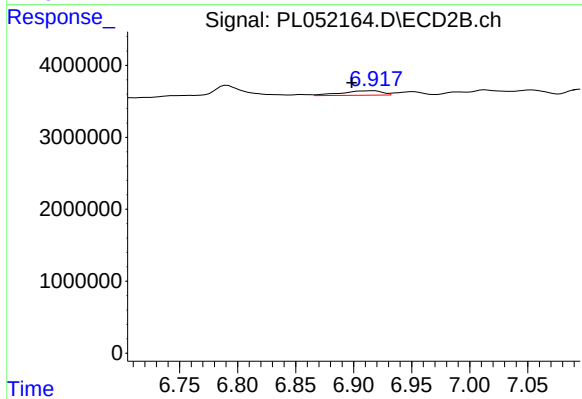


#27 Chlordane-5

R.T.: 6.917 min

Delta R.T.: 0.019 min


Response: 1495844

Conc: 15.17 ng/ml

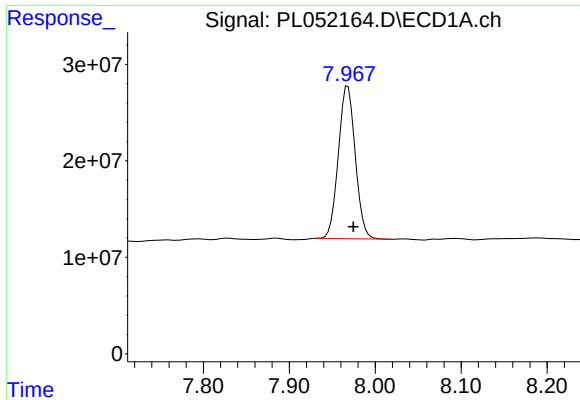

#28 Decachlorobiphenyl

R.T.: 7.968 min
Delta R.T.: -0.006 min
Response: 216166131
Conc: 17.81 ng/ml

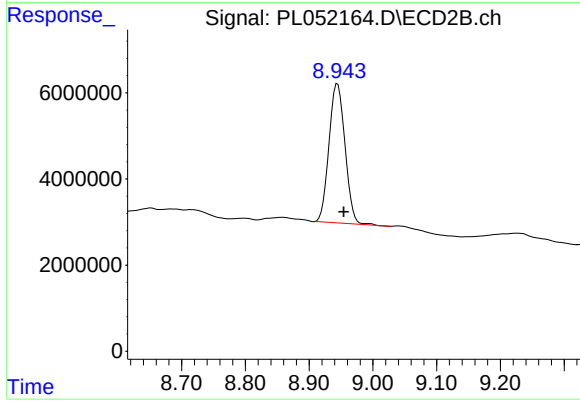

#28 Decachlorobiphenyl

R.T.: 8.945 min
Delta R.T.: -0.010 min
Response: 56619715
Conc: 18.60 ng/ml