

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083120\
 Data File : PL061080.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Aug 2020 12:26
 Operator : DD\AJ
 Sample : L3508-25
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 17:14:02 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 25 16:59:57 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.462	4.009	26751011	35932963	14.496	13.826
28)	SA Decachlor...	8.215	9.097	24732696	35006956	14.682	16.591
Target Compounds							
5)	MB Aldrin	0.000	5.474f	0	3698210	N.D.	1.097 #
10)	B gamma-Chl...	0.000	6.124	0	3101885	N.D.	0.999 #
11)	B alpha-Chl...	0.000	6.198	0	3786391	N.D.	1.218 #
12)	B 4,4'-DDE	0.000	6.351	0	3150394	N.D.	1.090 #
16)	A 4,4'-DDD	0.000	6.850	0	1872351	N.D.	0.802 #
17)	MA 4,4'-DDT	0.000	7.119f	0	1311293	N.D.	0.569 #
24)	Chlordane-2	0.000	5.474	0	3698210	N.D.	35.936 #
25)	Chlordane-3	0.000	6.124	0	3101885	N.D.	7.761 #
26)	Chlordane-4	0.000	6.198	0	3786391	N.D.	7.876 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083120\
Data File : PL061080.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Aug 2020 12:26
Operator : DD\AJ
Sample : L3508-25
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 17:14:02 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
Quant Title : GC Extractables
QLast Update : Tue Aug 25 16:59:57 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

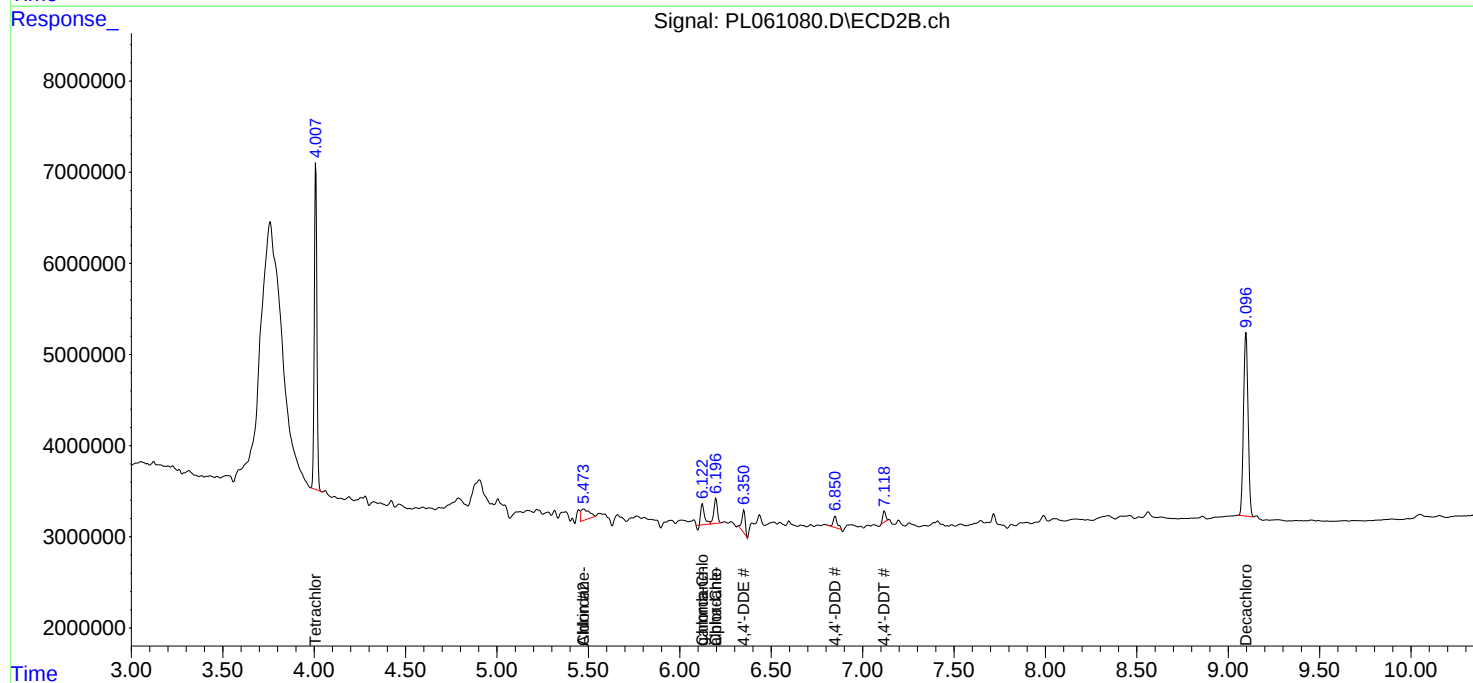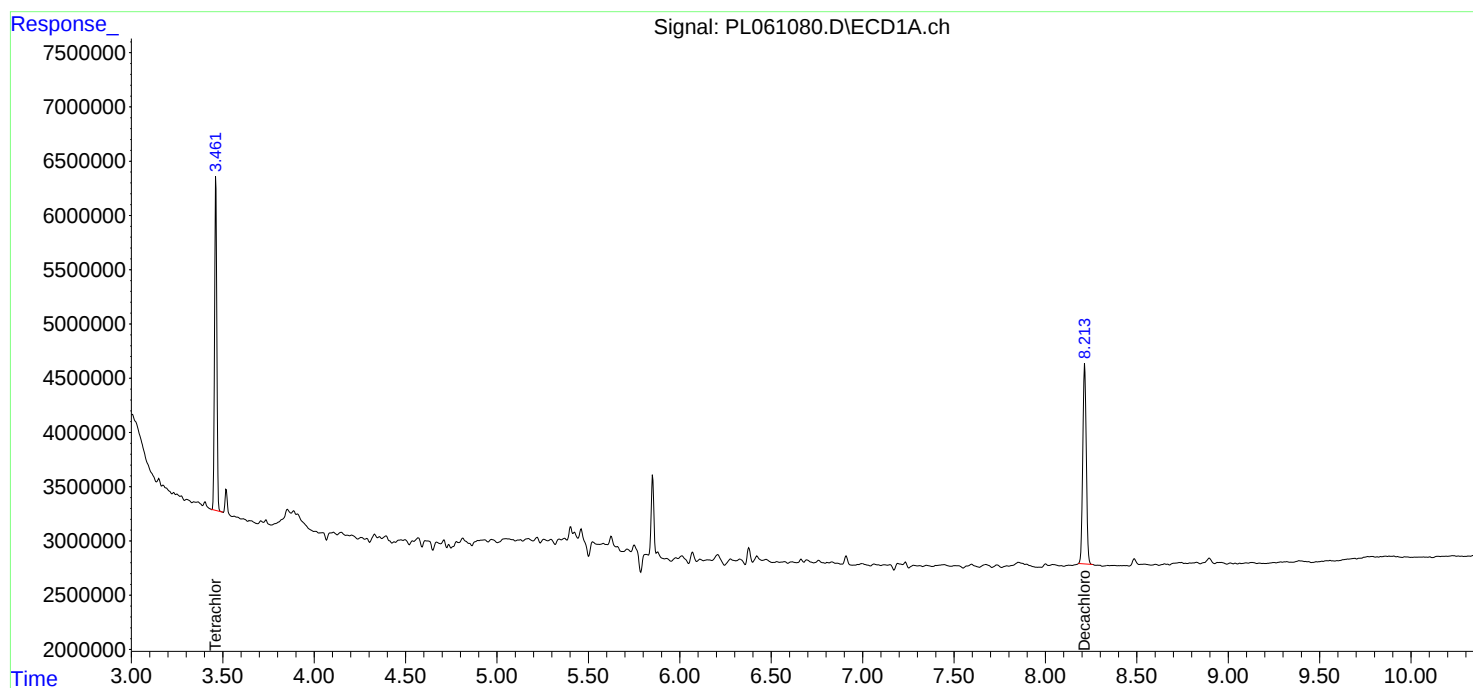


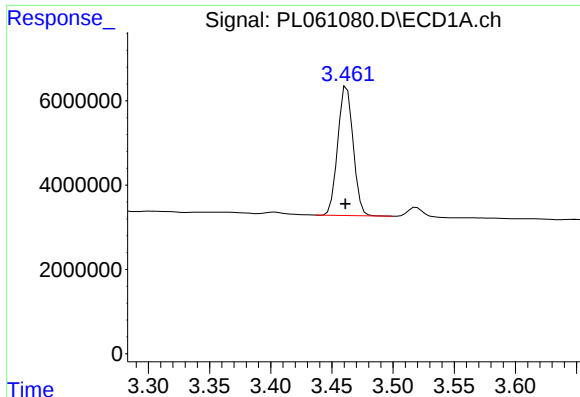

#1 Tetrachloro-m-xylene


R.T.: 3.462 min
Delta R.T.: 0.001 min
Response: 26751011
Conc: 14.50 ng/ml

Instrument :
ECD_L
ClientSampleId :

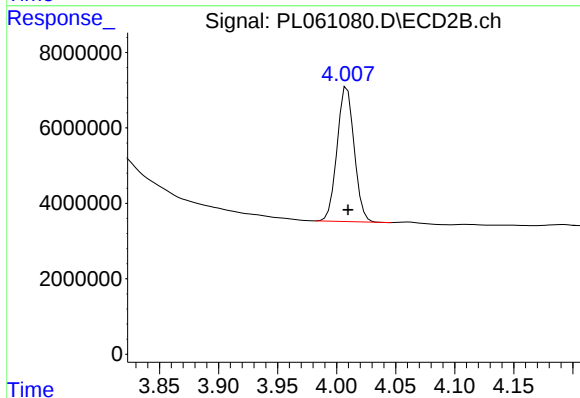


#1 Tetrachloro-m-xylene

R.T.: 4.009 min
Delta R.T.: 0.000 min
Response: 35932963
Conc: 13.83 ng/ml

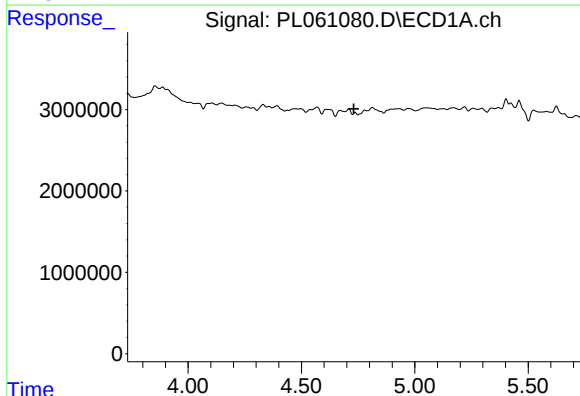


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.732 min
Response: 0
Conc: N.D.

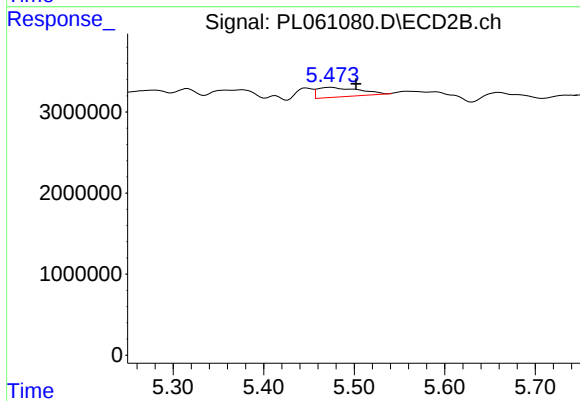

#5 Aldrin


R.T.: 5.474 min
Delta R.T.: -0.028 min
Response: 3698210
Conc: 1.10 ng/ml

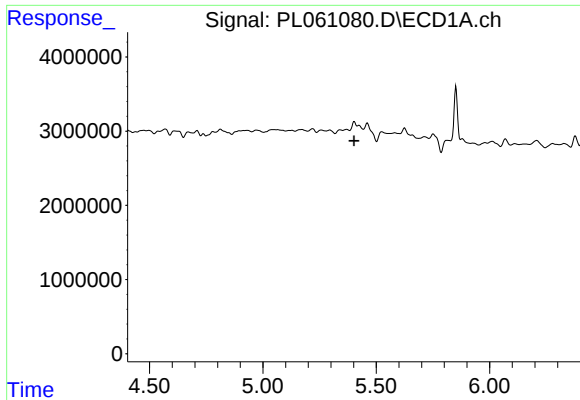

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.402 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

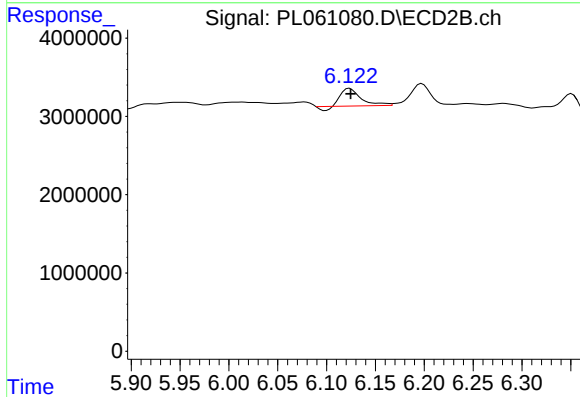


#10 gamma-Chlordane

R.T.: 6.124 min
Delta R.T.: -0.001 min
Response: 3101885
Conc: 1.00 ng/ml

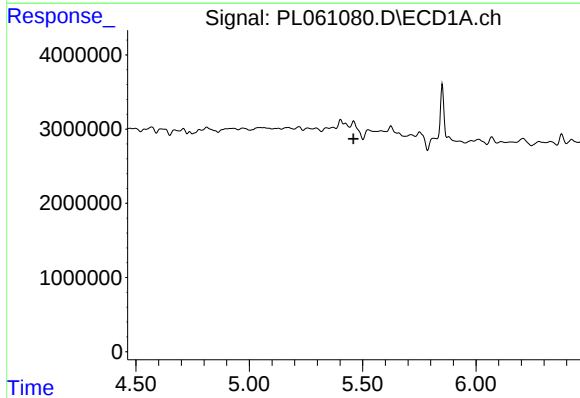


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.460 min
Response: 0
Conc: N.D.

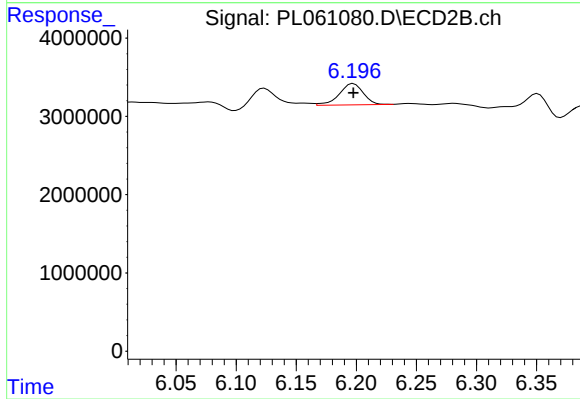

#11 alpha-Chlordane


R.T.: 6.198 min
Delta R.T.: 0.000 min
Response: 3786391
Conc: 1.22 ng/ml

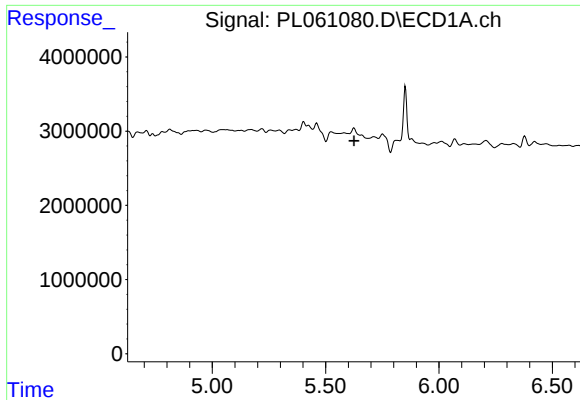

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 5.625 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

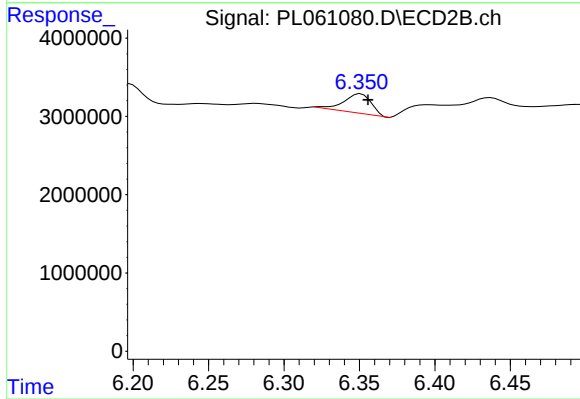


#12 4,4'-DDE

R.T.: 6.351 min
Delta R.T.: -0.005 min
Response: 3150394
Conc: 1.09 ng/ml

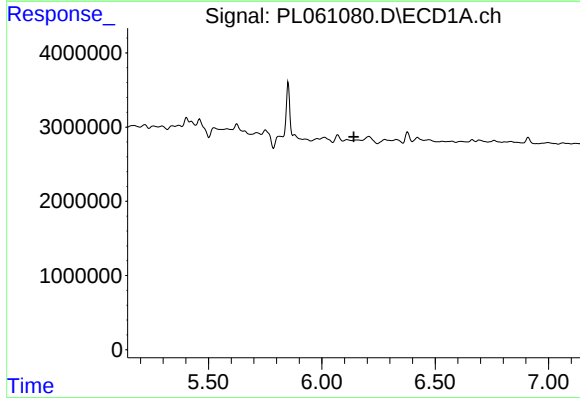


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.141 min
Response: 0
Conc: N.D.

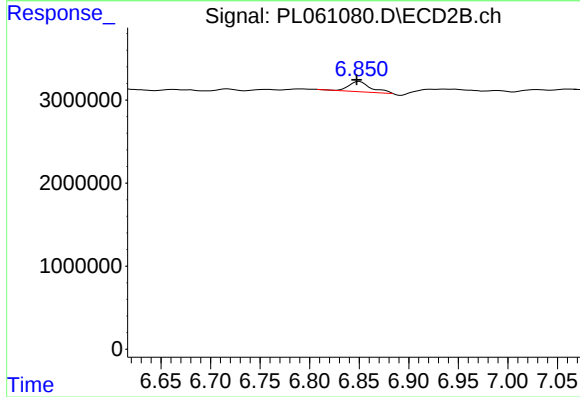

#16 4,4'-DDD


R.T.: 6.850 min
Delta R.T.: 0.003 min
Response: 1872351
Conc: 0.80 ng/ml

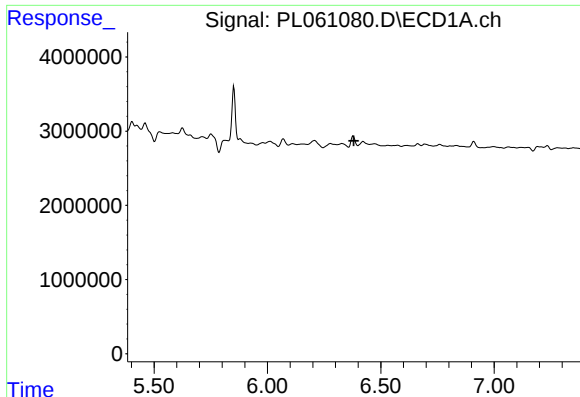

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

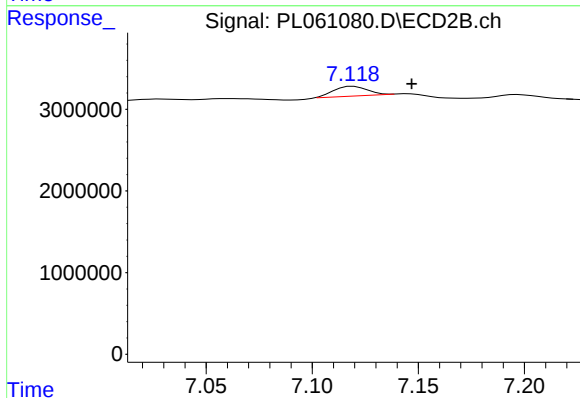


#17 4,4'-DDT

R.T.: 7.119 min
Delta R.T.: -0.027 min
Response: 1311293
Conc: 0.57 ng/ml

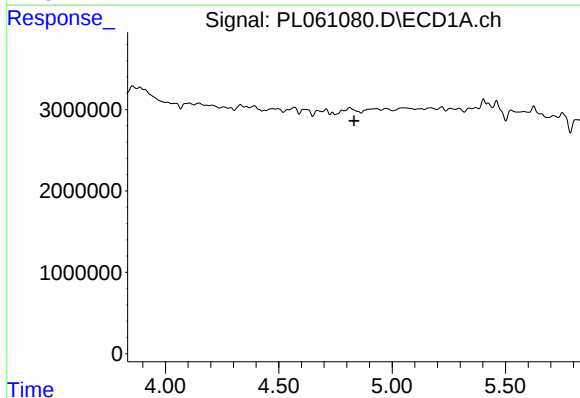


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 4.833 min
Response: 0
Conc: N.D.

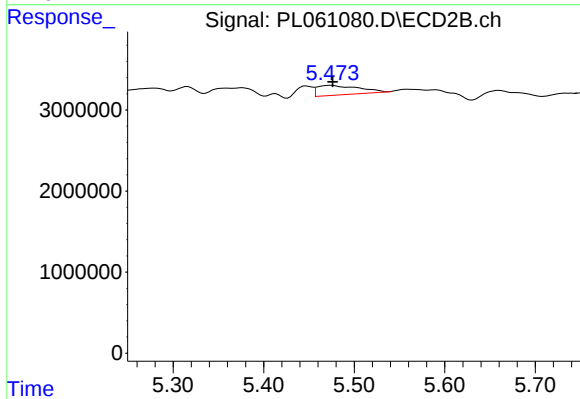

#24 Chlordane-2


R.T.: 5.474 min
Delta R.T.: -0.002 min
Response: 3698210
Conc: 35.94 ng/ml

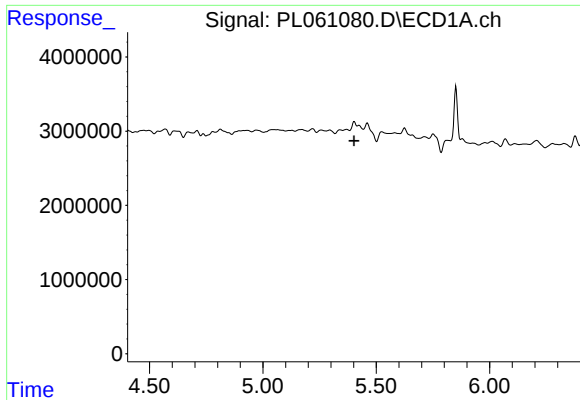

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.402 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

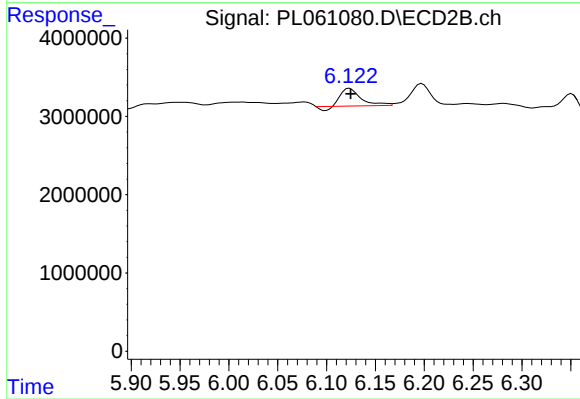


#25 Chlordane-3

R.T.: 6.124 min
Delta R.T.: -0.001 min
Response: 3101885
Conc: 7.76 ng/ml

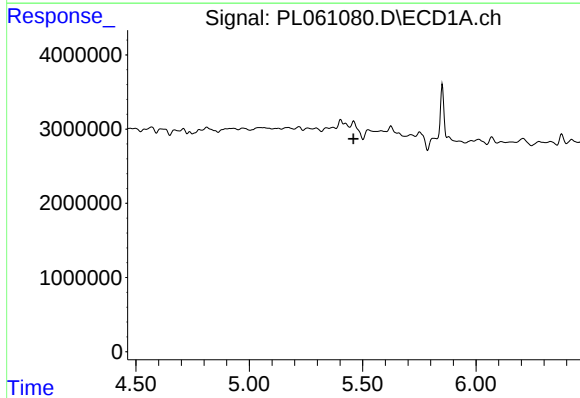


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.460 min
Response: 0
Conc: N.D.

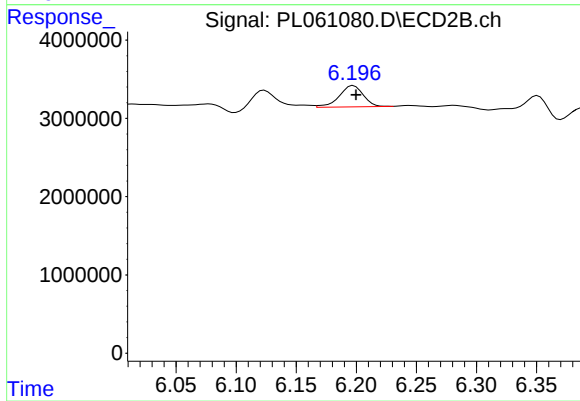

#26 Chlordane-4


R.T.: 6.198 min
Delta R.T.: -0.002 min
Response: 3786391
Conc: 7.88 ng/ml

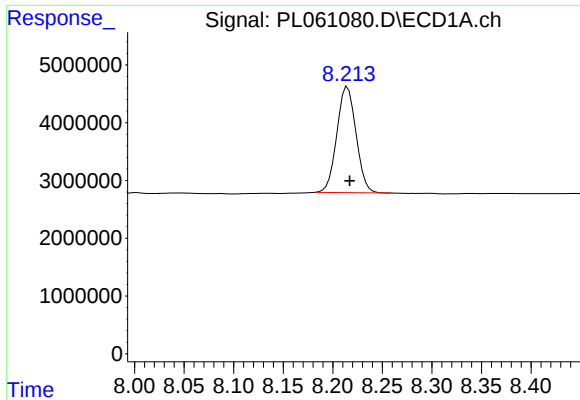

#28 Decachlorobiphenyl

R.T.: 8.215 min
Delta R.T.: -0.002 min
Response: 24732696
Conc: 14.68 ng/ml

Instrument :
ECD_L
ClientSampleId :

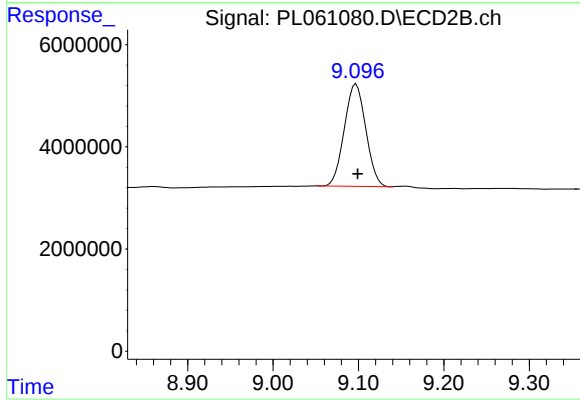

#28 Decachlorobiphenyl

R.T.: 9.097 min
Delta R.T.: -0.002 min
Response: 35006956
Conc: 16.59 ng/ml