

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083120\
 Data File : PL061082.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Aug 2020 12:54
 Operator : DD\AJ
 Sample : L3837-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 17:14:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 25 16:59:57 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.460	4.008	27292604	36210707	14.790	13.932
28)	SA Decachlor...	8.213	9.096	26757981	36390567	15.884	17.247
Target Compounds							
5)	MB Aldrin	0.000	5.523f	0	678447	N.D.	0.201 #
8)	B Heptachlo...	0.000	5.878	0	1489816	N.D.	0.570 #
10)	B gamma-Chl...	0.000	6.139	0	1960507	N.D.	0.631 #
12)	B 4,4'-DDE	0.000	6.351	0	6064349	N.D.	2.098 #
13)	MA Dieldrin	5.747	0.000	6845724	0	3.557	N.D. #
14)	MA Endrin	0.000	6.715	0	4315583	N.D.	1.699 #
16)	A 4,4'-DDD	0.000	6.851	0	4358777	N.D.	1.866 #
17)	MA 4,4'-DDT	6.376	7.144	4965141	2148852	3.285	0.933 #
25)	Chlordane-3	0.000	6.139	0	1960507	N.D.	4.905 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083120\
Data File : PL061082.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Aug 2020 12:54
Operator : DD\AJ
Sample : L3837-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 17:14:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
Quant Title : GC Extractables
QLast Update : Tue Aug 25 16:59:57 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

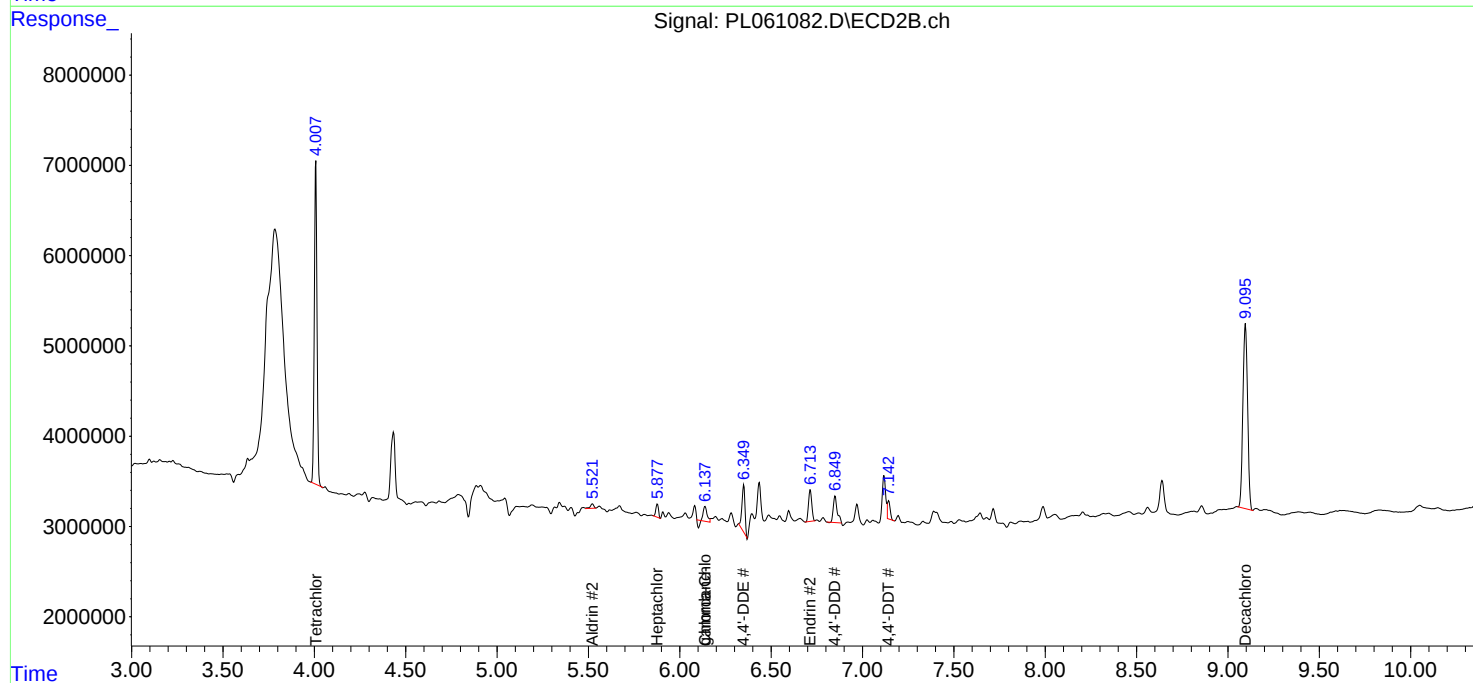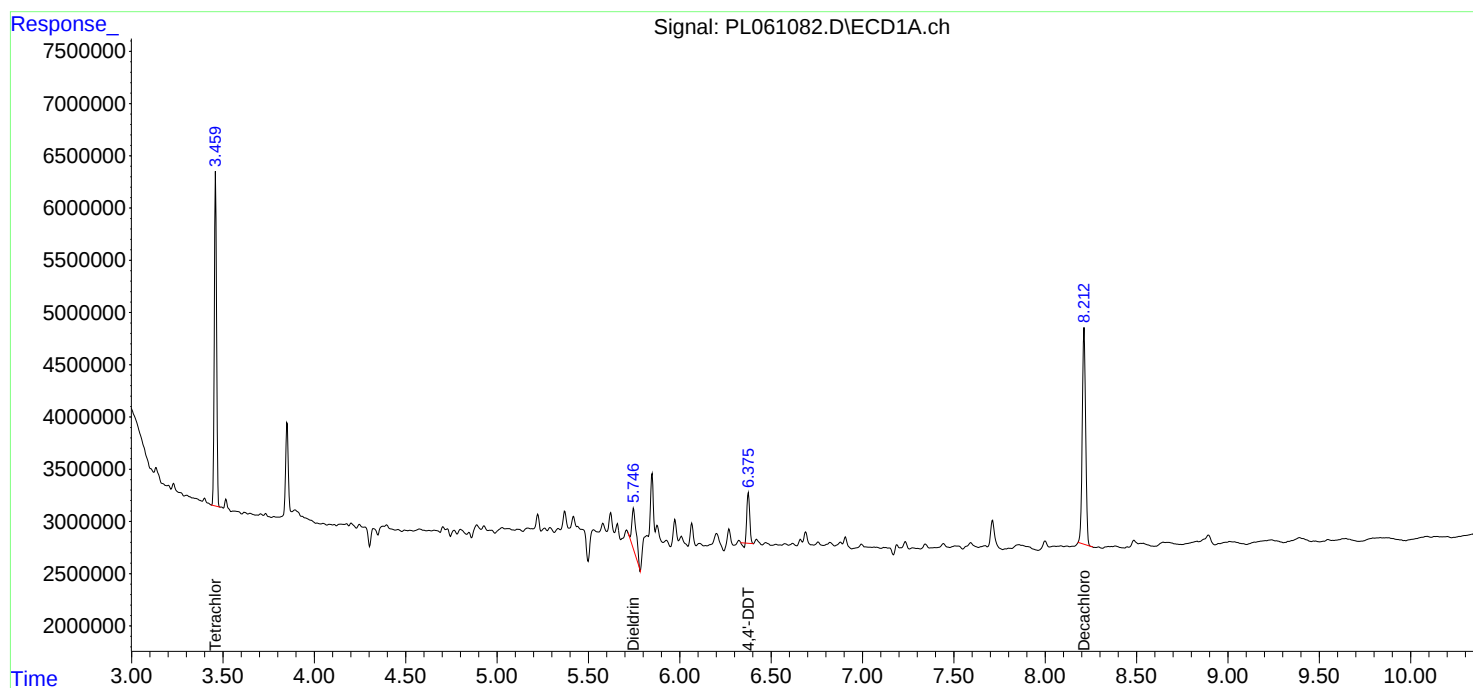


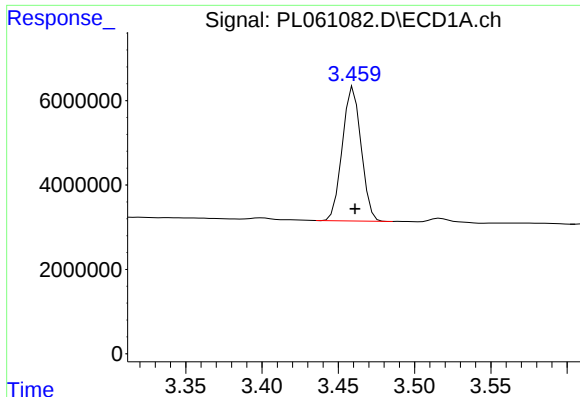

#1 Tetrachloro-m-xylene


R.T.: 3.460 min
Delta R.T.: 0.000 min
Response: 27292604
Conc: 14.79 ng/ml

Instrument :
ECD_L
ClientSampleId :

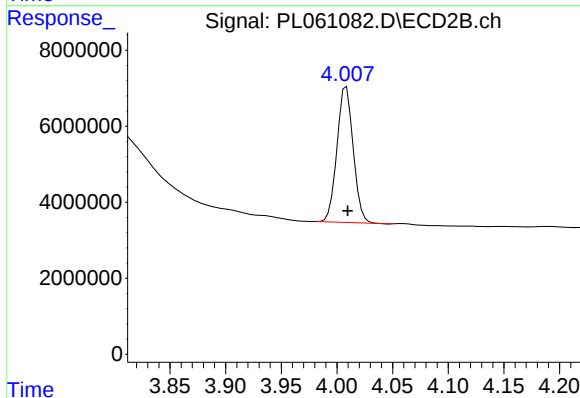


#1 Tetrachloro-m-xylene

R.T.: 4.008 min
Delta R.T.: -0.001 min
Response: 36210707
Conc: 13.93 ng/ml

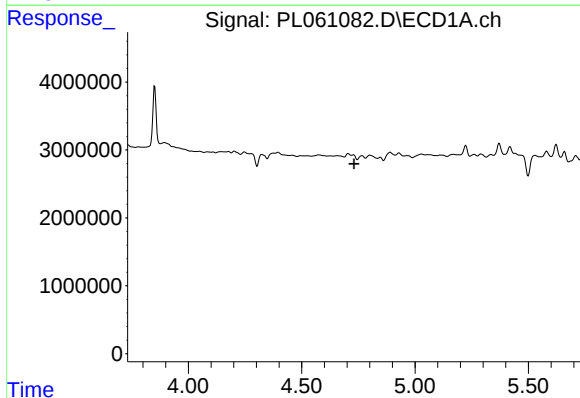


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.732 min
Response: 0
Conc: N.D.

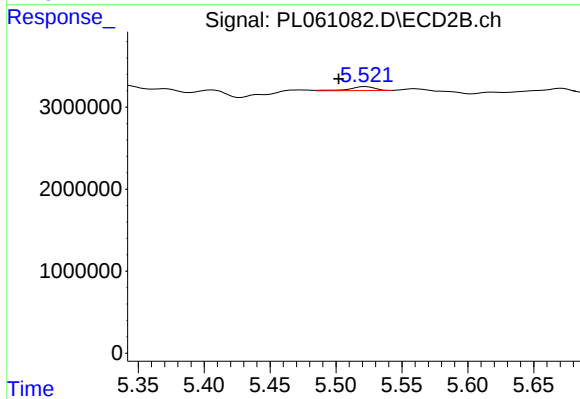

#5 Aldrin


R.T.: 5.523 min
Delta R.T.: 0.021 min
Response: 678447
Conc: 0.20 ng/ml

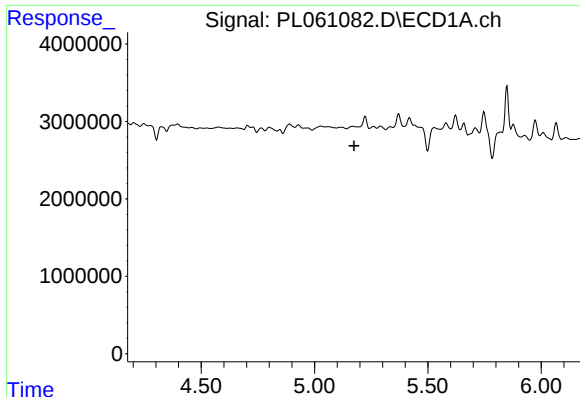

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.175 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

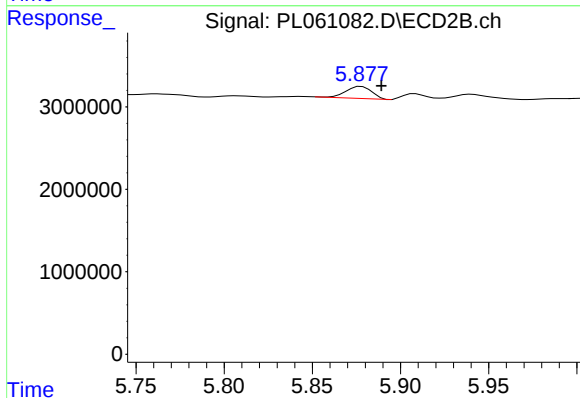


#8 Heptachlor epoxide

R.T.: 5.878 min
Delta R.T.: -0.011 min
Response: 1489816
Conc: 0.57 ng/ml

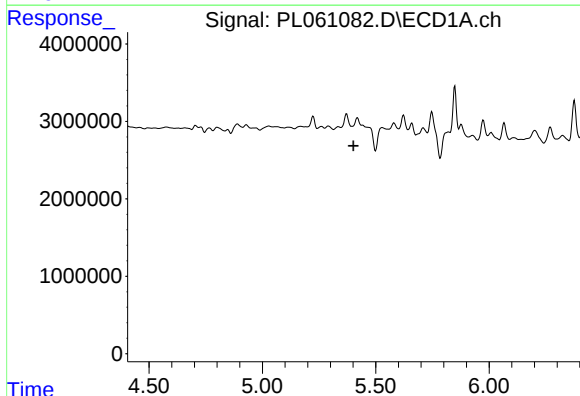


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.402 min
Response: 0
Conc: N.D.

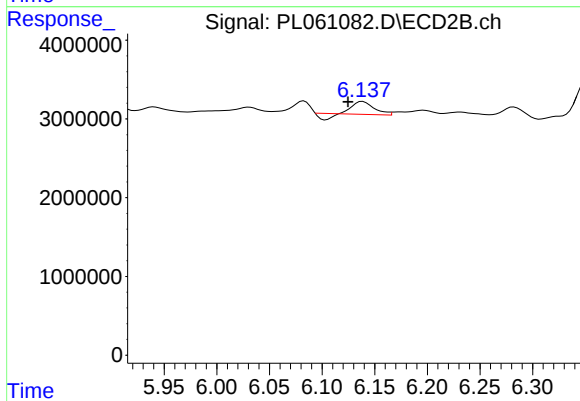

#10 gamma-Chlordane


R.T.: 6.139 min
Delta R.T.: 0.014 min
Response: 1960507
Conc: 0.63 ng/ml

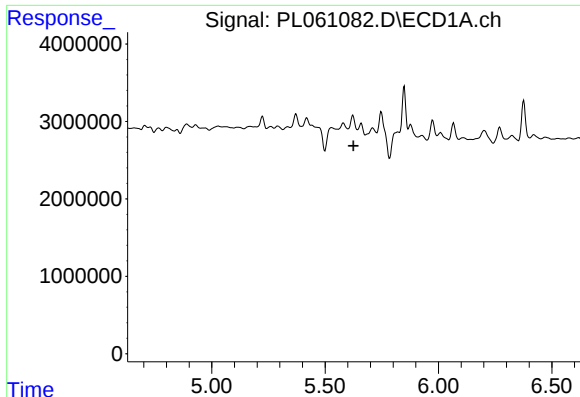

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 5.625 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

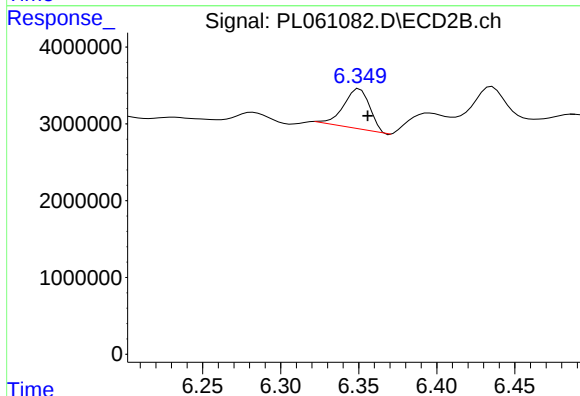


#12 4,4'-DDE

R.T.: 6.351 min
Delta R.T.: -0.005 min
Response: 6064349
Conc: 2.10 ng/ml

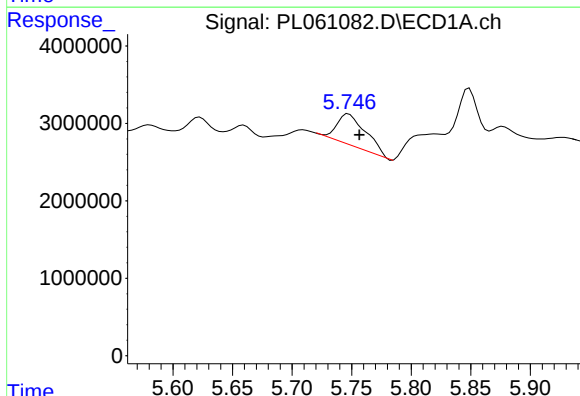


#13 Dieldrin

R.T.: 5.747 min
Delta R.T.: -0.009 min
Response: 6845724
Conc: 3.56 ng/ml

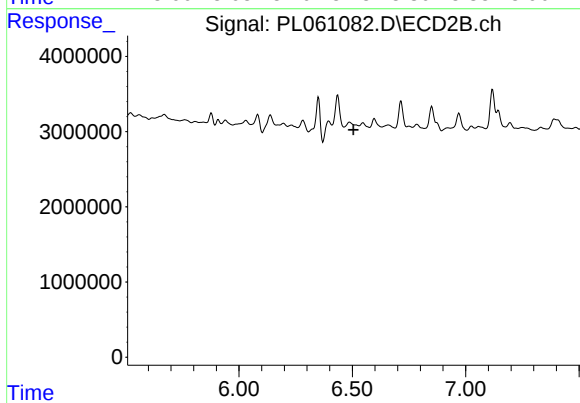

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.506 min
Response: 0
Conc: N.D.

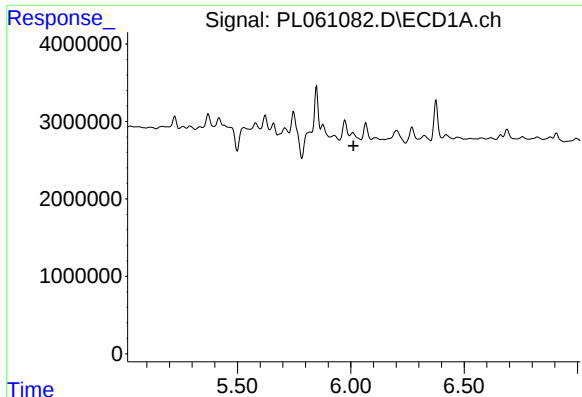

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.013 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

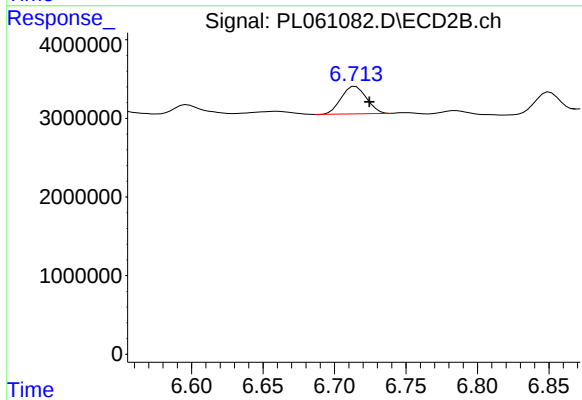


#14 Endrin

R.T.: 6.715 min
Delta R.T.: -0.010 min
Response: 4315583
Conc: 1.70 ng/ml

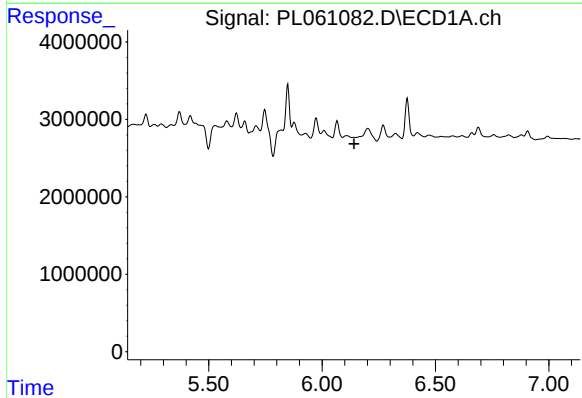


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.141 min
Response: 0
Conc: N.D.

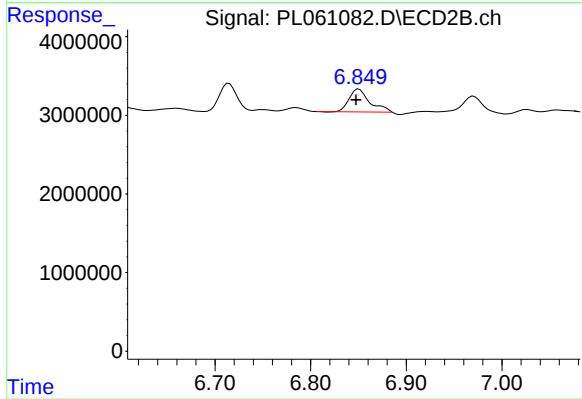

#16 4,4'-DDD


R.T.: 6.851 min
Delta R.T.: 0.003 min
Response: 4358777
Conc: 1.87 ng/ml

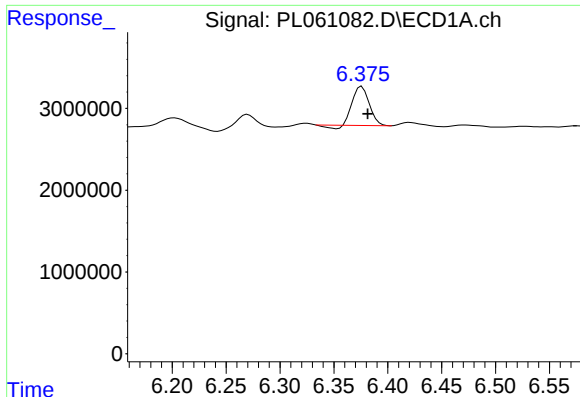

#17 4,4'-DDT


R.T.: 6.376 min
Delta R.T.: -0.006 min
Response: 4965141
Conc: 3.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

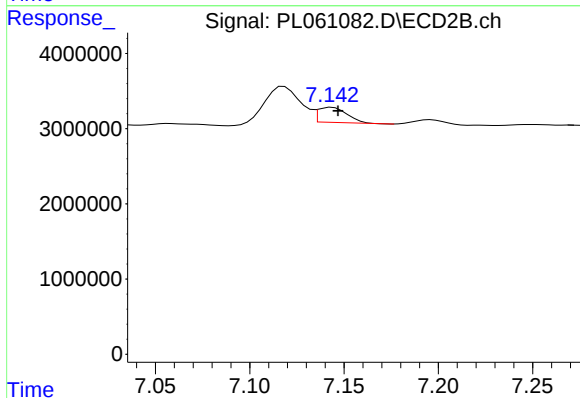


#17 4,4'-DDT

R.T.: 7.144 min
Delta R.T.: -0.003 min
Response: 2148852
Conc: 0.93 ng/ml

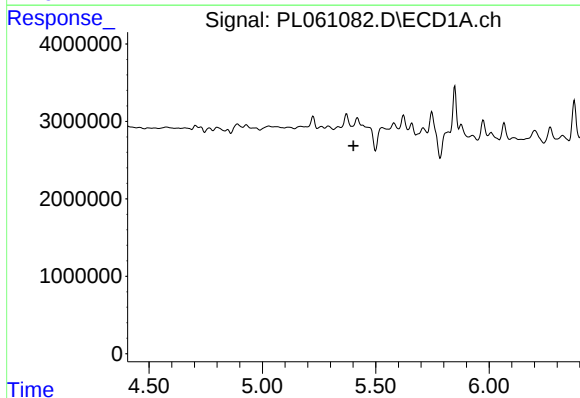


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.402 min
Response: 0
Conc: N.D.

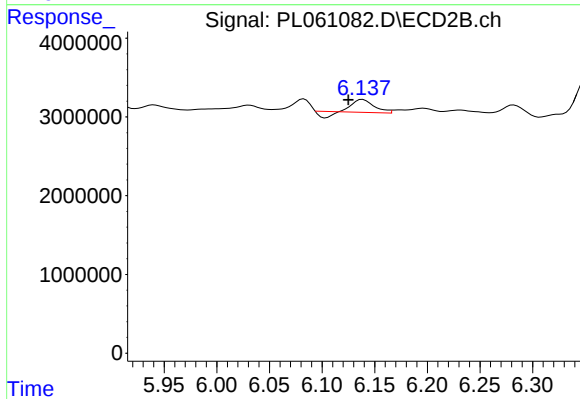

#25 Chlordane-3


R.T.: 6.139 min
Delta R.T.: 0.014 min
Response: 1960507
Conc: 4.91 ng/ml

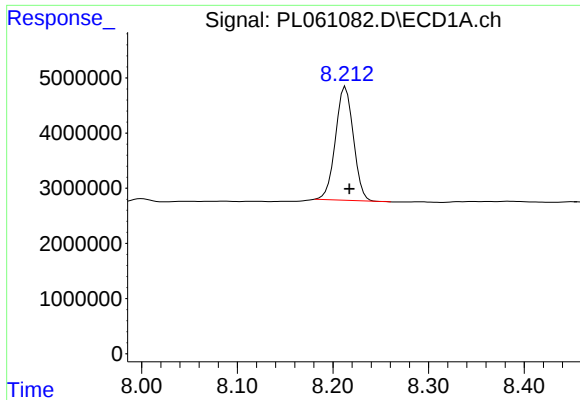

#28 Decachlorobiphenyl

R.T.: 8.213 min
Delta R.T.: -0.004 min
Response: 26757981
Conc: 15.88 ng/ml

Instrument :
ECD_L
ClientSampleId :

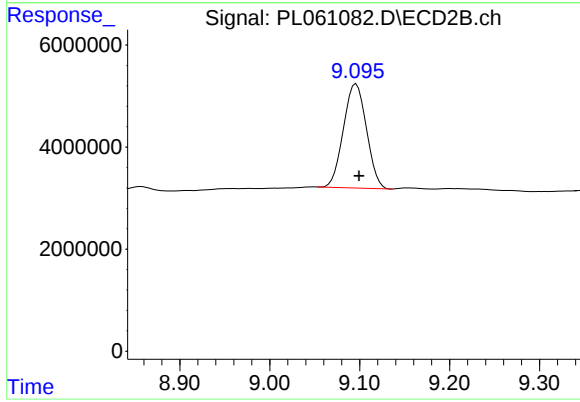

#28 Decachlorobiphenyl

R.T.: 9.096 min
Delta R.T.: -0.003 min
Response: 36390567
Conc: 17.25 ng/ml