

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083120\
 Data File : PL061083.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Aug 2020 13:09
 Operator : DD\AJ
 Sample : L3837-07
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 17:14:35 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 25 16:59:57 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.460	4.008	25469432	34817660	13.802	13.396
28)	SA Decachlor...	8.212	9.097	26376801	35206163	15.657	16.685
Target Compounds							
9)	A Endosulfan I	0.000	6.234	0	1234677	N.D.	0.429 #
10)	B gamma-Chl...	0.000	6.137	0	2854097	N.D.	0.919 #
11)	B alpha-Chl...	0.000	6.195	0	1878315	N.D.	0.604 #
12)	B 4,4'-DDE	0.000	6.350	0	4747769	N.D.	1.643 #
16)	A 4,4'-DDD	0.000	6.849	0	2262478	N.D.	0.969 #
17)	MA 4,4'-DDT	6.377	7.144	2990185	2407065	1.978	1.045 #
20)	A Methoxychlor	0.000	7.624f	0	966116	N.D.	0.747 #
23)	Chlordane-1	4.325	0.000	3361801	0	55.059	N.D. #
25)	Chlordane-3	0.000	6.137	0	2854097	N.D.	7.141 #
26)	Chlordane-4	0.000	6.195	0	1878315	N.D.	3.907 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083120\
Data File : PL061083.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Aug 2020 13:09
Operator : DD\AJ
Sample : L3837-07
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 17:14:35 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
Quant Title : GC Extractables
QLast Update : Tue Aug 25 16:59:57 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

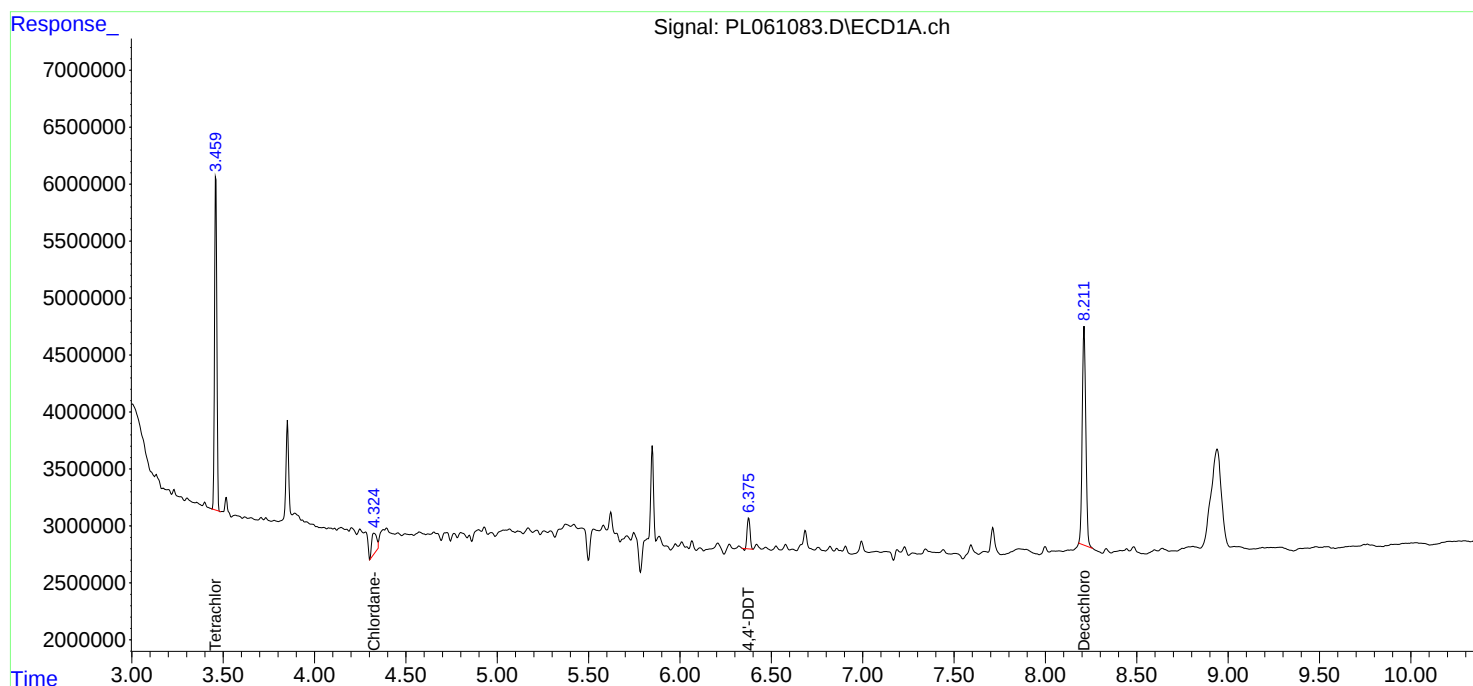


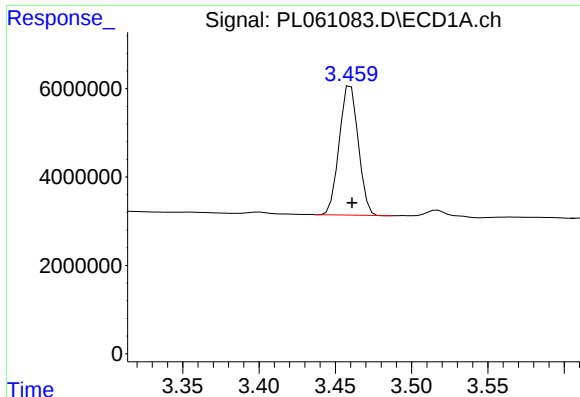

#1 Tetrachloro-m-xylene


R.T.: 3.460 min
Delta R.T.: 0.000 min
Response: 25469432
Conc: 13.80 ng/ml

Instrument :
ECD_L
ClientSampleId :

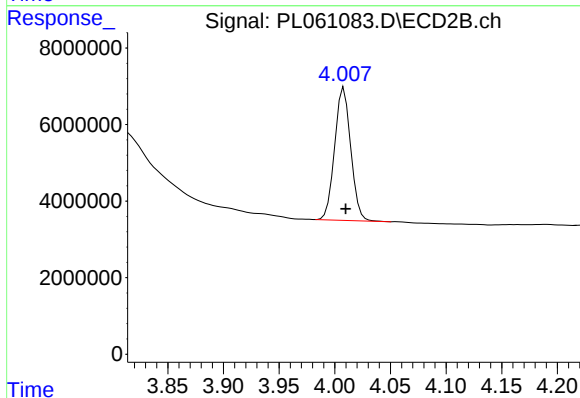


#1 Tetrachloro-m-xylene

R.T.: 4.008 min
Delta R.T.: -0.002 min
Response: 34817660
Conc: 13.40 ng/ml

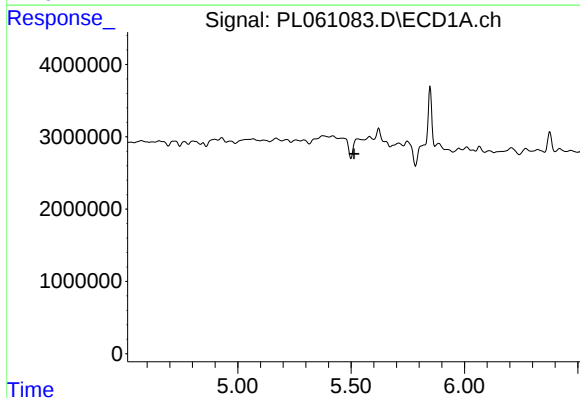


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.513 min
Response: 0
Conc: N.D.

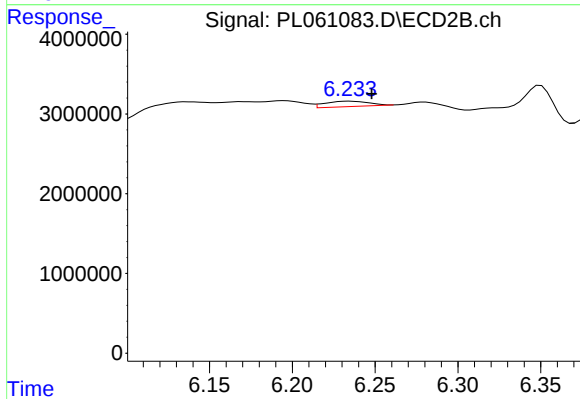

#9 Endosulfan I


R.T.: 6.234 min
Delta R.T.: -0.013 min
Response: 1234677
Conc: 0.43 ng/ml

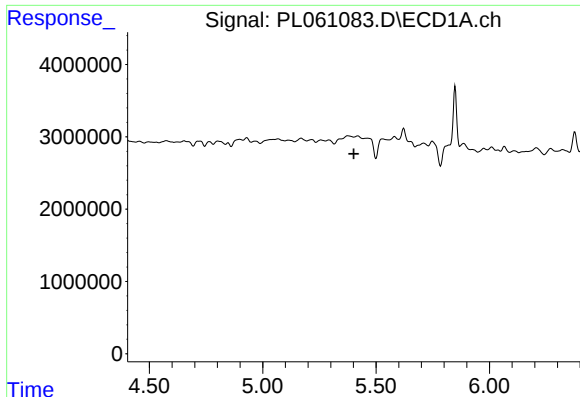

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.402 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

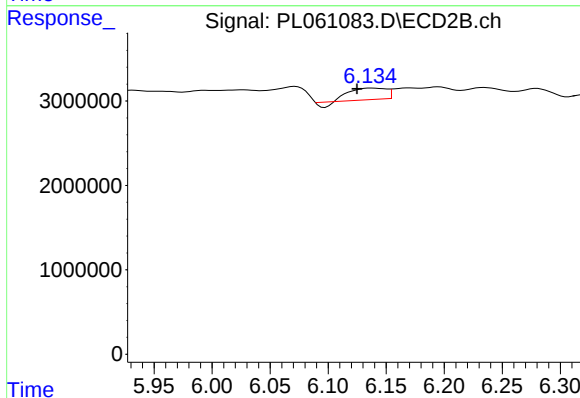


#10 gamma-Chlordane

R.T.: 6.137 min
Delta R.T.: 0.012 min
Response: 2854097
Conc: 0.92 ng/ml

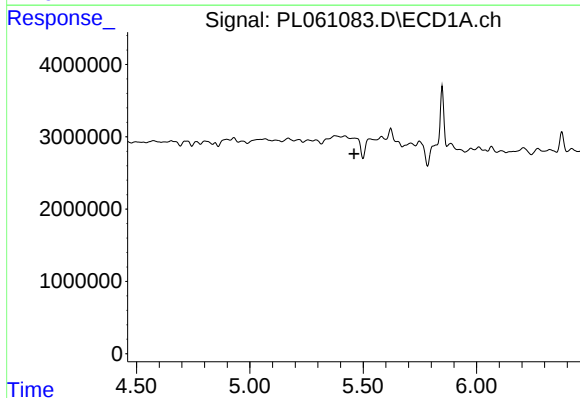


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.460 min
Response: 0
Conc: N.D.

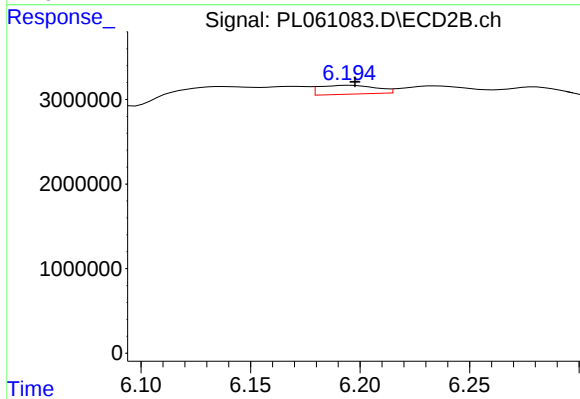

#11 alpha-Chlordane


R.T.: 6.195 min
Delta R.T.: -0.002 min
Response: 1878315
Conc: 0.60 ng/ml

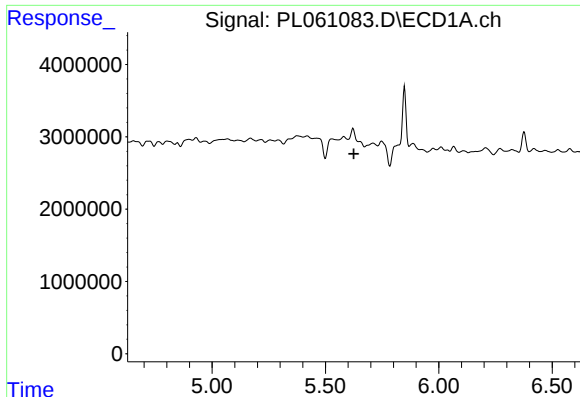

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 5.625 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

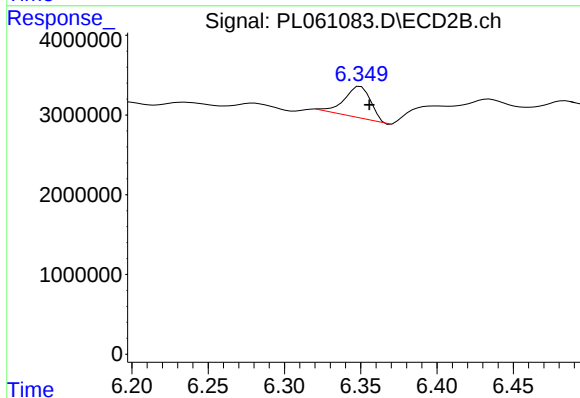


#12 4,4'-DDE

R.T.: 6.350 min
Delta R.T.: -0.006 min
Response: 4747769
Conc: 1.64 ng/ml

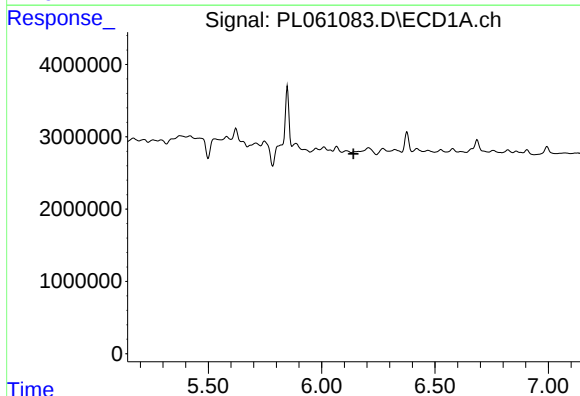


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.141 min
Response: 0
Conc: N.D.

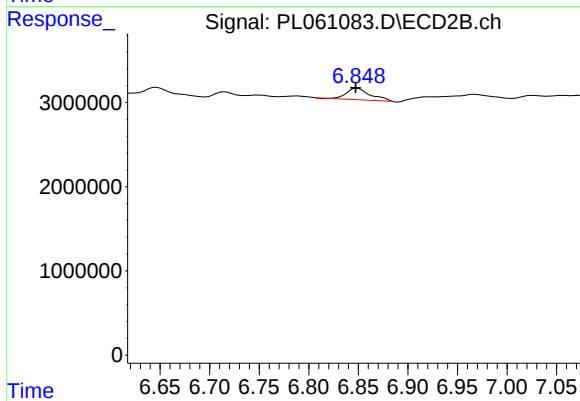

#16 4,4'-DDD


R.T.: 6.849 min
Delta R.T.: 0.002 min
Response: 2262478
Conc: 0.97 ng/ml

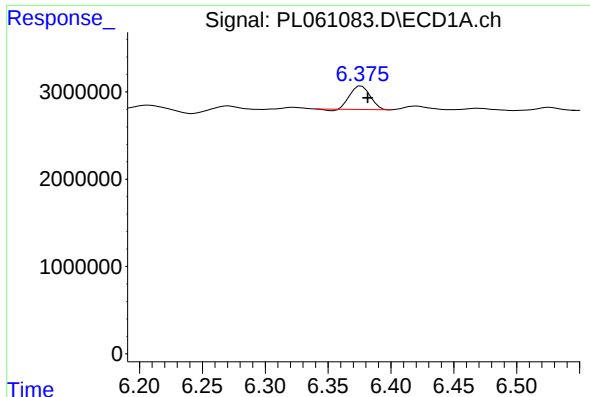

#17 4,4'-DDT


R.T.: 6.377 min
Delta R.T.: -0.005 min
Response: 2990185
Conc: 1.98 ng/ml

Instrument :
ECD_L
ClientSampleId :

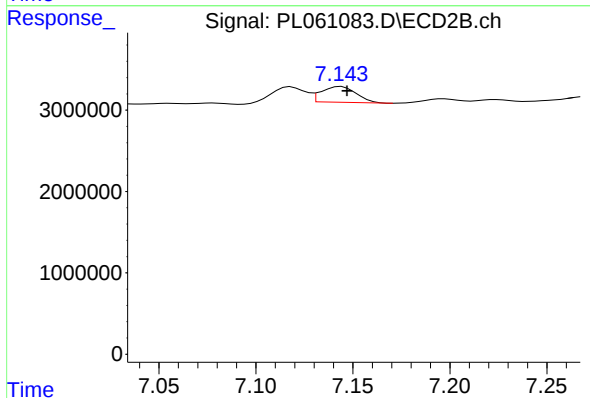


#17 4,4'-DDT

R.T.: 7.144 min
Delta R.T.: -0.003 min
Response: 2407065
Conc: 1.05 ng/ml

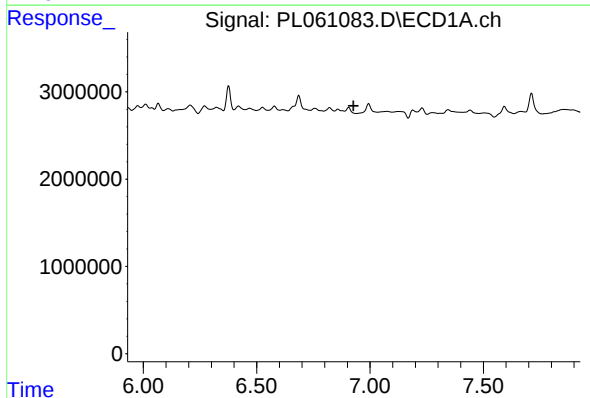


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.928 min
Response: 0
Conc: N.D.

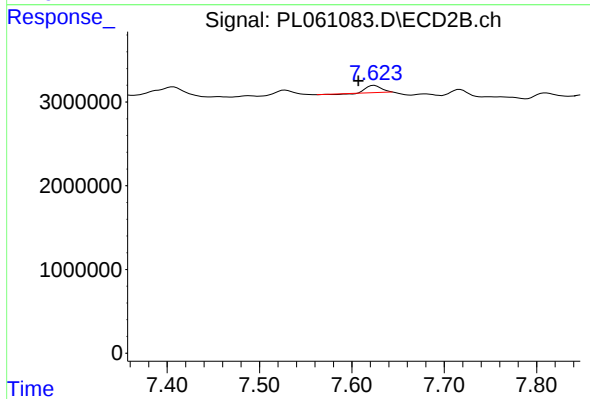

#20 Methoxychlor


R.T.: 7.624 min
Delta R.T.: 0.017 min
Response: 966116
Conc: 0.75 ng/ml

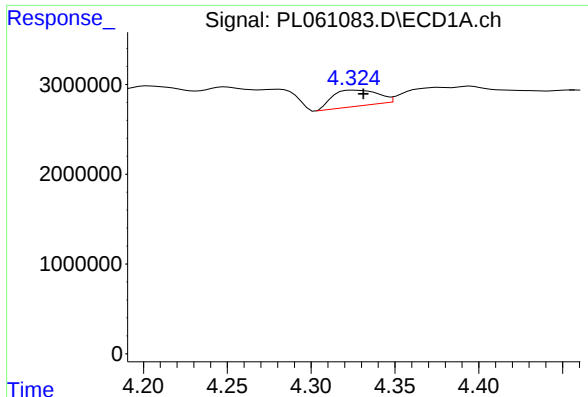

#23 Chlordane-1


R.T.: 4.325 min
Delta R.T.: -0.006 min
Response: 3361801
Conc: 55.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

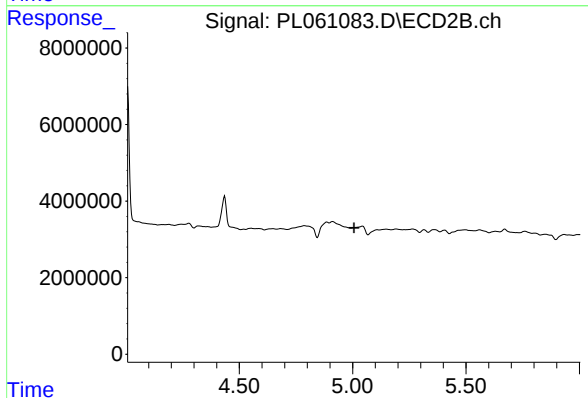


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.007 min
Response: 0
Conc: N.D.

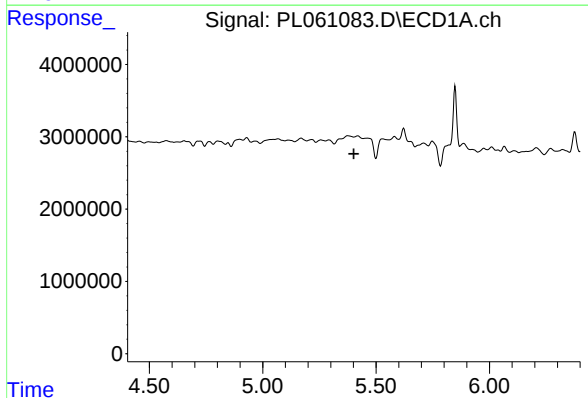


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.402 min
Response: 0
Conc: N.D.

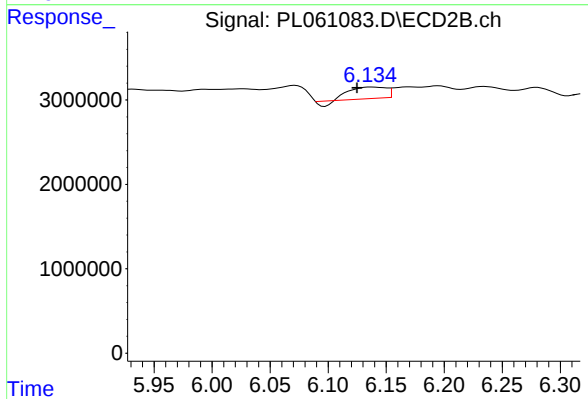

#25 Chlordane-3


R.T.: 6.137 min
Delta R.T.: 0.012 min
Response: 2854097
Conc: 7.14 ng/ml

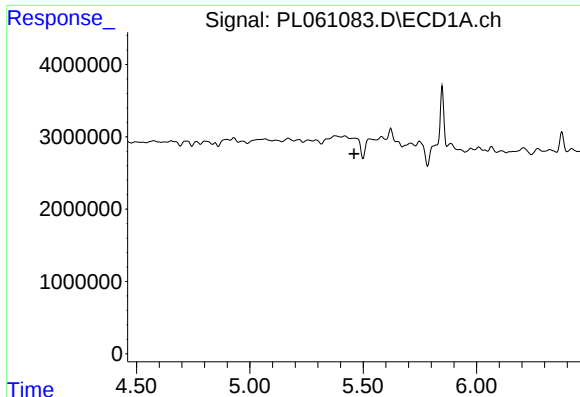

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.460 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

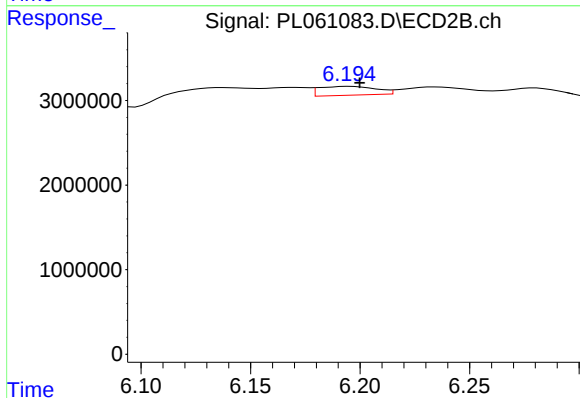


#26 Chlordane-4

R.T.: 6.195 min
Delta R.T.: -0.005 min
Response: 1878315
Conc: 3.91 ng/ml

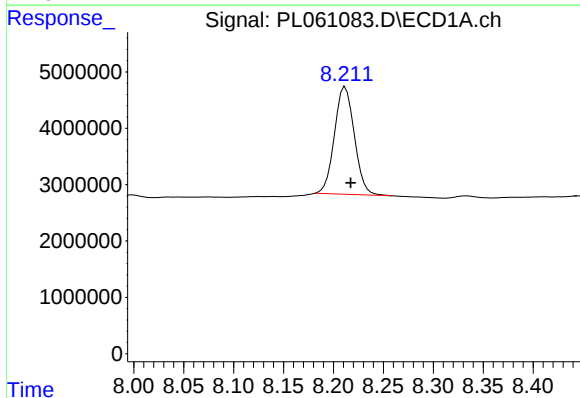

#28 Decachlorobiphenyl

R.T.: 8.212 min
Delta R.T.: -0.005 min
Response: 26376801
Conc: 15.66 ng/ml

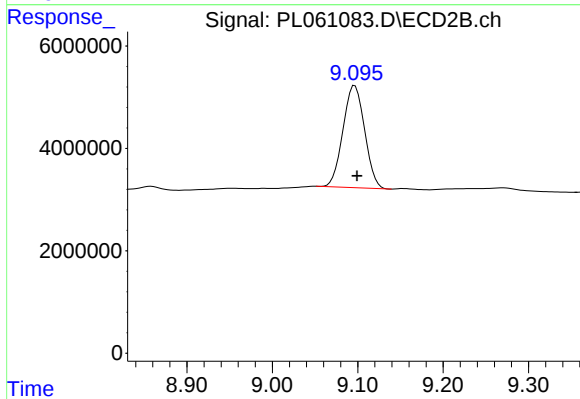

#28 Decachlorobiphenyl

R.T.: 9.097 min
Delta R.T.: -0.003 min
Response: 35206163
Conc: 16.69 ng/ml