

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083120\
 Data File : PL061096.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Aug 2020 16:46
 Operator : DD\AJ
 Sample : L3837-16
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 02:25:07 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 25 16:59:57 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
6) B	beta-BHC	0.000	4.883f	0	462106	N.D. 0.310 #
9) A	Endosulfan I	0.000	6.240	0	701184	N.D. 0.244 #
10) B	gamma-Chl...	0.000	6.135	0	1093259	N.D. 0.352 #
11) B	alpha-Chl...	0.000	6.202	0	3473570	N.D. 1.117 #
12) B	4,4'-DDE	5.630	6.357	45173998	65871793	24.551 22.791
14) MA	Endrin	0.000	6.754f	0	1805624	N.D. 0.711 #
15) B	Endosulfa...	0.000	6.946	0	111799	N.D. 0.043 #
16) A	4,4'-DDD	0.000	6.853	0	2398208	N.D. 1.027 #
17) MA	4,4'-DDT	6.386	7.149	14036014	22426104	9.286 9.738
22)	Mirex	0.000	8.212	0	2709961	N.D. 1.557 #
25)	Chlordane-3	0.000	6.135	0	1093259	N.D. 2.735 #
26)	Chlordane-4	0.000	6.202	0	3473570	N.D. 7.226 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083120\
Data File : PL061096.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Aug 2020 16:46
Operator : DD\AJ
Sample : L3837-16
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 02:25:07 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
Quant Title : GC Extractables
QLast Update : Tue Aug 25 16:59:57 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

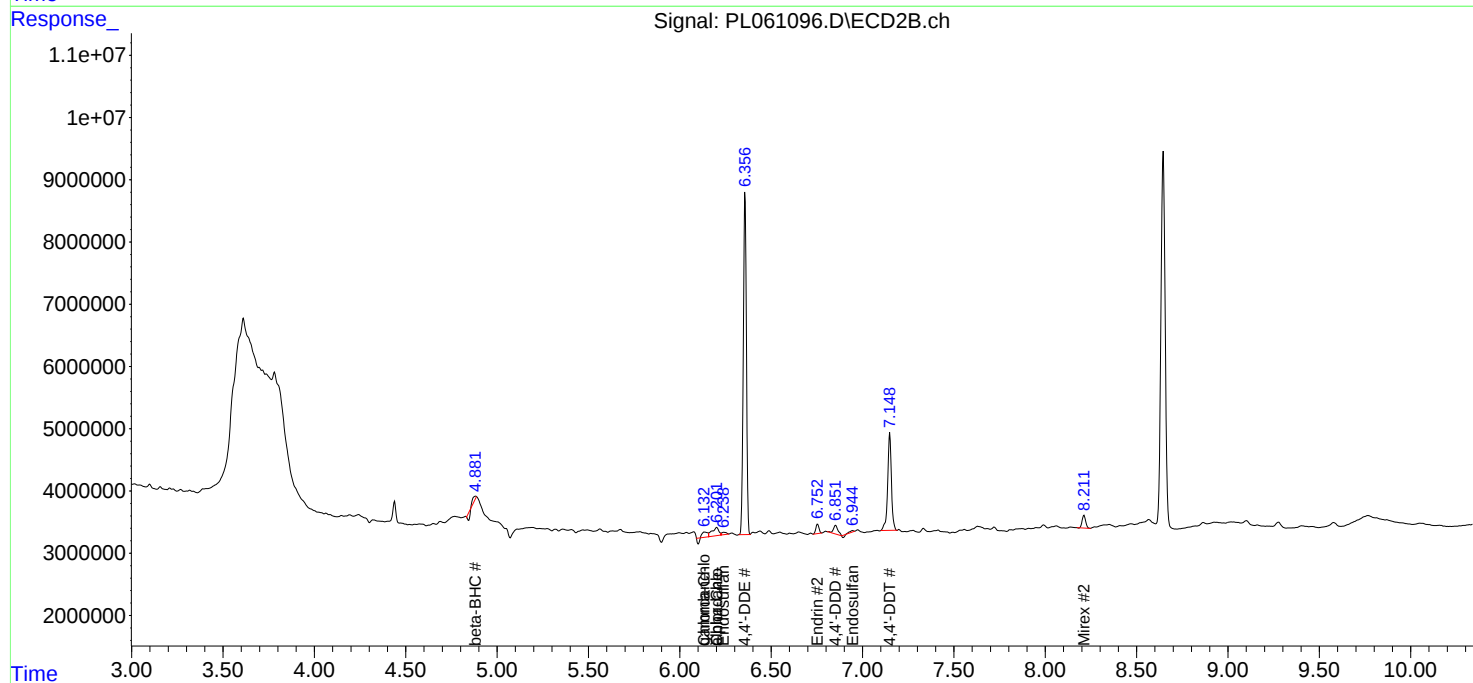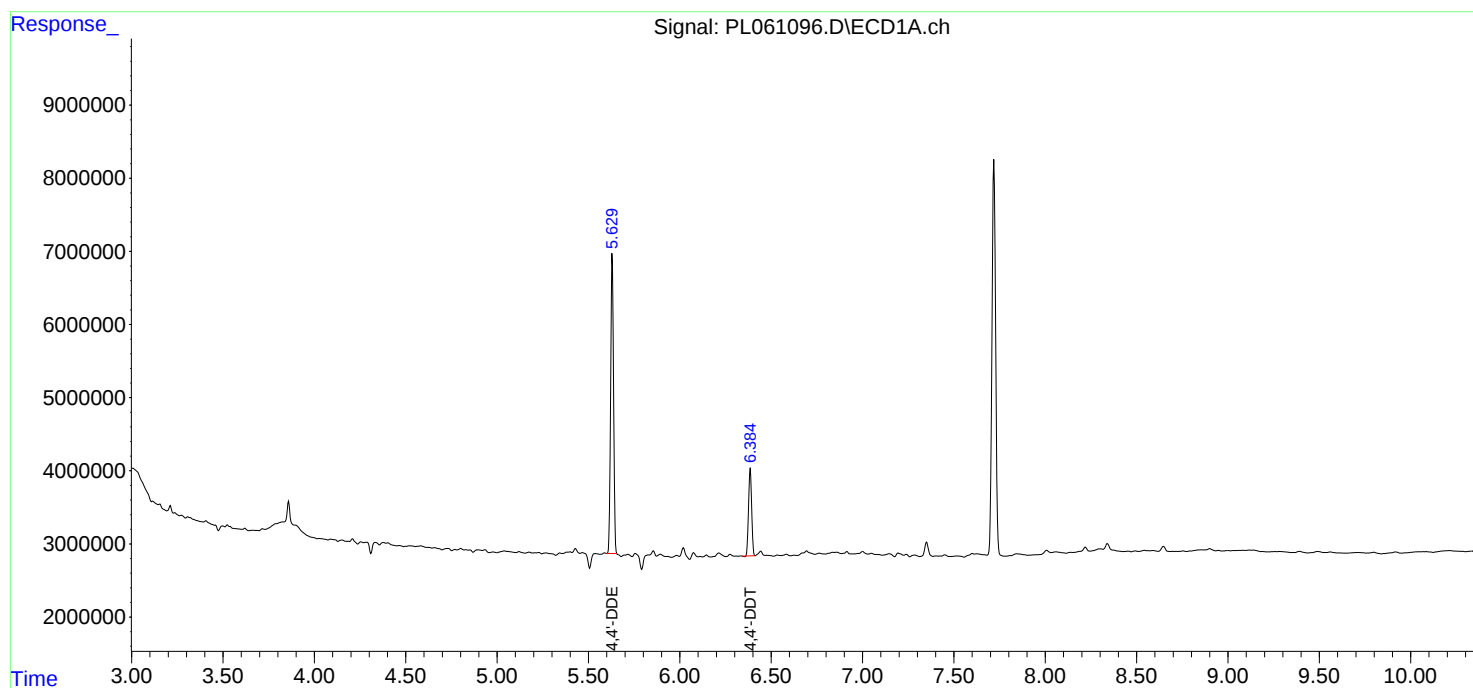


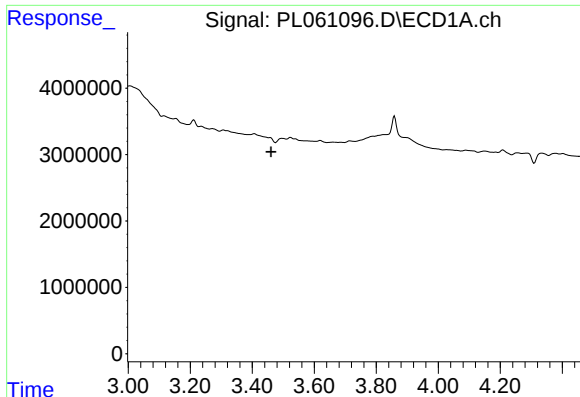

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.461 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

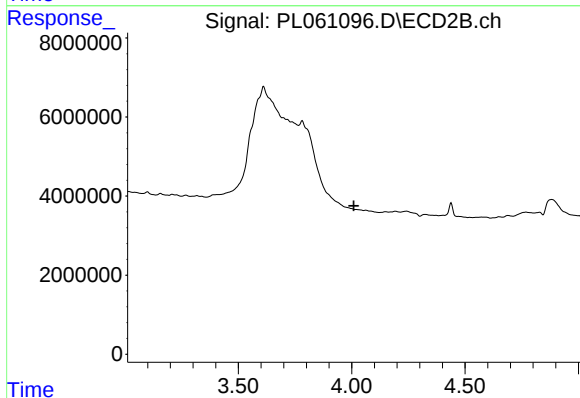


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.010 min
Response: 0
Conc: N.D.

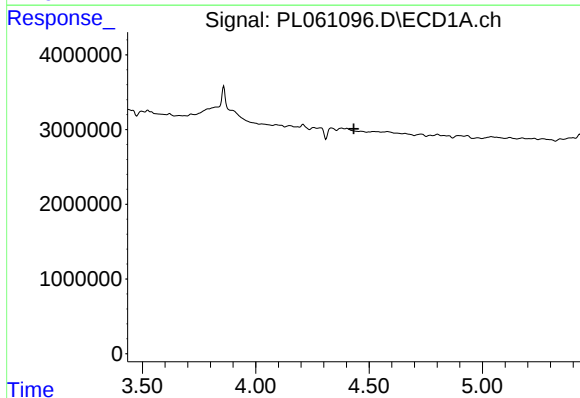


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.432 min
Response: 0
Conc: N.D.

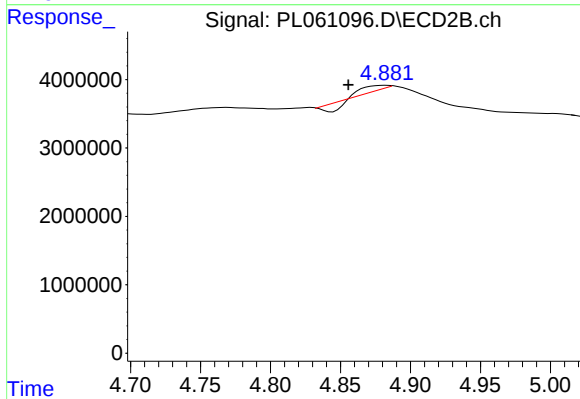

#6 beta-BHC


R.T.: 4.883 min
Delta R.T.: 0.027 min
Response: 462106
Conc: 0.31 ng/ml

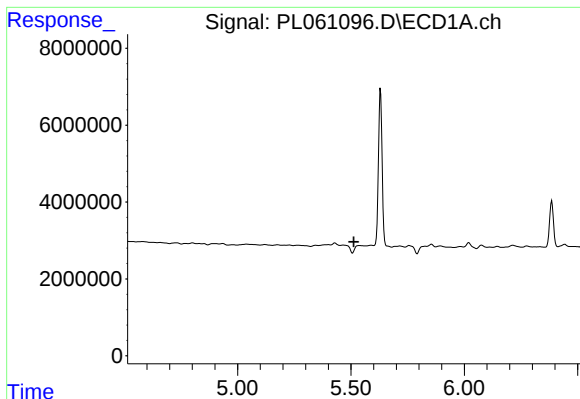

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.513 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

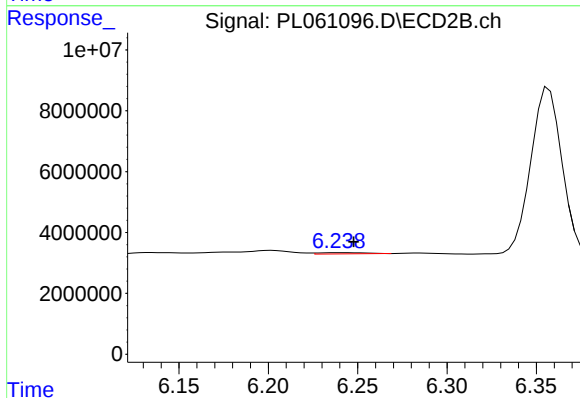


#9 Endosulfan I

R.T.: 6.240 min
Delta R.T.: -0.007 min
Response: 701184
Conc: 0.24 ng/ml

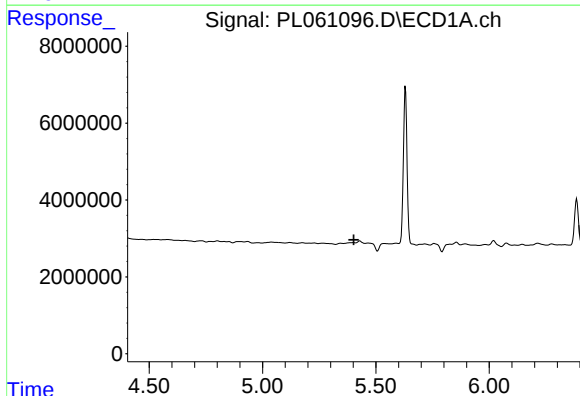


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.402 min
Response: 0
Conc: N.D.

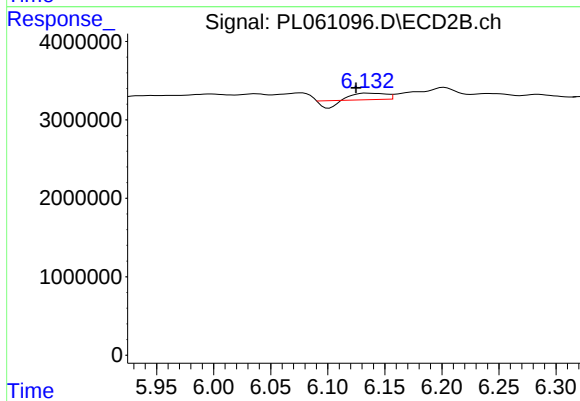

#10 gamma-Chlordane


R.T.: 6.135 min
Delta R.T.: 0.010 min
Response: 1093259
Conc: 0.35 ng/ml

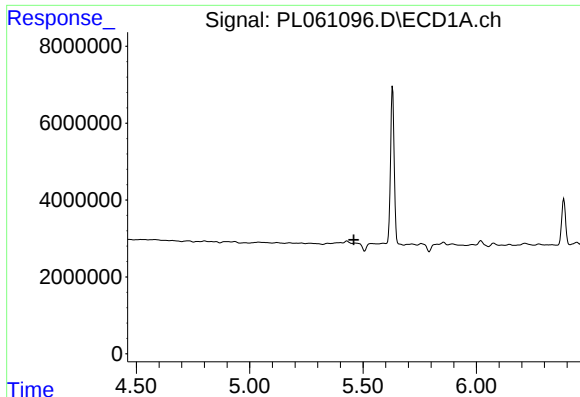

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.460 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

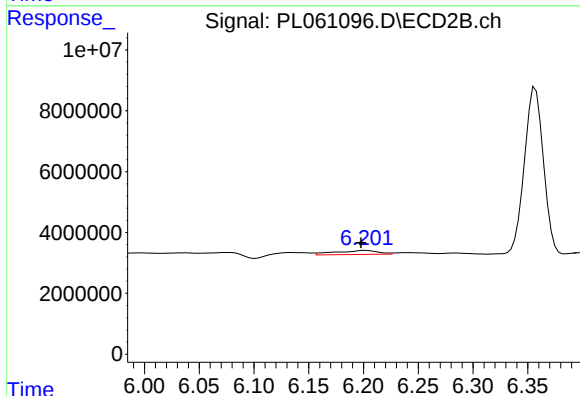


#11 alpha-Chlordane

R.T.: 6.202 min
Delta R.T.: 0.004 min
Response: 3473570
Conc: 1.12 ng/ml

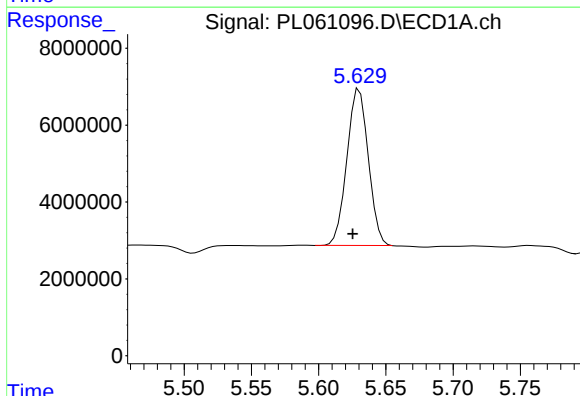


#12 4,4'-DDE

R.T.: 5.630 min
Delta R.T.: 0.005 min
Response: 45173998
Conc: 24.55 ng/ml

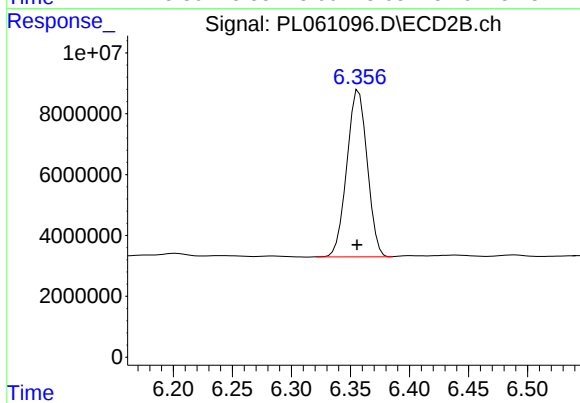

#12 4,4'-DDE


R.T.: 6.357 min
Delta R.T.: 0.001 min
Response: 65871793
Conc: 22.79 ng/ml

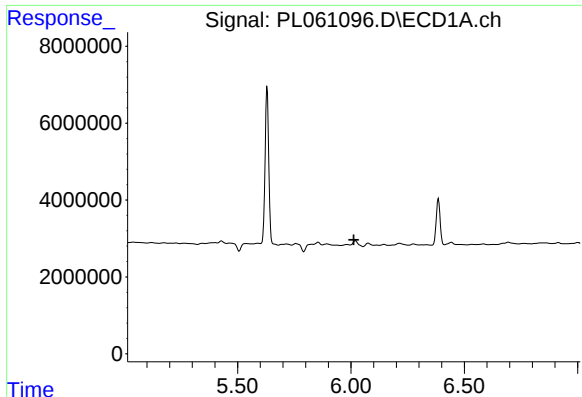

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.013 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

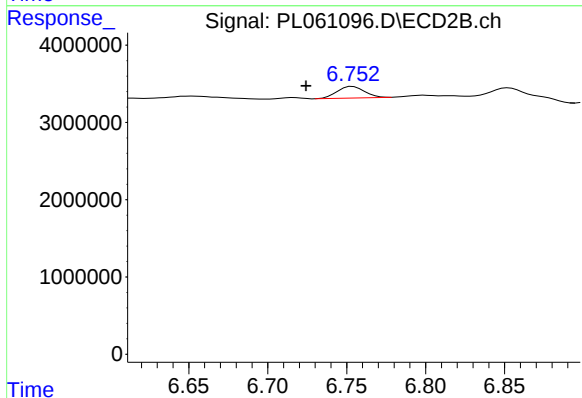


#14 Endrin

R.T.: 6.754 min
Delta R.T.: 0.029 min
Response: 1805624
Conc: 0.71 ng/ml

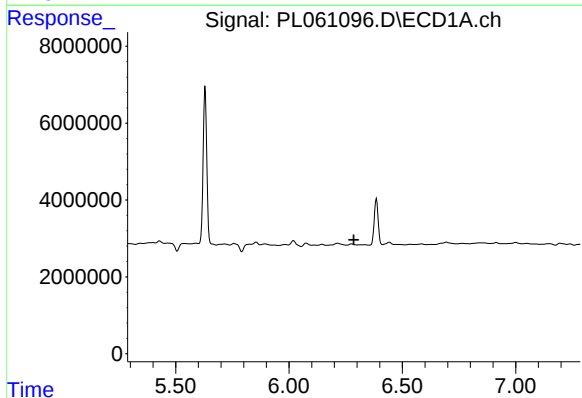


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.286 min
Response: 0
Conc: N.D.

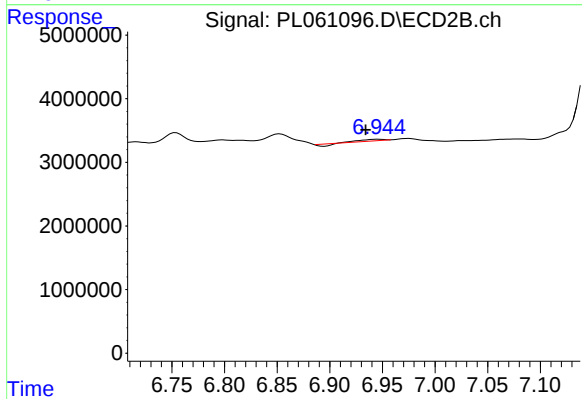

#15 Endosulfan II


R.T.: 6.946 min
Delta R.T.: 0.011 min
Response: 111799
Conc: 0.04 ng/ml

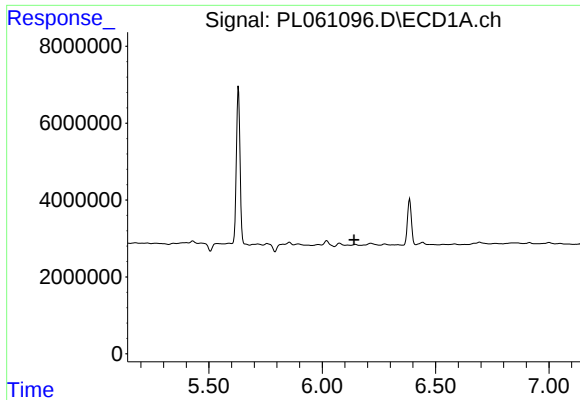

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.141 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

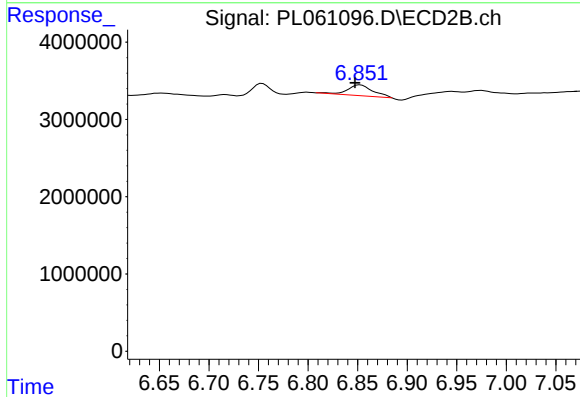


#16 4,4'-DDD

R.T.: 6.853 min
Delta R.T.: 0.005 min
Response: 2398208
Conc: 1.03 ng/ml

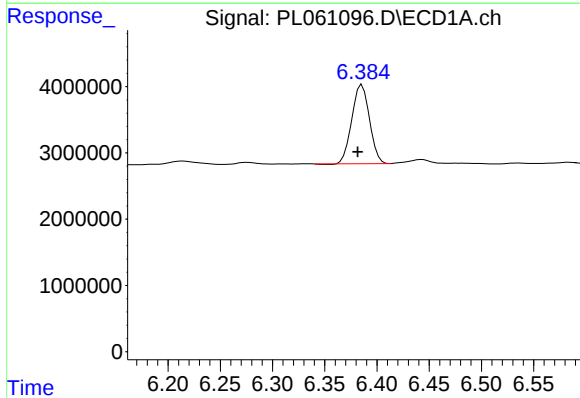


#17 4,4'-DDT

R.T.: 6.386 min
Delta R.T.: 0.004 min
Response: 14036014
Conc: 9.29 ng/ml

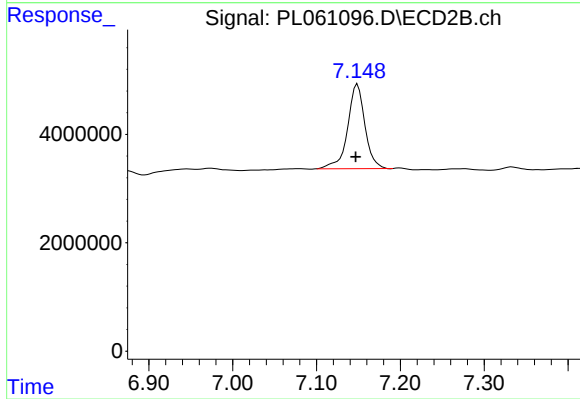

#17 4,4'-DDT


R.T.: 7.149 min
Delta R.T.: 0.002 min
Response: 22426104
Conc: 9.74 ng/ml

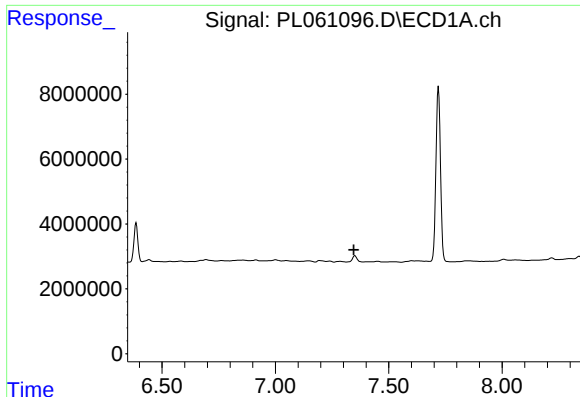

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 7.346 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

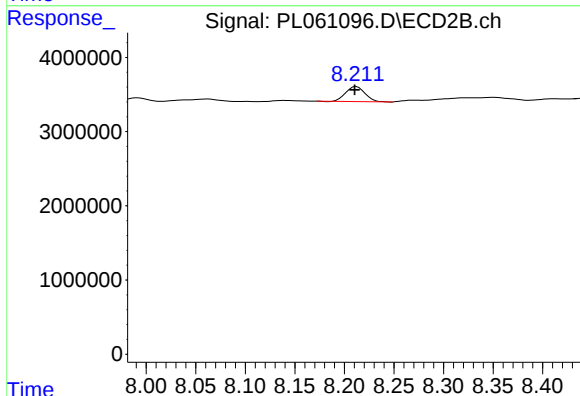


#22 Mirex

R.T.: 8.212 min
Delta R.T.: 0.002 min
Response: 2709961
Conc: 1.56 ng/ml

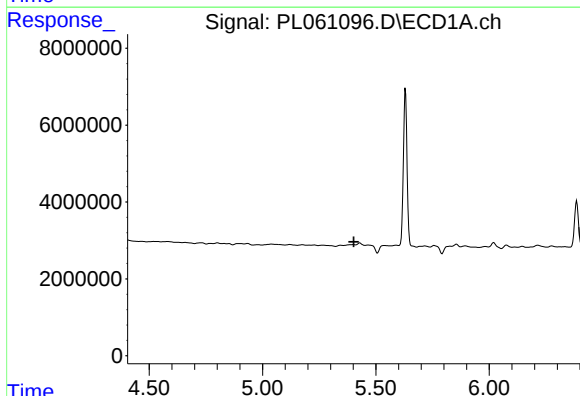


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.402 min
Response: 0
Conc: N.D.

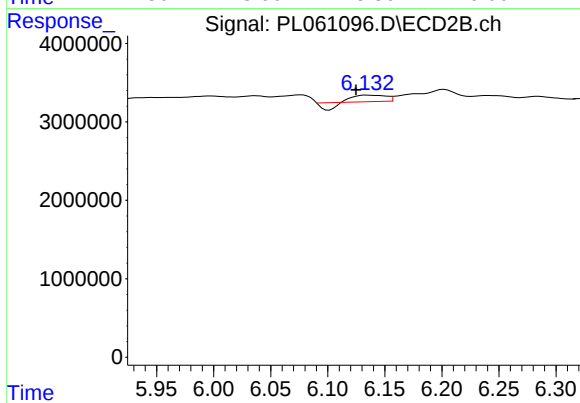

#25 Chlordane-3


R.T.: 6.135 min
Delta R.T.: 0.010 min
Response: 1093259
Conc: 2.74 ng/ml

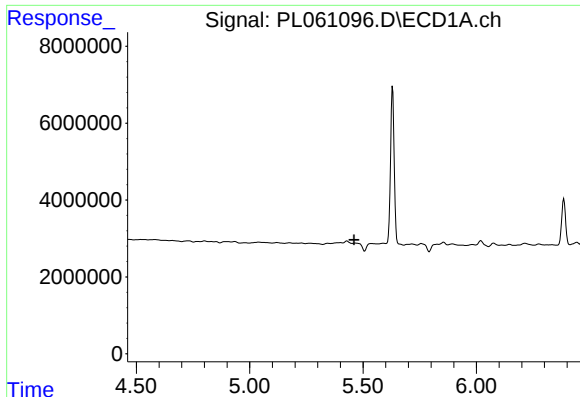

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.460 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

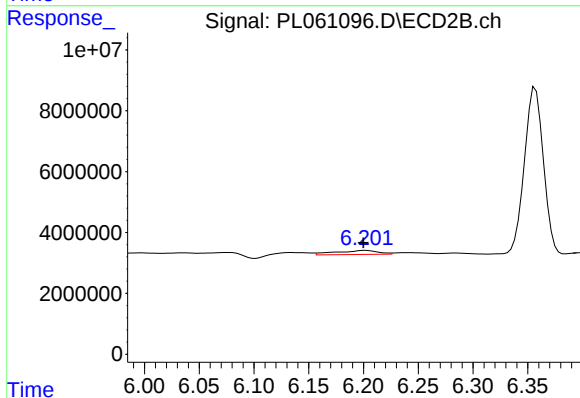


#26 Chlordane-4

R.T.: 6.202 min
Delta R.T.: 0.002 min
Response: 3473570
Conc: 7.23 ng/ml

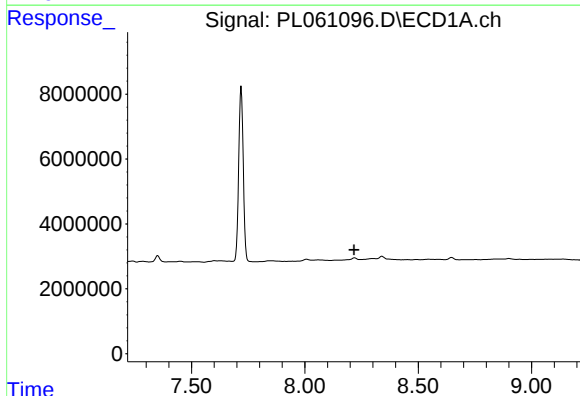

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 8.217 min
Response: 0
Conc: N.D.

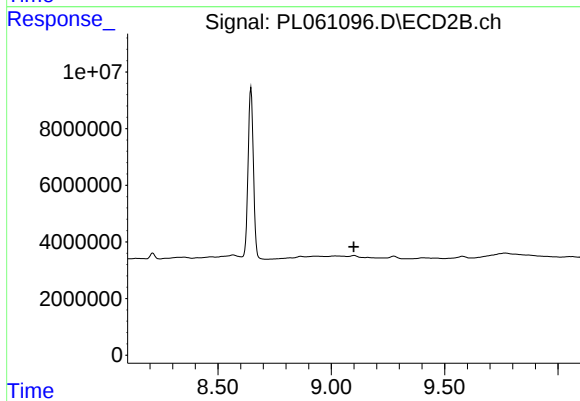

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 9.099 min
Response: 0
Conc: N.D.