

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083120\
 Data File : PL061103.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Aug 2020 18:25
 Operator : DD\AJ
 Sample : L3847-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 02:26:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 25 16:59:57 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.461	4.009	22577604	28405982	12.235	10.929
28)	SA Decachlor...	8.214	9.097	19592429	28089996	11.630	13.313
Target Compounds							
5)	MB Aldrin	0.000	5.499	0	5250297	N.D.	1.558 #
9)	A Endosulfan I	5.526	6.244	1841367	5050848	1.013	1.757 #
10)	B gamma-Chl...	0.000	6.128	0	2595239	N.D.	0.836 #
11)	B alpha-Chl...	0.000	6.196	0	12673145	N.D.	4.076 #
12)	B 4,4'-DDE	0.000	6.348	0	3966448	N.D.	1.372 #
16)	A 4,4'-DDD	0.000	6.843	0	1944438	N.D.	0.833 #
17)	MA 4,4'-DDT	0.000	7.145	0	2301525	N.D.	0.999 #
18)	B Endrin al...	0.000	7.058	0	451365	N.D.	0.207 #
24)	Chlordane-2	0.000	5.499f	0	5250297	N.D.	51.018 #
25)	Chlordane-3	0.000	6.128	0	2595239	N.D.	6.493 #
26)	Chlordane-4	0.000	6.196	0	12673145	N.D.	26.362 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083120\
Data File : PL061103.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Aug 2020 18:25
Operator : DD\AJ
Sample : L3847-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 02:26:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
Quant Title : GC Extractables
QLast Update : Tue Aug 25 16:59:57 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

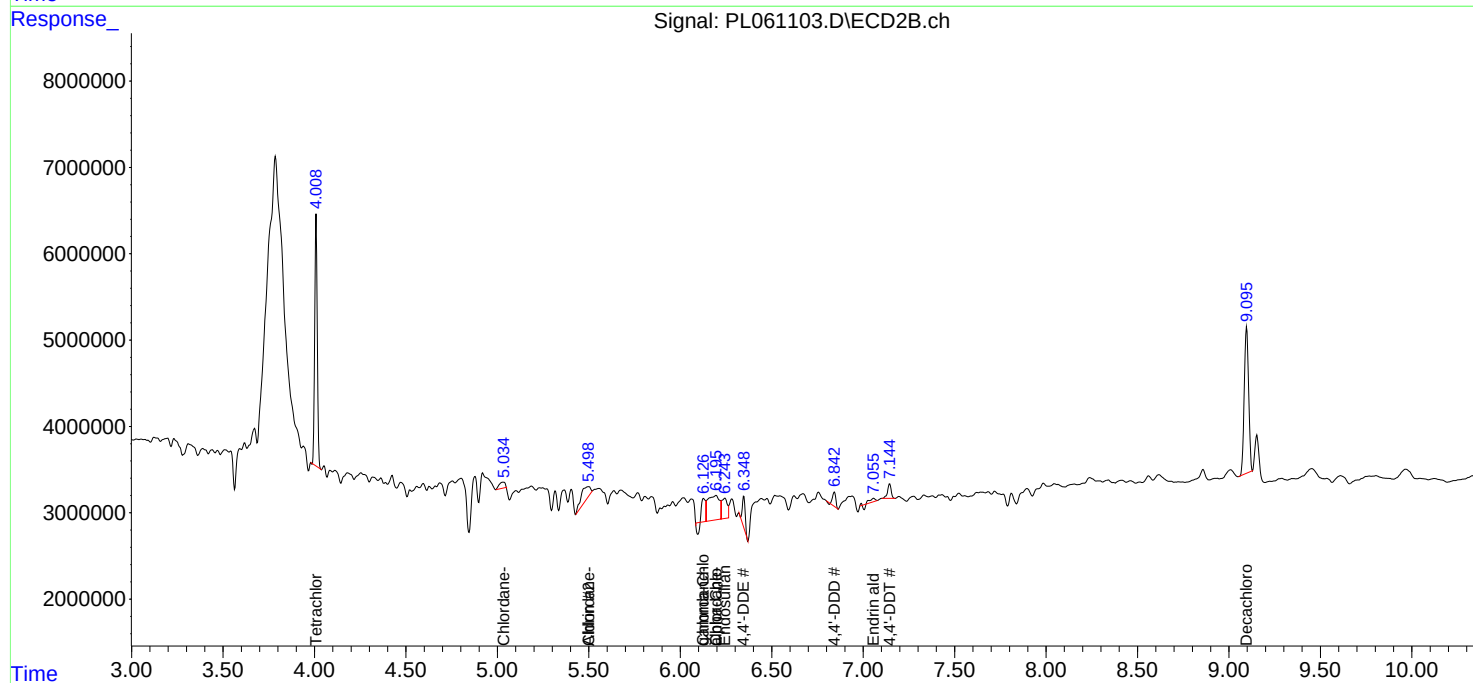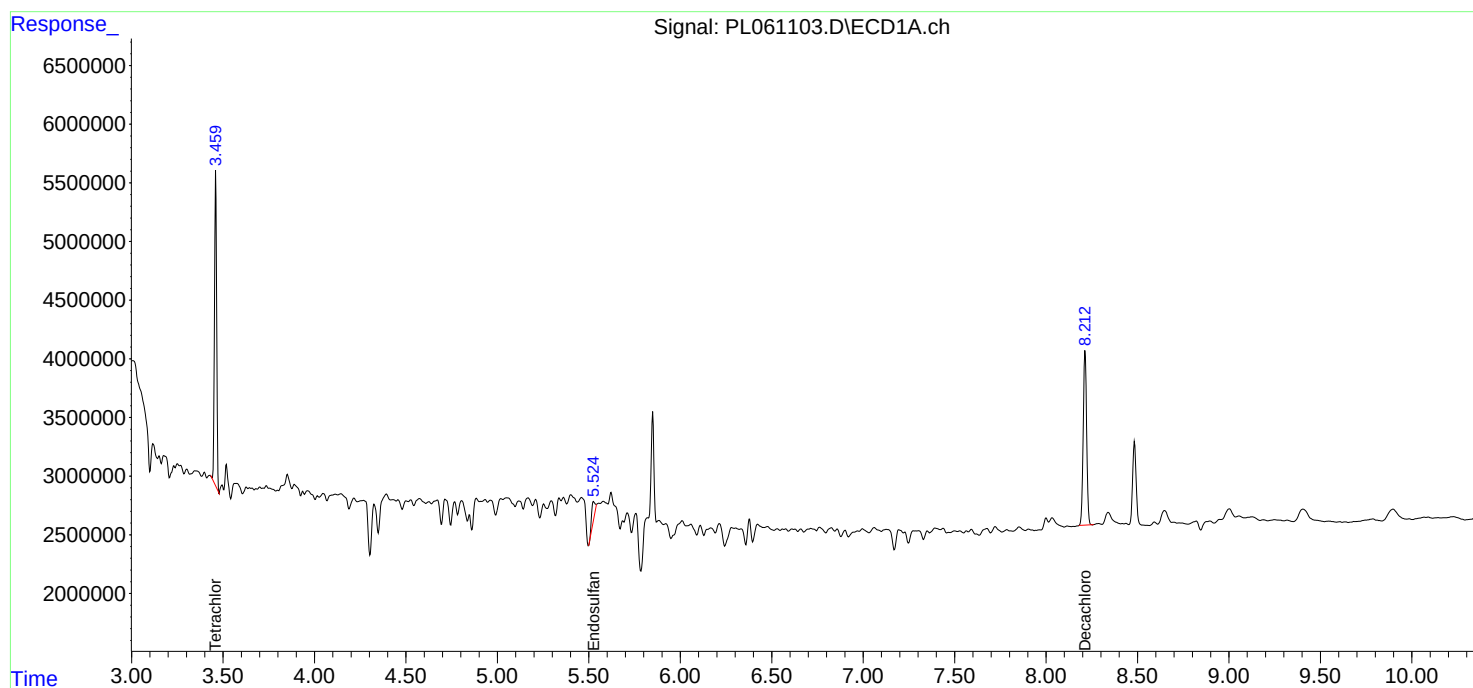


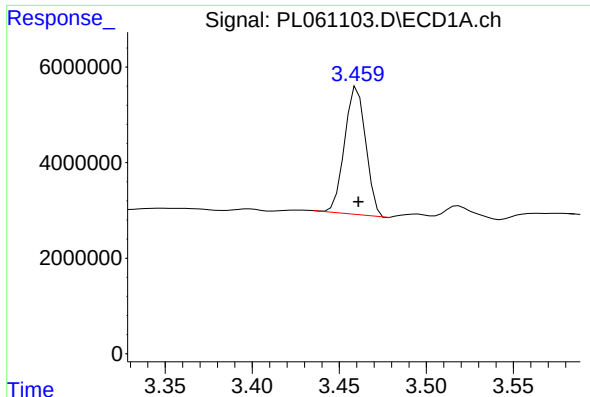

#1 Tetrachloro-m-xylene


R.T.: 3.461 min
Delta R.T.: 0.000 min
Response: 22577604
Conc: 12.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

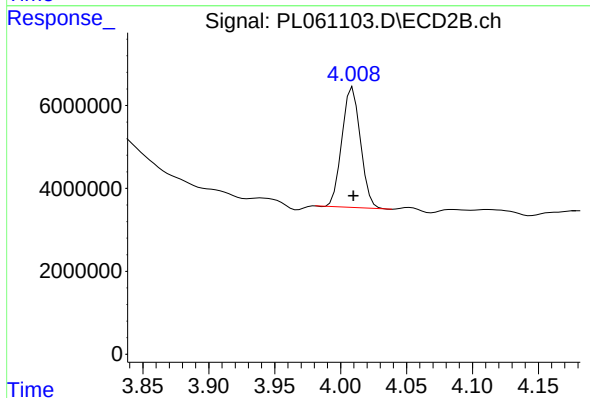


#1 Tetrachloro-m-xylene

R.T.: 4.009 min
Delta R.T.: 0.000 min
Response: 28405982
Conc: 10.93 ng/ml

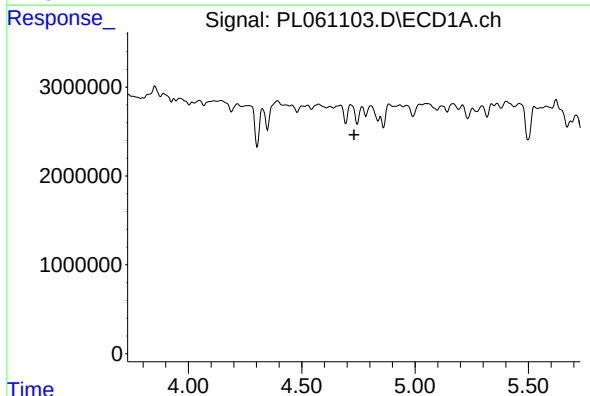


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.732 min
Response: 0
Conc: N.D.

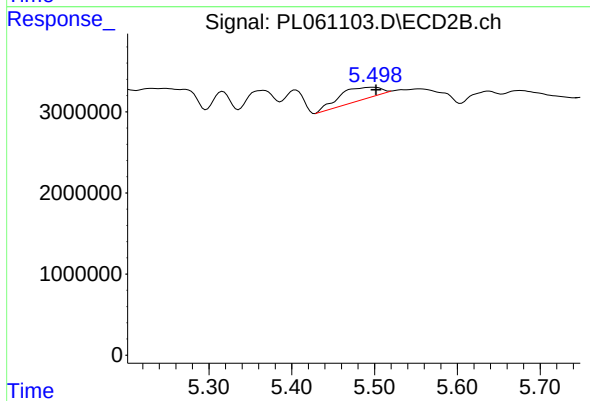

#5 Aldrin


R.T.: 5.499 min
Delta R.T.: -0.003 min
Response: 5250297
Conc: 1.56 ng/ml

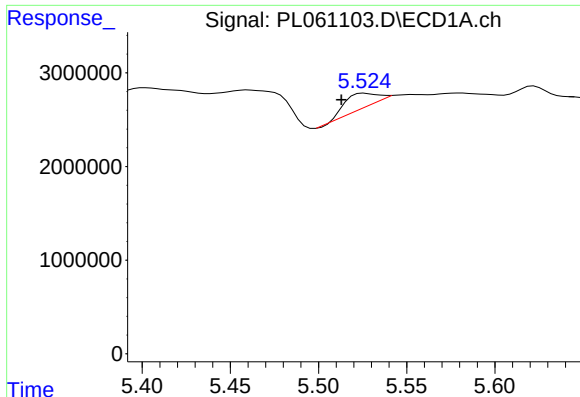

#9 Endosulfan I


R.T.: 5.526 min
Delta R.T.: 0.013 min
Response: 1841367
Conc: 1.01 ng/ml

Instrument :
ECD_L
ClientSampleId :

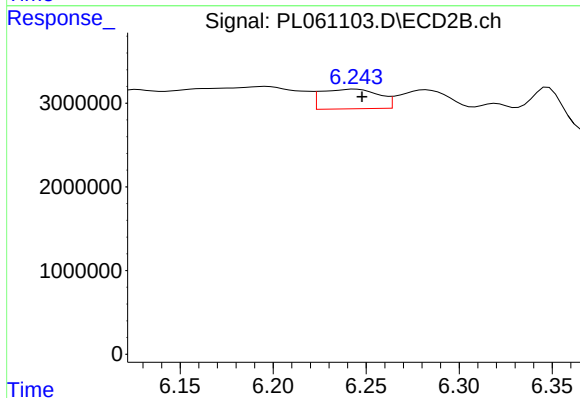


#9 Endosulfan I

R.T.: 6.244 min
Delta R.T.: -0.004 min
Response: 5050848
Conc: 1.76 ng/ml

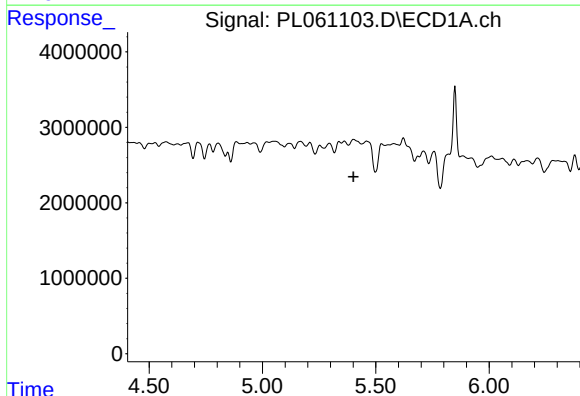


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.402 min
Response: 0
Conc: N.D.

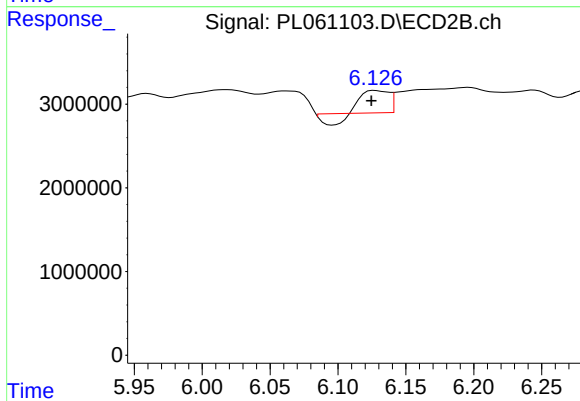

#10 gamma-Chlordane


R.T.: 6.128 min
Delta R.T.: 0.003 min
Response: 2595239
Conc: 0.84 ng/ml

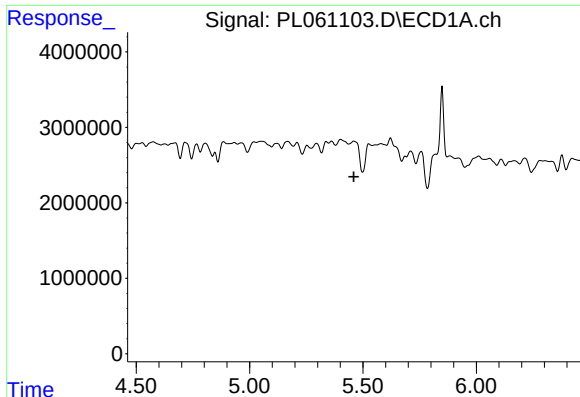

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.460 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

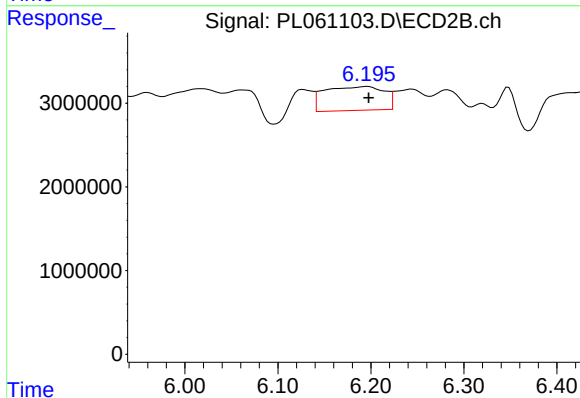


#11 alpha-Chlordane

R.T.: 6.196 min
Delta R.T.: -0.002 min
Response: 12673145
Conc: 4.08 ng/ml

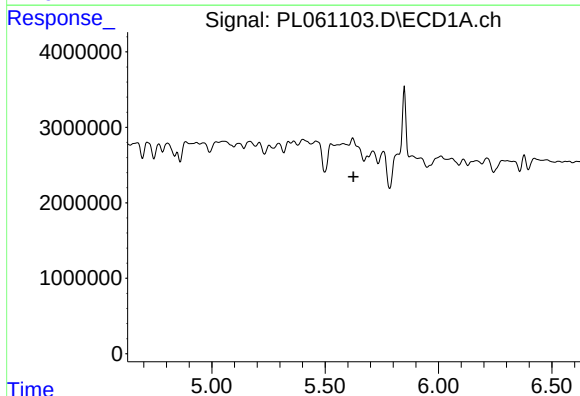


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 5.625 min
Response: 0
Conc: N.D.

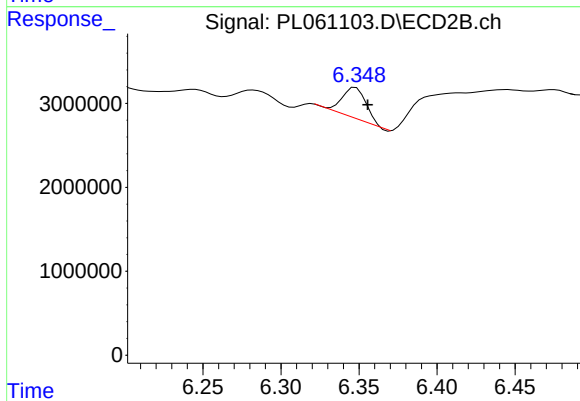

#12 4,4'-DDE


R.T.: 6.348 min
Delta R.T.: -0.008 min
Response: 3966448
Conc: 1.37 ng/ml

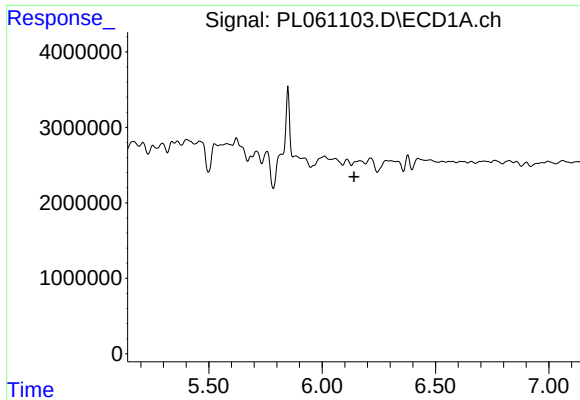

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.141 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

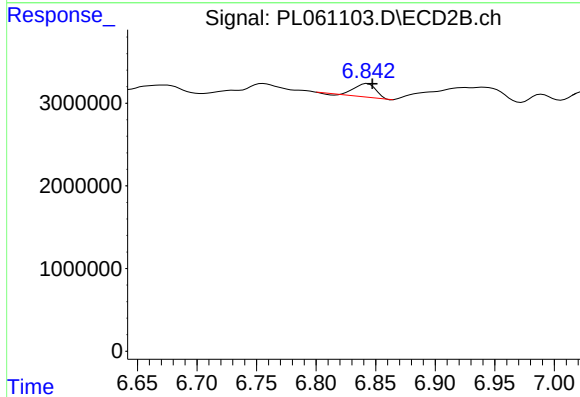


#16 4,4'-DDD

R.T.: 6.843 min
Delta R.T.: -0.004 min
Response: 1944438
Conc: 0.83 ng/ml

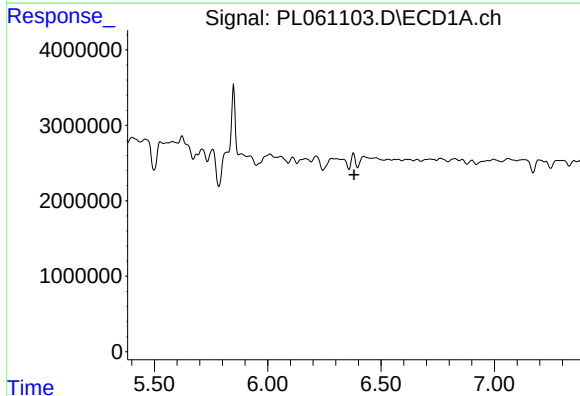


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 6.382 min
Response: 0
Conc: N.D.

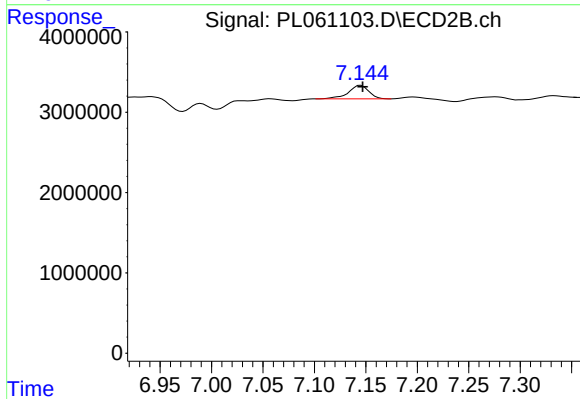

#17 4,4'-DDT


R.T.: 7.145 min
Delta R.T.: -0.002 min
Response: 2301525
Conc: 1.00 ng/ml

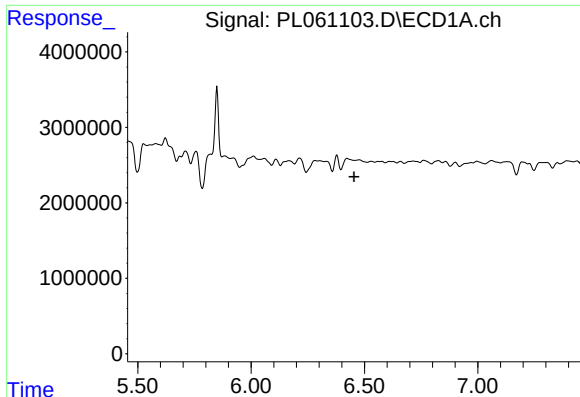

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.454 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

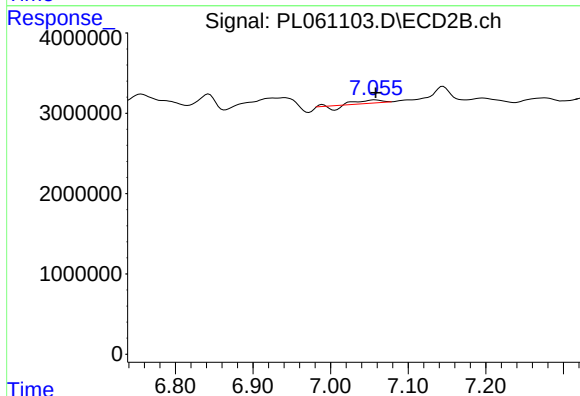


#18 Endrin aldehyde

R.T.: 7.058 min
Delta R.T.: 0.000 min
Response: 451365
Conc: 0.21 ng/ml

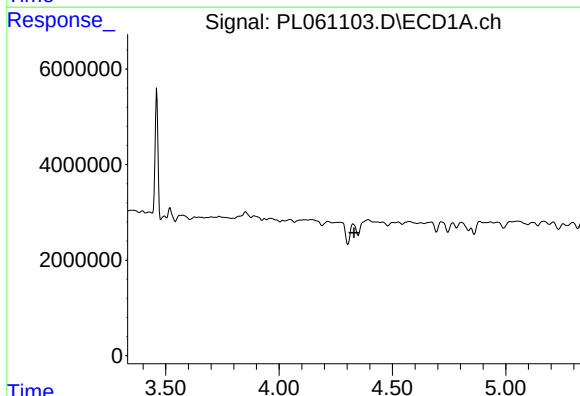


#23 Chlordane-1

R.T.: 4.327 min
Delta R.T.: -0.005 min
Response: -1054433
Conc: N.D.

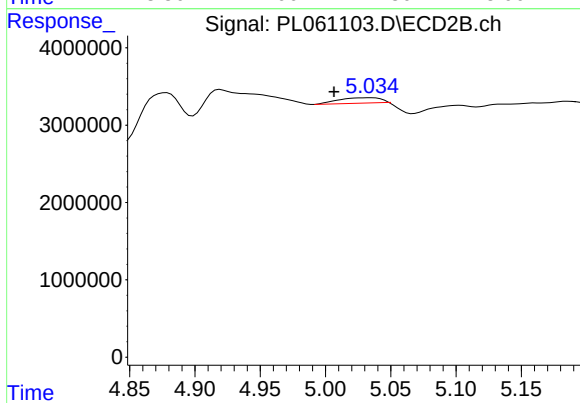

#23 Chlordane-1


R.T.: 5.035 min
Delta R.T.: 0.028 min
Response: 1553217
Conc: 12.77 ng/ml

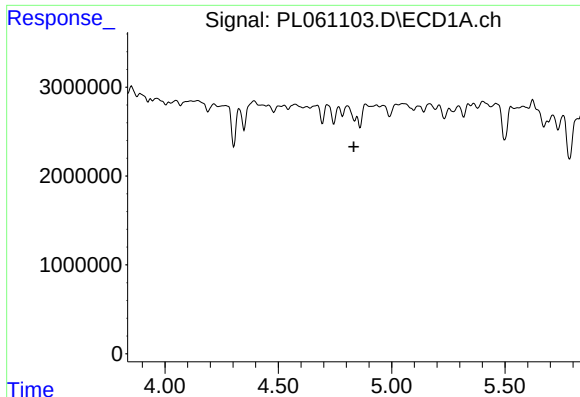

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.833 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

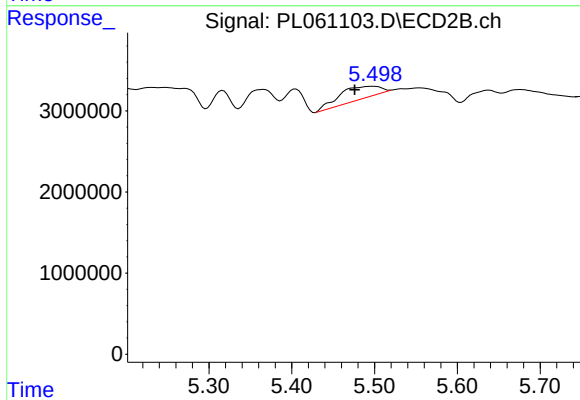


#24 Chlordane-2

R.T.: 5.499 min
Delta R.T.: 0.022 min
Response: 5250297
Conc: 51.02 ng/ml

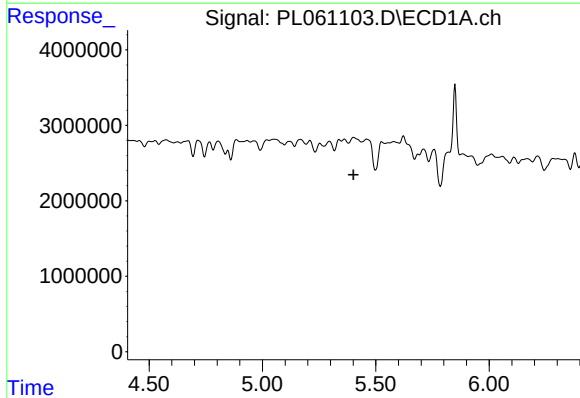


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.402 min
Response: 0
Conc: N.D.

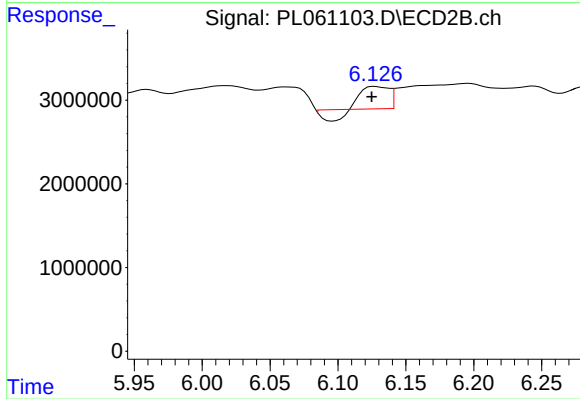

#25 Chlordane-3


R.T.: 6.128 min
Delta R.T.: 0.003 min
Response: 2595239
Conc: 6.49 ng/ml

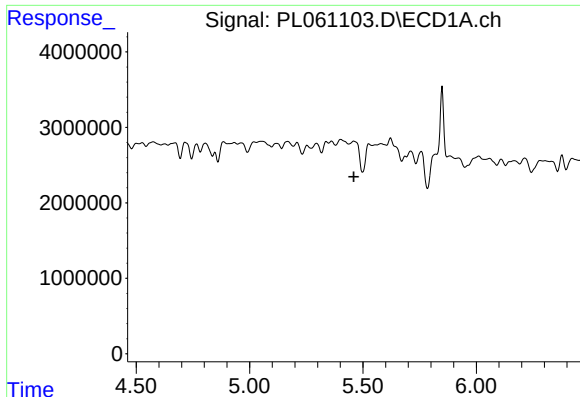

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.460 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

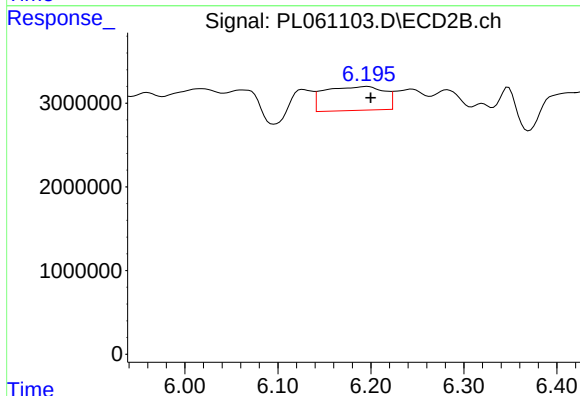


#26 Chlordane-4

R.T.: 6.196 min
Delta R.T.: -0.004 min
Response: 12673145
Conc: 26.36 ng/ml

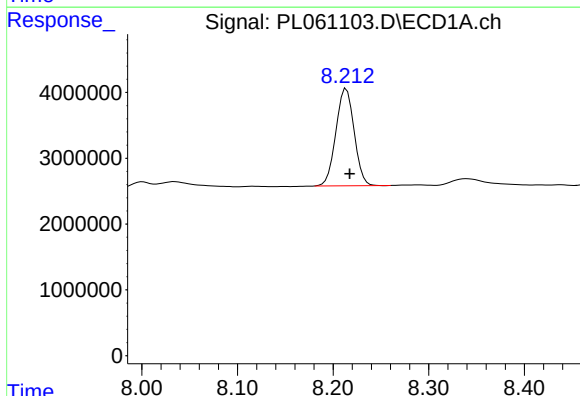

#28 Decachlorobiphenyl

R.T.: 8.214 min
Delta R.T.: -0.003 min
Response: 19592429
Conc: 11.63 ng/ml

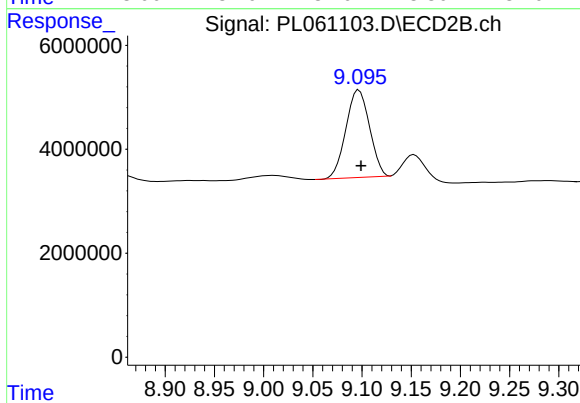

#28 Decachlorobiphenyl

R.T.: 9.097 min
Delta R.T.: -0.002 min
Response: 28089996
Conc: 13.31 ng/ml