

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083120\
 Data File : PL061108.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Aug 2020 19:36
 Operator : DD\AJ
 Sample : L3848-03
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 02:27:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 25 16:59:57 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.461	4.009	23169052	31291189	12.555	12.040
28)	SA Decachlor...	8.214	9.097	16961497	25846338	10.068	12.249
Target Compounds							
5)	MB Aldrin	4.710f	5.503	8717774	6314836	4.178	1.874 #
8)	B Heptachlo...	5.171	0.000	3602999	0	1.827	N.D. #
9)	A Endosulfan I	5.519	6.272f	15350686	1391029	8.448	0.484 #
12)	B 4,4'-DDE	5.622	6.353	6631754	10958699	3.604	3.792
16)	A 4,4'-DDD	6.138	6.846	2974232	5687165	1.881	2.435 #
17)	MA 4,4'-DDT	6.378	7.145	2289890	3826630	1.515	1.662
23)	Chlordane-1	4.335	0.000	4261025	0	69.787	N.D. #
24)	Chlordane-2	4.851f	5.503f	2473019	6314836	38.454	61.362 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083120\
Data File : PL061108.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Aug 2020 19:36
Operator : DD\AJ
Sample : L3848-03
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 02:27:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
Quant Title : GC Extractables
QLast Update : Tue Aug 25 16:59:57 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

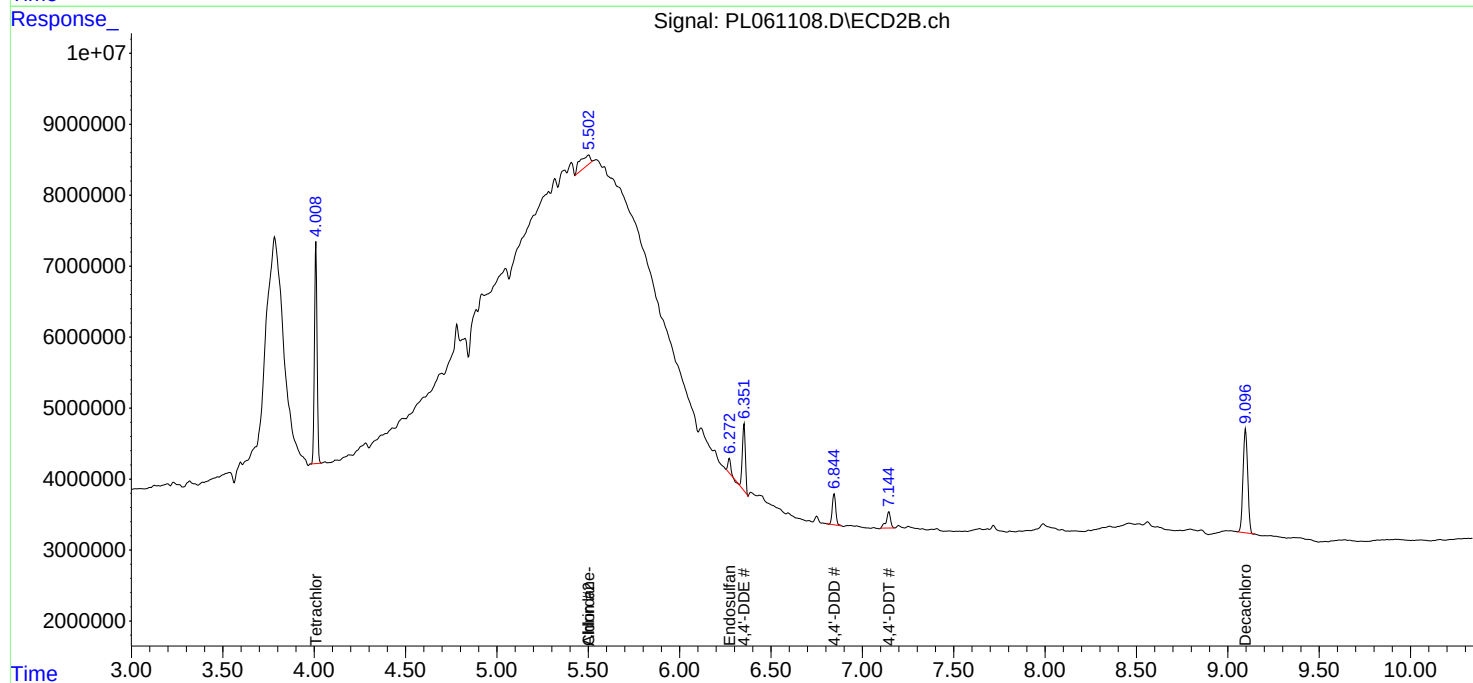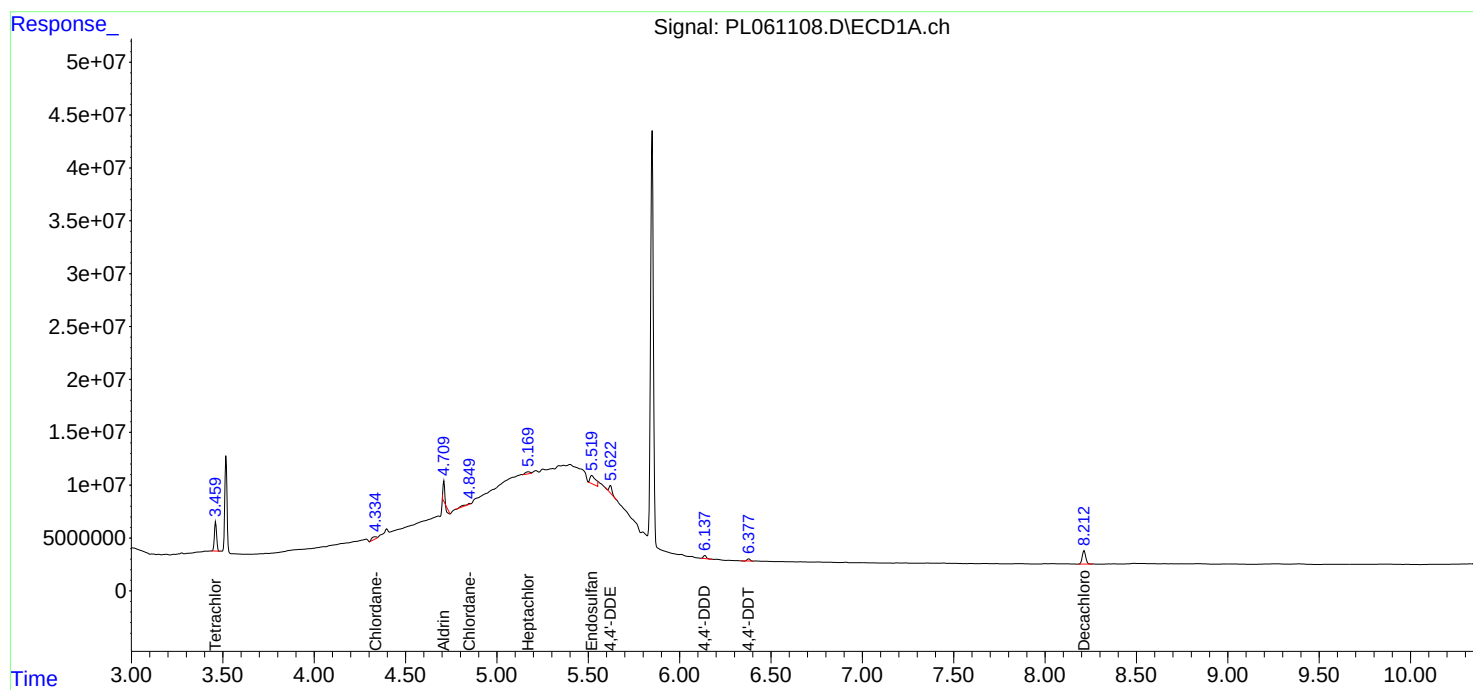


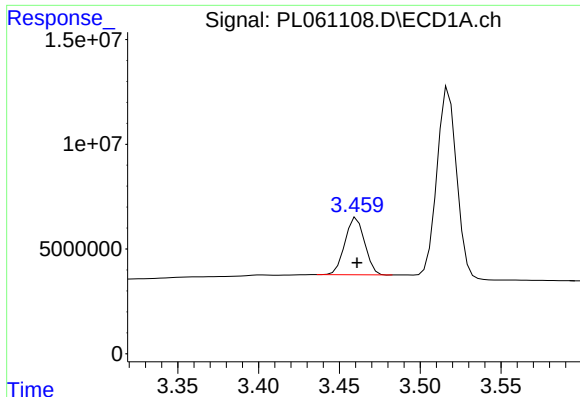

#1 Tetrachloro-m-xylene


R.T.: 3.461 min
Delta R.T.: 0.000 min
Response: 23169052
Conc: 12.56 ng/ml

Instrument :
ECD_L
ClientSampleId :

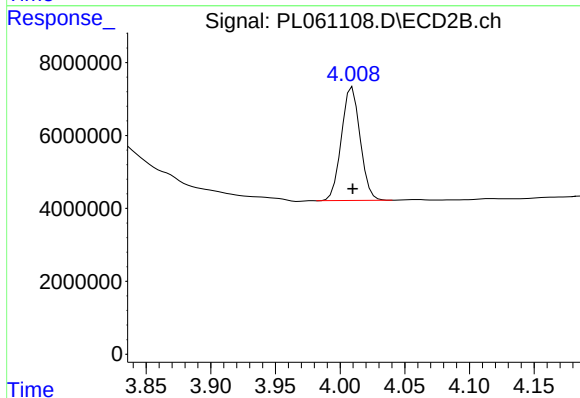


#1 Tetrachloro-m-xylene

R.T.: 4.009 min
Delta R.T.: 0.000 min
Response: 31291189
Conc: 12.04 ng/ml

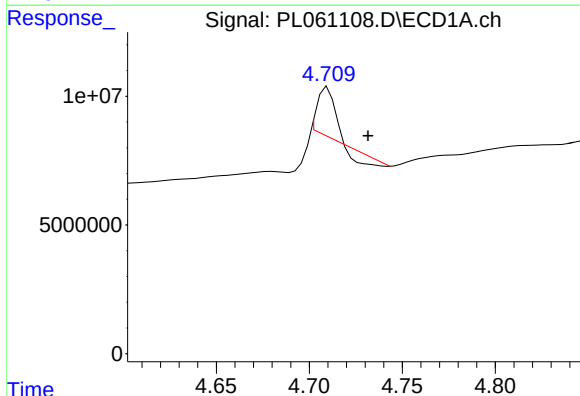


#5 Aldrin

R.T.: 4.710 min
Delta R.T.: -0.021 min
Response: 8717774
Conc: 4.18 ng/ml

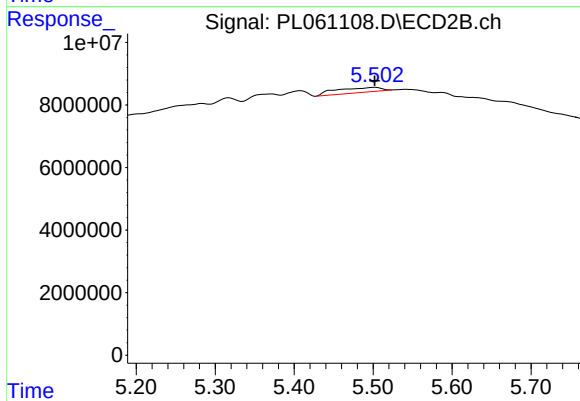

#5 Aldrin


R.T.: 5.503 min
Delta R.T.: 0.000 min
Response: 6314836
Conc: 1.87 ng/ml

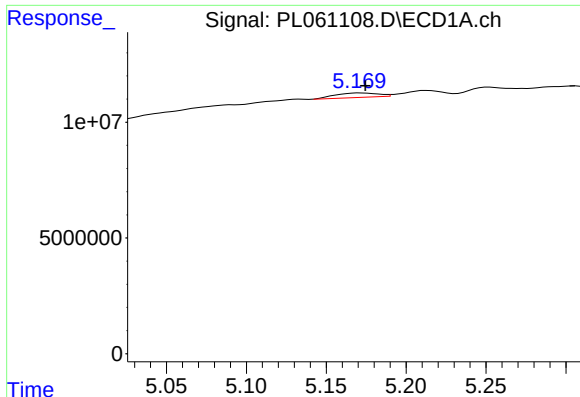

#8 Heptachlor epoxide


R.T.: 5.171 min
Delta R.T.: -0.004 min
Response: 3602999
Conc: 1.83 ng/ml

Instrument :
ECD_L
ClientSampleId :

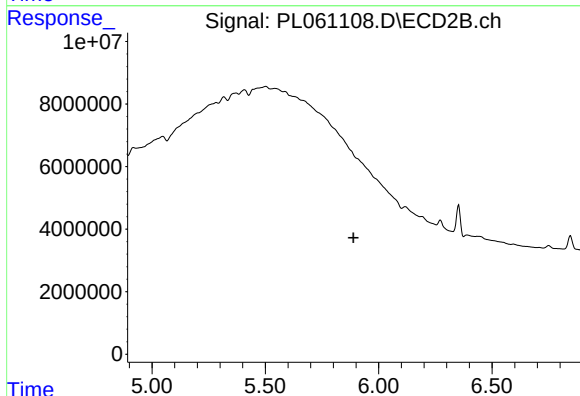


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.889 min
Response: 0
Conc: N.D.

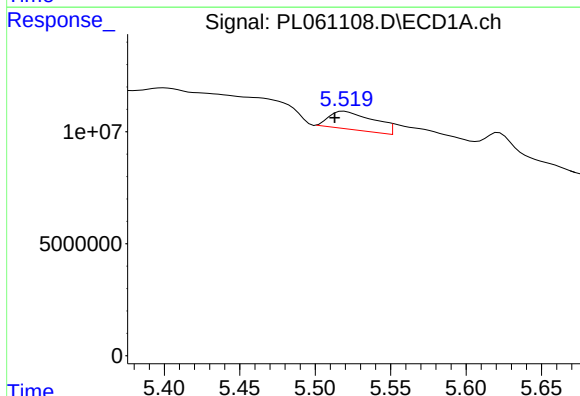


#9 Endosulfan I

R.T.: 5.519 min
Delta R.T.: 0.006 min
Response: 15350686
Conc: 8.45 ng/ml

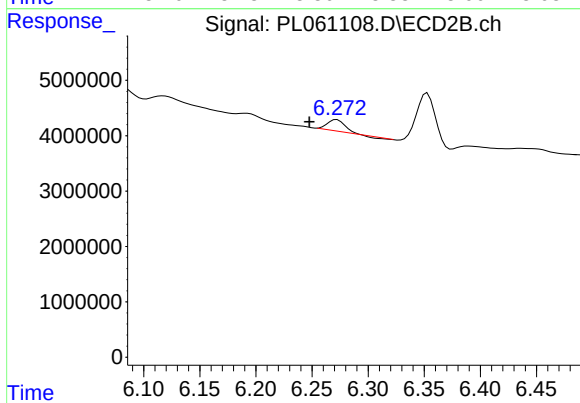

#9 Endosulfan I


R.T.: 6.272 min
Delta R.T.: 0.024 min
Response: 1391029
Conc: 0.48 ng/ml

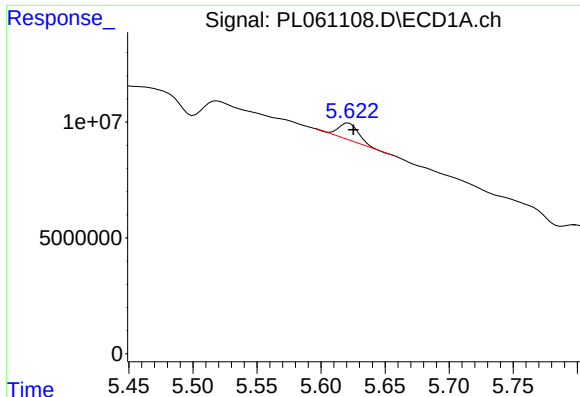

#12 4,4'-DDE


R.T.: 5.622 min
Delta R.T.: -0.004 min
Response: 6631754
Conc: 3.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

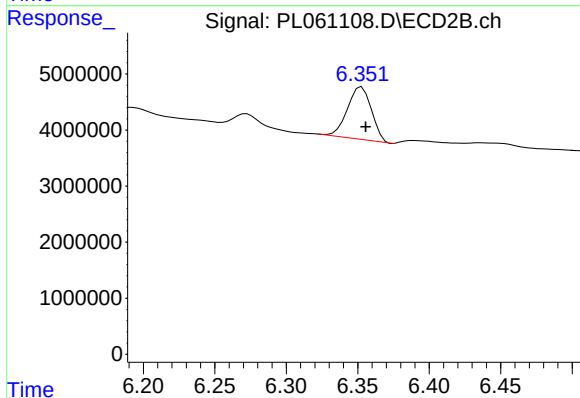


#12 4,4'-DDE

R.T.: 6.353 min
Delta R.T.: -0.003 min
Response: 10958699
Conc: 3.79 ng/ml

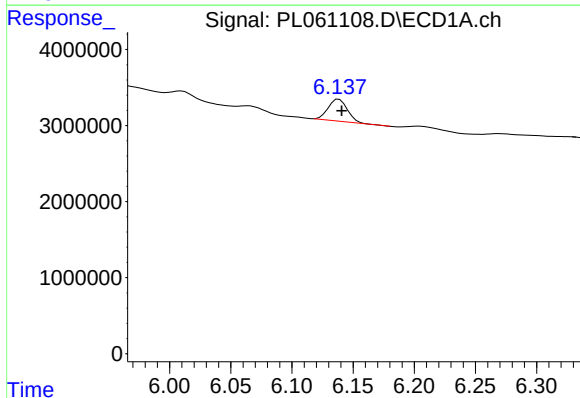


#16 4,4'-DDD

R.T.: 6.138 min
Delta R.T.: -0.002 min
Response: 2974232
Conc: 1.88 ng/ml

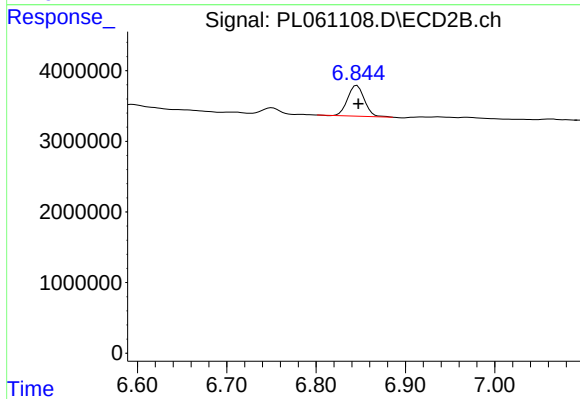

#16 4,4'-DDD


R.T.: 6.846 min
Delta R.T.: -0.002 min
Response: 5687165
Conc: 2.44 ng/ml

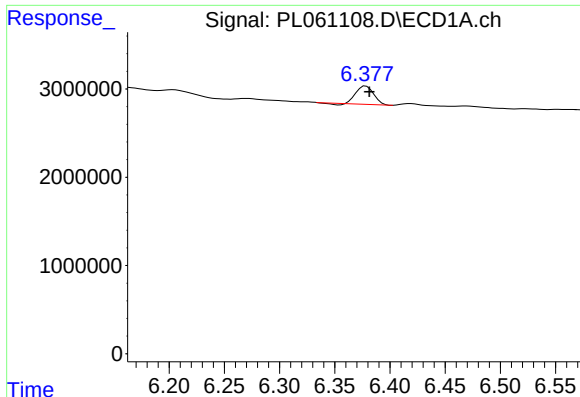

#17 4,4'-DDT


R.T.: 6.378 min
Delta R.T.: -0.003 min
Response: 2289890
Conc: 1.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

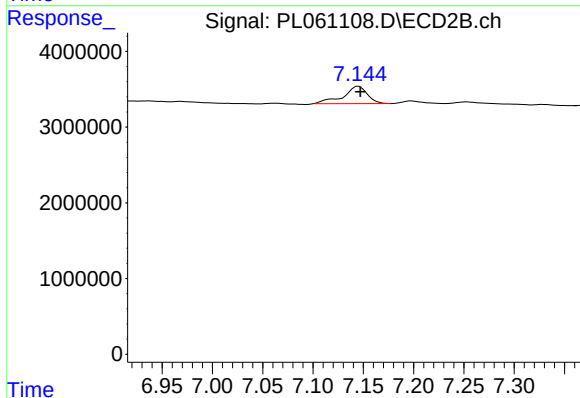


#17 4,4'-DDT

R.T.: 7.145 min
Delta R.T.: -0.002 min
Response: 3826630
Conc: 1.66 ng/ml

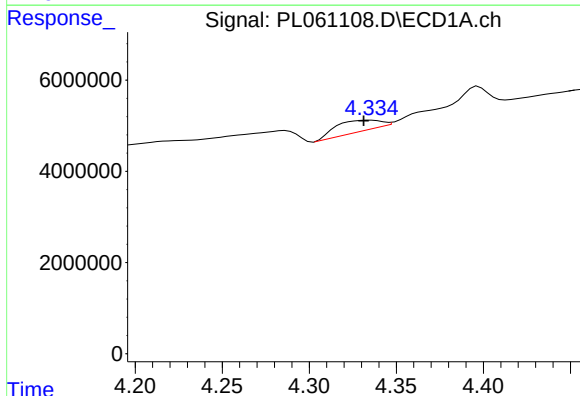


#23 Chlordane-1

R.T.: 4.335 min
Delta R.T.: 0.004 min
Response: 4261025
Conc: 69.79 ng/ml

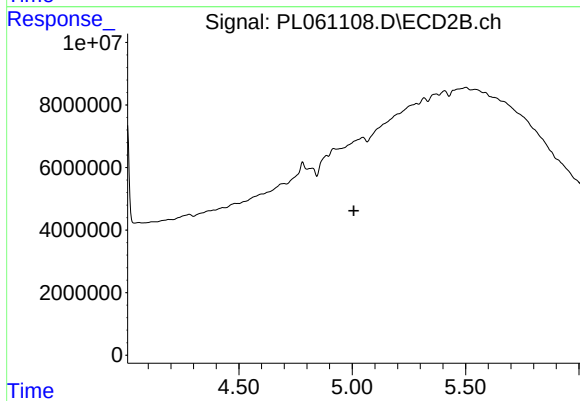

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.007 min
Response: 0
Conc: N.D.

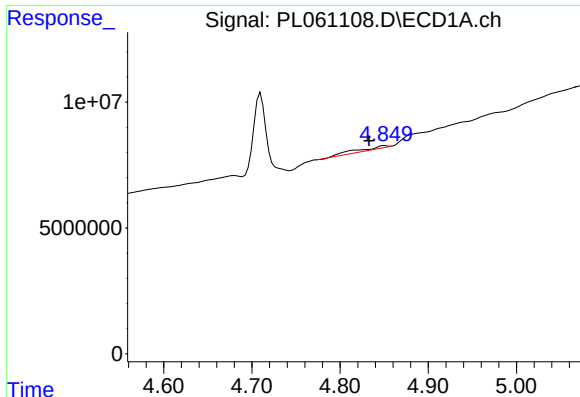

#24 Chlordane-2


R.T.: 4.851 min
Delta R.T.: 0.018 min
Response: 2473019
Conc: 38.45 ng/ml

Instrument :
ECD_L
ClientSampleId :

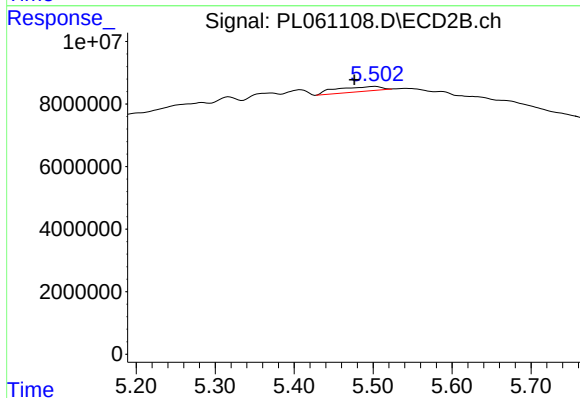


#24 Chlordane-2

R.T.: 5.503 min
Delta R.T.: 0.027 min
Response: 6314836
Conc: 61.36 ng/ml

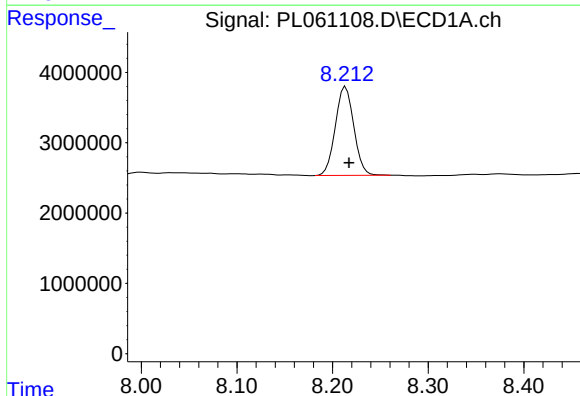

#28 Decachlorobiphenyl

R.T.: 8.214 min
Delta R.T.: -0.004 min
Response: 16961497
Conc: 10.07 ng/ml

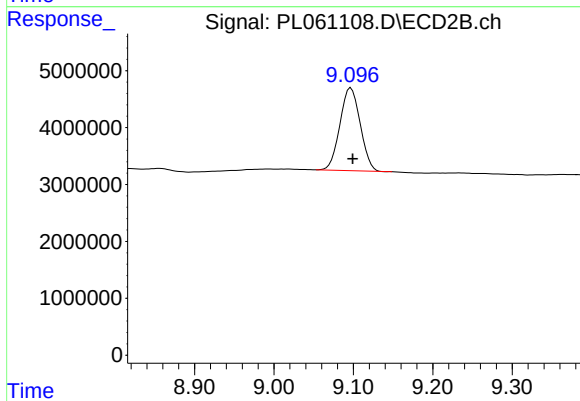

#28 Decachlorobiphenyl

R.T.: 9.097 min
Delta R.T.: -0.002 min
Response: 25846338
Conc: 12.25 ng/ml