

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083120\
 Data File : PL061098.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Aug 2020 17:15
 Operator : DD\AJ
 Sample : L3837-18
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 789UMR-TP11-2430-01

Manual Integrations
 APPROVED

Ankita
 9/1/2020 1:29:17 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 02:25:35 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 25 16:59:57 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
12) B	4,4'-DDE	5.623	6.353	24658059	32858098	11.369
16) A	4,4'-DDD	6.139	6.843	1576375	2868952	1.228m
17) MA	4,4'-DDT	6.379	7.145	11453327	17740082	7.703

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083120\
Data File : PL061098.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Aug 2020 17:15
Operator : DD\AJ
Sample : L3837-18
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
789UMR-TP11-2430-01


Manual Integrations
APPROVED

Ankita
9/1/2020 1:29:17 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 02:25:35 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
Quant Title : GC Extractables
QLast Update : Tue Aug 25 16:59:57 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

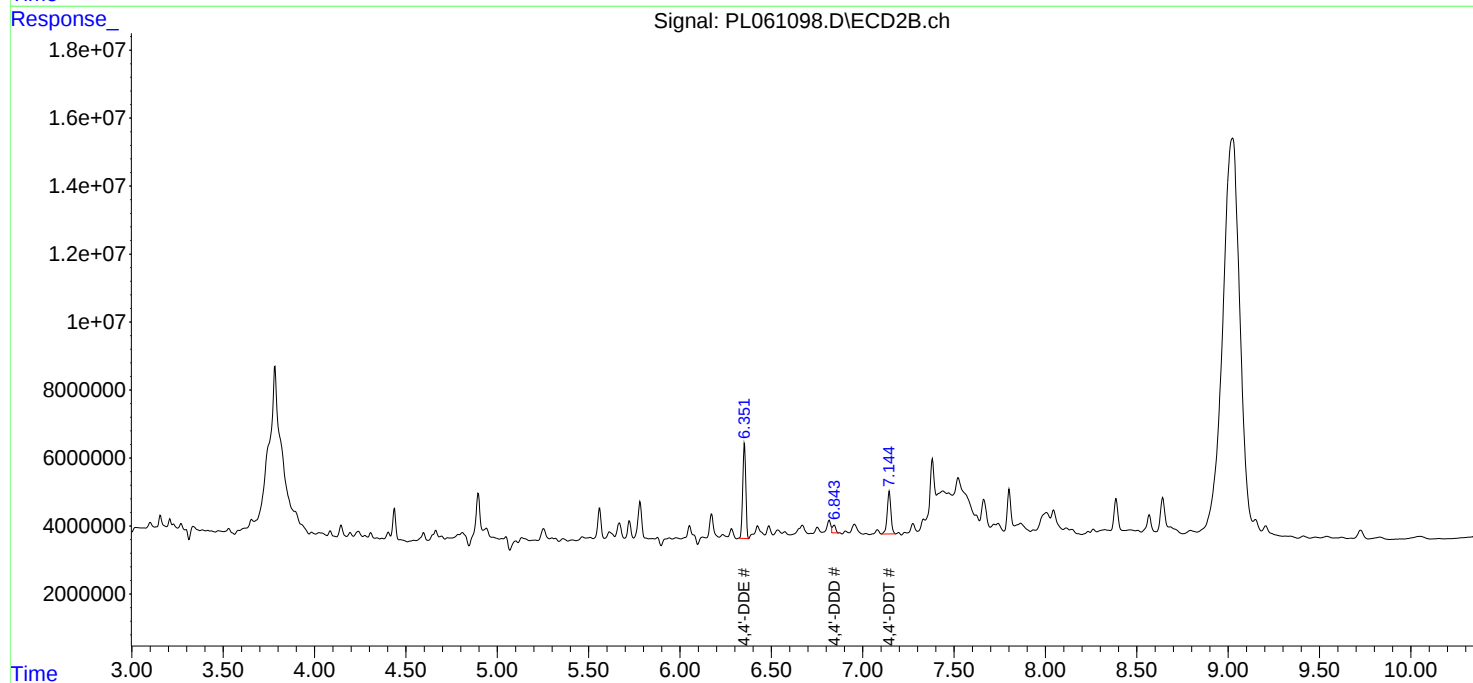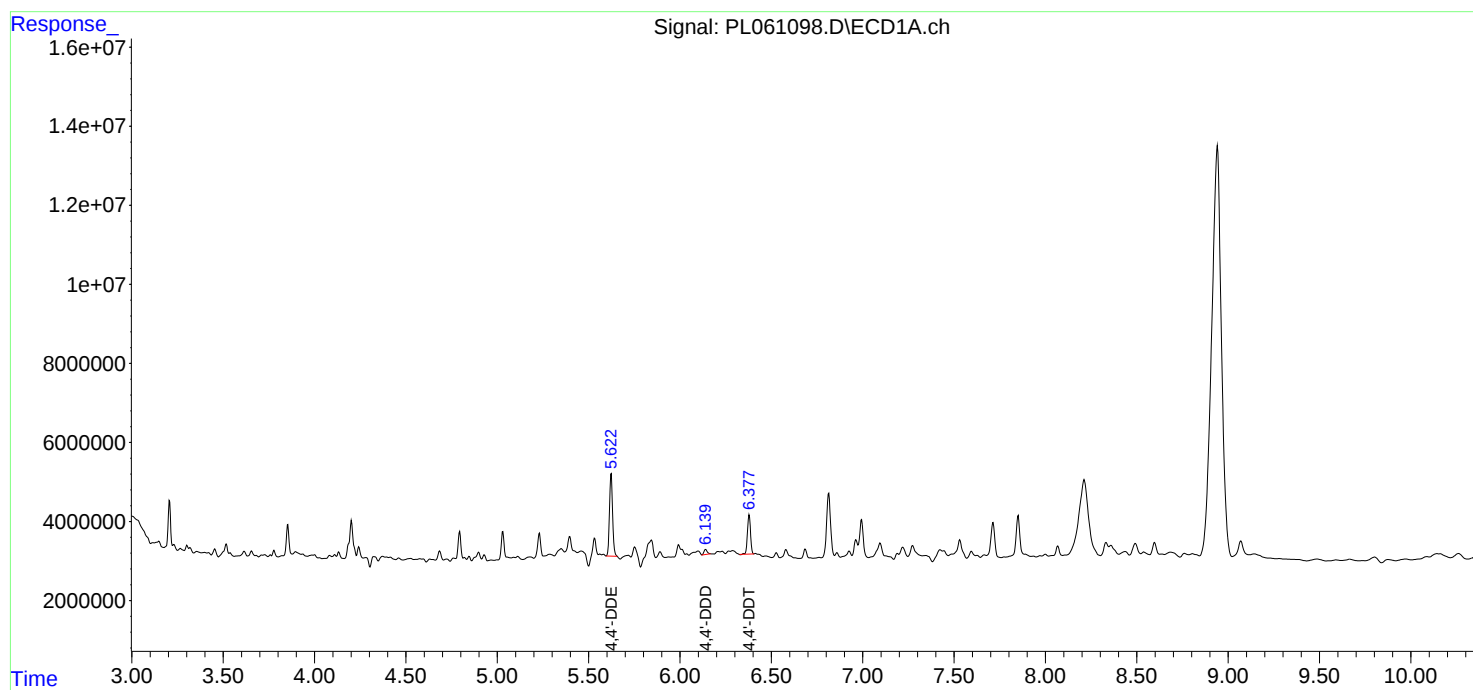

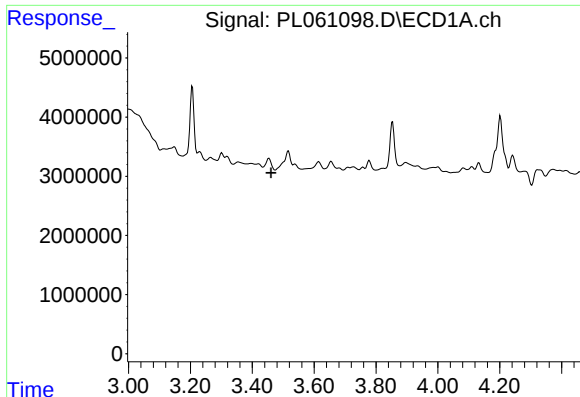


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 3.461 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
789UMR-TP11-2430-01


Manual Integrations
APPROVED

Ankita
9/1/2020 1:29:17 PM

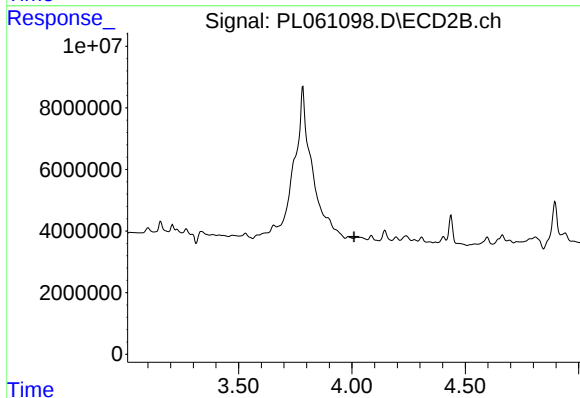


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 4.010 min
Response: 0
Conc: N.D.

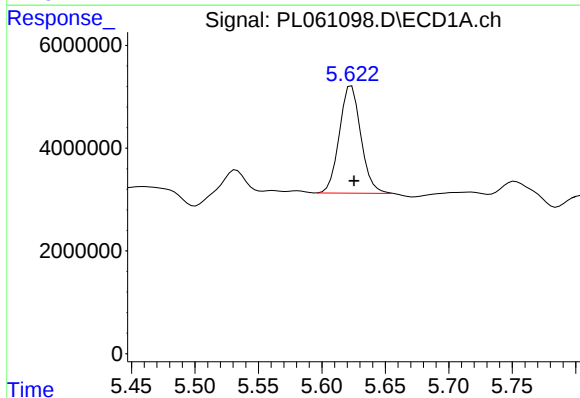


#12 4,4'-DDE

R.T.: 5.623 min
Delta R.T.: -0.002 min
Response: 24658059
Conc: 13.40 ng/ml

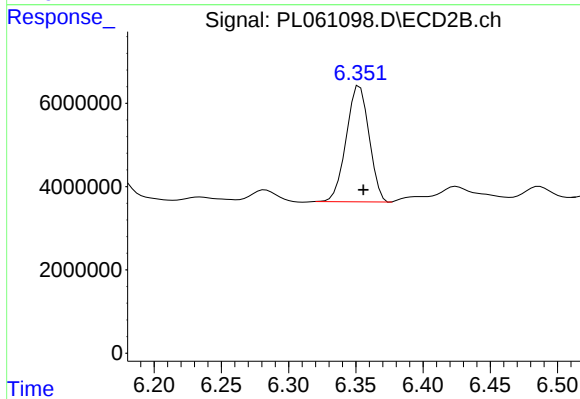

#12 4,4'-DDE

R.T.: 6.353 min
Delta R.T.: -0.003 min
Response: 32858098
Conc: 11.37 ng/ml

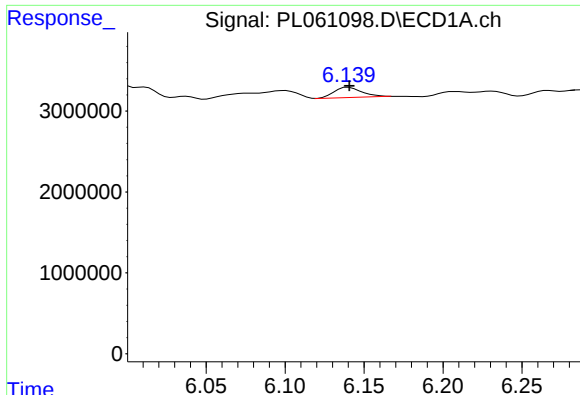


#16 4,4'-DDD

R.T.: 6.139 min
Delta R.T.: -0.002 min
Response: 1576375
Conc: 1.00 ng/ml m

Instrument :
ECD_L
ClientSampleId :
789UMR-TP11-2430-01


Manual Integrations
APPROVED

Ankita
9/1/2020 1:29:17 PM

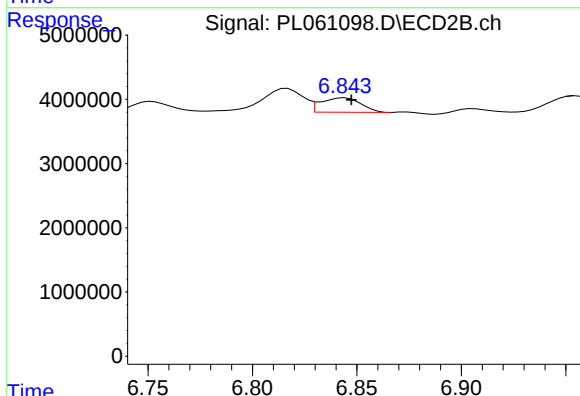


#16 4,4'-DDD

R.T.: 6.843 min
Delta R.T.: -0.004 min
Response: 2868952
Conc: 1.23 ng/ml m

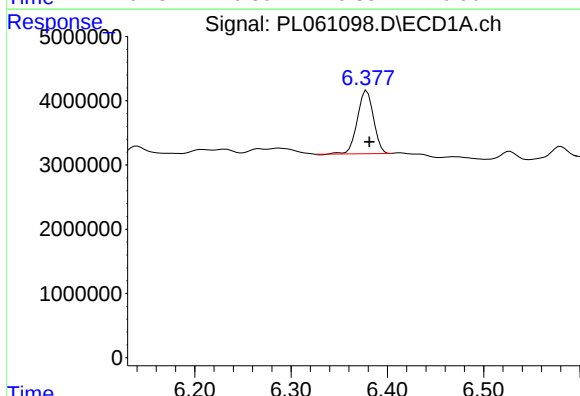


#17 4,4'-DDT

R.T.: 6.379 min
Delta R.T.: -0.003 min
Response: 11453327
Conc: 7.58 ng/ml

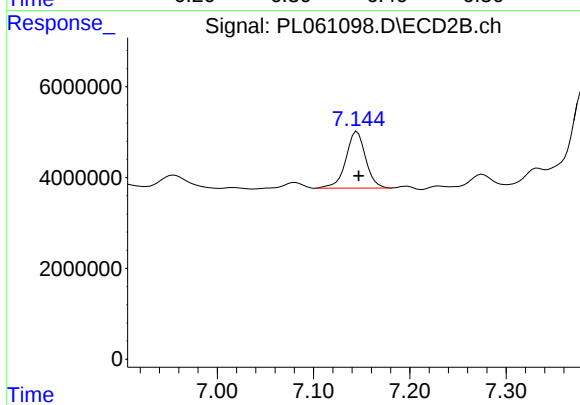

#17 4,4'-DDT

R.T.: 7.145 min
Delta R.T.: -0.002 min
Response: 17740082
Conc: 7.70 ng/ml

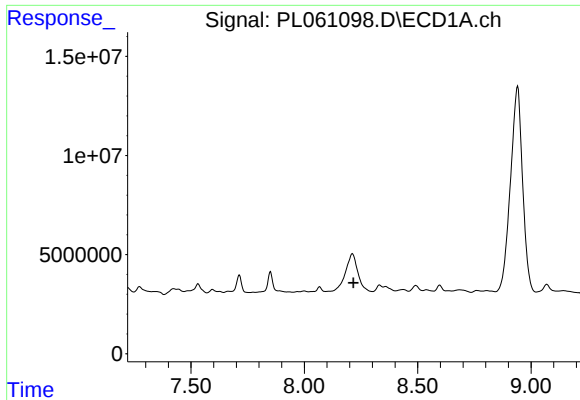


#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.217 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
789UMR-TP11-2430-01

Manual Integrations
APPROVED

Ankita
9/1/2020 1:29:17 PM

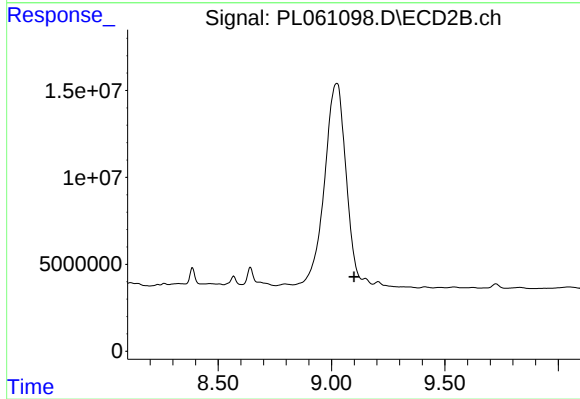

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.099 min
Response: 0
Conc: N.D.