

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083120\
 Data File : PL061103.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Aug 2020 18:25
 Operator : DD\AJ
 Sample : L3847-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 LINDEN-JOP-BH-08-A

Manual Integrations
 APPROVED

Ankita
 9/1/2020 1:29:25 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 02:26:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 25 16:59:57 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.461	4.009	22577604	28405982	12.235	10.929
28)	SA Decachlor...	8.214	9.097	19592429	28089996	11.630	13.313
Target Compounds							
12)	B 4,4'-DDE	5.621	6.348	1040186	3966448	0.565m	1.372 #
17)	MA 4,4'-DDT	6.377	7.145	2380375	2301525	1.575m	0.999 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083120\
Data File : PL061103.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Aug 2020 18:25
Operator : DD\AJ
Sample : L3847-01
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
LINDEN-JOP-BH-08-A


Manual Integrations
APPROVED

Ankita
9/1/2020 1:29:25 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 02:26:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
Quant Title : GC Extractables
QLast Update : Tue Aug 25 16:59:57 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

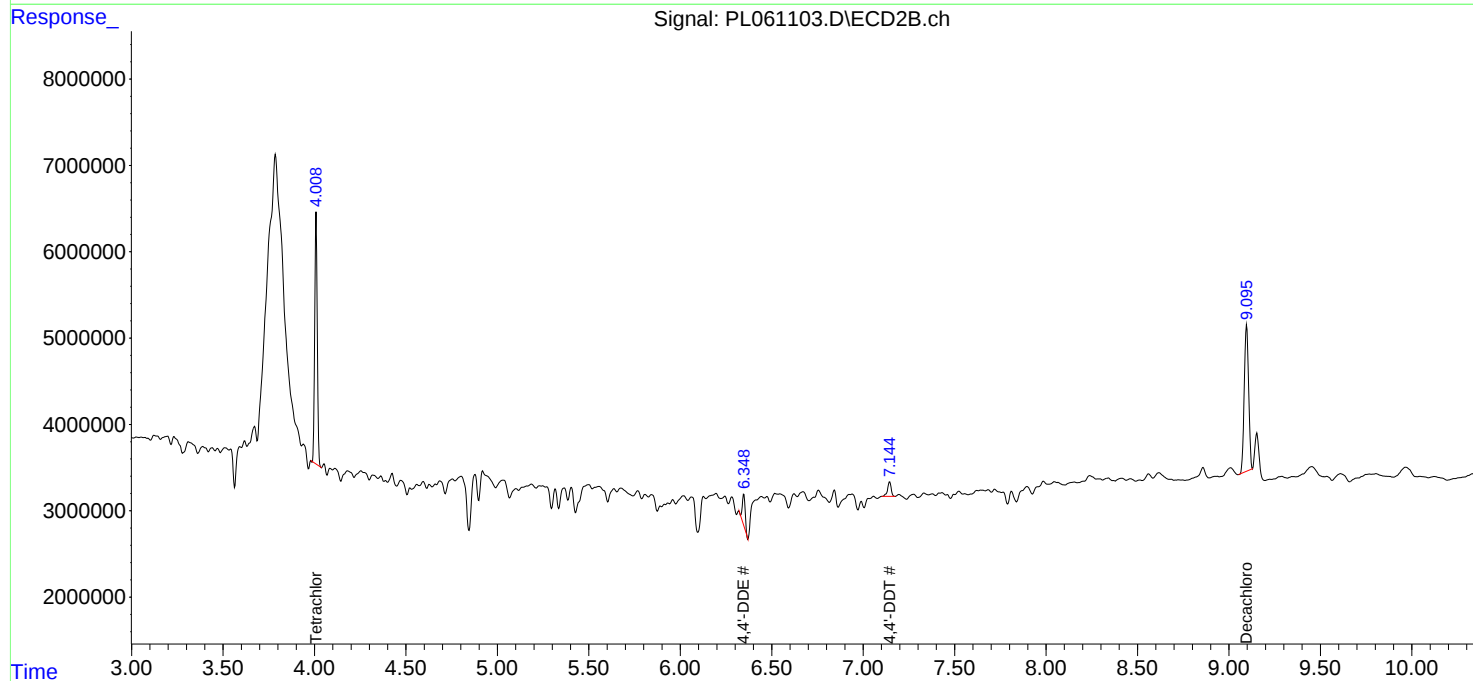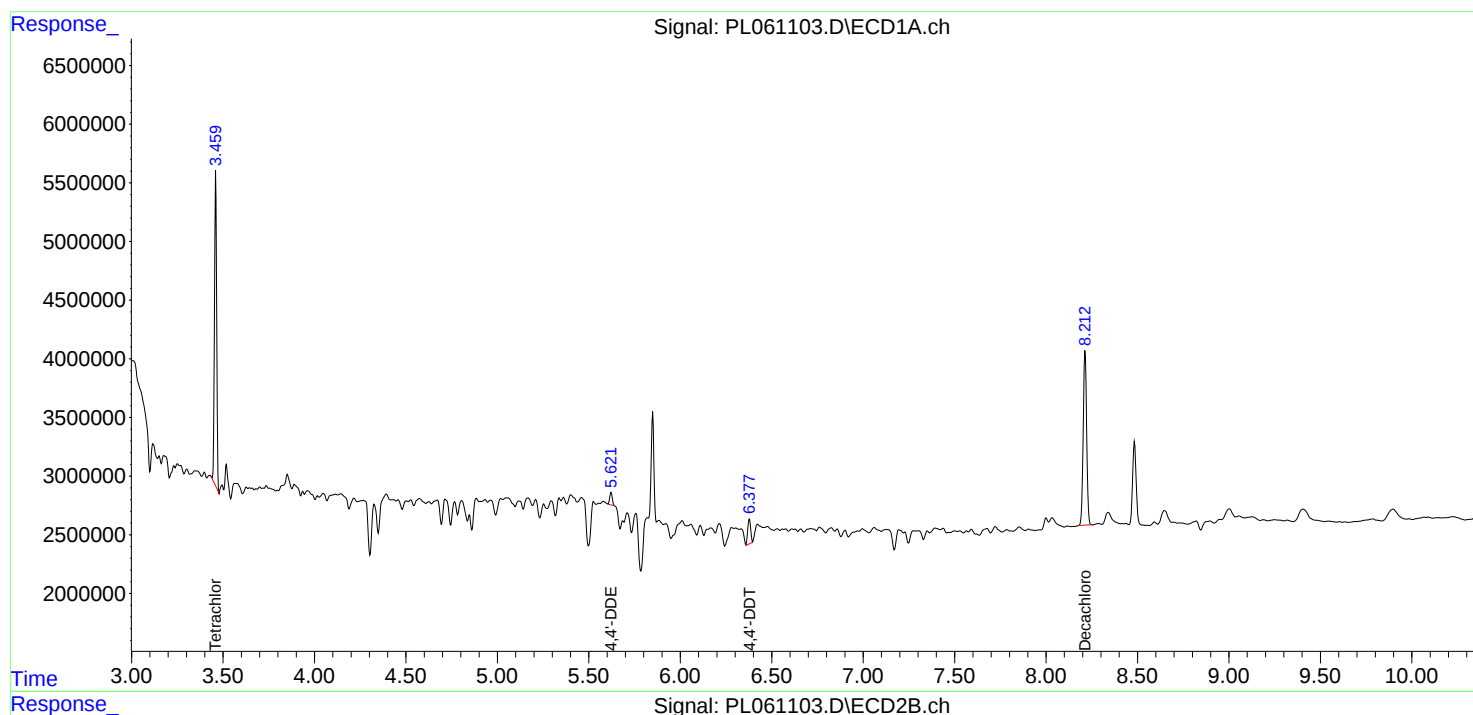

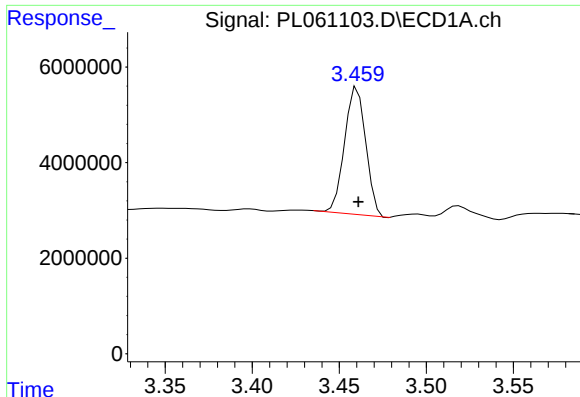


#1 Tetrachloro-m-xylene

R.T.: 3.461 min
Delta R.T.: 0.000 min
Response: 22577604
Conc: 12.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
LINDEN-JOP-BH-08-A


Manual Integrations
APPROVED

Ankita
9/1/2020 1:29:25 PM

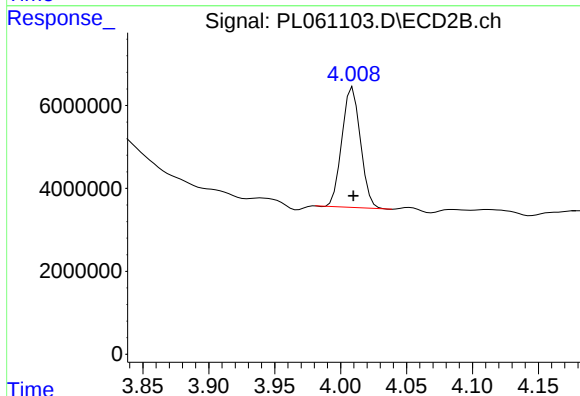


#1 Tetrachloro-m-xylene

R.T.: 4.009 min
Delta R.T.: 0.000 min
Response: 28405982
Conc: 10.93 ng/ml

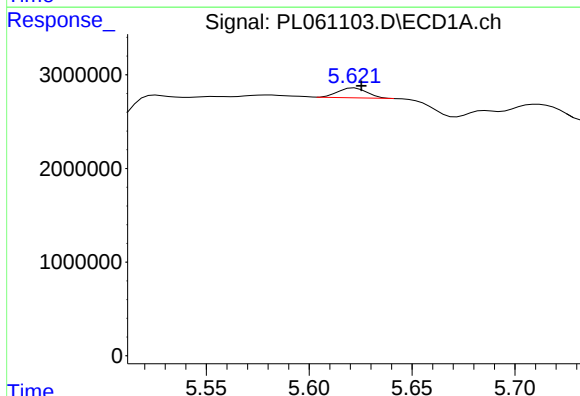


#12 4,4'-DDE

R.T.: 5.621 min
Delta R.T.: -0.005 min
Response: 1040186
Conc: 0.57 ng/ml m

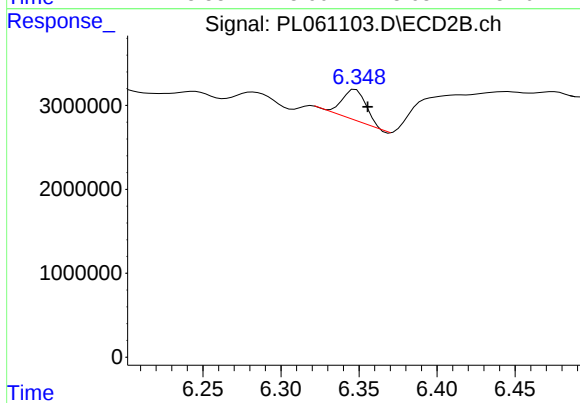

#12 4,4'-DDE

R.T.: 6.348 min
Delta R.T.: -0.008 min
Response: 3966448
Conc: 1.37 ng/ml

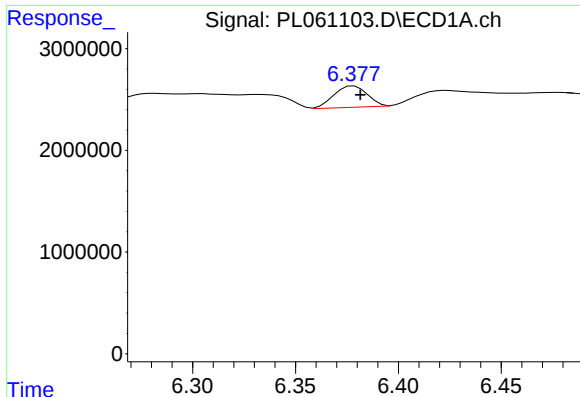


#17 4,4'-DDT

R.T.: 6.377 min
Delta R.T.: -0.005 min
Response: 2380375
Conc: 1.57 ng/ml m

Instrument :
ECD_L
ClientSampleId :
LINDEN-JOP-BH-08-A


Manual Integrations
APPROVED

Ankita
9/1/2020 1:29:25 PM

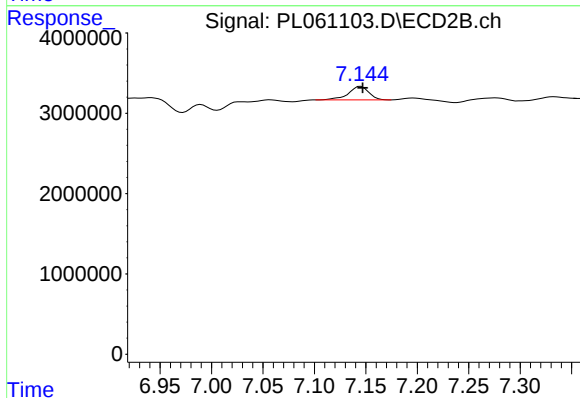


#17 4,4'-DDT

R.T.: 7.145 min
Delta R.T.: -0.002 min
Response: 2301525
Conc: 1.00 ng/ml

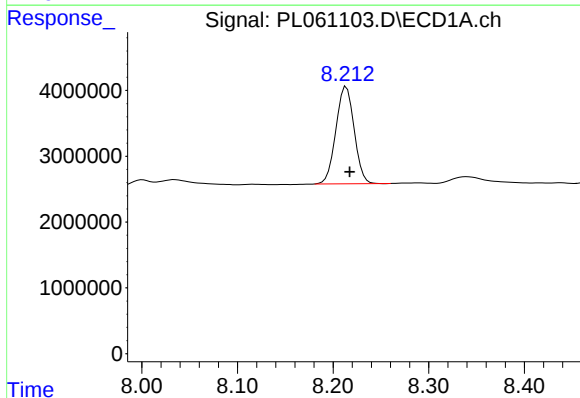

#28 Decachlorobiphenyl

R.T.: 8.214 min
Delta R.T.: -0.003 min
Response: 19592429
Conc: 11.63 ng/ml

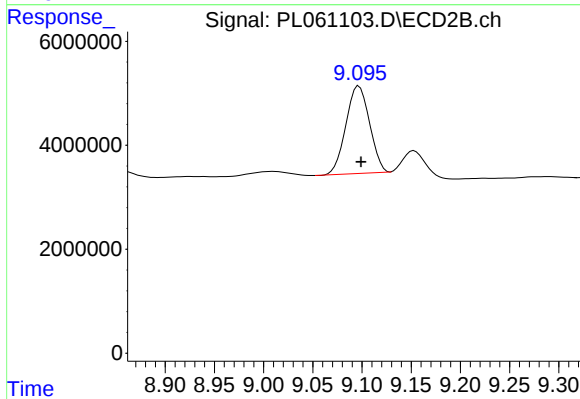

#28 Decachlorobiphenyl

R.T.: 9.097 min
Delta R.T.: -0.002 min
Response: 28089996
Conc: 13.31 ng/ml