

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083120\
 Data File : PL061104.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Aug 2020 18:39
 Operator : DD\AJ
 Sample : L3847-07
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 LINDEN-JOP-BH-09-A

Manual Integrations
 APPROVED

Ankita
 9/1/2020 1:29:26 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 02:26:49 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 25 16:59:57 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.461	4.009	24622367	29246163	13.343	11.253
28)	SA Decachlor...	8.213	9.096	23493990	35633160	13.946	16.888m
Target Compounds							
17)	MA 4,4'-DDT	6.377	7.144	3013110	2243212	1.993m	0.974 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083120\
Data File : PL061104.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Aug 2020 18:39
Operator : DD\AJ
Sample : L3847-07
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
LINDEN-JOP-BH-09-A


Manual Integrations
APPROVED

Ankita
9/1/2020 1:29:26 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 02:26:49 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
Quant Title : GC Extractables
QLast Update : Tue Aug 25 16:59:57 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

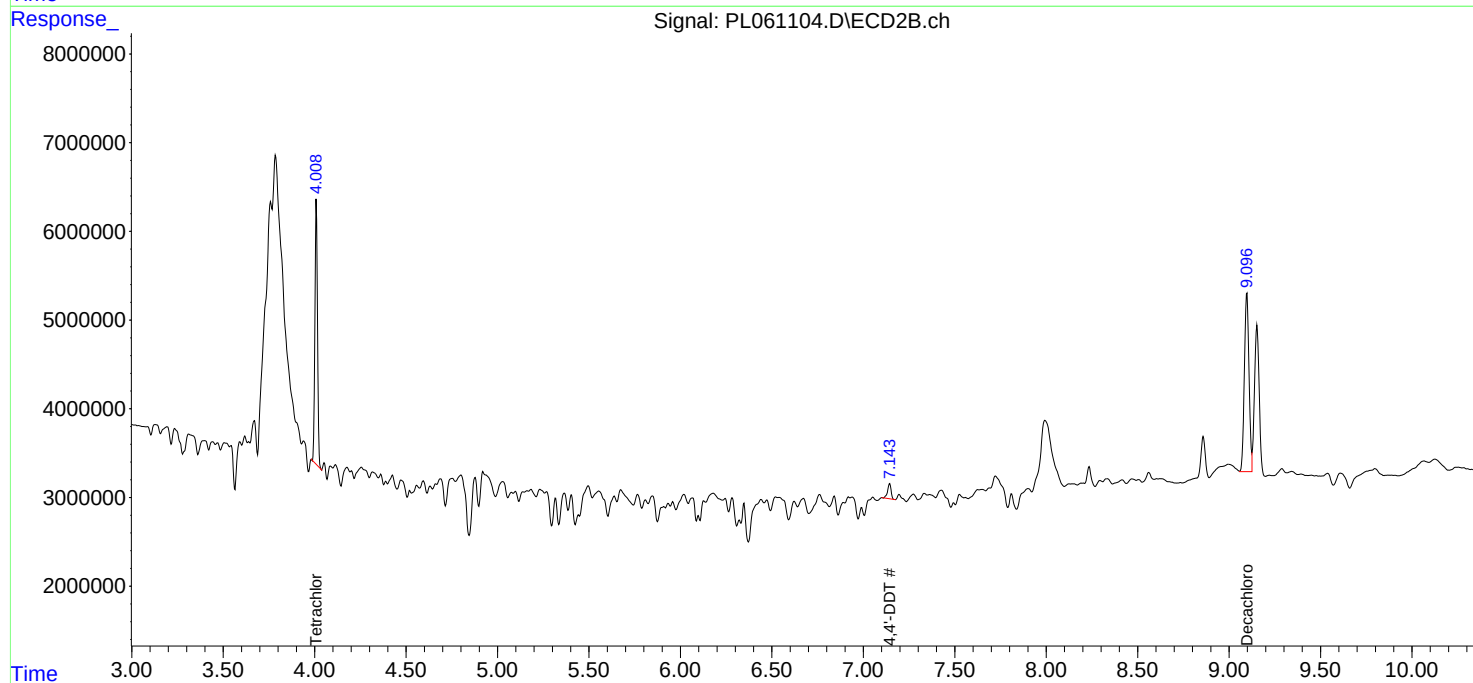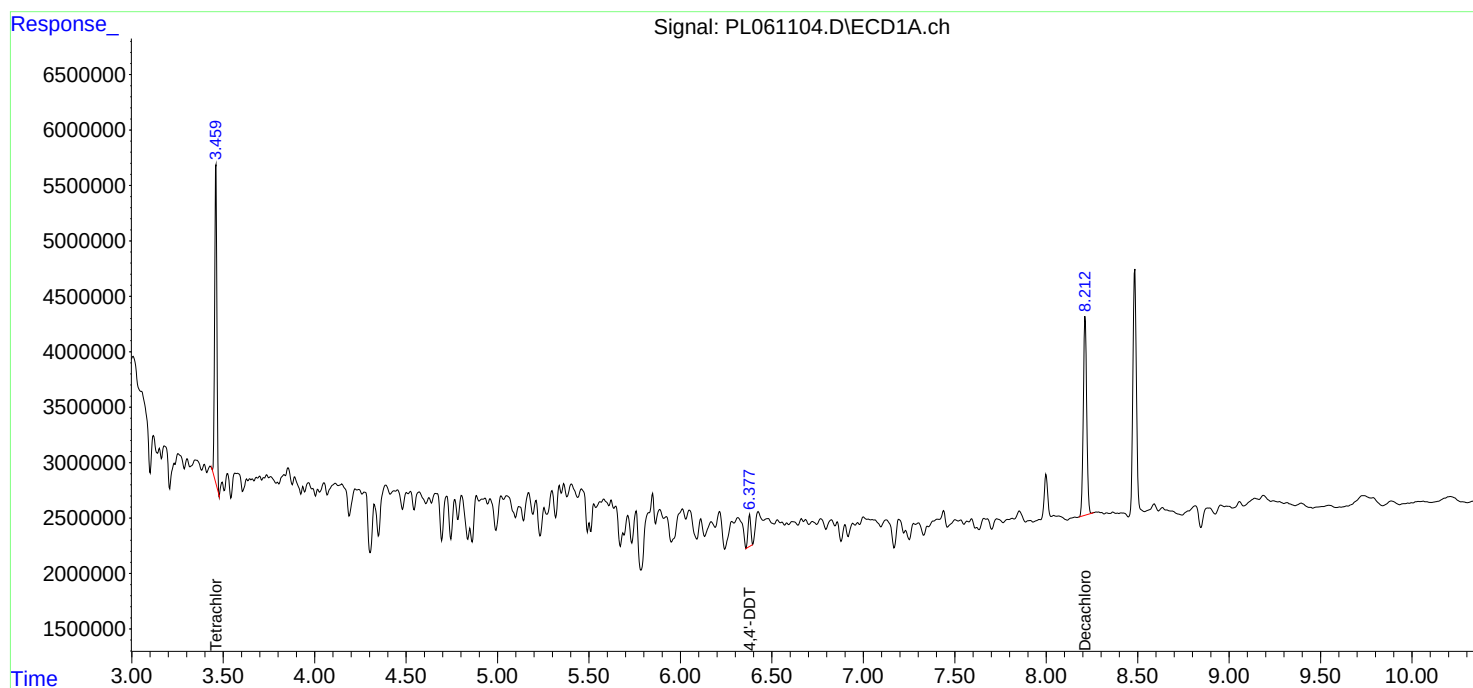

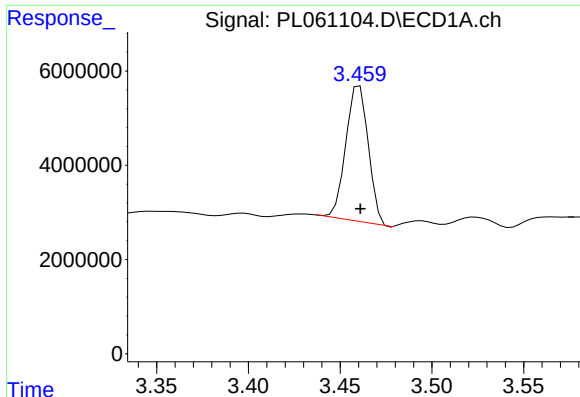


#1 Tetrachloro-m-xylene

R.T.: 3.461 min
Delta R.T.: 0.000 min
Response: 24622367
Conc: 13.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
LINDEN-JOP-BH-09-A


Manual Integrations
APPROVED

Ankita
9/1/2020 1:29:26 PM

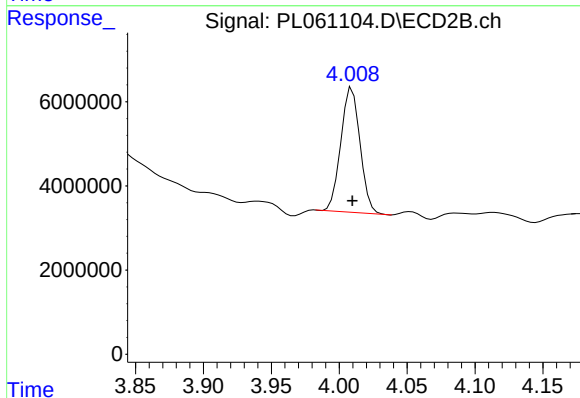


#1 Tetrachloro-m-xylene

R.T.: 4.009 min
Delta R.T.: 0.000 min
Response: 29246163
Conc: 11.25 ng/ml

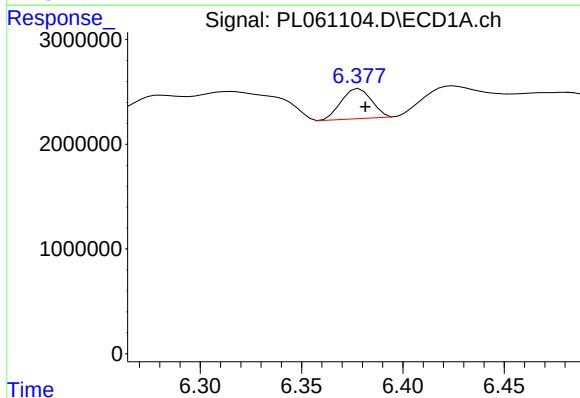


#17 4,4'-DDT

R.T.: 6.377 min
Delta R.T.: -0.004 min
Response: 3013110
Conc: 1.99 ng/ml m

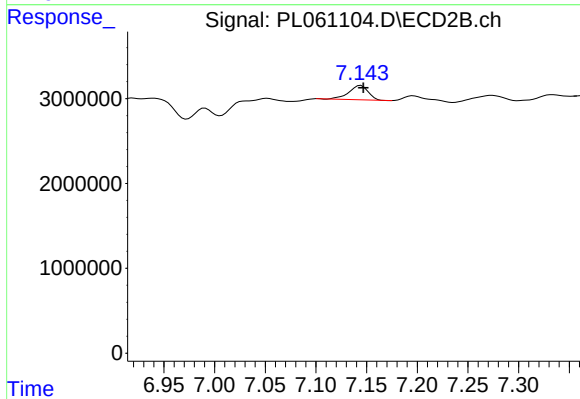

#17 4,4'-DDT

R.T.: 7.144 min
Delta R.T.: -0.003 min
Response: 2243212
Conc: 0.97 ng/ml

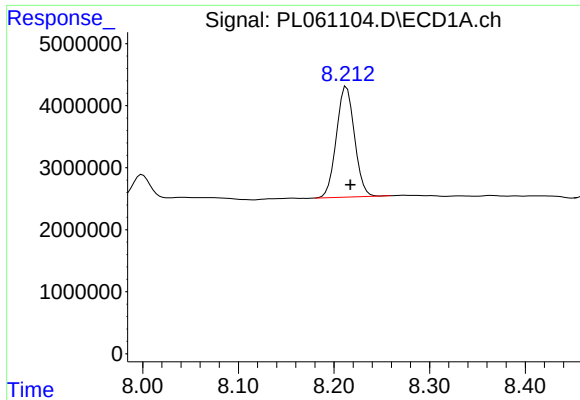


#28 Decachlorobiphenyl

R.T.: 8.213 min
Delta R.T.: -0.004 min
Response: 23493990
Conc: 13.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
LINDEN-JOP-BH-09-A

Manual Integrations
APPROVED

Ankita
9/1/2020 1:29:26 PM

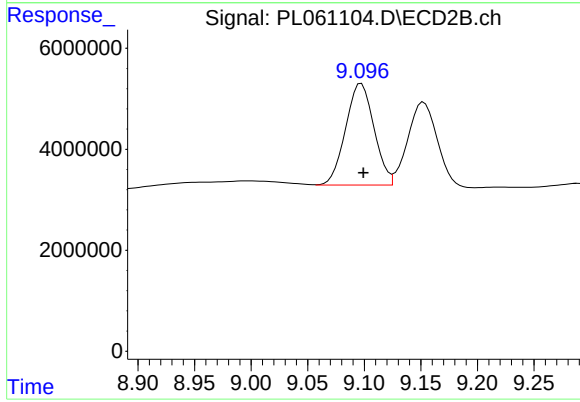

#28 Decachlorobiphenyl

R.T.: 9.096 min
Delta R.T.: -0.003 min
Response: 35633160
Conc: 16.89 ng/ml m