

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083120\
 Data File : PL061108.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Aug 2020 19:36
 Operator : DD\AJ
 Sample : L3848-03
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 LINDEN-BH-02-A

Manual Integrations
 APPROVED

Ankita
 9/1/2020 1:29:32 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 02:27:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 25 16:59:57 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.461	4.009	23169052	31291189	12.555	12.040
28)	SA Decachlor...	8.214	9.097	16961497	25846338	10.068	12.249
Target Compounds							
12)	B 4,4'-DDE	5.622	6.353	6631754	10958699	3.604	3.792
16)	A 4,4'-DDD	6.138	6.846	2974232	5687165	1.881	2.435 #
17)	MA 4,4'-DDT	6.377	7.144	2604432	3278004	1.723m	1.423m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083120\
Data File : PL061108.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Aug 2020 19:36
Operator : DD\AJ
Sample : L3848-03
Misc :
ALS Vial : 32 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
LINDEN-BH-02-A


Manual Integrations
APPROVED

Ankita
9/1/2020 1:29:32 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 02:27:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
Quant Title : GC Extractables
QLast Update : Tue Aug 25 16:59:57 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

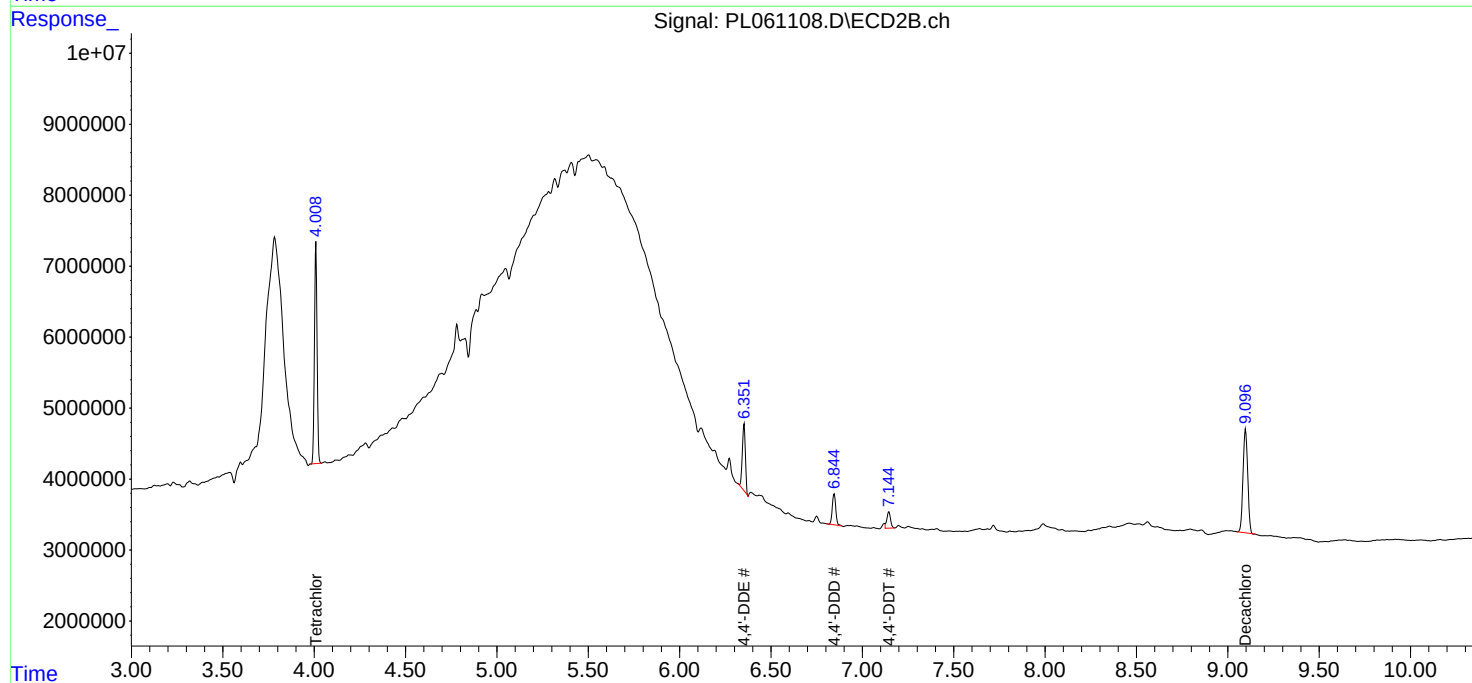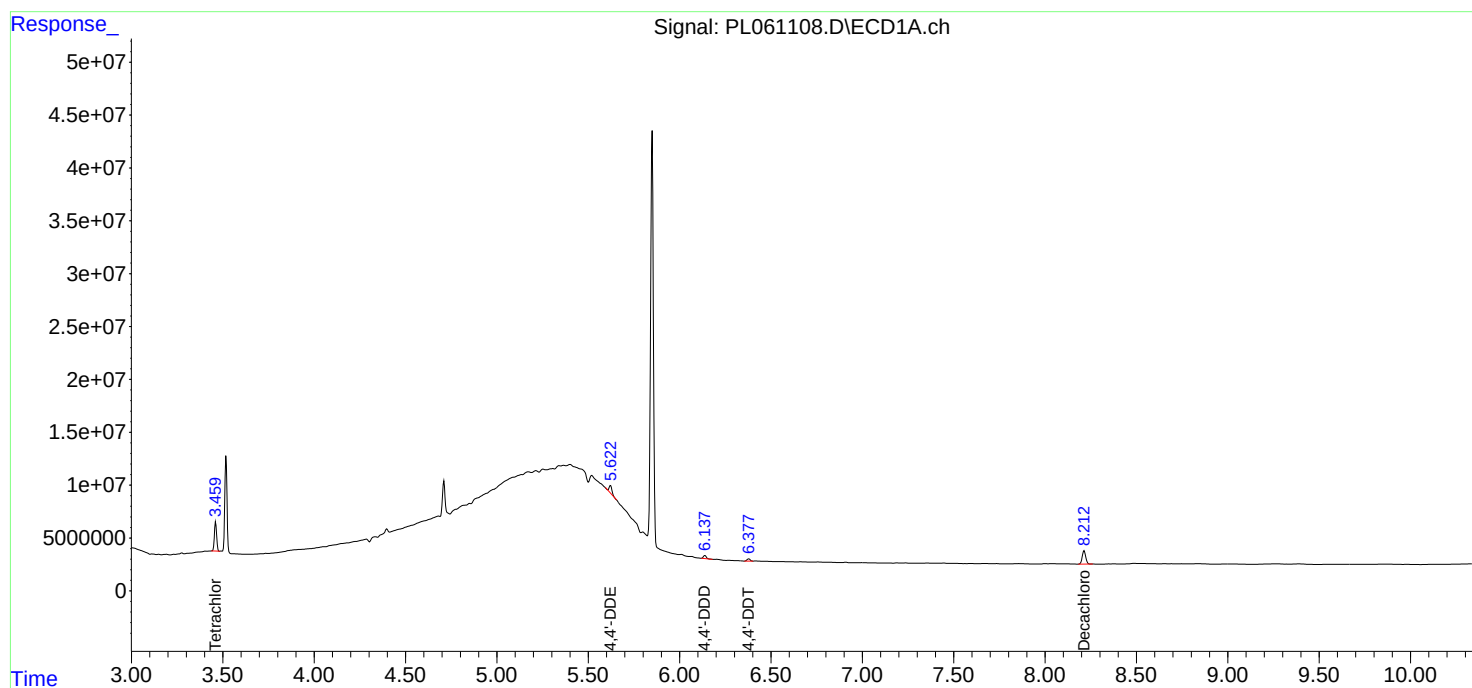

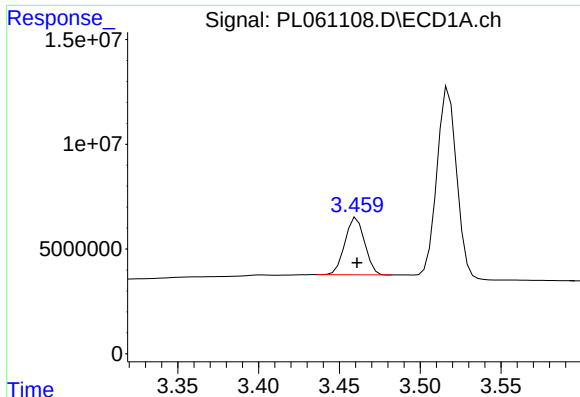


#1 Tetrachloro-m-xylene

R.T.: 3.461 min
Delta R.T.: 0.000 min
Response: 23169052
Conc: 12.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
LINDEN-BH-02-A


Manual Integrations
APPROVED

Ankita
9/1/2020 1:29:32 PM

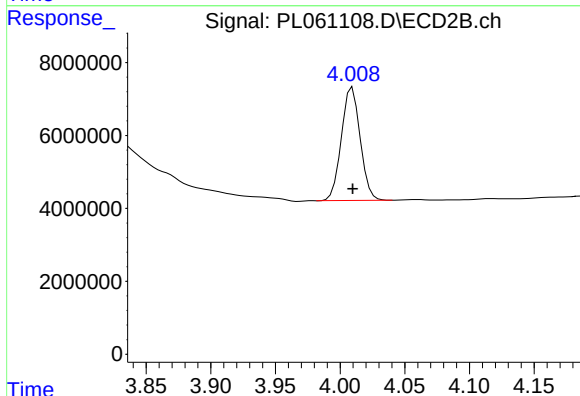


#1 Tetrachloro-m-xylene

R.T.: 4.009 min
Delta R.T.: 0.000 min
Response: 31291189
Conc: 12.04 ng/ml

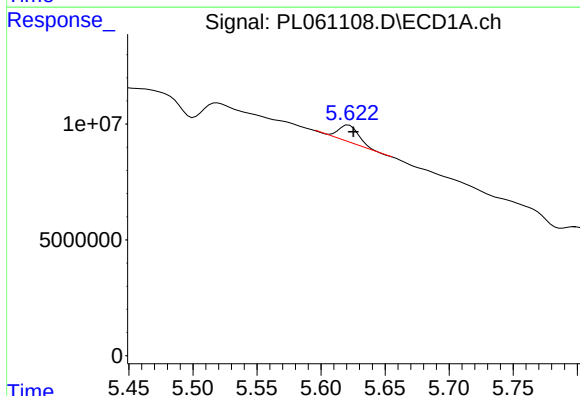


#12 4,4'-DDE

R.T.: 5.622 min
Delta R.T.: -0.004 min
Response: 6631754
Conc: 3.60 ng/ml

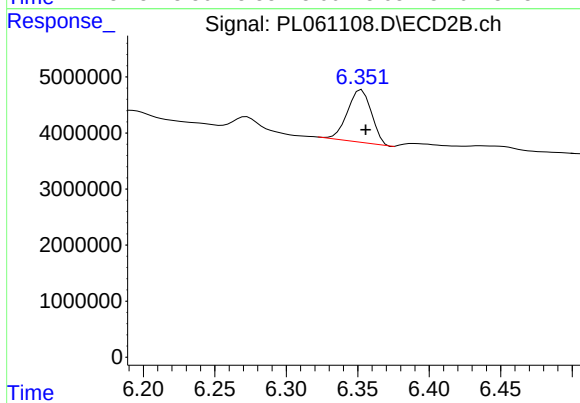

#12 4,4'-DDE

R.T.: 6.353 min
Delta R.T.: -0.003 min
Response: 10958699
Conc: 3.79 ng/ml

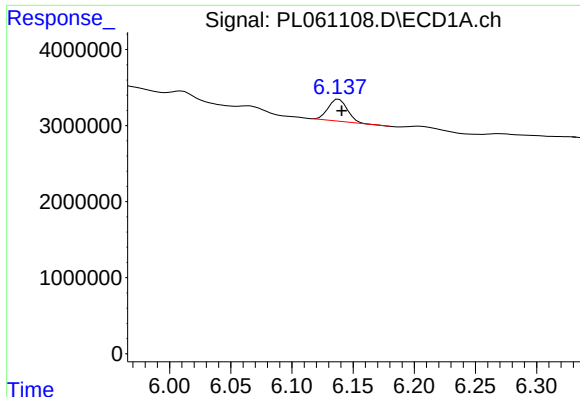


#16 4,4'-DDD

R.T.: 6.138 min
Delta R.T.: -0.002 min
Response: 2974232
Conc: 1.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
LINDEN-BH-02-A


Manual Integrations
APPROVED

Ankita
9/1/2020 1:29:32 PM

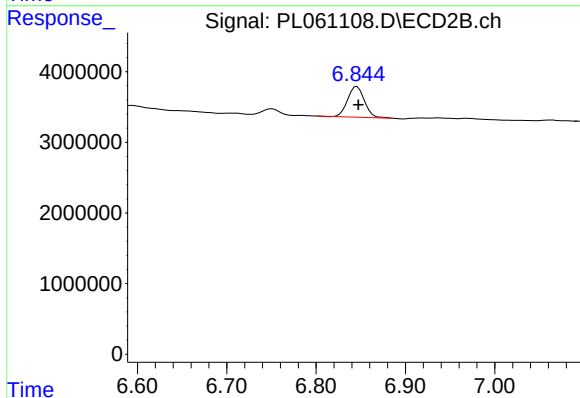


#16 4,4'-DDD

R.T.: 6.846 min
Delta R.T.: -0.002 min
Response: 5687165
Conc: 2.44 ng/ml

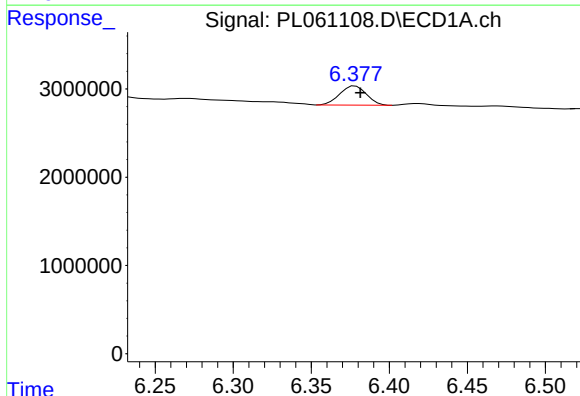


#17 4,4'-DDT

R.T.: 6.377 min
Delta R.T.: -0.005 min
Response: 2604432
Conc: 1.72 ng/ml m

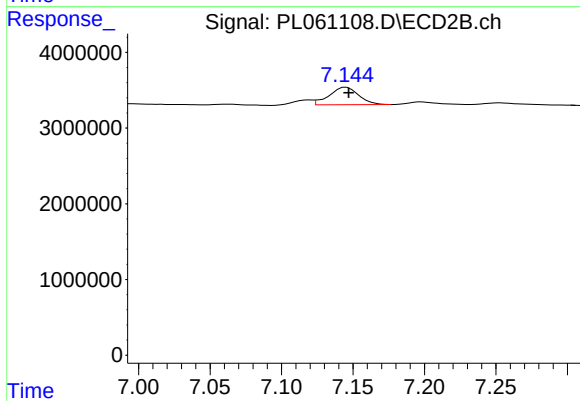

#17 4,4'-DDT

R.T.: 7.144 min
Delta R.T.: -0.003 min
Response: 3278004
Conc: 1.42 ng/ml m

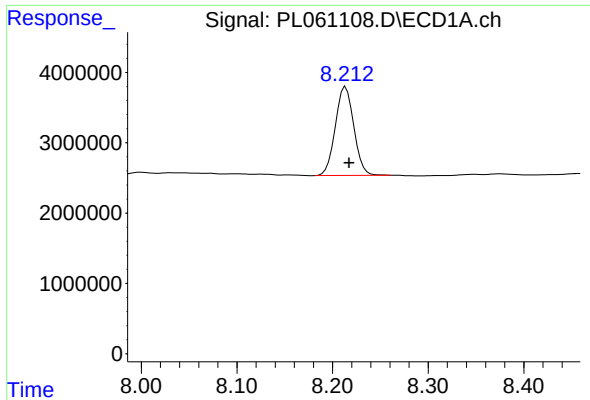


#28 Decachlorobiphenyl

R.T.: 8.214 min
Delta R.T.: -0.004 min
Response: 16961497
Conc: 10.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
LINDEN-BH-02-A

Manual Integrations
APPROVED

Ankita
9/1/2020 1:29:32 PM

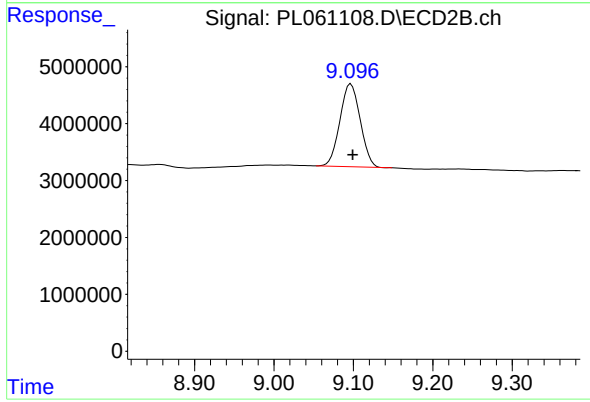

#28 Decachlorobiphenyl

R.T.: 9.097 min
Delta R.T.: -0.002 min
Response: 25846338
Conc: 12.25 ng/ml