

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083120\
 Data File : PL061109.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Aug 2020 19:50
 Operator : DD\AJ
 Sample : L3848-09
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 LINDEN-BH-01-A

Manual Integrations
 APPROVED

Ankita
 9/1/2020 1:29:34 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 02:27:47 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 25 16:59:57 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.461	4.010	25150320	34626807	13.629	13.323
28)	SA Decachlor...	8.213	9.097	20909637	31409662	12.412	14.886
Target Compounds							
12)	B 4,4'-DDE	5.622	6.352	1017790	1649547	0.553m	0.571

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083120\
Data File : PL061109.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Aug 2020 19:50
Operator : DD\AJ
Sample : L3848-09
Misc :
ALS Vial : 33 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampleId :
LINDEN-BH-01-A


Manual Integrations
APPROVED

Ankita
9/1/2020 1:29:34 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 02:27:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
Quant Title : GC Extractables
QLast Update : Tue Aug 25 16:59:57 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

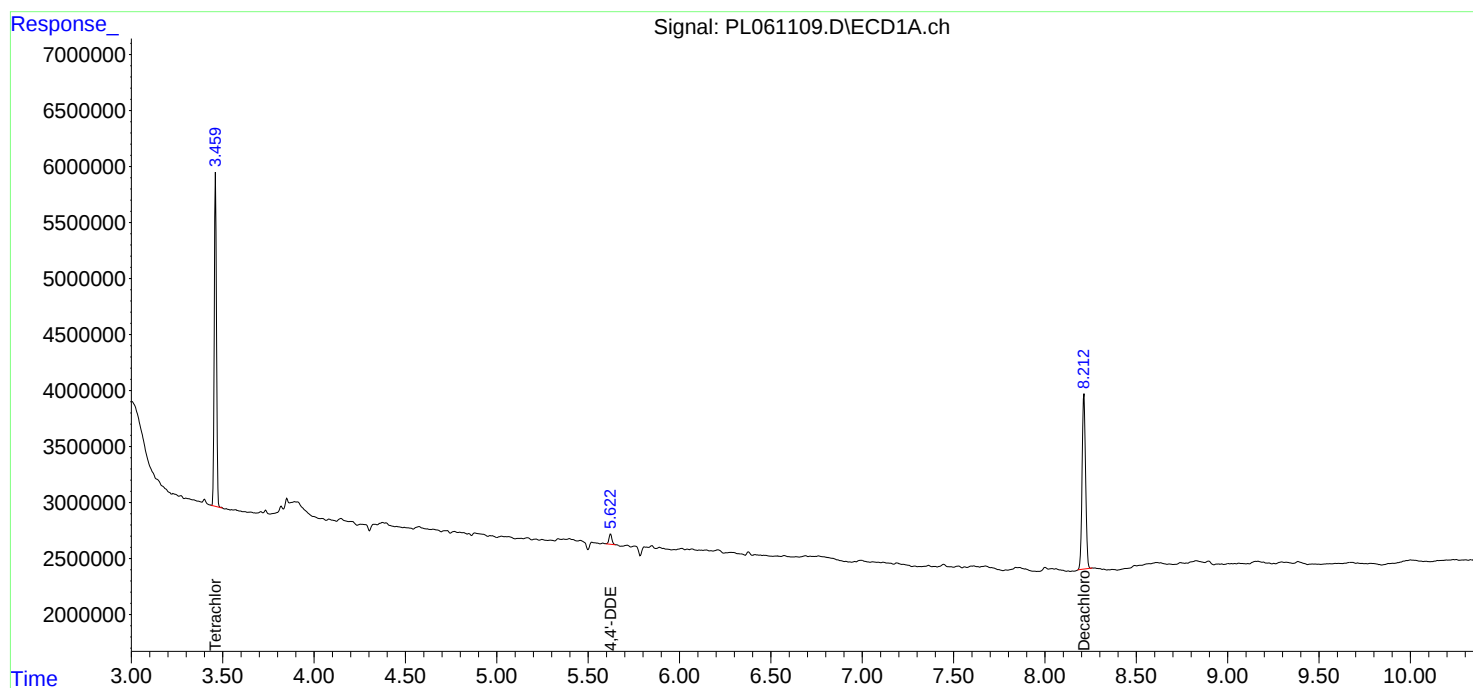

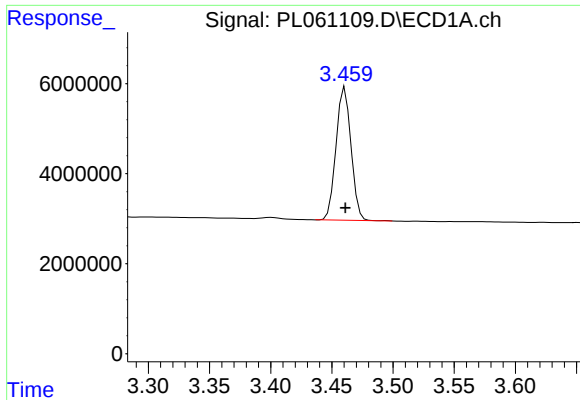


#1 Tetrachloro-m-xylene

R.T.: 3.461 min
Delta R.T.: 0.000 min
Response: 25150320
Conc: 13.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
LINDEN-BH-01-A


Manual Integrations
APPROVED

Ankita
9/1/2020 1:29:34 PM

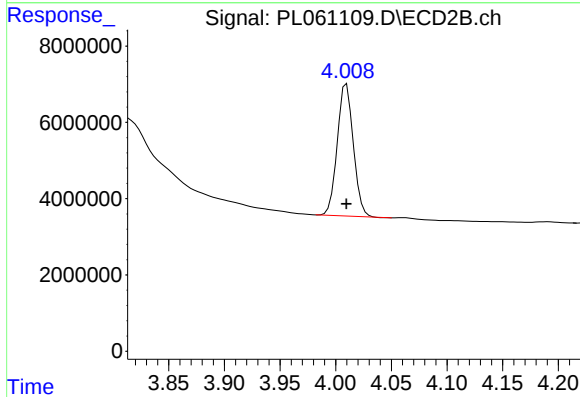


#1 Tetrachloro-m-xylene

R.T.: 4.010 min
Delta R.T.: 0.000 min
Response: 34626807
Conc: 13.32 ng/ml

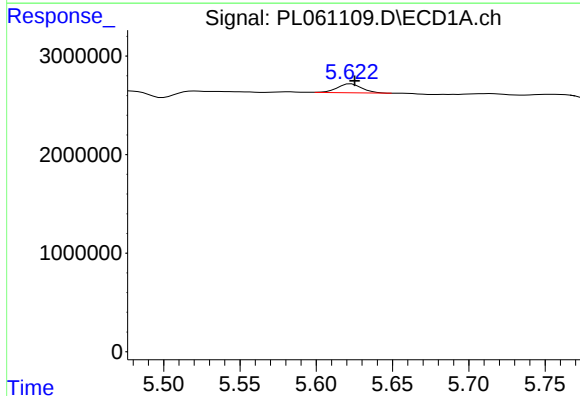


#12 4,4'-DDE

R.T.: 5.622 min
Delta R.T.: -0.004 min
Response: 1017790
Conc: 0.55 ng/ml m

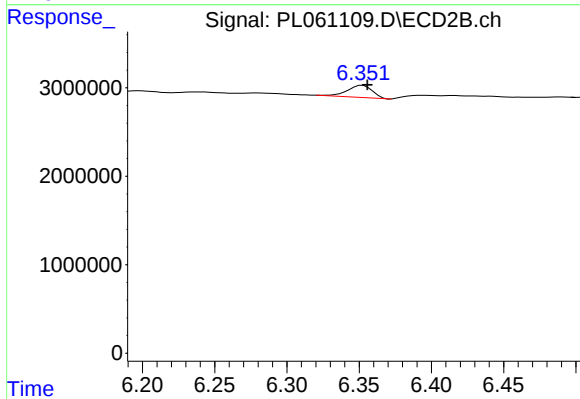

#12 4,4'-DDE

R.T.: 6.352 min
Delta R.T.: -0.003 min
Response: 1649547
Conc: 0.57 ng/ml

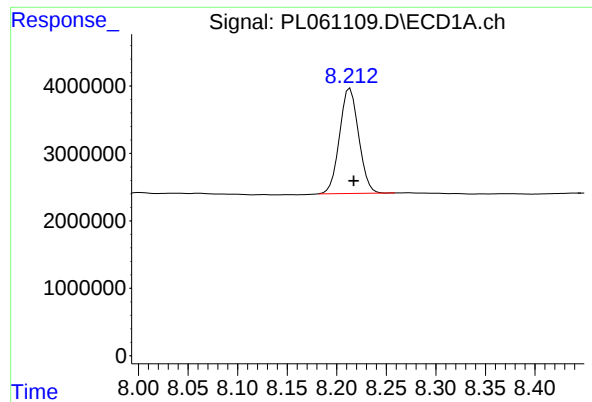


#28 Decachlorobiphenyl

R.T.: 8.213 min
Delta R.T.: -0.004 min
Response: 20909637
Conc: 12.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
LINDEN-BH-01-A

Manual Integrations
APPROVED

Ankita
9/1/2020 1:29:34 PM

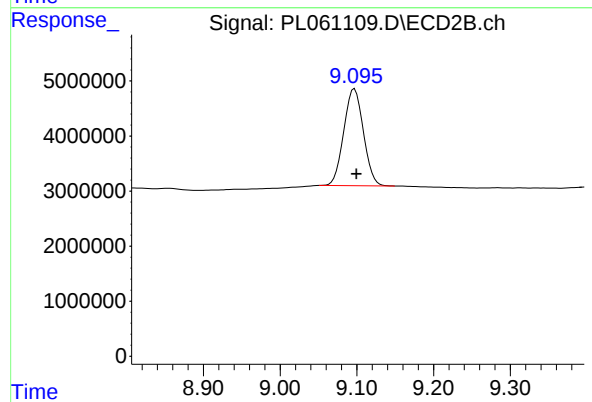

#28 Decachlorobiphenyl

R.T.: 9.097 min
Delta R.T.: -0.002 min
Response: 31409662
Conc: 14.89 ng/ml