

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083121\
 Data File : PL069630.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Aug 2021 15:32
 Operator : AR\AJ
 Sample : M3597-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RO-PSC124042

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 01:29:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL083021.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 31 01:49:30 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.634	5.570	7207377	25872890	23.152	20.565
28)	SA Decachlor...	10.406	11.497	11179829	20193570	18.957	17.895
Target Compounds							
9)	A Endosulfan I	7.505f	0.000	1270695	0	2.688	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083121\
Data File : PL069630.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Aug 2021 15:32
Operator : AR\AJ
Sample : M3597-03
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
RO-PSC124042

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 01:29:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL083021.M
Quant Title : GC Extractables
QLast Update : Tue Aug 31 01:49:30 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

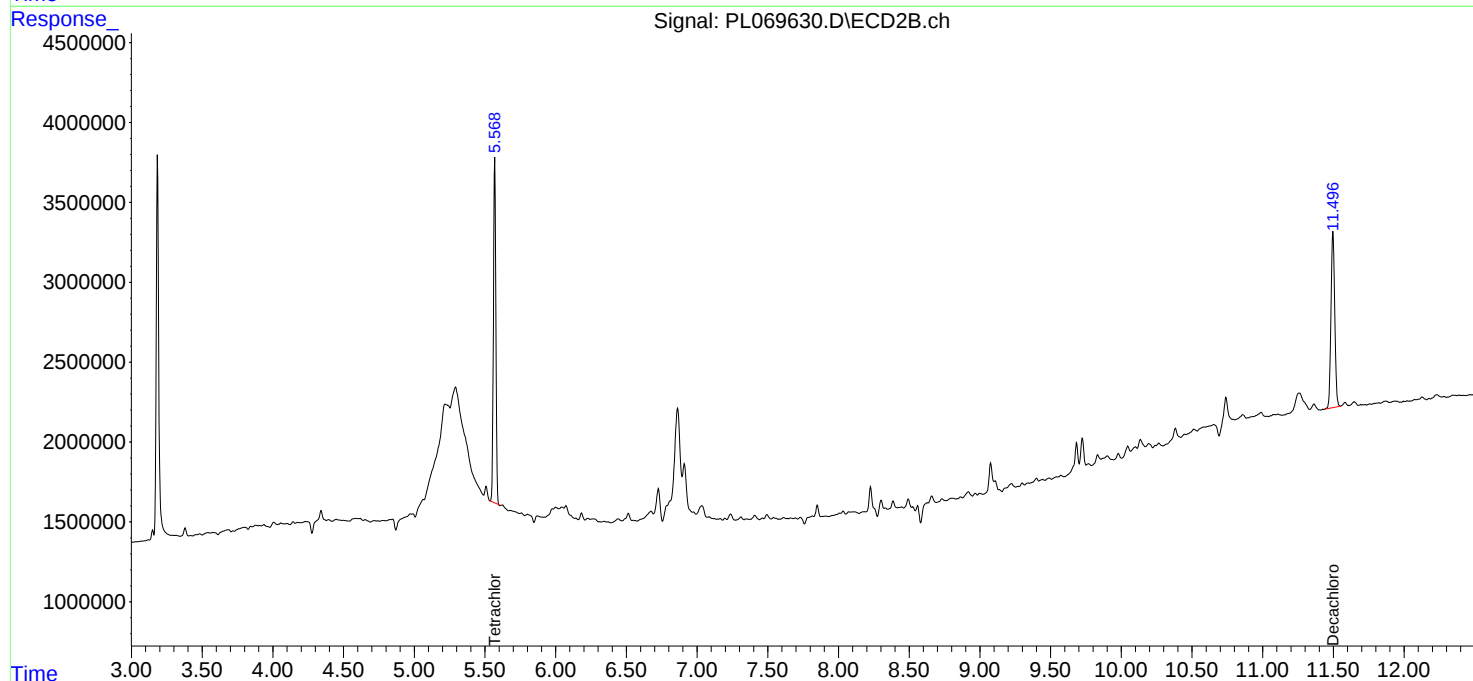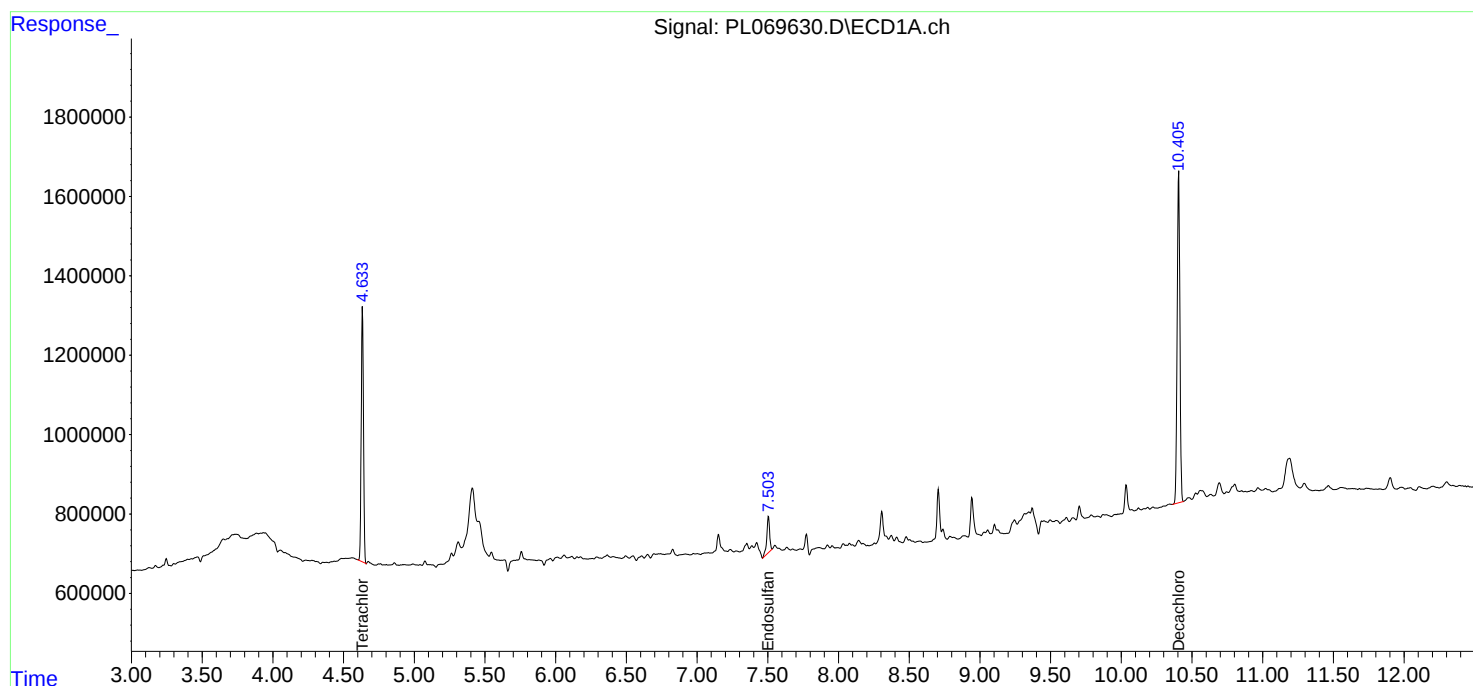


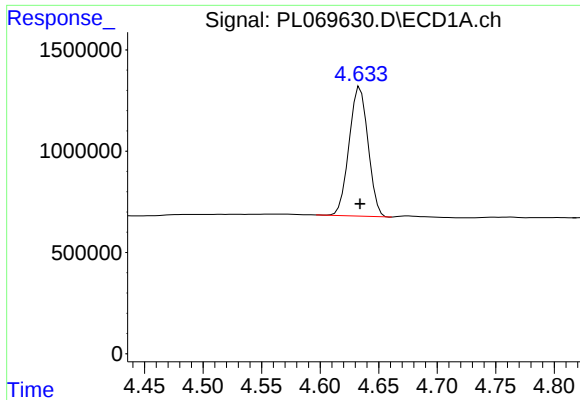

#1 Tetrachloro-m-xylene


R.T.: 4.634 min
Delta R.T.: 0.000 min
Response: 7207377
Conc: 23.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
RO-PSC124042

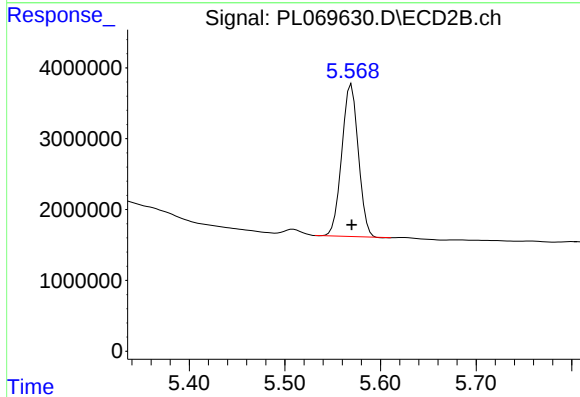


#1 Tetrachloro-m-xylene

R.T.: 5.570 min
Delta R.T.: 0.000 min
Response: 25872890
Conc: 20.57 ng/ml

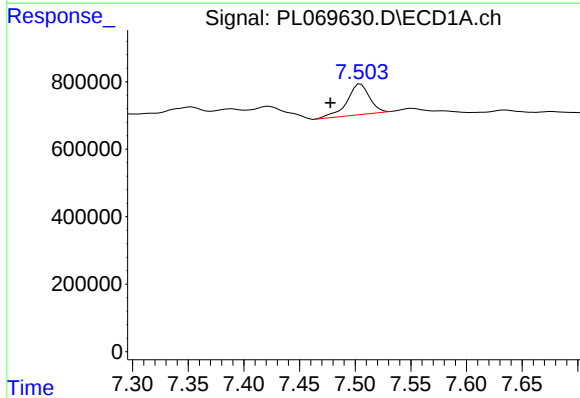


#9 Endosulfan I

R.T.: 7.505 min
Delta R.T.: 0.027 min
Response: 1270695
Conc: 2.69 ng/ml

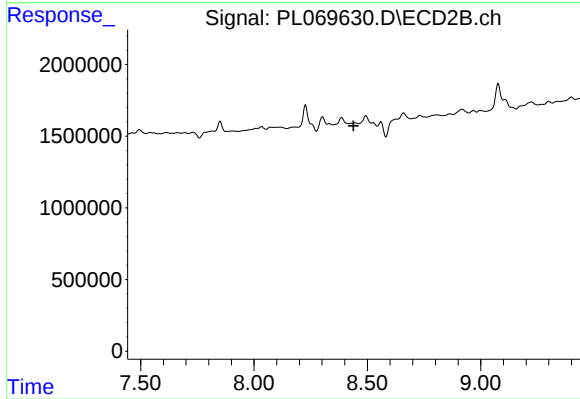

#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 8.439 min
Response: 0
Conc: N.D.

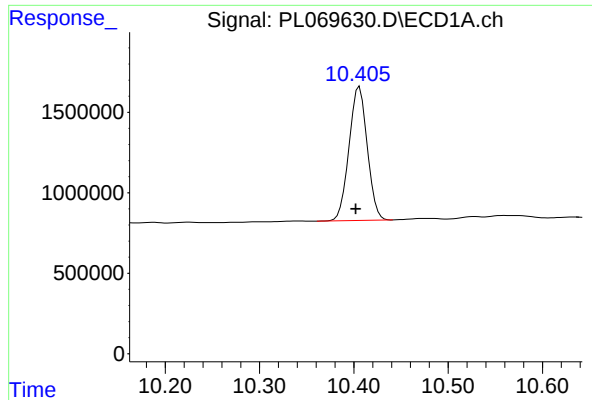

#28 Decachlorobiphenyl


R.T.: 10.406 min

Delta R.T.: 0.004 min

Response: 11179829

Conc: 18.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
RO-PSC124042

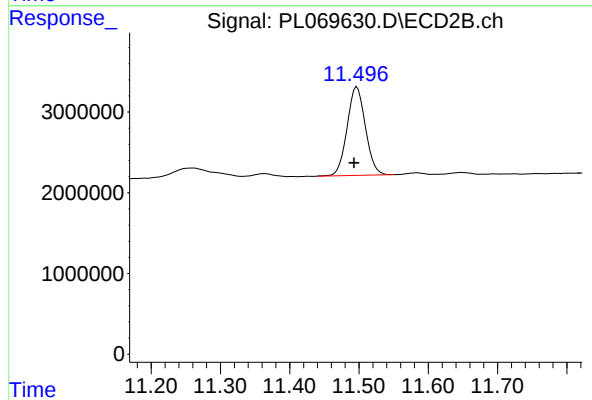

#28 Decachlorobiphenyl

R.T.: 11.497 min

Delta R.T.: 0.004 min

Response: 20193570

Conc: 17.90 ng/ml