

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083121\
 Data File : PL069631.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Aug 2021 15:48
 Operator : AR\AJ
 Sample : M3577-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 191-0827-B1-0-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 01:29:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL083021.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 31 01:49:30 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.634	5.570	5138913	18470218	16.507	14.681
28)	SA Decachlor...	10.405	11.497	8446781	15623977	14.323	13.846
Target Compounds							
10)	B gamma-Chl...	0.000	8.304	0	1485100	N.D.	1.069 #
11)	B alpha-Chl...	0.000	8.387	0	2250830	N.D.	1.645 #
25)	Chlordane-3	0.000	8.304	0	1485100	N.D.	7.189 #
26)	Chlordane-4	0.000	8.387	0	2250830	N.D.	9.075 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083121\
Data File : PL069631.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Aug 2021 15:48
Operator : AR\AJ
Sample : M3577-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
191-0827-B1-0-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 01:29:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL083021.M
Quant Title : GC Extractables
QLast Update : Tue Aug 31 01:49:30 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

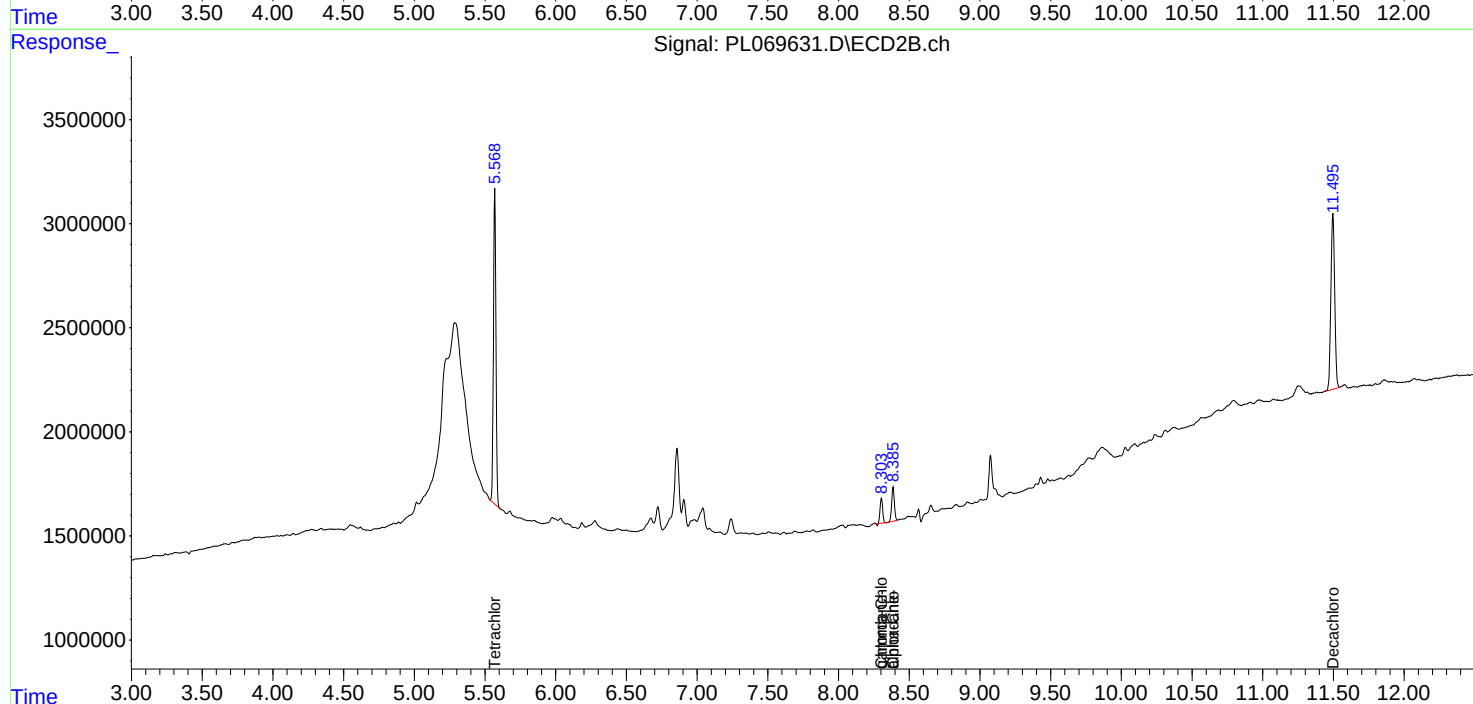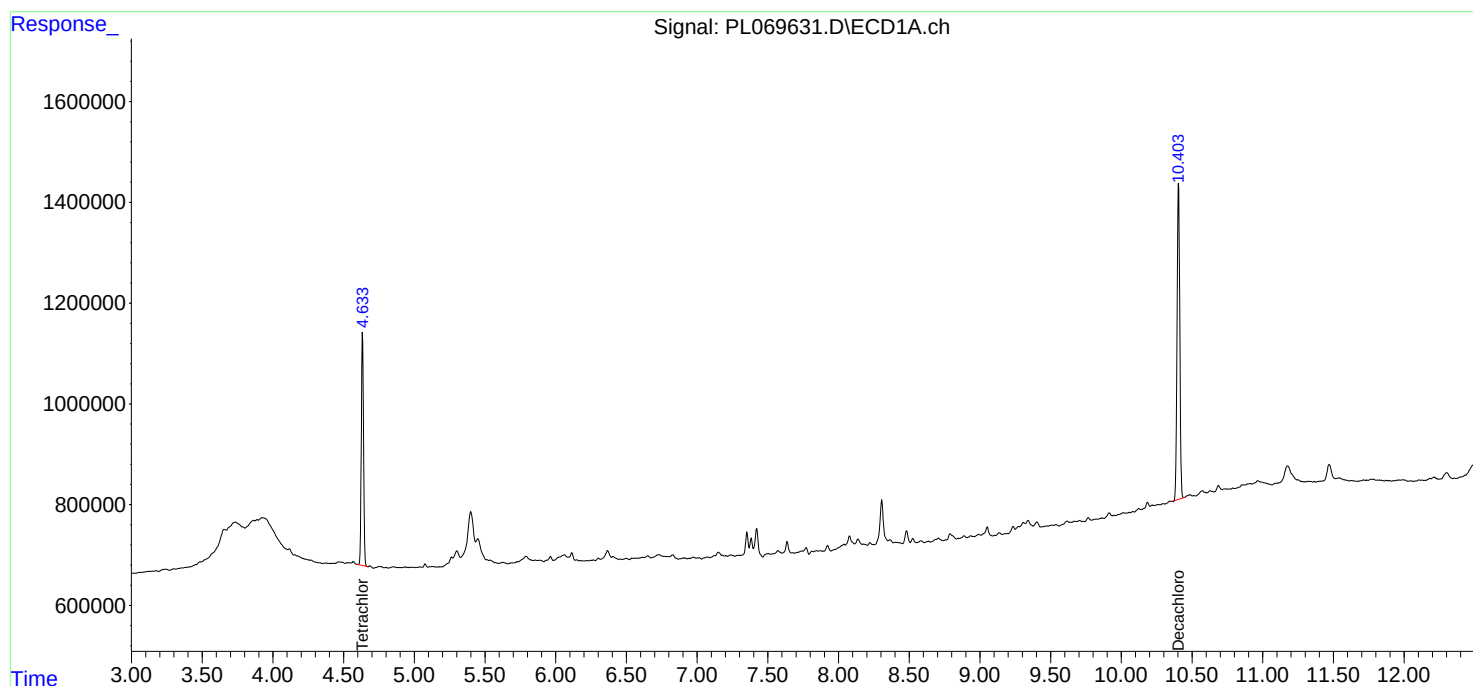


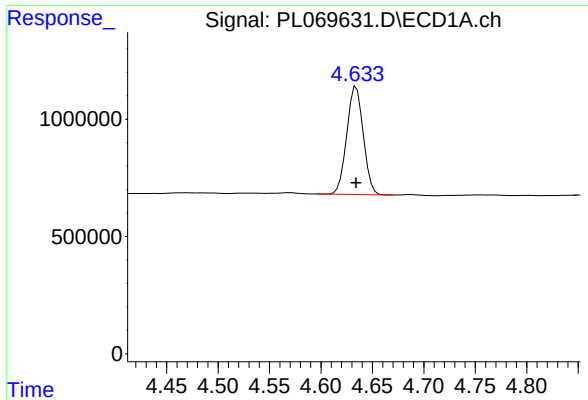

#1 Tetrachloro-m-xylene


R.T.: 4.634 min
Delta R.T.: 0.000 min
Response: 5138913
Conc: 16.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
191-0827-B1-0-2

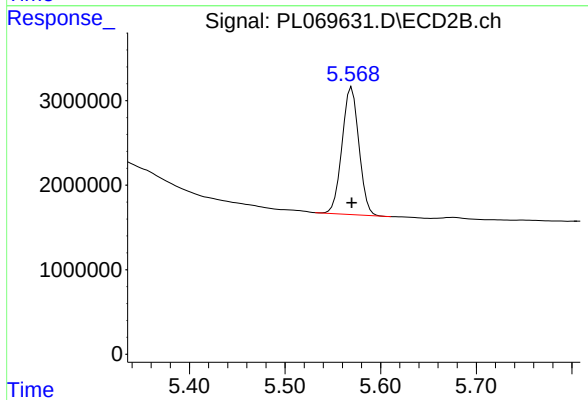


#1 Tetrachloro-m-xylene

R.T.: 5.570 min
Delta R.T.: 0.000 min
Response: 18470218
Conc: 14.68 ng/ml

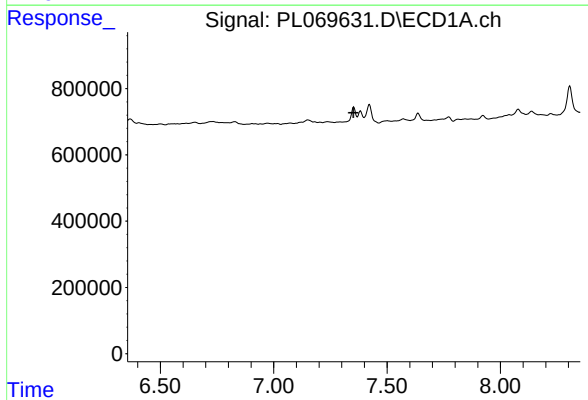


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.352 min
Response: 0
Conc: N.D.

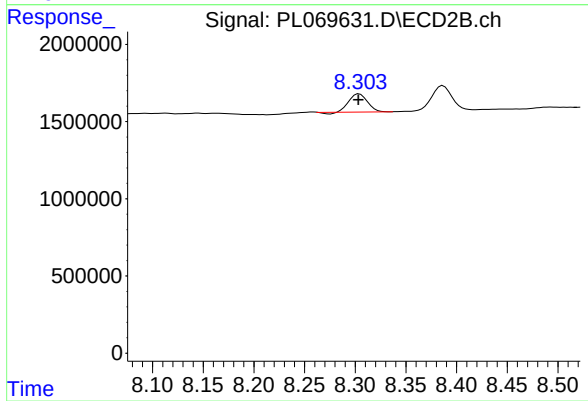

#10 gamma-Chlordane


R.T.: 8.304 min
Delta R.T.: 0.000 min
Response: 1485100
Conc: 1.07 ng/ml

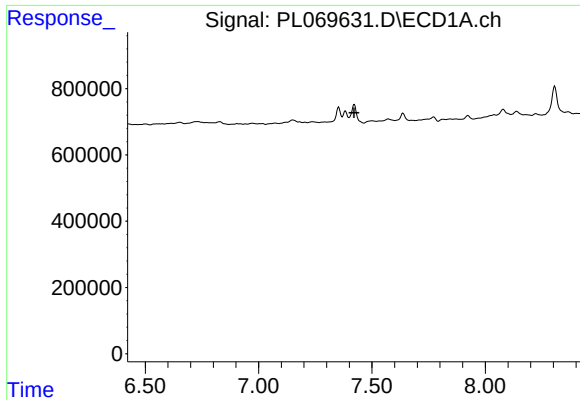

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.422 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
191-0827-B1-0-2

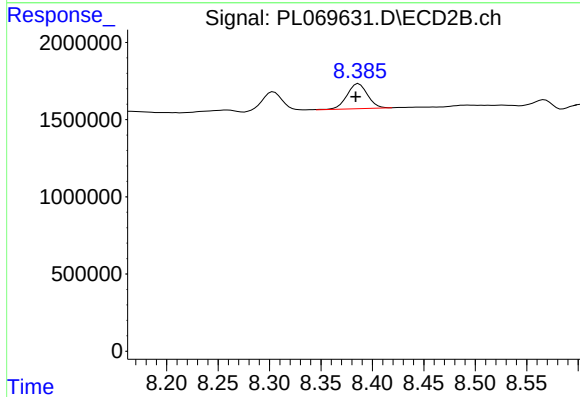


#11 alpha-Chlordane

R.T.: 8.387 min
Delta R.T.: 0.003 min
Response: 2250830
Conc: 1.64 ng/ml

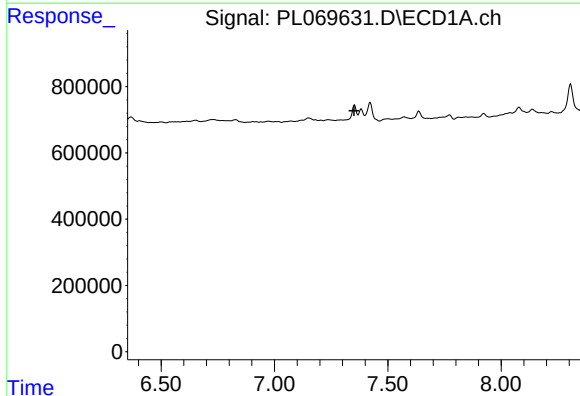


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.351 min
Response: 0
Conc: N.D.

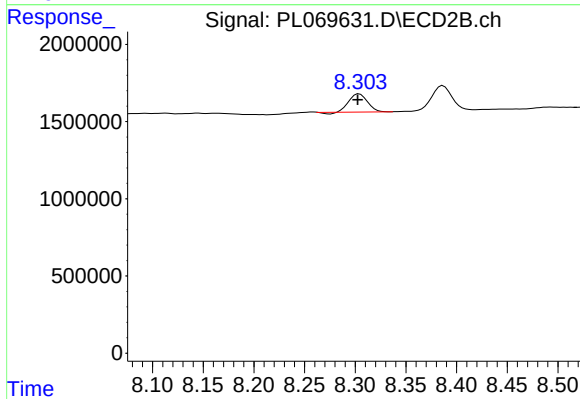

#25 Chlordane-3


R.T.: 8.304 min
Delta R.T.: 0.001 min
Response: 1485100
Conc: 7.19 ng/ml

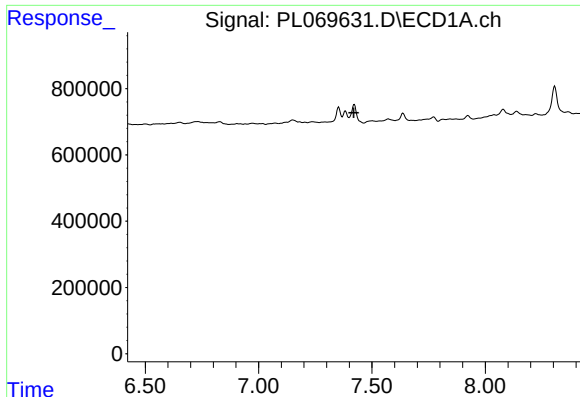

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.420 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
191-0827-B1-0-2

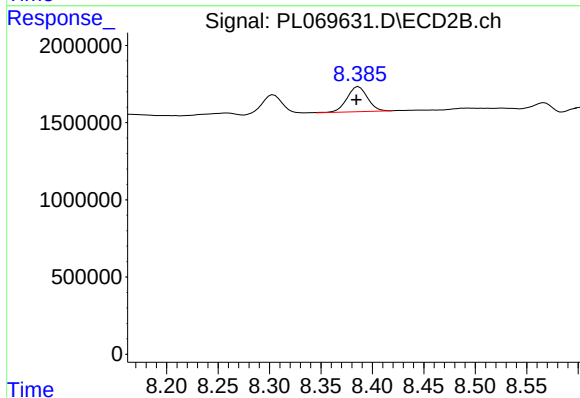


#26 Chlordane-4

R.T.: 8.387 min
Delta R.T.: 0.002 min
Response: 2250830
Conc: 9.07 ng/ml

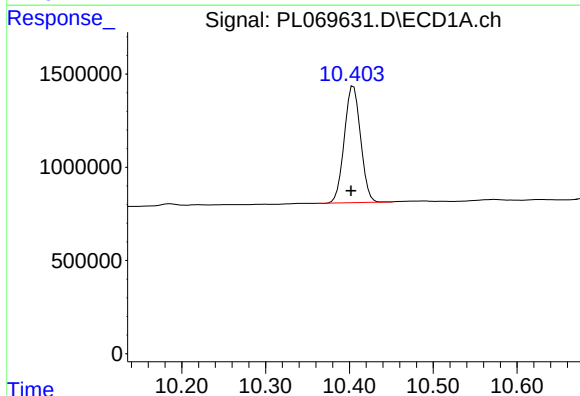

#28 Decachlorobiphenyl

R.T.: 10.405 min
Delta R.T.: 0.003 min
Response: 8446781
Conc: 14.32 ng/ml

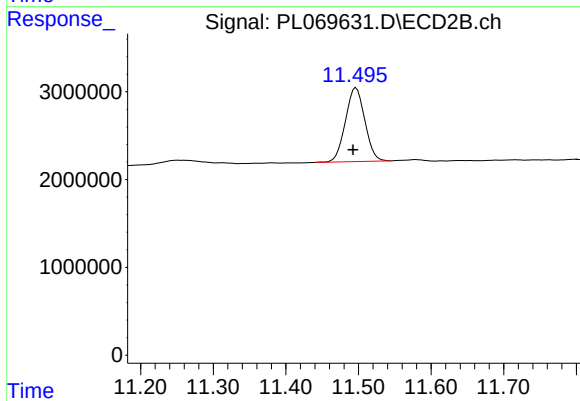

#28 Decachlorobiphenyl

R.T.: 11.497 min
Delta R.T.: 0.004 min
Response: 15623977
Conc: 13.85 ng/ml