

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083121\
 Data File : PL069651.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Aug 2021 23:00
 Operator : AR\AJ
 Sample : M3607-01
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 20211021-SITE-WATER

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 01:34:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL083021.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 31 01:49:30 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.633	5.568	6547179	24739664	21.031	19.665
28)	SA Decachlor...	10.400	11.491	10614262	19294302	17.998	17.098
Target Compounds							
6)	B beta-BHC	6.114f	0.000	7157971	0	29.827	N.D. #
7)	B delta-BHC	0.000	7.045f	0	2264992	N.D.	1.416 #
23)	Chlordane-1	5.988f	0.000	1694654	0	122.071	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083121\
Data File : PL069651.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Aug 2021 23:00
Operator : AR\AJ
Sample : M3607-01
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
20211021-SITE-WATER

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 01:34:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL083021.M
Quant Title : GC Extractables
QLast Update : Tue Aug 31 01:49:30 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

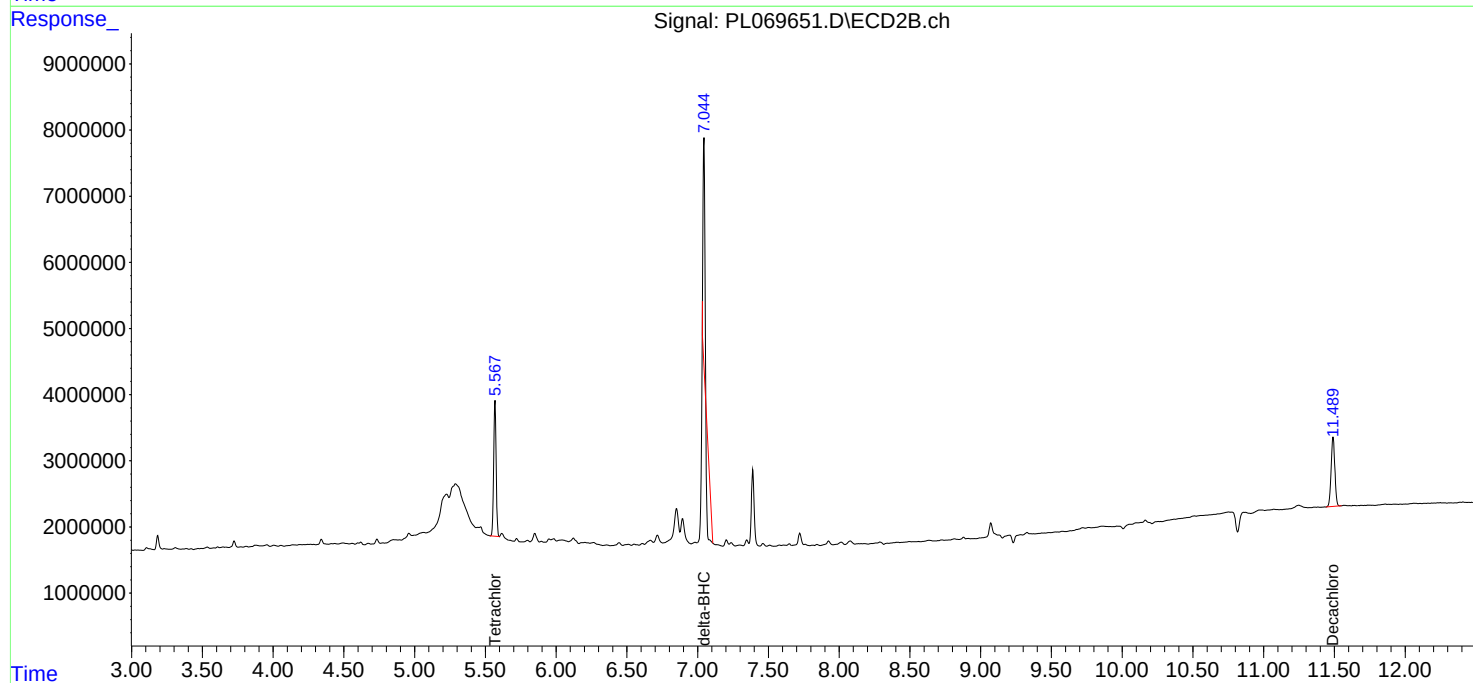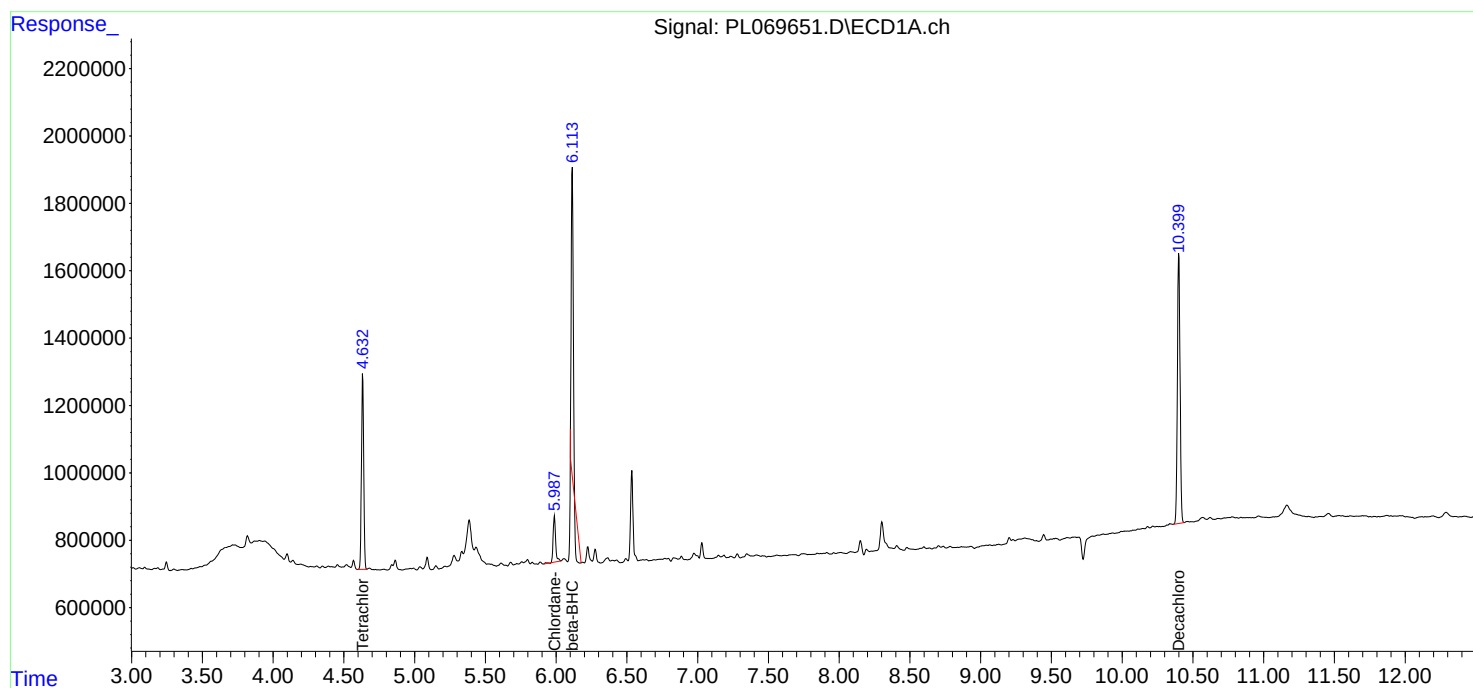


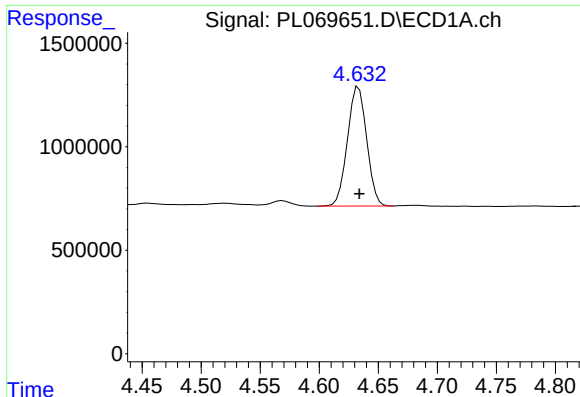

#1 Tetrachloro-m-xylene


R.T.: 4.633 min
Delta R.T.: 0.000 min
Response: 6547179
Conc: 21.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
20211021-SITE-WATER

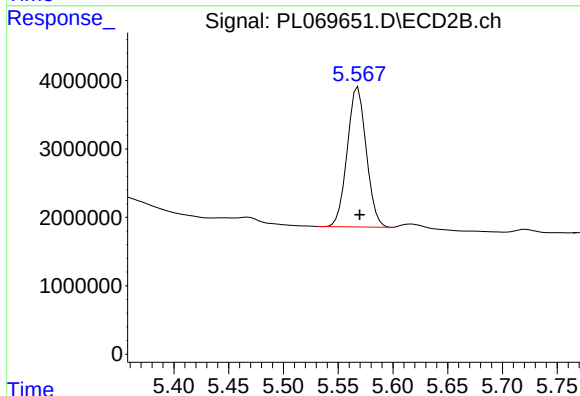


#1 Tetrachloro-m-xylene

R.T.: 5.568 min
Delta R.T.: -0.002 min
Response: 24739664
Conc: 19.66 ng/ml

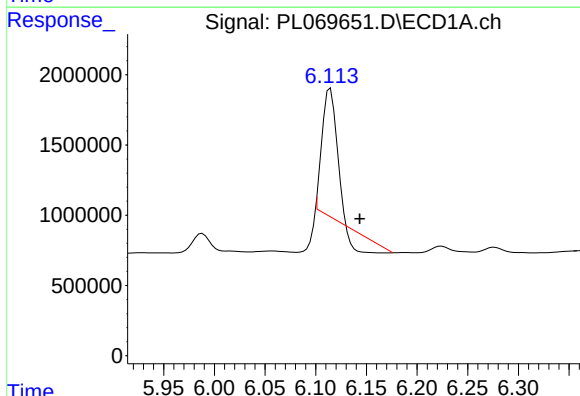


#6 beta-BHC

R.T.: 6.114 min
Delta R.T.: -0.029 min
Response: 7157971
Conc: 29.83 ng/ml

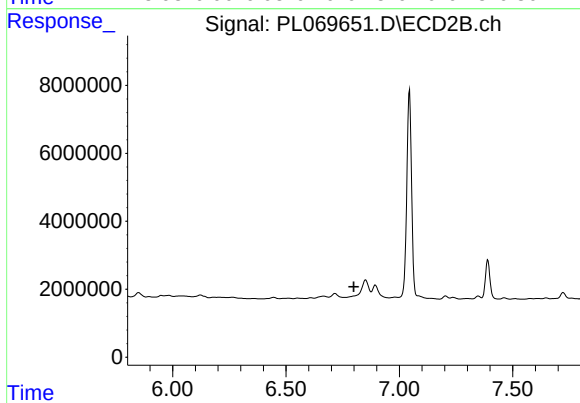

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.800 min
Response: 0
Conc: N.D.

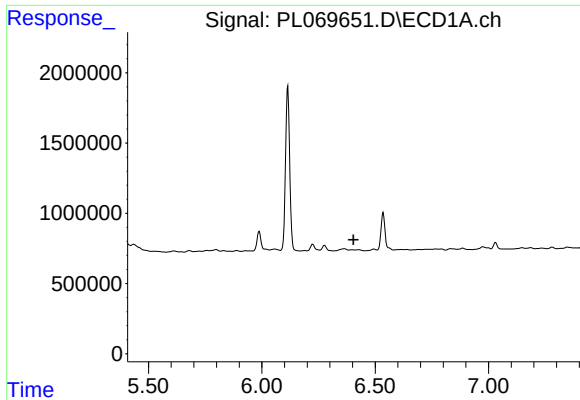

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.405 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
20211021-SITE-WATER

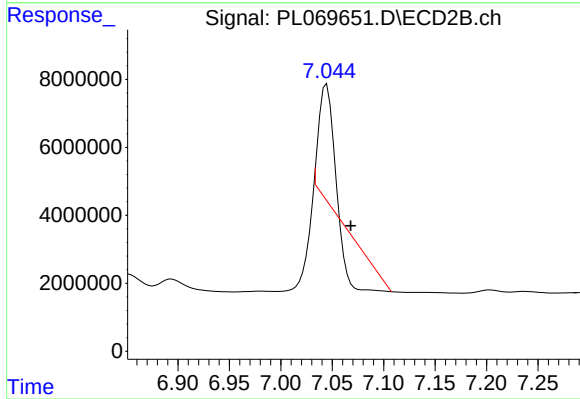


#7 delta-BHC

R.T.: 7.045 min
Delta R.T.: -0.023 min
Response: 2264992
Conc: 1.42 ng/ml

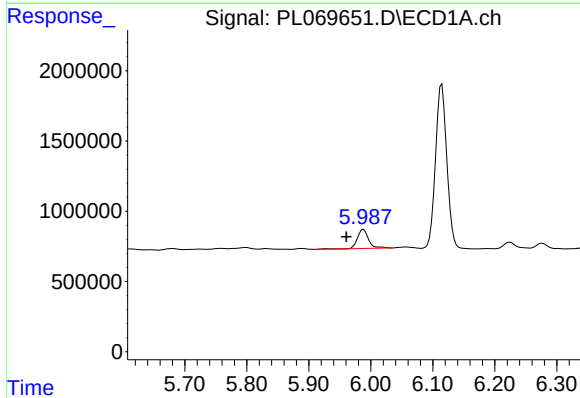


#23 Chlordane-1

R.T.: 5.988 min
Delta R.T.: 0.028 min
Response: 1694654
Conc: 122.07 ng/ml

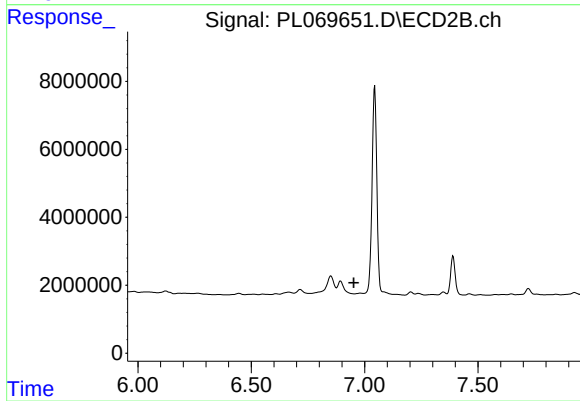

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 6.953 min
Response: 0
Conc: N.D.

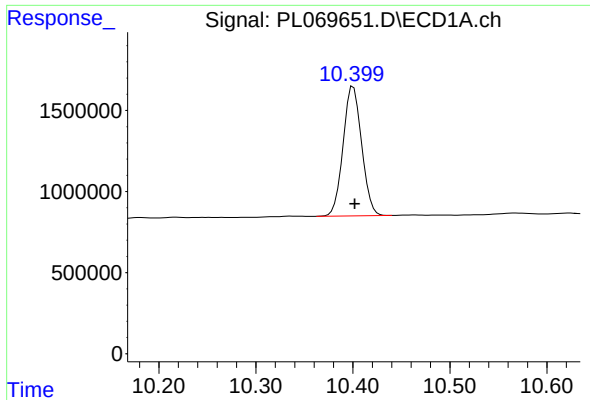

#28 Decachlorobiphenyl

R.T.: 10.400 min
Delta R.T.: -0.002 min
Response: 10614262
Conc: 18.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
20211021-SITE-WATER

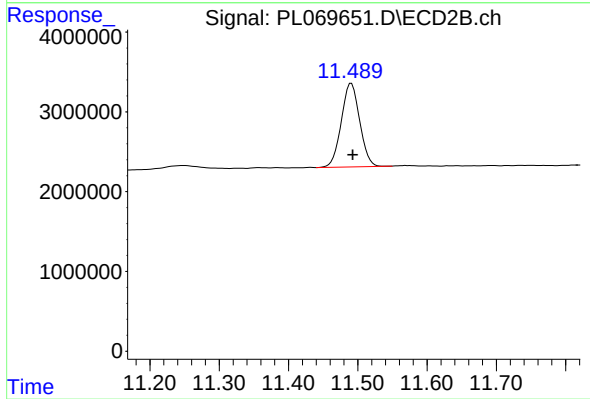

#28 Decachlorobiphenyl

R.T.: 11.491 min
Delta R.T.: -0.002 min
Response: 19294302
Conc: 17.10 ng/ml