

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083121\
 Data File : PL069623.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Aug 2021 12:23
 Operator : AR\AJ
 Sample : M3493-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 20211008-MANASQUAN-WATER

Manual Integrations
 APPROVED

Ankita
 9/1/2021 11:01:36 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 01:27:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL083021.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 31 01:49:30 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.633	5.570	5374344	19146182	17.263m	15.219
28) SA Decachlor...	10.404	11.494	8513329	14156150	14.436	12.545
Target Compounds						
3) MA gamma-BHC...	5.757	6.550	245738	1446307	0.562m	0.890m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083121\
Data File : PL069623.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Aug 2021 12:23
Operator : AR\AJ
Sample : M3493-01
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
20211008-MANASQUAN-WATER


Manual Integrations
APPROVED

Ankita
9/1/2021 11:01:36 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 01:27:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL083021.M
Quant Title : GC Extractables
QLast Update : Tue Aug 31 01:49:30 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

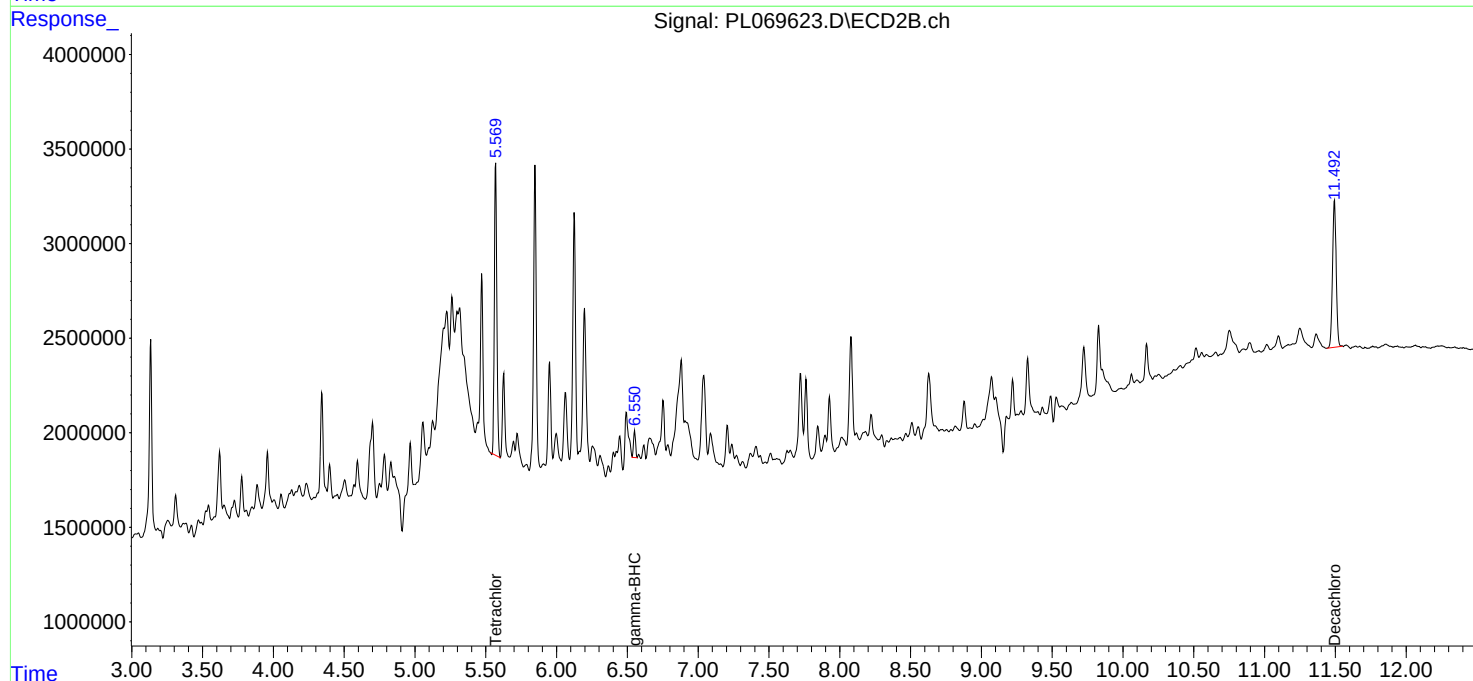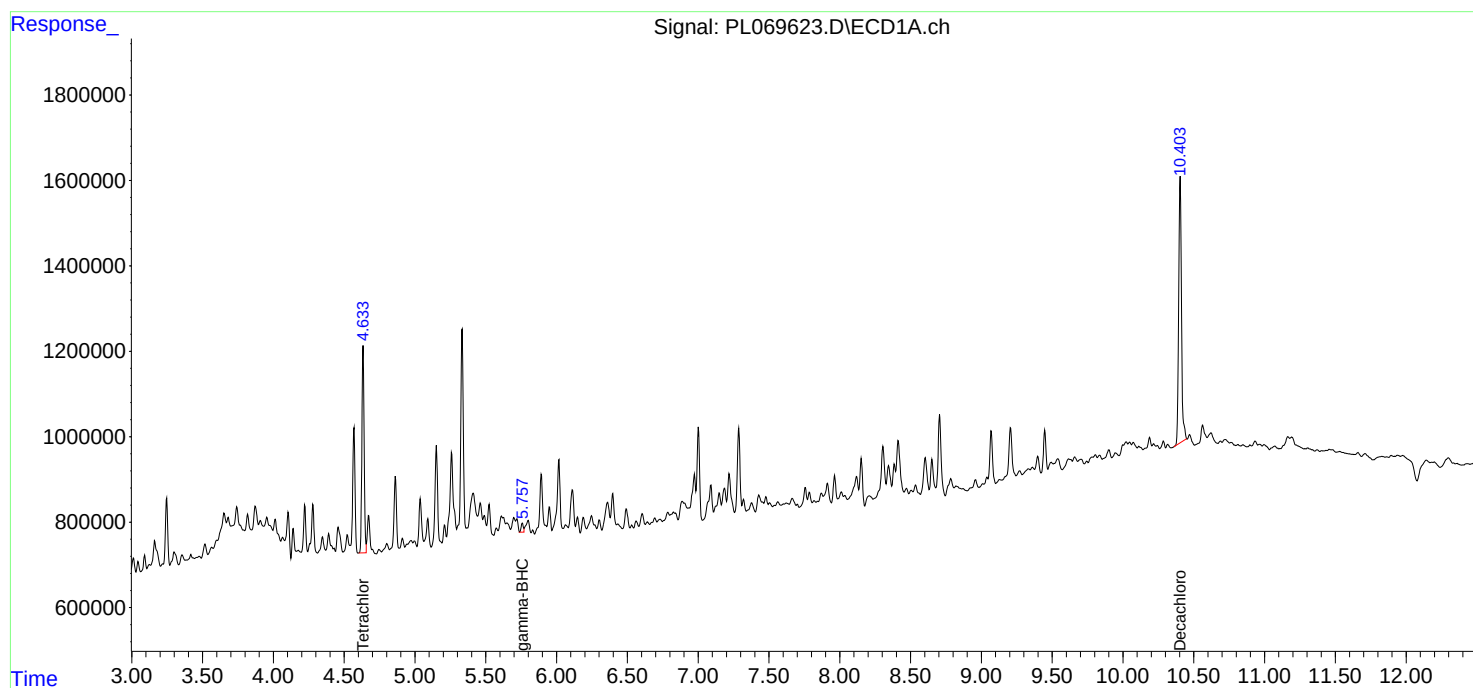

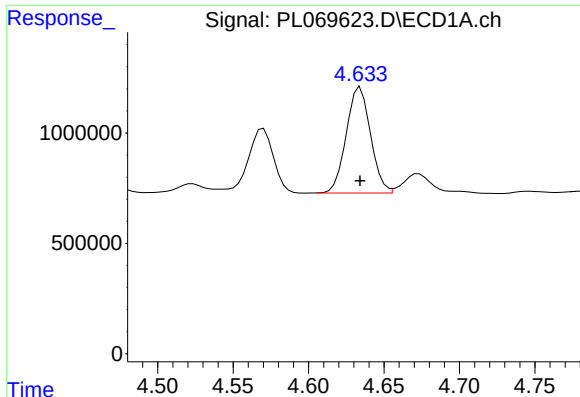


#1 Tetrachloro-m-xylene

R.T.: 4.633 min
Delta R.T.: -0.001 min
Response: 5374344
Conc: 17.26 ng/ml m

Instrument :
ECD_L
ClientSampleId :
20211008-MANASQUAN-WATER


Manual Integrations
APPROVED

Ankita
9/1/2021 11:01:36 AM

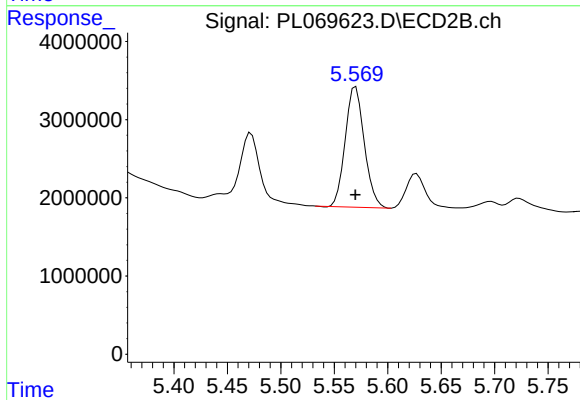


#1 Tetrachloro-m-xylene

R.T.: 5.570 min
Delta R.T.: 0.000 min
Response: 19146182
Conc: 15.22 ng/ml

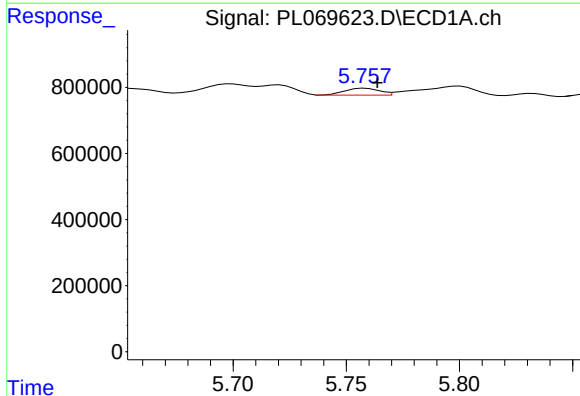


#3 gamma-BHC (Lindane)

R.T.: 5.757 min
Delta R.T.: -0.007 min
Response: 245738
Conc: 0.56 ng/ml m

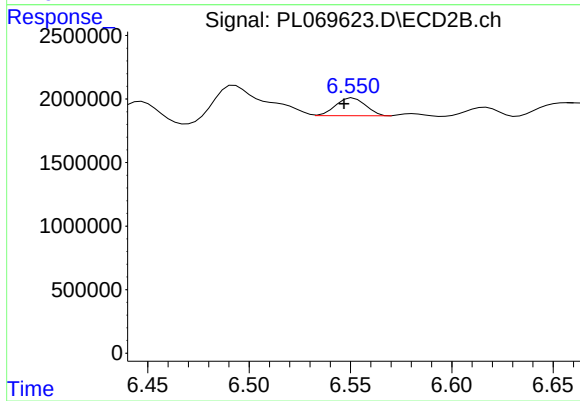

#3 gamma-BHC (Lindane)

R.T.: 6.550 min
Delta R.T.: 0.003 min
Response: 1446307
Conc: 0.89 ng/ml m

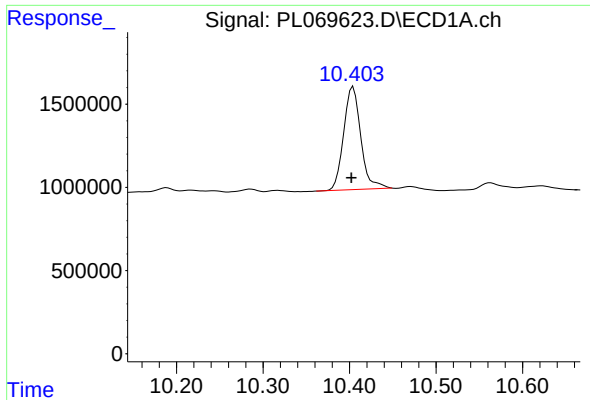

#28 Decachlorobiphenyl

R.T.: 10.404 min

Delta R.T.: 0.002 min


Response: 8513329

Conc: 14.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
20211008-MANASQUAN-WATER

Manual Integrations
APPROVED

Ankita
9/1/2021 11:01:36 AM

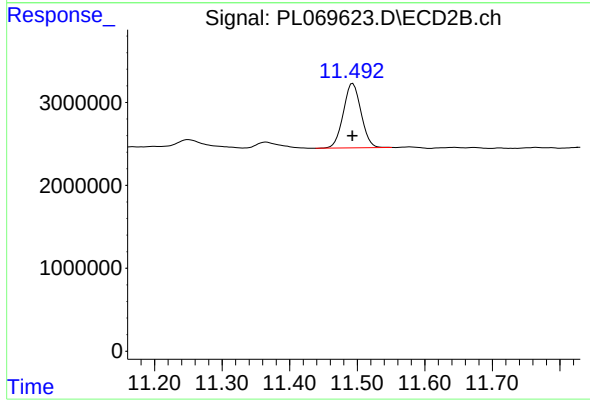

#28 Decachlorobiphenyl

R.T.: 11.494 min

Delta R.T.: 0.000 min

Response: 14156150

Conc: 12.54 ng/ml