

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083121\
 Data File : PL069632.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Aug 2021 16:05
 Operator : AR\AJ
 Sample : M3577-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 191-0827-B1-DP

Manual Integrations
 APPROVED

Ankita
 9/1/2021 11:01:41 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 01:29:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL083021.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 31 01:49:30 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.634	5.571	5291776	18714784	16.998	14.876
28)	SA Decachlor...	10.405	11.496	9386914	16966856	15.917	15.036
Target Compounds							
10)	B gamma-Chl...	7.353	8.304	681812	1940631	1.329m	1.397m
11)	B alpha-Chl...	7.424	8.388	1159857	2573419	2.232	1.881
17)	MA 4,4'-DDT	8.481	9.431	422713	483147	0.910m	0.443m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083121\
Data File : PL069632.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Aug 2021 16:05
Operator : AR\AJ
Sample : M3577-02
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
191-0827-B1-DP


Manual Integrations
APPROVED

Ankita
9/1/2021 11:01:41 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 01:29:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL083021.M
Quant Title : GC Extractables
QLast Update : Tue Aug 31 01:49:30 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

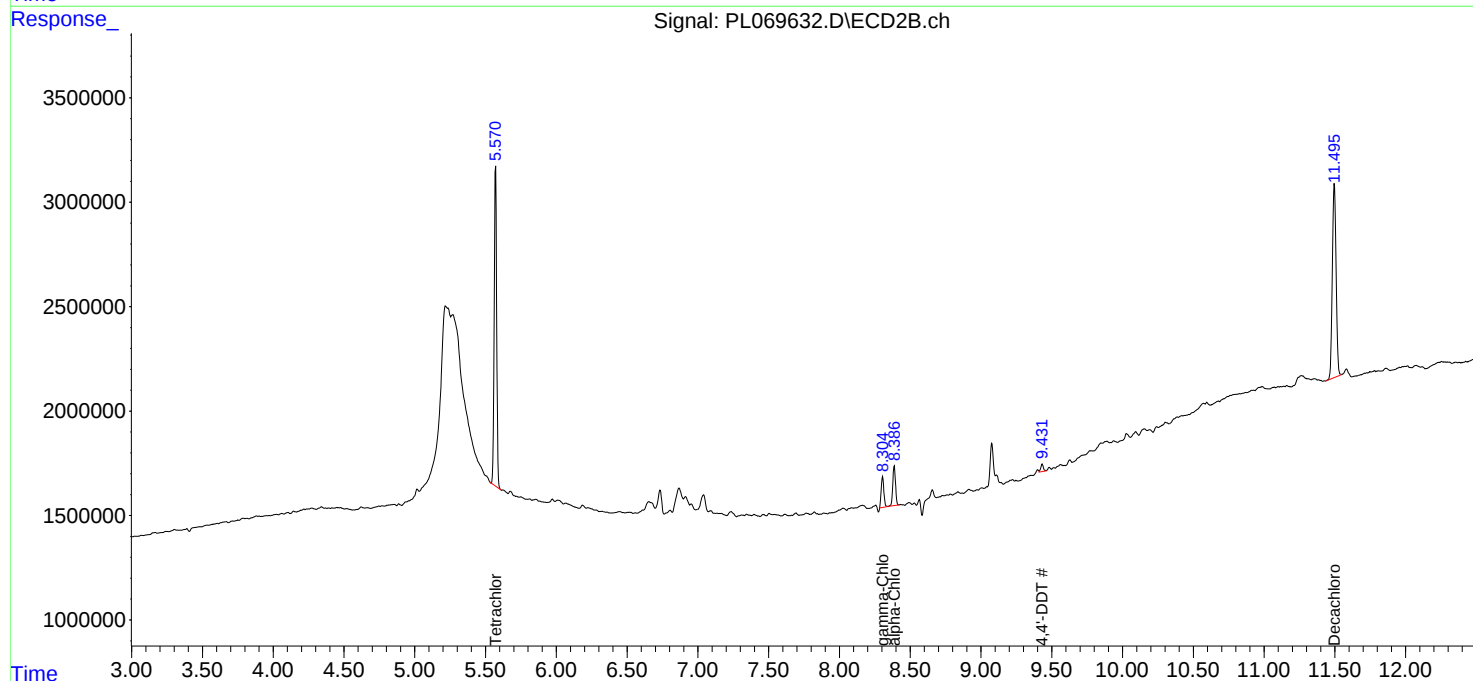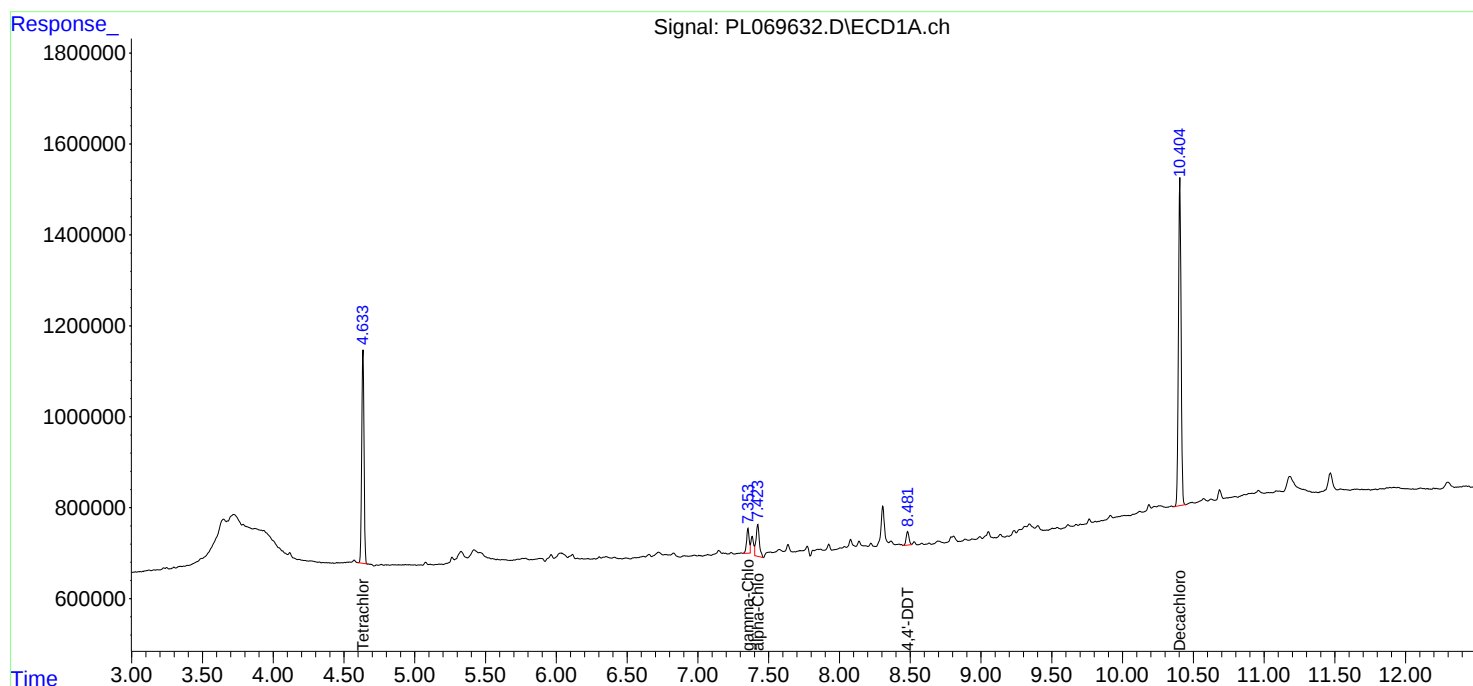

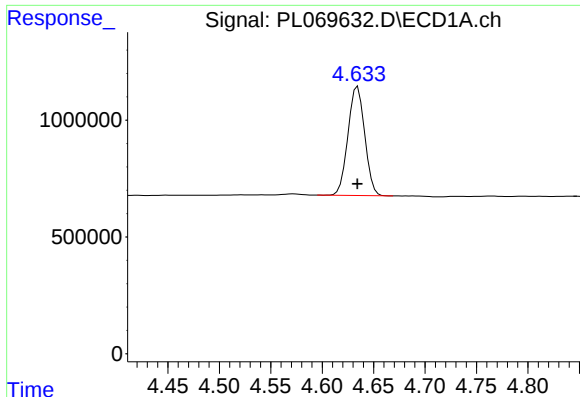


#1 Tetrachloro-m-xylene

R.T.: 4.634 min
Delta R.T.: 0.000 min
Response: 5291776
Conc: 17.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
191-0827-B1-DP


Manual Integrations
APPROVED

Ankita
9/1/2021 11:01:41 AM

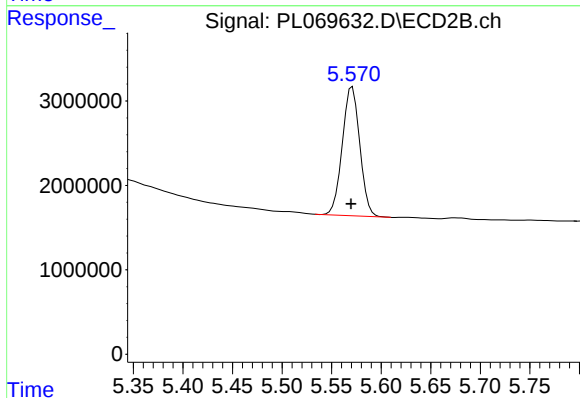


#1 Tetrachloro-m-xylene

R.T.: 5.571 min
Delta R.T.: 0.001 min
Response: 18714784
Conc: 14.88 ng/ml

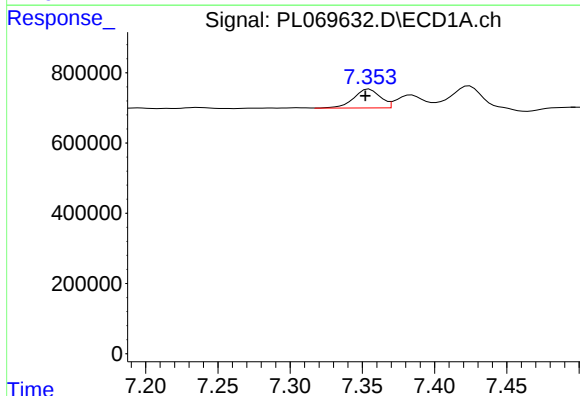


#10 gamma-Chlordane

R.T.: 7.353 min
Delta R.T.: 0.001 min
Response: 681812
Conc: 1.33 ng/ml m

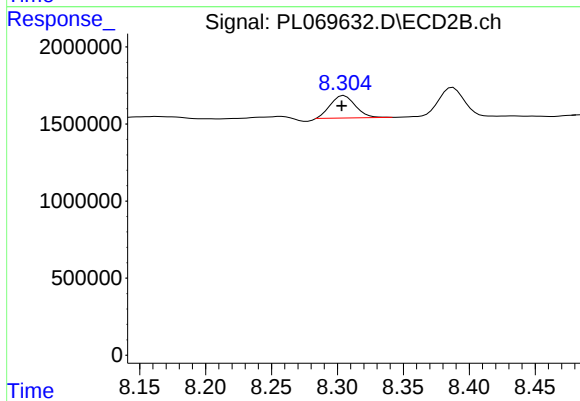

#10 gamma-Chlordane

R.T.: 8.304 min
Delta R.T.: 0.000 min
Response: 1940631
Conc: 1.40 ng/ml m

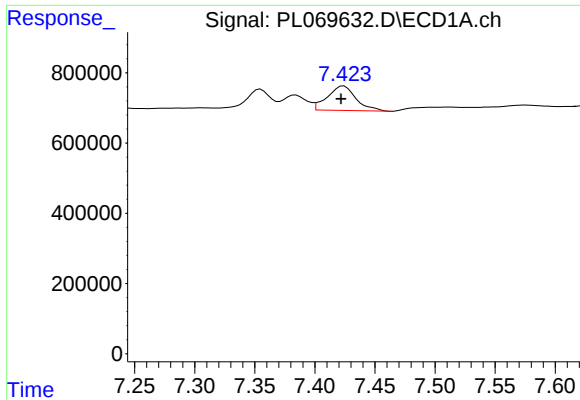


#11 alpha-Chlordane

R.T.: 7.424 min
Delta R.T.: 0.002 min
Response: 1159857
Conc: 2.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
191-0827-B1-DP


Manual Integrations
APPROVED

Ankita
9/1/2021 11:01:41 AM

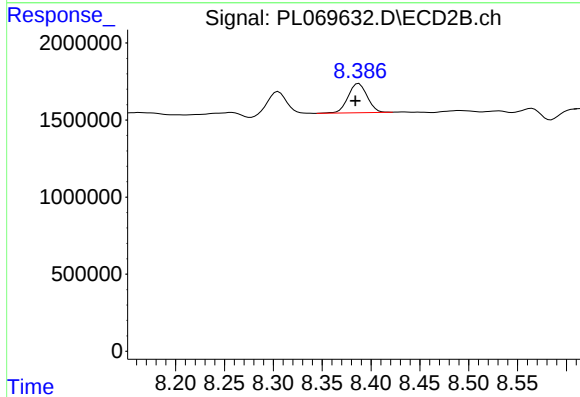


#11 alpha-Chlordane

R.T.: 8.388 min
Delta R.T.: 0.004 min
Response: 2573419
Conc: 1.88 ng/ml

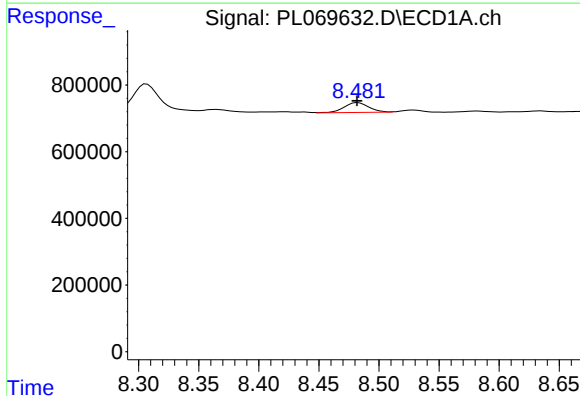


#17 4,4'-DDT

R.T.: 8.481 min
Delta R.T.: 0.000 min
Response: 422713
Conc: 0.91 ng/ml m

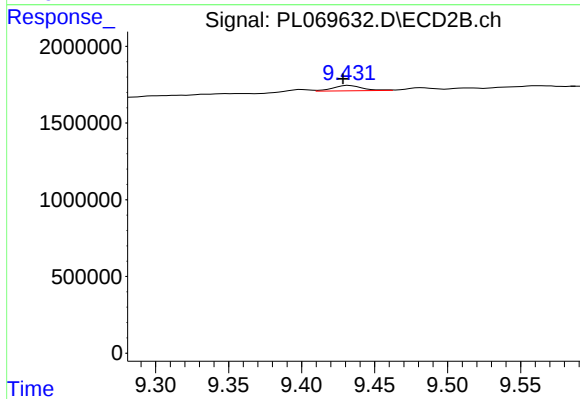

#17 4,4'-DDT

R.T.: 9.431 min
Delta R.T.: 0.002 min
Response: 483147
Conc: 0.44 ng/ml m

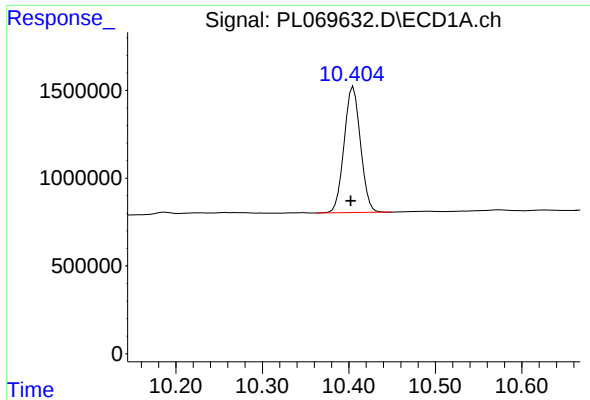


#28 Decachlorobiphenyl

R.T.: 10.405 min
Delta R.T.: 0.003 min
Response: 9386914
Conc: 15.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
191-0827-B1-DP

Manual Integrations
APPROVED

Ankita
9/1/2021 11:01:41 AM

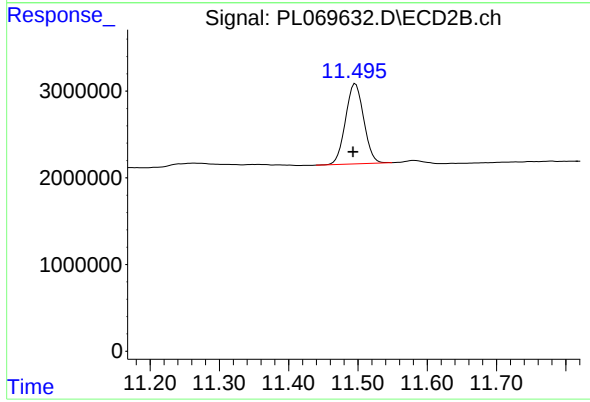

#28 Decachlorobiphenyl

R.T.: 11.496 min
Delta R.T.: 0.004 min
Response: 16966856
Conc: 15.04 ng/ml