

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083121\
 Data File : PL069633.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Aug 2021 16:21
 Operator : AR\AJ
 Sample : M3602-09
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-1COMP

Manual Integrations
 APPROVED

Ankita
 9/1/2021 11:01:43 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 01:29:56 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL083021.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 31 01:49:30 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.634	5.569	4935578	17483303	15.854	13.897
28)	SA Decachlor...	10.402	11.493	8354344	14889154	14.166	13.195
Target Compounds							
17)	MA 4,4'-DDT	8.479	9.426	326872	473028	0.703m	0.434m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083121\
Data File : PL069633.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Aug 2021 16:21
Operator : AR\AJ
Sample : M3602-09
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
TP-1COMP


Manual Integrations
APPROVED

Ankita
9/1/2021 11:01:43 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 01:29:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL083021.M
Quant Title : GC Extractables
QLast Update : Tue Aug 31 01:49:30 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

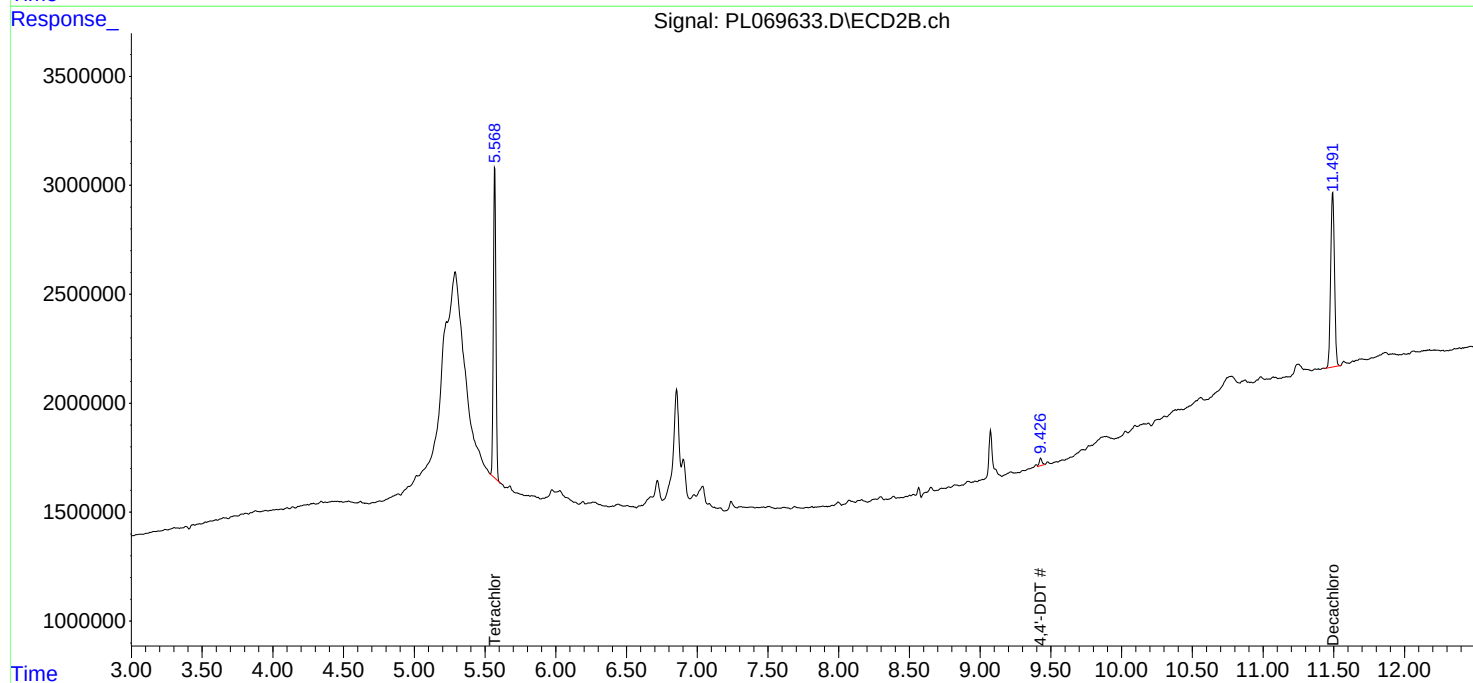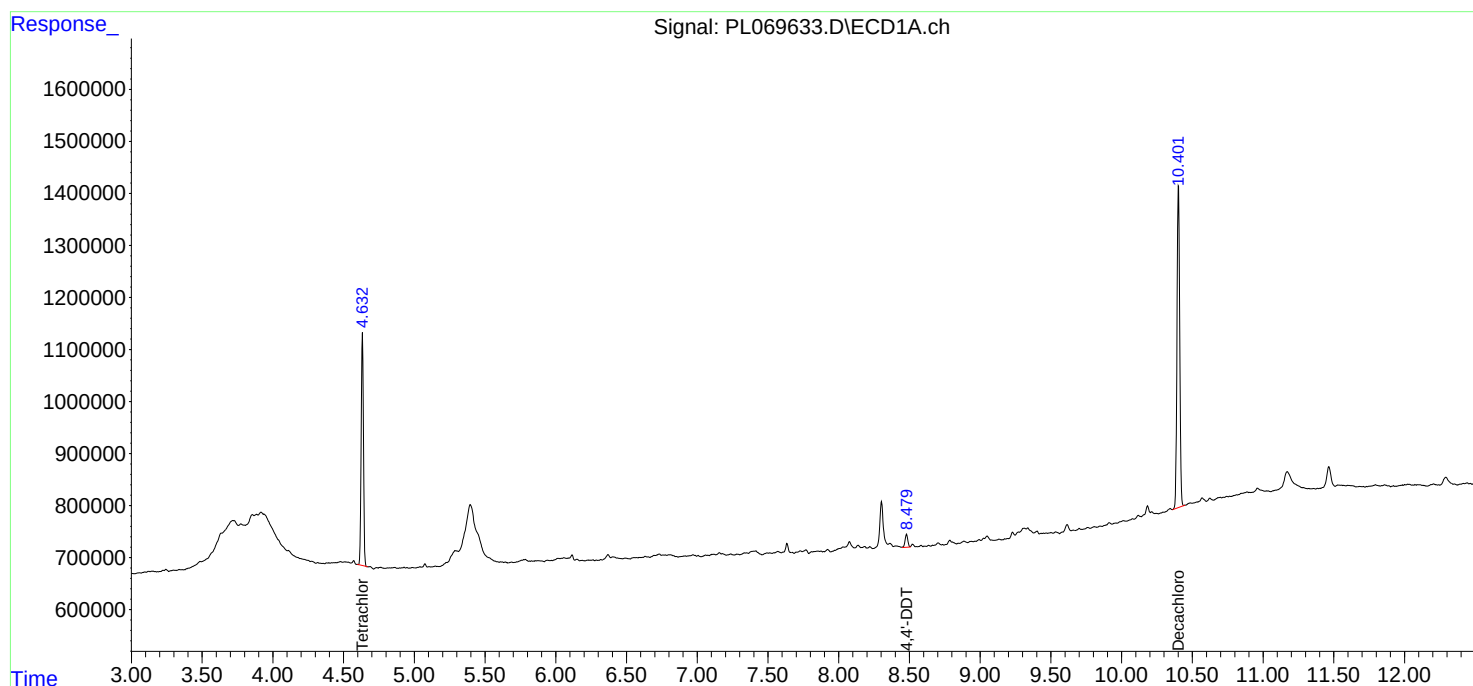

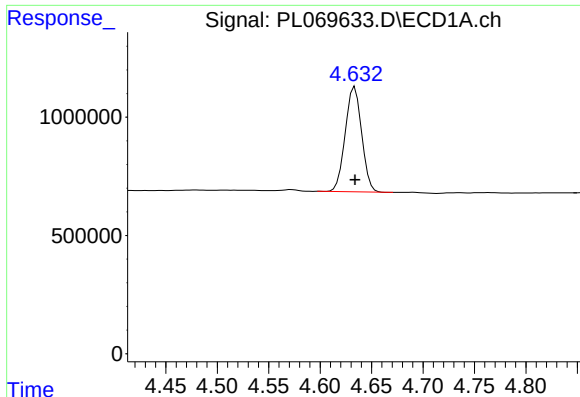


#1 Tetrachloro-m-xylene

R.T.: 4.634 min
Delta R.T.: 0.000 min
Response: 4935578
Conc: 15.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1COMP


Manual Integrations
APPROVED

Ankita
9/1/2021 11:01:43 AM

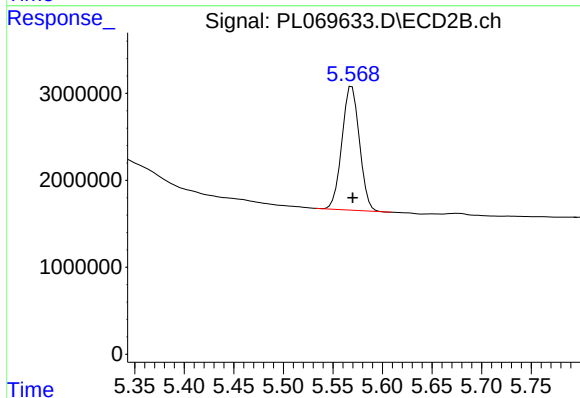


#1 Tetrachloro-m-xylene

R.T.: 5.569 min
Delta R.T.: 0.000 min
Response: 17483303
Conc: 13.90 ng/ml

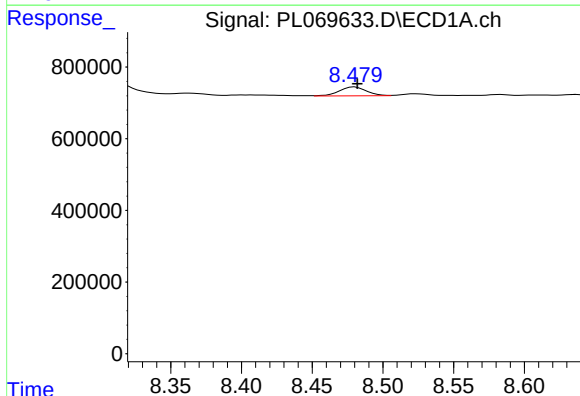


#17 4,4'-DDT

R.T.: 8.479 min
Delta R.T.: -0.003 min
Response: 326872
Conc: 0.70 ng/ml m

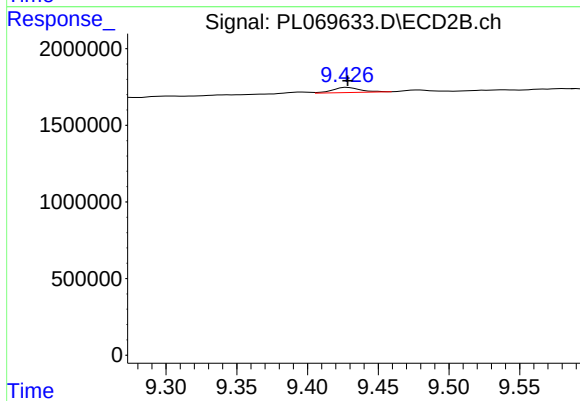

#17 4,4'-DDT

R.T.: 9.426 min
Delta R.T.: -0.002 min
Response: 473028
Conc: 0.43 ng/ml m

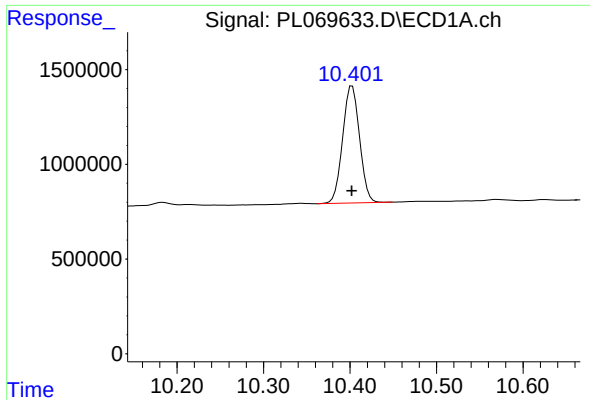


#28 Decachlorobiphenyl

R.T.: 10.402 min
Delta R.T.: 0.000 min
Response: 8354344
Conc: 14.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1COMP

Manual Integrations
APPROVED

Ankita
9/1/2021 11:01:43 AM

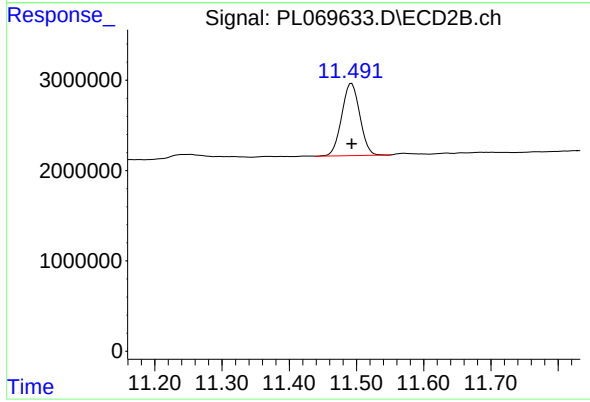

#28 Decachlorobiphenyl

R.T.: 11.493 min
Delta R.T.: 0.000 min
Response: 14889154
Conc: 13.19 ng/ml