

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083122\
 Data File : PL077400.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Aug 2022 12:37
 Operator : AR\AJ
 Sample : PB147371BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 15:52:57 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082222.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 23 05:36:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.423	2.632	24169770	49106896	17.763	15.979
28)	SA Decachlor...	8.916	7.739	22232281	46858381	18.971	16.793
Target Compounds							
2)	A alpha-BHC	0.000	3.115	0	220940	N.D.	0.051 #
7)	B delta-BHC	4.651f	0.000	762153	0	0.493	N.D. #
10)	B gamma-Chl...	0.000	4.793	0	1486335	N.D.	0.445 #
14)	MA Endrin	0.000	5.479f	0	600093	N.D.	0.220 #
15)	B Endosulfa...	6.705f	0.000	143566	0	0.131	N.D. #
16)	A 4,4'-DDD	0.000	5.618	0	1494961	N.D.	0.559 #
21)	B Endrin ke...	7.570f	0.000	411788	0	0.338	N.D. #
25)	Chlordane-3	0.000	4.793	0	1486335	N.D.	4.868 #
27)	Chlordane-5	0.000	5.557f	0	2535841	N.D.	28.963 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083122\
Data File : PL077400.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Aug 2022 12:37
Operator : AR\AJ
Sample : PB147371BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 15:52:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082222.M
Quant Title : GC Extractables
QLast Update : Tue Aug 23 05:36:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

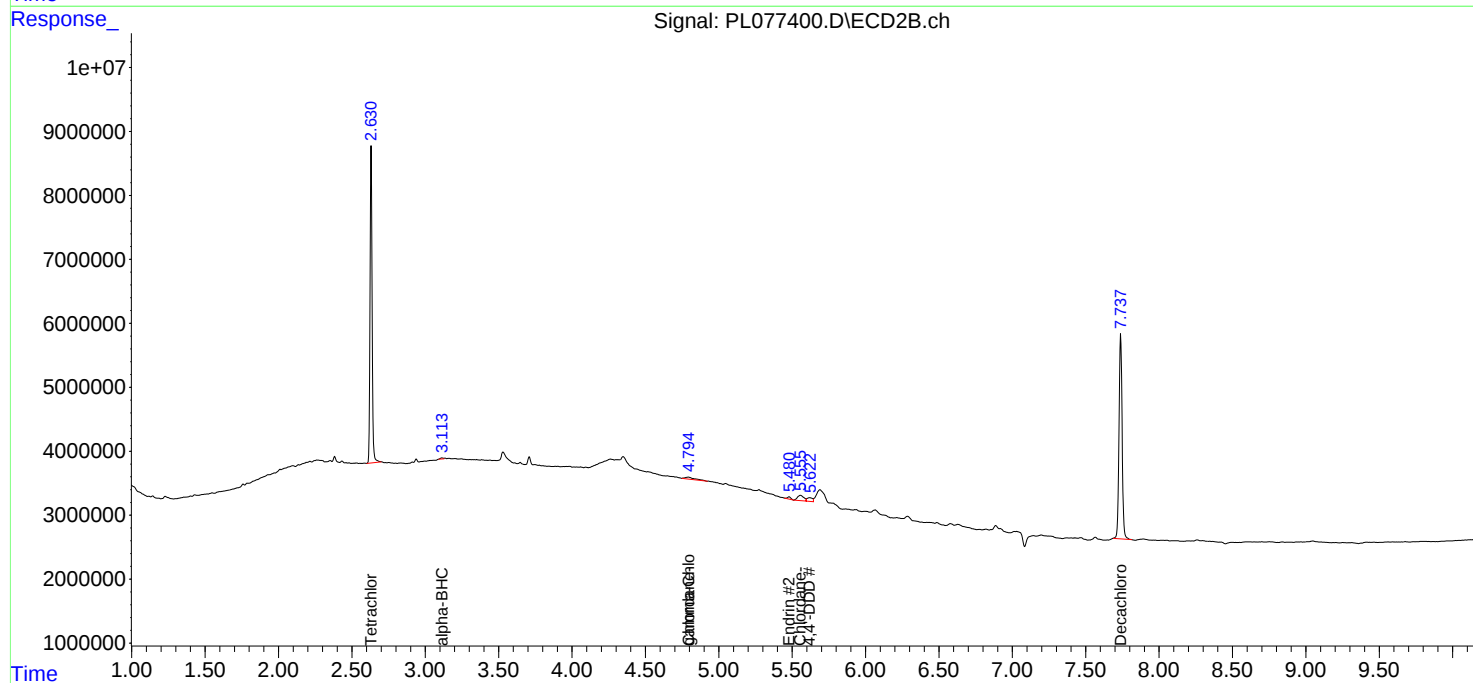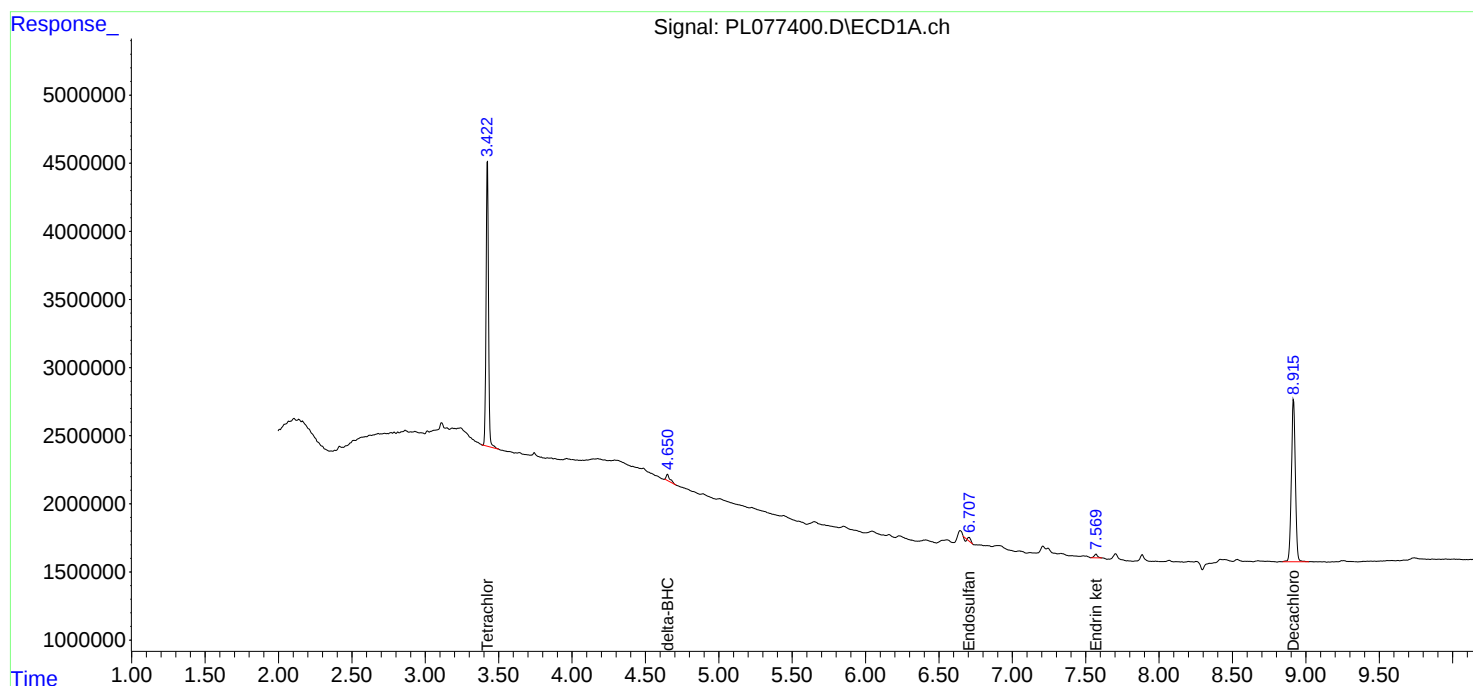


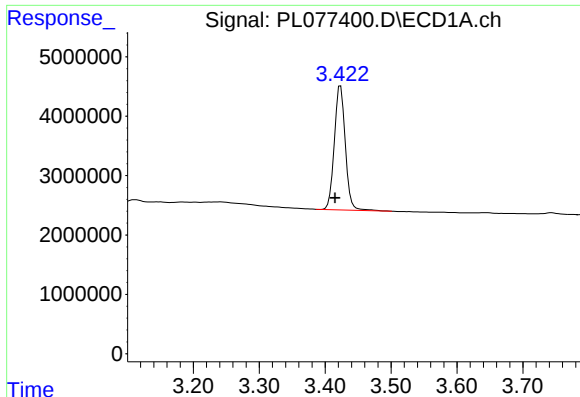

#1 Tetrachloro-m-xylene


R.T.: 3.423 min
Delta R.T.: 0.008 min
Response: 24169770
Conc: 17.76 ng/ml

Instrument :
ECD_L
ClientSampleId :

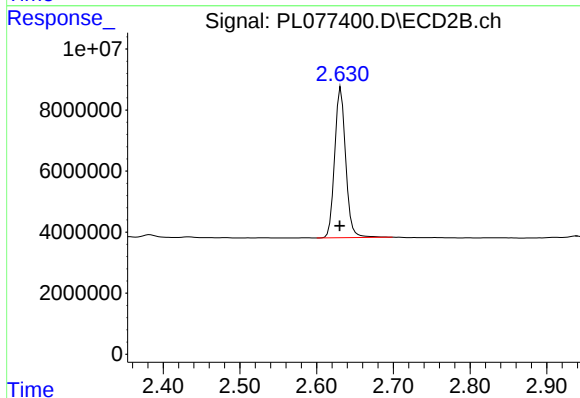


#1 Tetrachloro-m-xylene

R.T.: 2.632 min
Delta R.T.: 0.001 min
Response: 49106896
Conc: 15.98 ng/ml

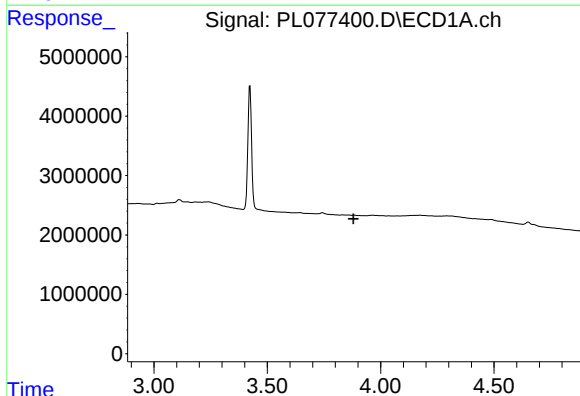


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.880 min
Response: 0
Conc: N.D.

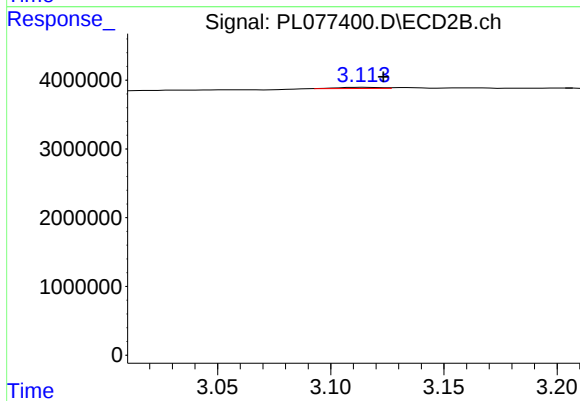

#2 alpha-BHC


R.T.: 3.115 min
Delta R.T.: -0.009 min
Response: 220940
Conc: 0.05 ng/ml

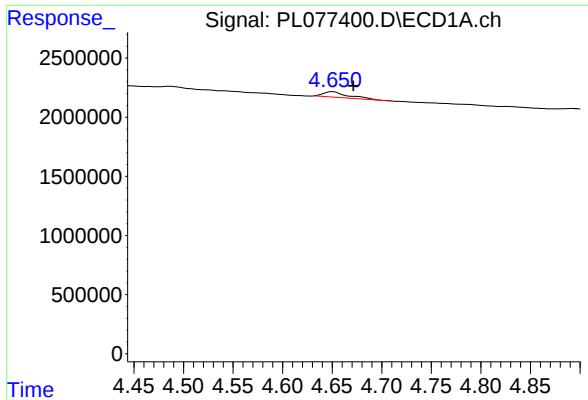

#7 delta-BHC


R.T.: 4.651 min
Delta R.T.: -0.021 min
Response: 762153
Conc: 0.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

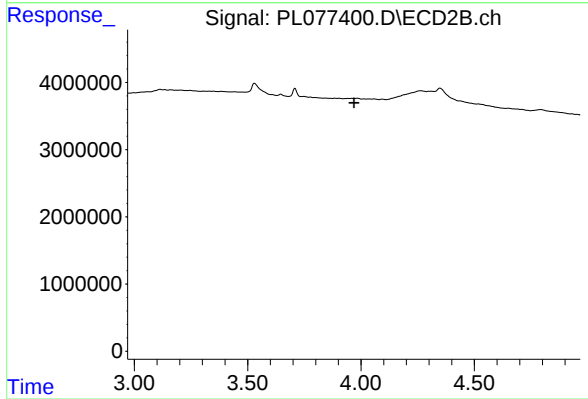


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 3.970 min
Response: 0
Conc: N.D.

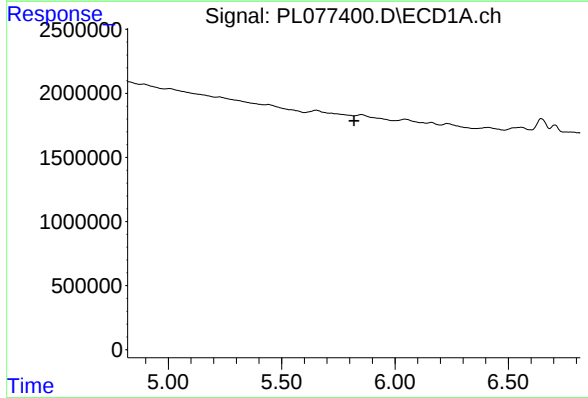


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.820 min
Response: 0
Conc: N.D.

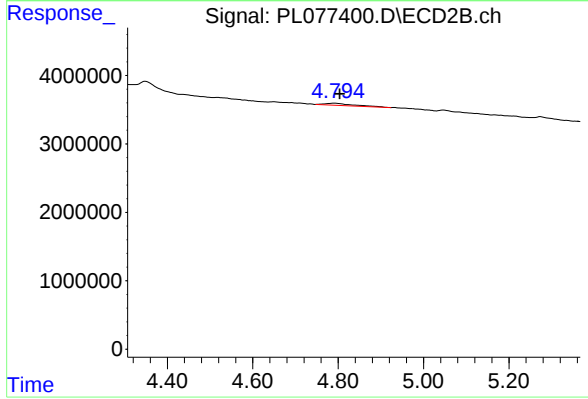

#10 gamma-Chlordane


R.T.: 4.793 min
Delta R.T.: -0.010 min
Response: 1486335
Conc: 0.44 ng/ml

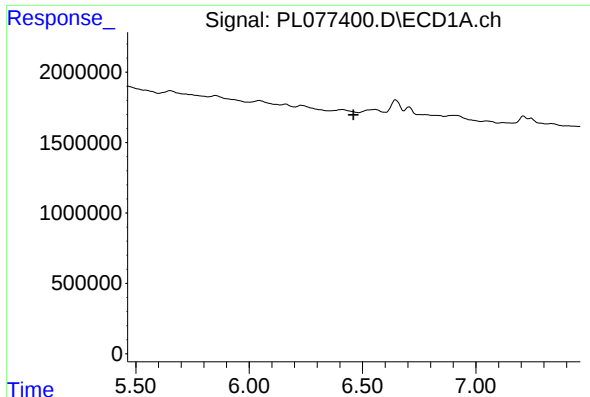

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.460 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

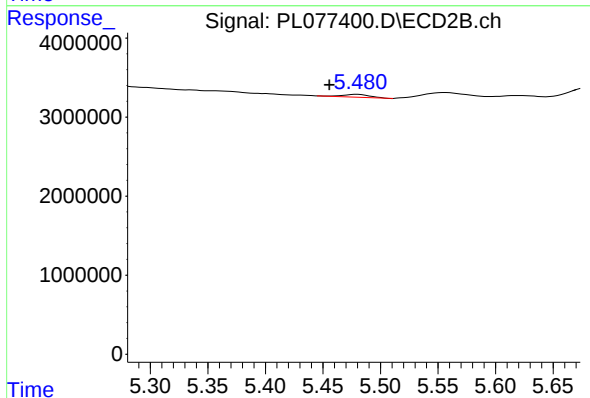


#14 Endrin

R.T.: 5.479 min
Delta R.T.: 0.024 min
Response: 600093
Conc: 0.22 ng/ml

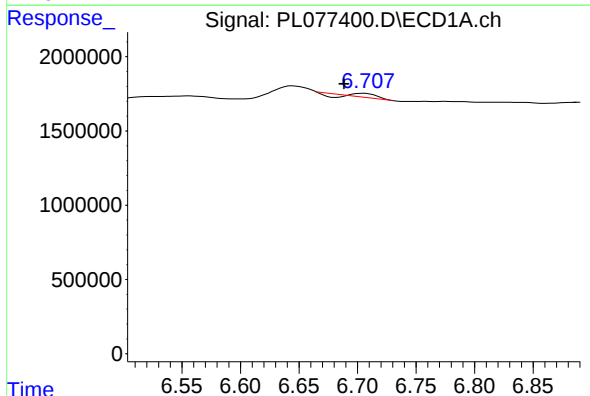


#15 Endosulfan II

R.T.: 6.705 min
Delta R.T.: 0.017 min
Response: 143566
Conc: 0.13 ng/ml

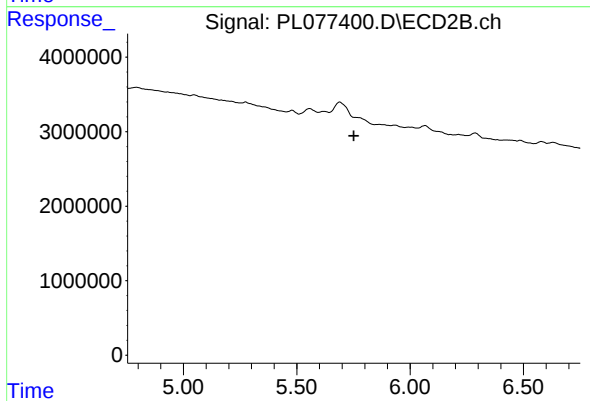

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.752 min
Response: 0
Conc: N.D.

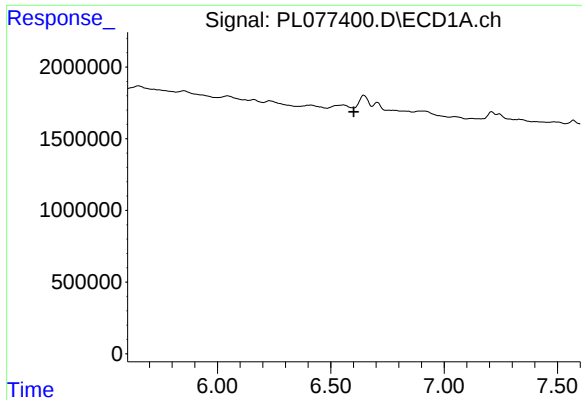

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.602 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

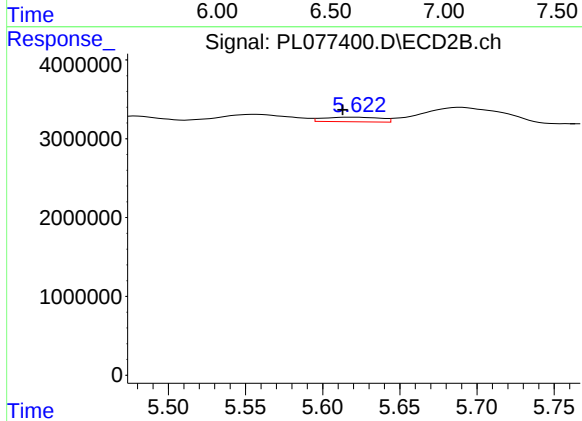


#16 4,4'-DDD

R.T.: 5.618 min
Delta R.T.: 0.005 min
Response: 1494961
Conc: 0.56 ng/ml

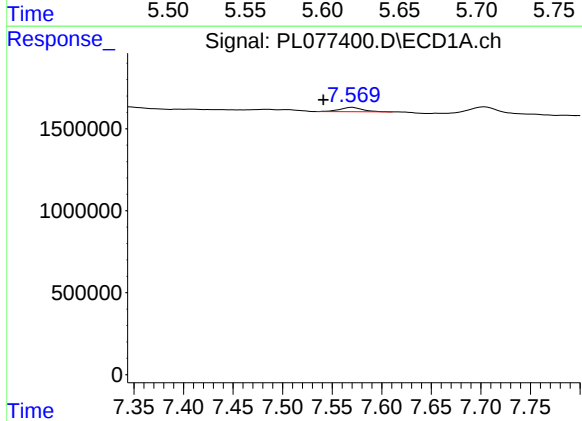


#21 Endrin ketone

R.T.: 7.570 min
Delta R.T.: 0.029 min
Response: 411788
Conc: 0.34 ng/ml

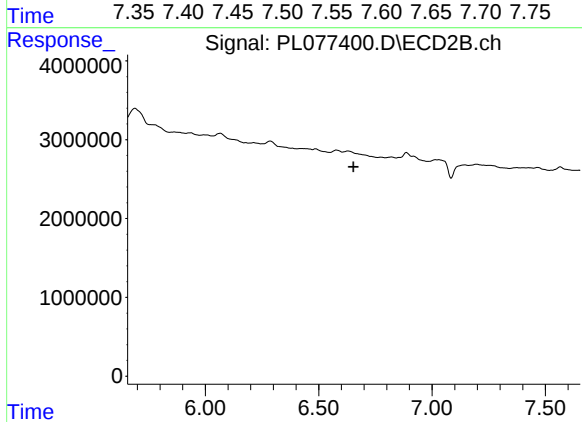

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 6.654 min
Response: 0
Conc: N.D.

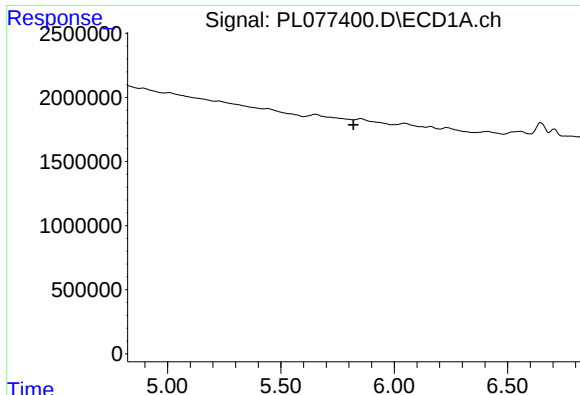

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.821 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

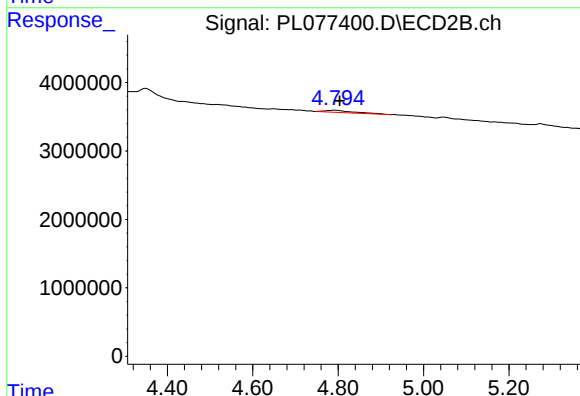


#25 Chlordane-3

R.T.: 4.793 min
Delta R.T.: -0.011 min
Response: 1486335
Conc: 4.87 ng/ml

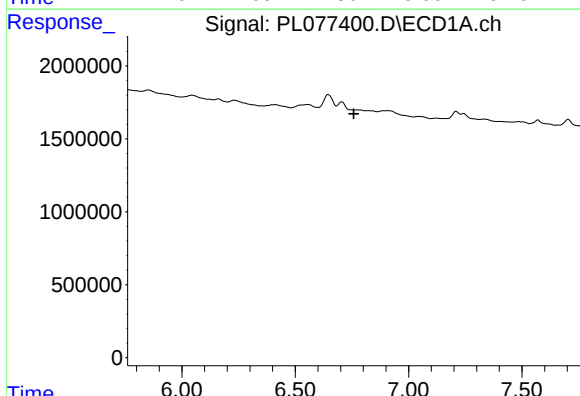


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.758 min
Response: 0
Conc: N.D.

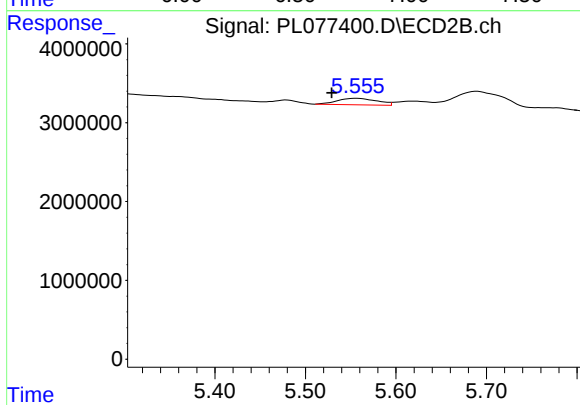

#27 Chlordane-5


R.T.: 5.557 min
Delta R.T.: 0.027 min
Response: 2535841
Conc: 28.96 ng/ml

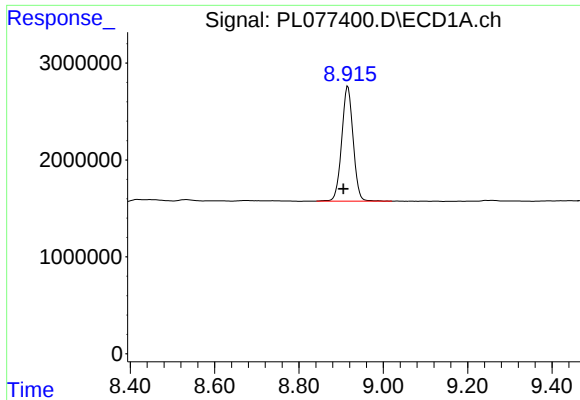

#28 Decachlorobiphenyl

R.T.: 8.916 min
Delta R.T.: 0.011 min
Response: 22232281
Conc: 18.97 ng/ml

Instrument :
ECD_L
ClientSampleId :

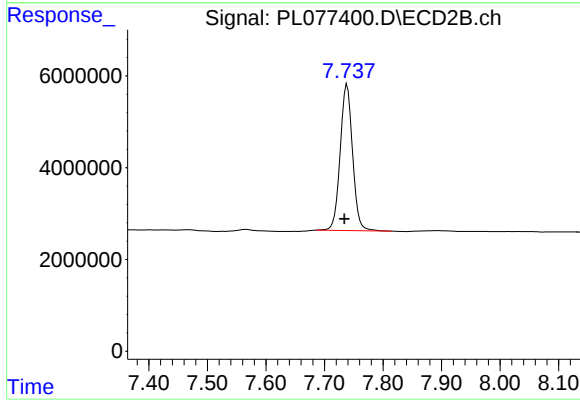

#28 Decachlorobiphenyl

R.T.: 7.739 min
Delta R.T.: 0.004 min
Response: 46858381
Conc: 16.79 ng/ml