

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083122\
 Data File : PL077405.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Aug 2022 14:06
 Operator : AR\AJ
 Sample : N4433-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 EP-BLIND-DUPLICATE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 15:53:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082222.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 23 05:36:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.417	2.631	16188741	35303672	11.898	11.487
28)	SA Decachlor...	8.907	7.733	16906532	35170650	14.427	12.605
Target Compounds							
12)	B 4,4'-DDE	6.074	5.059	1217631	3493336	0.938	1.082
17)	MA 4,4'-DDT	6.914	5.860	2888809	5541979	2.586	2.104


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083122\
Data File : PL077405.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Aug 2022 14:06
Operator : AR\AJ
Sample : N4433-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
EP-BLIND-DUPLICATE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 15:53:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082222.M
Quant Title : GC Extractables
QLast Update : Tue Aug 23 05:36:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

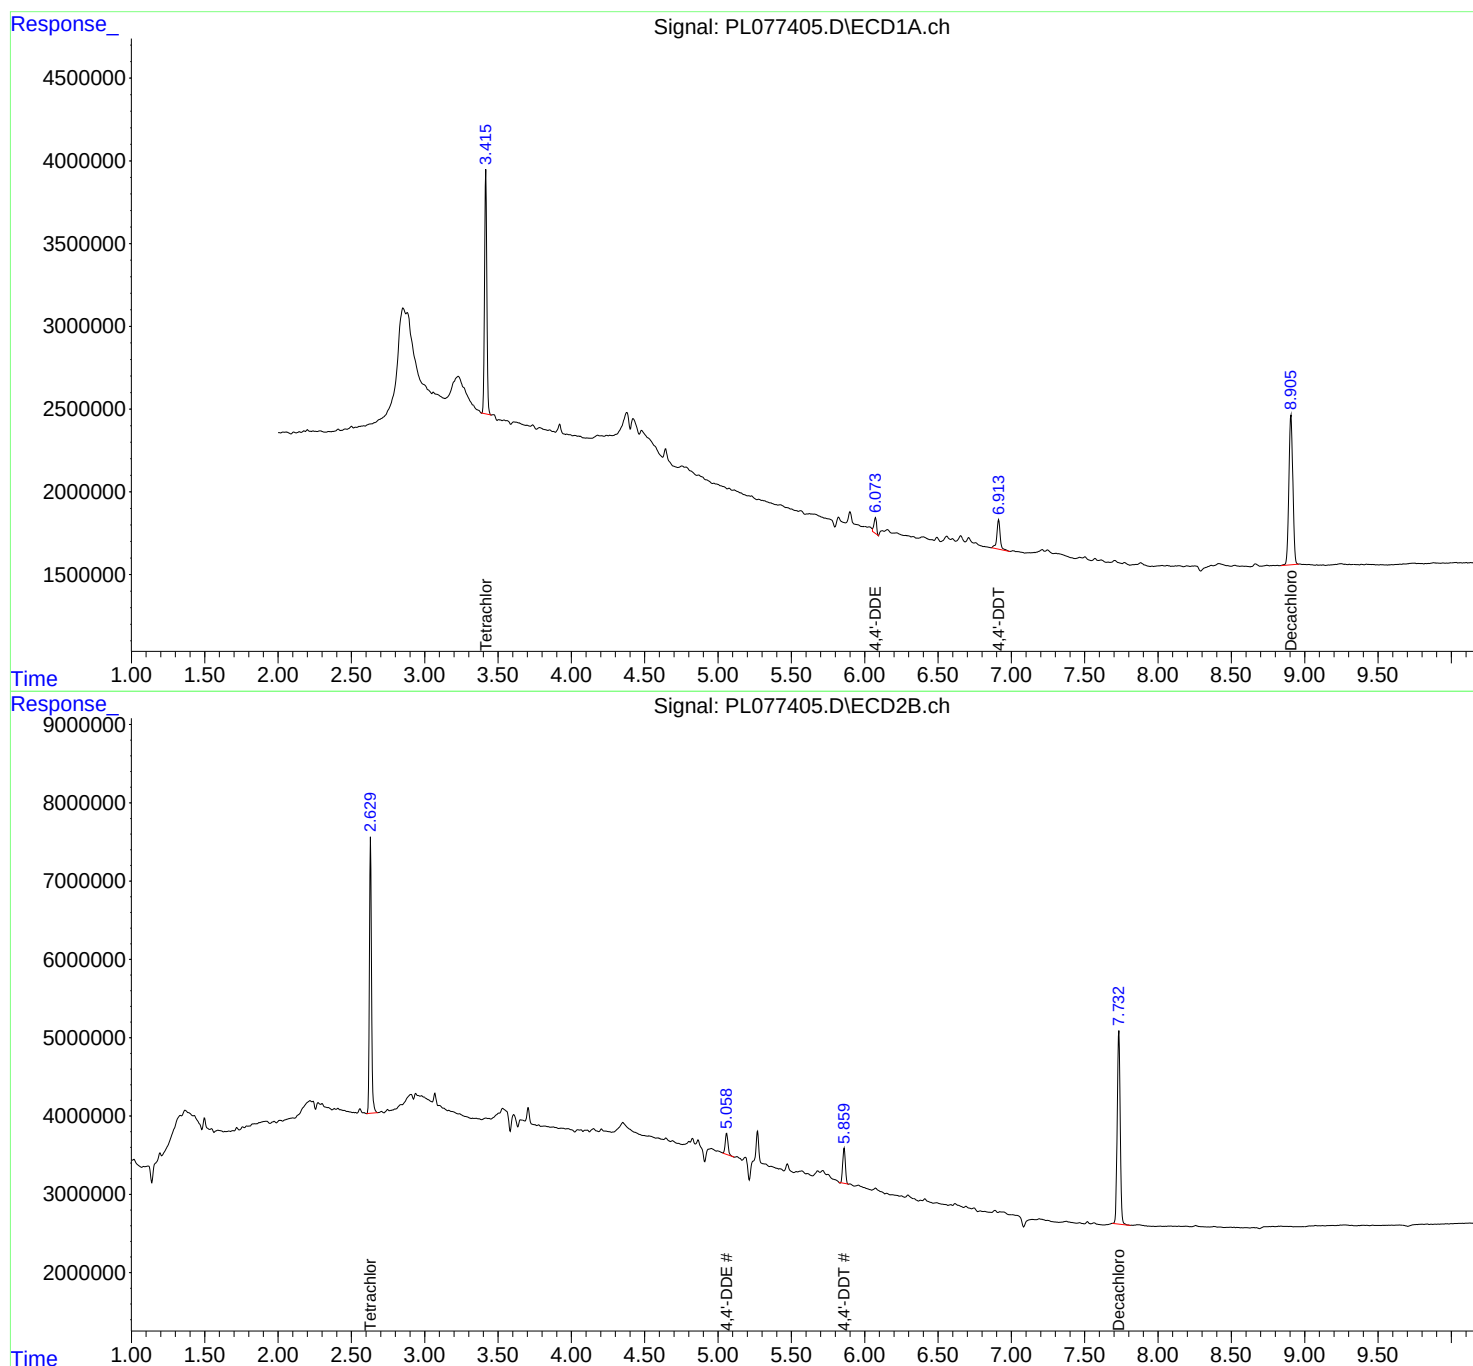


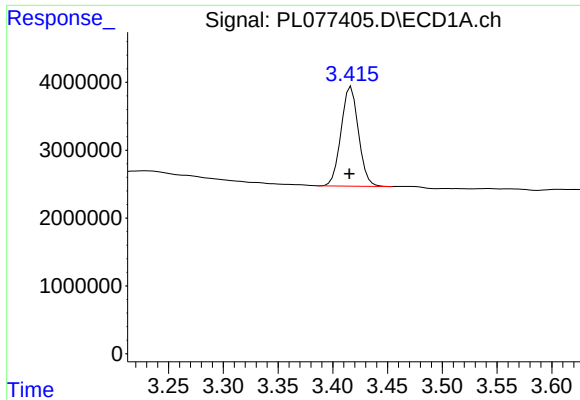

#1 Tetrachloro-m-xylene


R.T.: 3.417 min
Delta R.T.: 0.002 min
Response: 16188741
Conc: 11.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
EP-BLIND-DUPLICATE

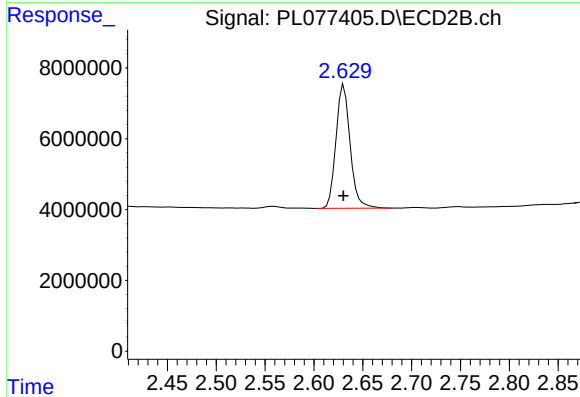


#1 Tetrachloro-m-xylene

R.T.: 2.631 min
Delta R.T.: 0.000 min
Response: 35303672
Conc: 11.49 ng/ml

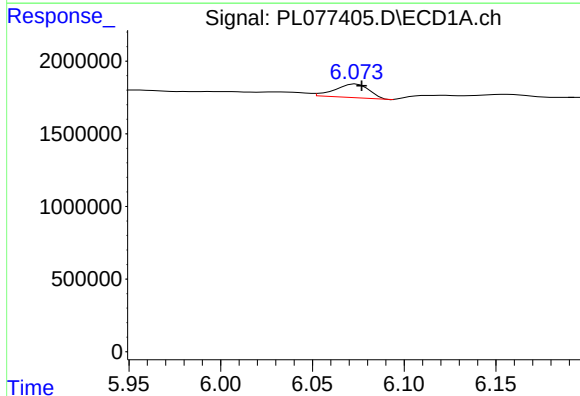


#12 4,4'-DDE

R.T.: 6.074 min
Delta R.T.: -0.003 min
Response: 1217631
Conc: 0.94 ng/ml

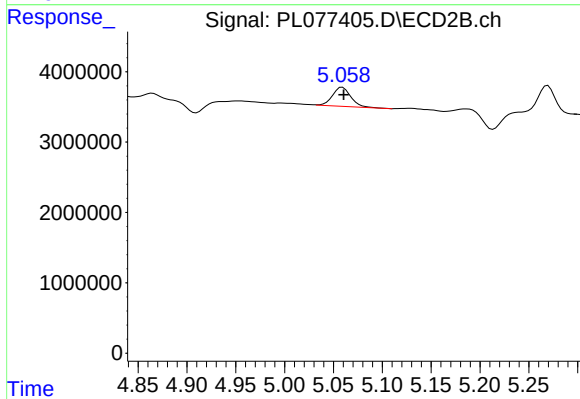

#12 4,4'-DDE


R.T.: 5.059 min
Delta R.T.: -0.001 min
Response: 3493336
Conc: 1.08 ng/ml

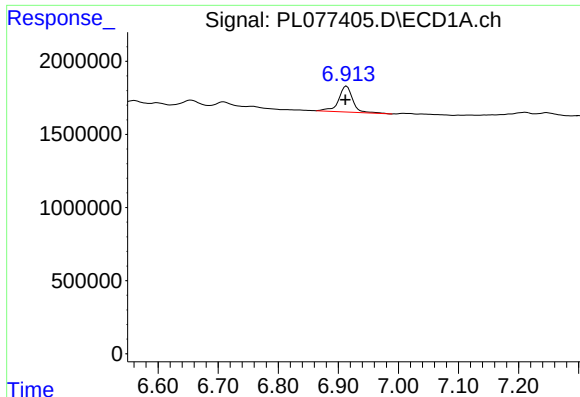

#17 4,4'-DDT


R.T.: 6.914 min
Delta R.T.: 0.002 min
Response: 2888809
Conc: 2.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
EP-BLIND-DUPLICATE

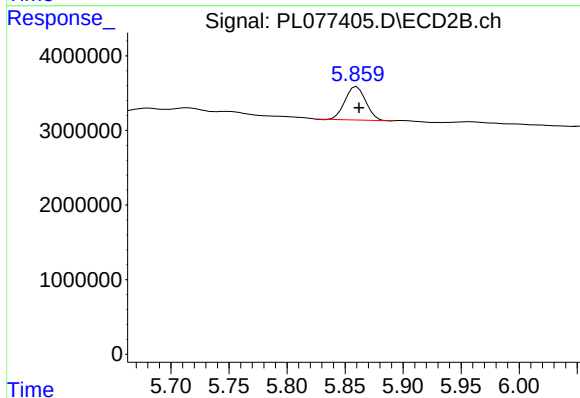


#17 4,4'-DDT

R.T.: 5.860 min
Delta R.T.: -0.002 min
Response: 5541979
Conc: 2.10 ng/ml

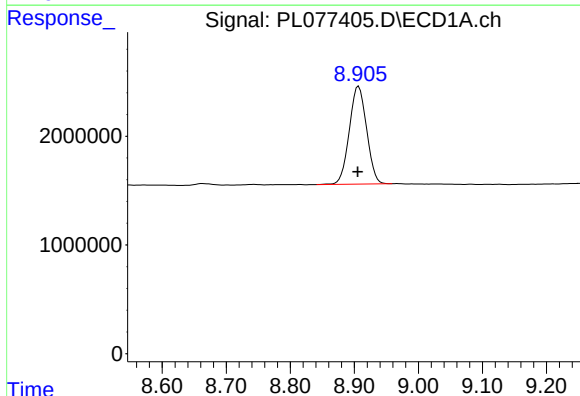

#28 Decachlorobiphenyl

R.T.: 8.907 min
Delta R.T.: 0.001 min
Response: 16906532
Conc: 14.43 ng/ml

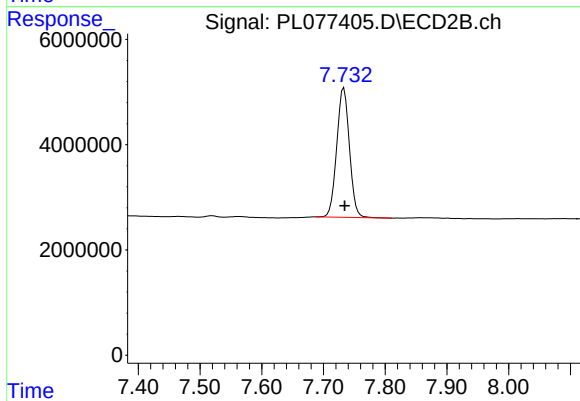

#28 Decachlorobiphenyl

R.T.: 7.733 min
Delta R.T.: -0.001 min
Response: 35170650
Conc: 12.60 ng/ml