

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083122\
 Data File : PL077429.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Aug 2022 19:41
 Operator : AR\AJ
 Sample : N4438-01
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 KTS2-WC-S-TR-01-02-03

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/01/2022
 Supervised By : Ankita Jodhani 09/01/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 03:02:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082222.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 23 05:36:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.415	2.630	22737754	44145520	16.711m	14.364
28) SA Decachlor...	8.905	7.731	13487816	26110301	11.509	9.357

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083122\
Data File : PL077429.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Aug 2022 19:41
Operator : AR\AJ
Sample : N4438-01
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
KTS2-WC-S-TR-01-02-03


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 09/01/2022
Supervised By : Ankita Jodhani 09/01/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 03:02:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082222.M
Quant Title : GC Extractables
QLast Update : Tue Aug 23 05:36:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

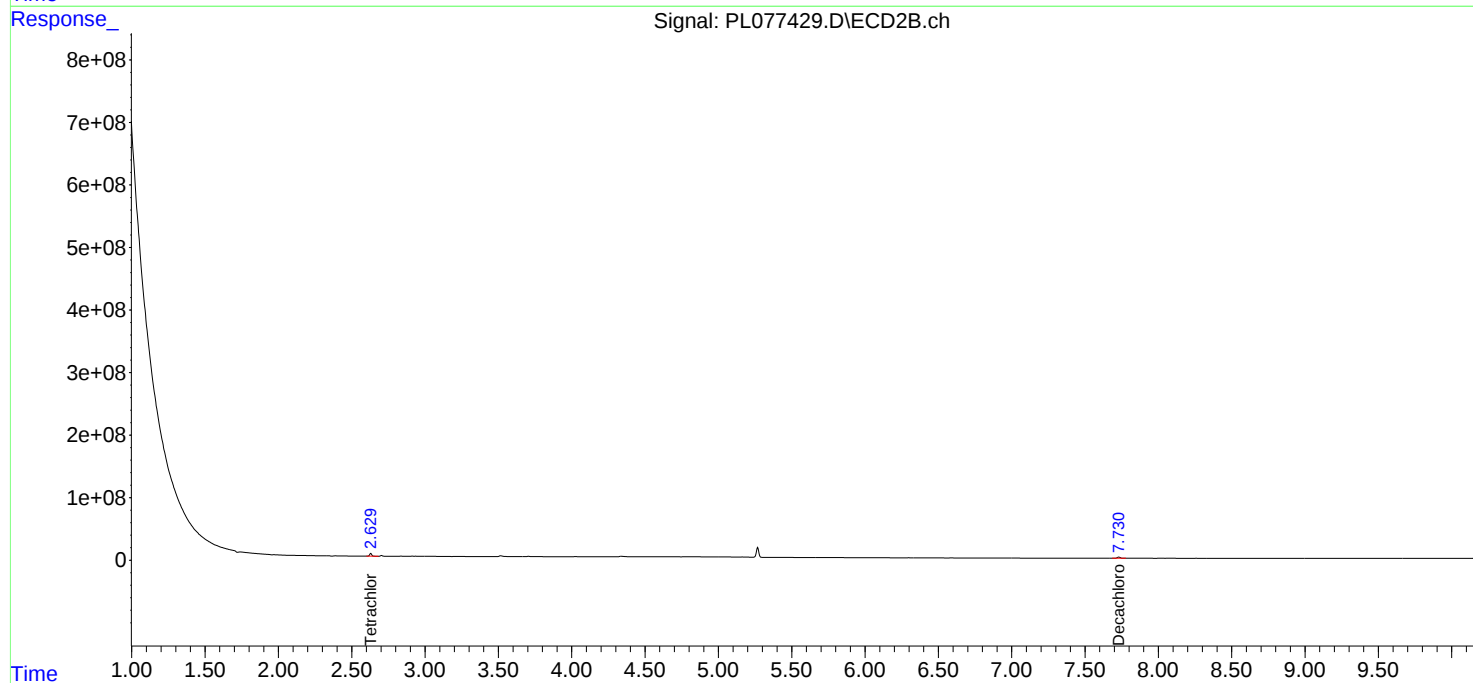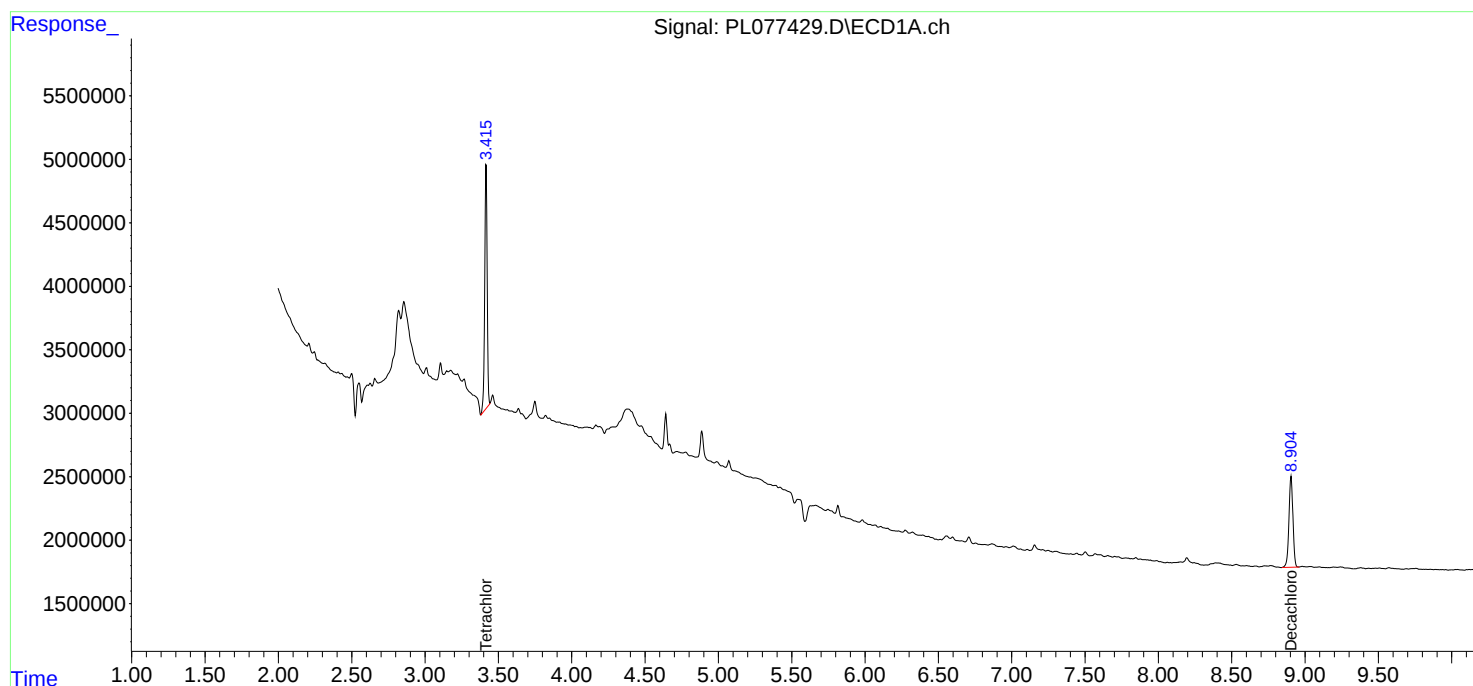

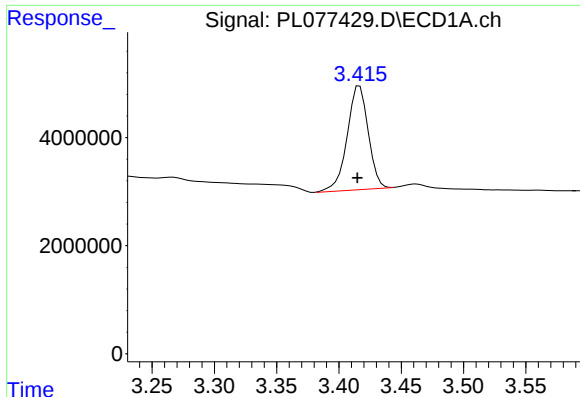


#1 Tetrachloro-m-xylene

R.T.: 3.415 min
Delta R.T.: 0.000 min
Response: 22737754
Conc: 16.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
KTS2-WC-S-TR-01-02-03


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/01/2022
Supervised By :Ankita Jodhani 09/01/2022

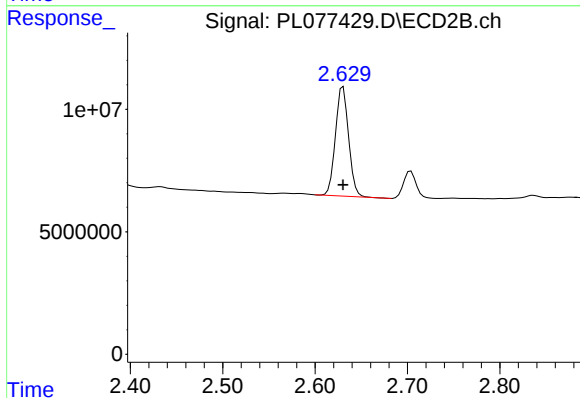


#1 Tetrachloro-m-xylene

R.T.: 2.630 min
Delta R.T.: 0.000 min
Response: 44145520
Conc: 14.36 ng/ml

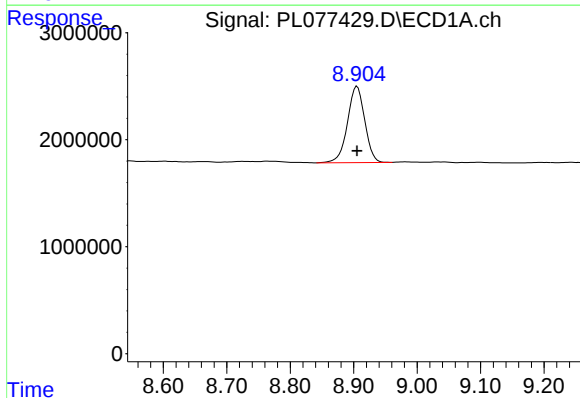

#28 Decachlorobiphenyl

R.T.: 8.905 min
Delta R.T.: 0.000 min
Response: 13487816
Conc: 11.51 ng/ml

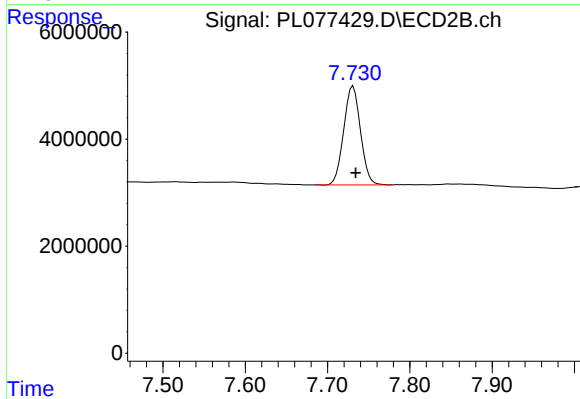

#28 Decachlorobiphenyl

R.T.: 7.731 min
Delta R.T.: -0.003 min
Response: 26110301
Conc: 9.36 ng/ml