

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090120\
 Data File : PL061122.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Sep 2020 09:57
 Operator : DD\AJ
 Sample : L3847-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 14:49:45 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 25 16:59:57 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.459	4.008	22461149	28352646	12.171	10.909
28)	SA Decachlor...	8.213	9.094	20228691	27238944	12.008	12.909
Target Compounds							
5)	MB Aldrin	0.000	5.497	0	4462044	N.D.	1.324 #
9)	A Endosulfan I	5.525	0.000	1735735	0	0.955	N.D. #
10)	B gamma-Chl...	0.000	6.125	0	2784495	N.D.	0.897 #
11)	B alpha-Chl...	0.000	6.193	0	5533494	N.D.	1.780 #
17)	MA 4,4'-DDT	6.377	0.000	1086156	0	0.719	N.D. #
23)	Chlordane-1	4.325	0.000	5047923	0	82.675	N.D. #
24)	Chlordane-2	0.000	5.497 ^f	0	4462044	N.D.	43.358 #
25)	Chlordane-3	0.000	6.125	0	2784495	N.D.	6.967 #
26)	Chlordane-4	0.000	6.193	0	5533494	N.D.	11.511 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090120\
Data File : PL061122.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Sep 2020 09:57
Operator : DD\AJ
Sample : L3847-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 14:49:45 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
Quant Title : GC Extractables
QLast Update : Tue Aug 25 16:59:57 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

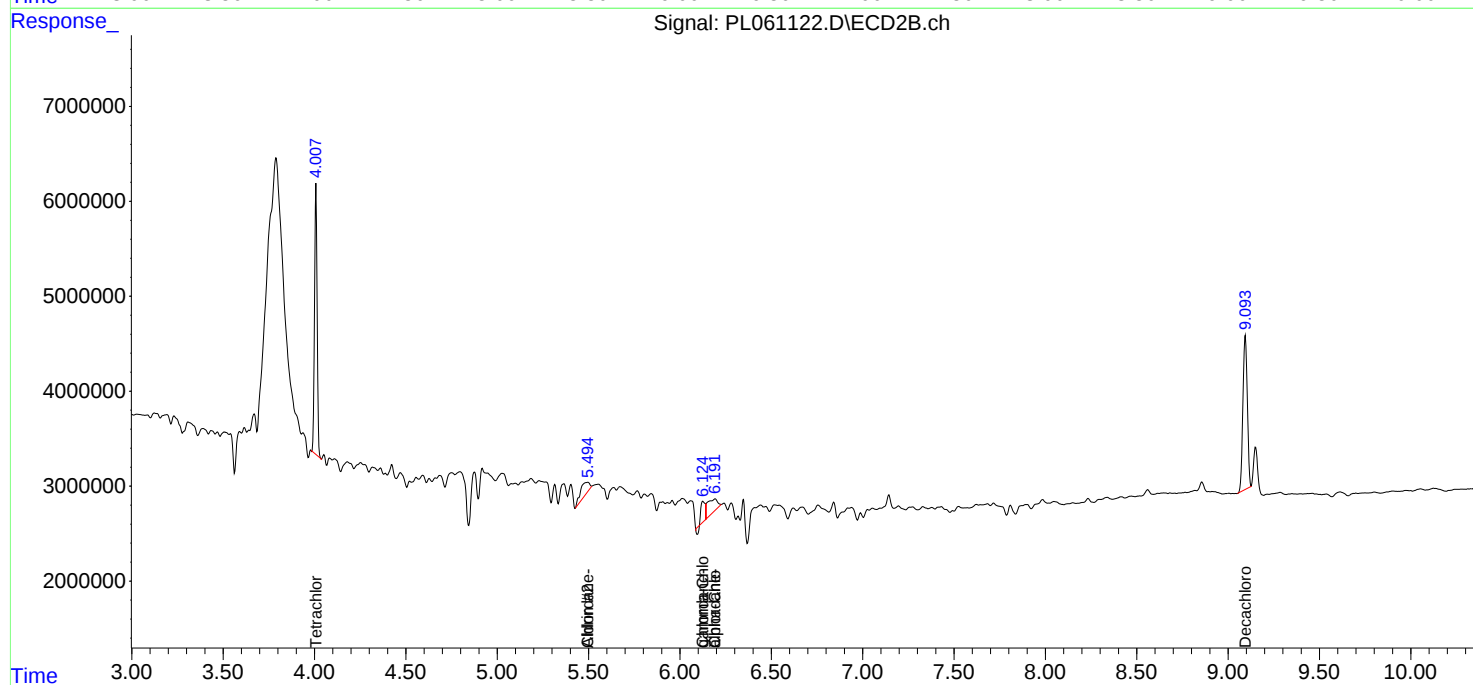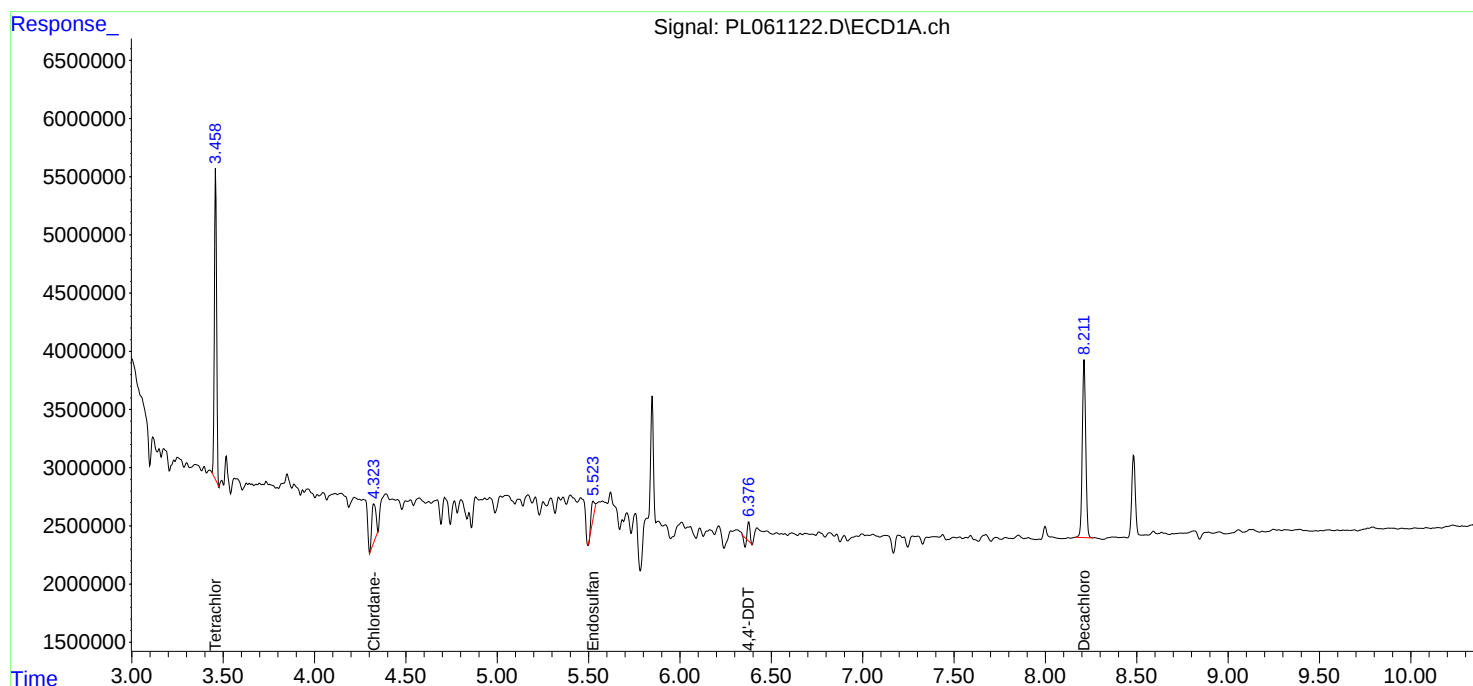


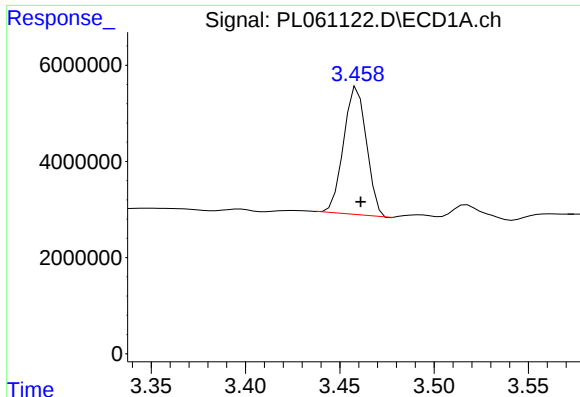

#1 Tetrachloro-m-xylene


R.T.: 3.459 min
Delta R.T.: -0.002 min
Response: 22461149
Conc: 12.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

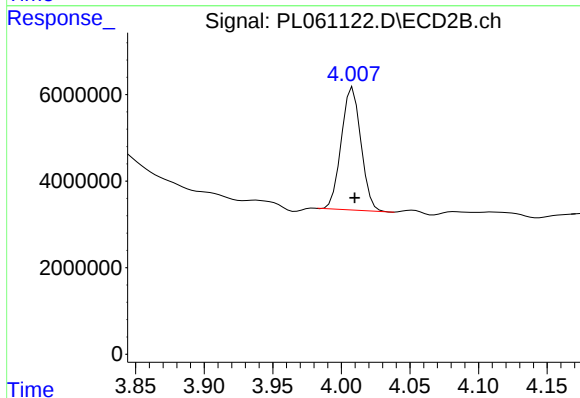


#1 Tetrachloro-m-xylene

R.T.: 4.008 min
Delta R.T.: -0.001 min
Response: 28352646
Conc: 10.91 ng/ml

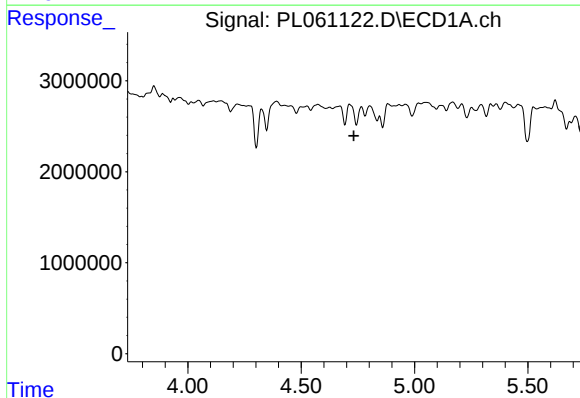


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.732 min
Response: 0
Conc: N.D.

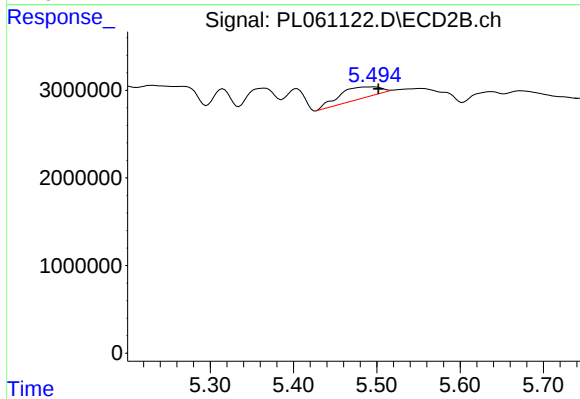

#5 Aldrin


R.T.: 5.497 min
Delta R.T.: -0.005 min
Response: 4462044
Conc: 1.32 ng/ml

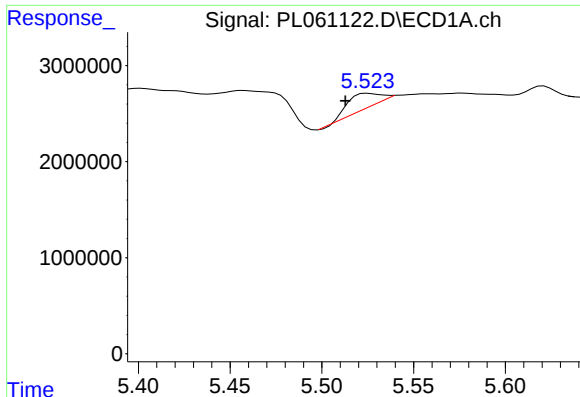

#9 Endosulfan I


R.T.: 5.525 min
Delta R.T.: 0.012 min
Response: 1735735
Conc: 0.96 ng/ml

Instrument :
ECD_L
ClientSampleId :

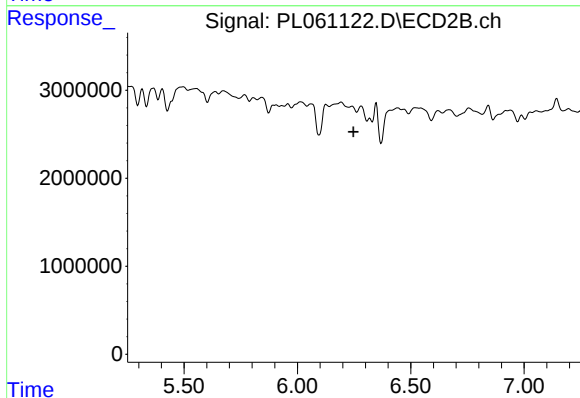


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.248 min
Response: 0
Conc: N.D.

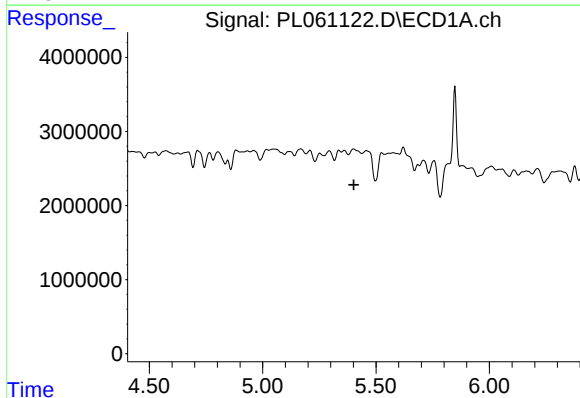


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.402 min
Response: 0
Conc: N.D.

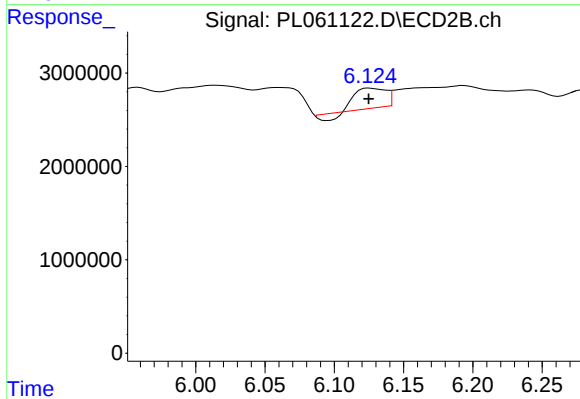

#10 gamma-Chlordane


R.T.: 6.125 min
Delta R.T.: 0.000 min
Response: 2784495
Conc: 0.90 ng/ml

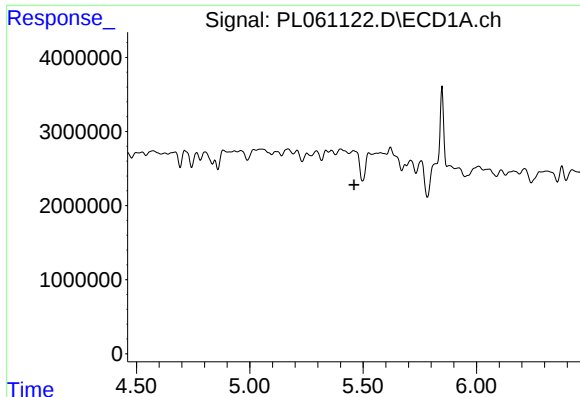

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.460 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

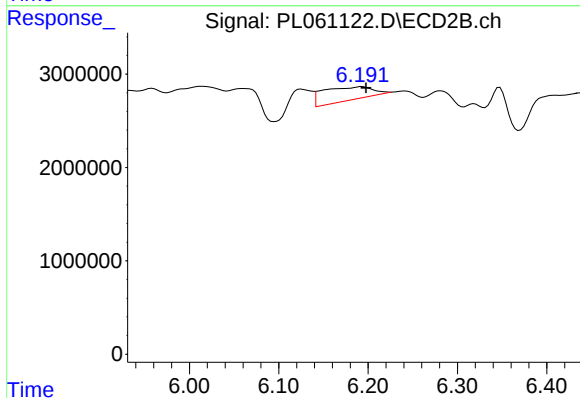


#11 alpha-Chlordane

R.T.: 6.193 min
Delta R.T.: -0.005 min
Response: 5533494
Conc: 1.78 ng/ml

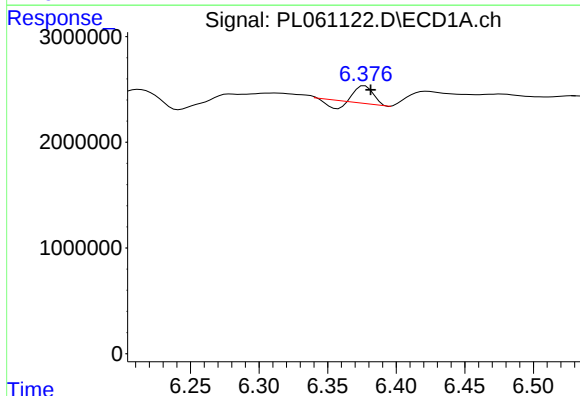


#17 4,4'-DDT

R.T.: 6.377 min
Delta R.T.: -0.004 min
Response: 1086156
Conc: 0.72 ng/ml

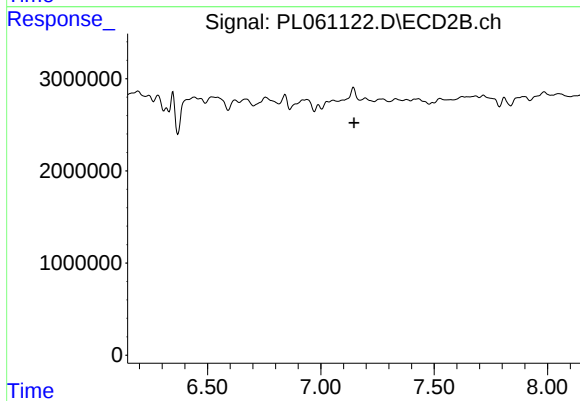

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.147 min
Response: 0
Conc: N.D.

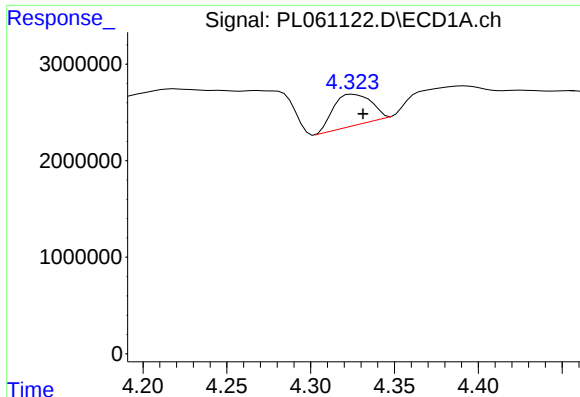

#23 Chlordane-1


R.T.: 4.325 min
Delta R.T.: -0.006 min
Response: 5047923
Conc: 82.67 ng/ml

Instrument :
ECD_L
ClientSampleId :

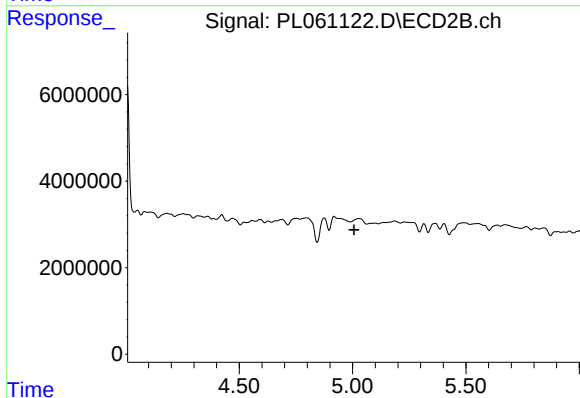


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.007 min
Response: 0
Conc: N.D.

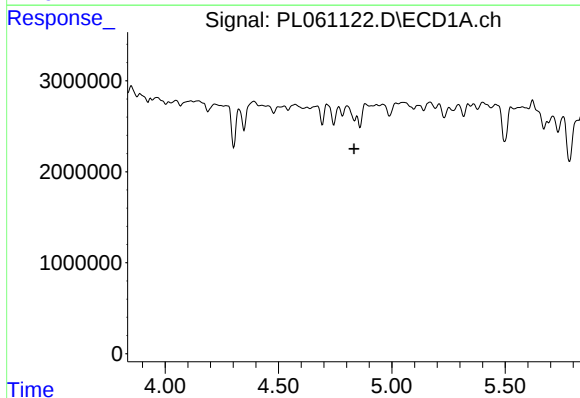


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.833 min
Response: 0
Conc: N.D.

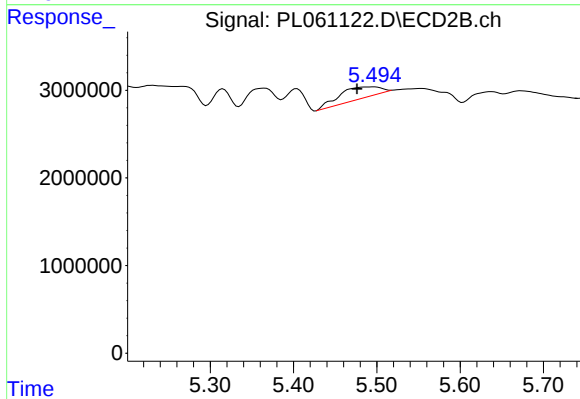

#24 Chlordane-2


R.T.: 5.497 min
Delta R.T.: 0.020 min
Response: 4462044
Conc: 43.36 ng/ml

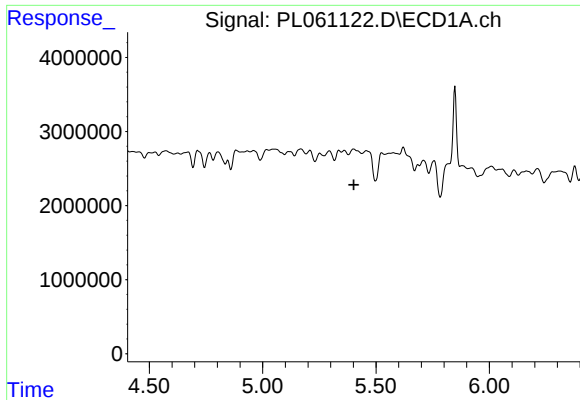

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 5.402 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

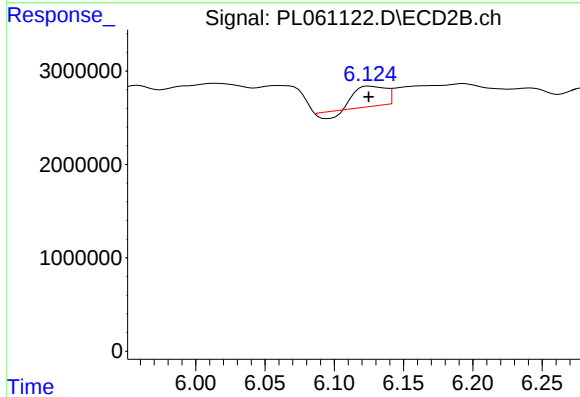


#25 Chlordane-3

R.T.: 6.125 min
Delta R.T.: 0.000 min
Response: 2784495
Conc: 6.97 ng/ml

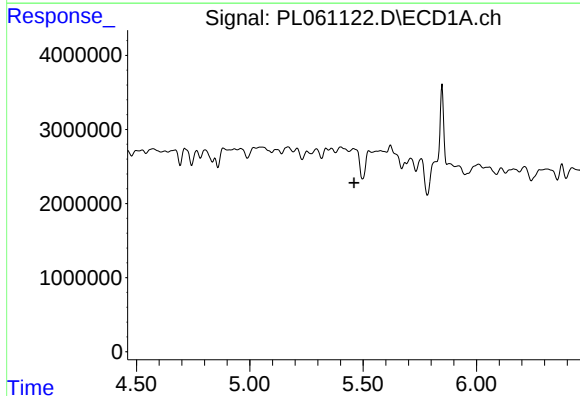


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.460 min
Response: 0
Conc: N.D.

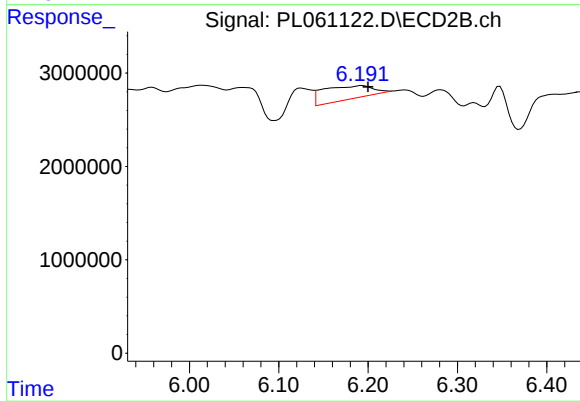

#26 Chlordane-4


R.T.: 6.193 min
Delta R.T.: -0.007 min
Response: 5533494
Conc: 11.51 ng/ml

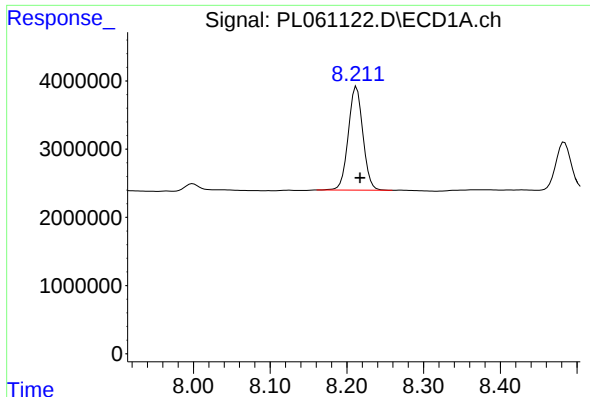

#28 Decachlorobiphenyl

R.T.: 8.213 min
Delta R.T.: -0.005 min
Response: 20228691
Conc: 12.01 ng/ml

Instrument :
ECD_L
ClientSampleId :

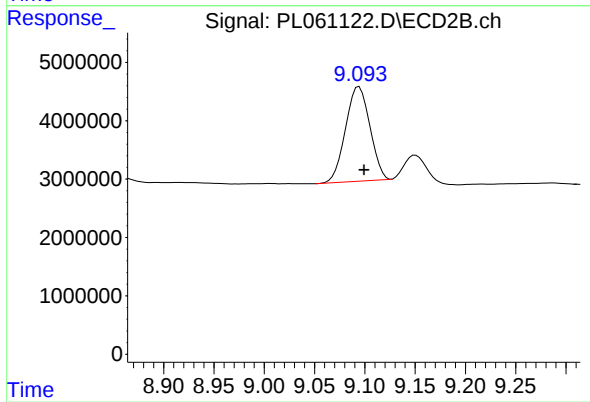

#28 Decachlorobiphenyl

R.T.: 9.094 min
Delta R.T.: -0.005 min
Response: 27238944
Conc: 12.91 ng/ml