

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090120\
 Data File : PL061123.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Sep 2020 10:11
 Operator : DD\AJ
 Sample : L3847-07
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 14:49:59 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 25 16:59:57 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.460	4.008	24666498	29187579	13.367	11.230
28)	SA Decachlor...	8.212	9.095	24240060	30016792	14.389	14.226
Target Compounds							
5)	MB Aldrin	4.721	5.496	5437361	5447049	2.606	1.616 #
6)	B beta-BHC	0.000	4.876f	0	313508	N.D.	0.211 #
8)	B Heptachlo...	5.168	0.000	5842092	0	2.963	N.D. #
9)	A Endosulfan I	5.526	0.000	1142732	0	0.629	N.D. #
11)	B alpha-Chl...	0.000	6.178f	0	5462497	N.D.	1.757 #
13)	MA Dieldrin	5.757	0.000	3982897	0	2.070	N.D. #
15)	B Endosulfa...	6.315f	0.000	9596956	0	5.377	N.D. #
17)	MA 4,4'-DDT	6.377	0.000	598142	0	0.396	N.D. #
23)	Chlordane-1	4.326	5.026f	4913267	3059409	80.469	25.163 #
24)	Chlordane-2	0.000	5.496f	0	5447049	N.D.	52.930 #
26)	Chlordane-4	0.000	6.178f	0	5462497	N.D.	11.363 #
27)	Chlordane-5	6.315f	0.000	9596956	0	153.366	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090120\
Data File : PL061123.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Sep 2020 10:11
Operator : DD\AJ
Sample : L3847-07
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 14:49:59 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
Quant Title : GC Extractables
QLast Update : Tue Aug 25 16:59:57 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

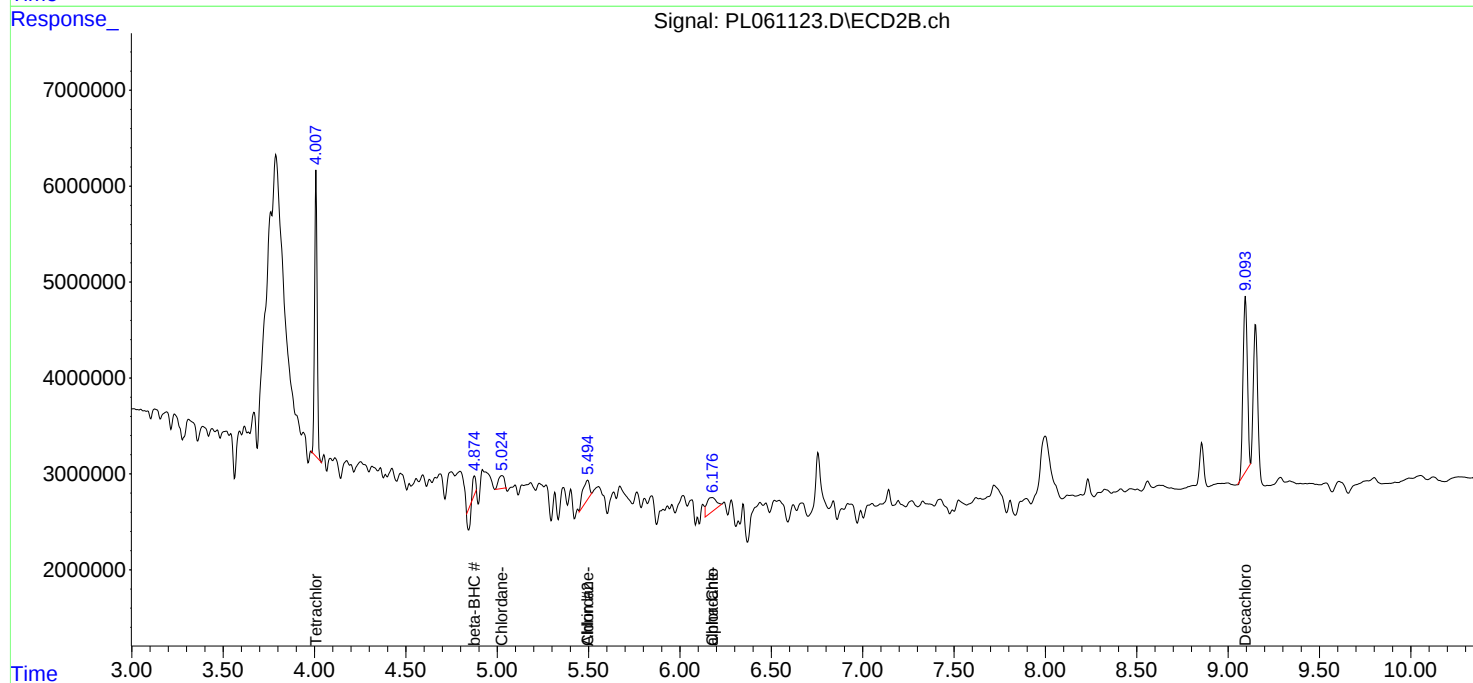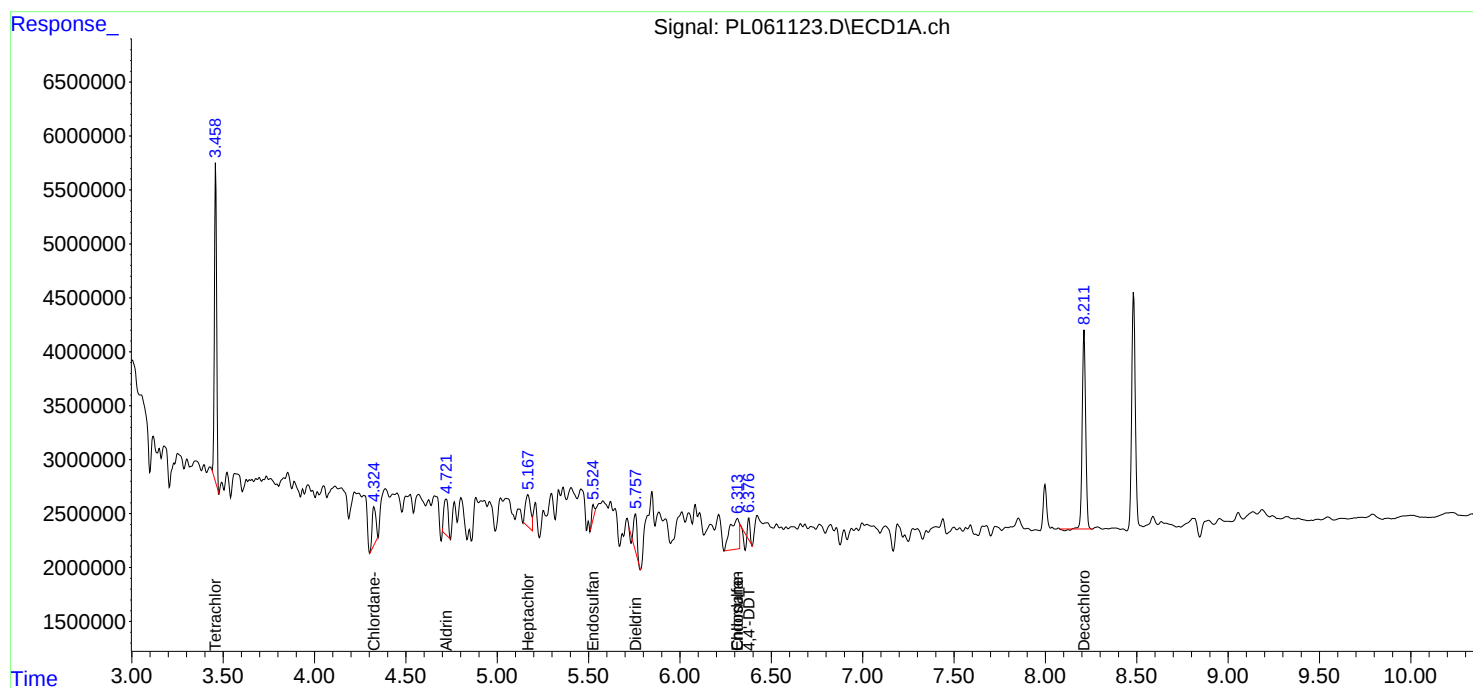


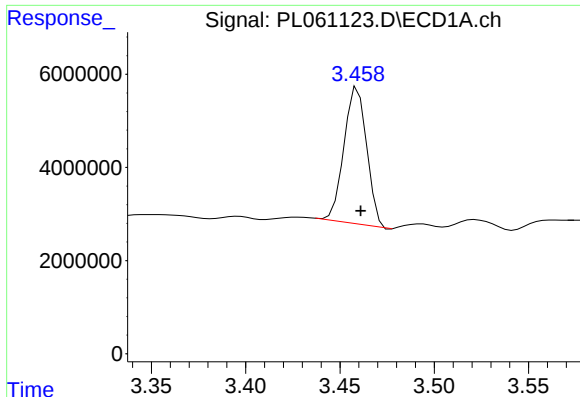

#1 Tetrachloro-m-xylene


R.T.: 3.460 min
Delta R.T.: -0.001 min
Response: 24666498
Conc: 13.37 ng/ml

Instrument :
ECD_L
ClientSampleId :

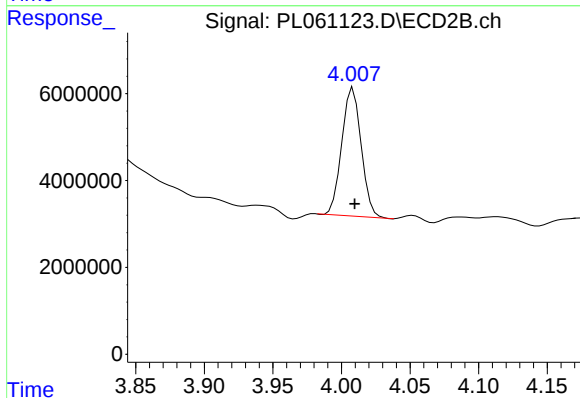


#1 Tetrachloro-m-xylene

R.T.: 4.008 min
Delta R.T.: -0.001 min
Response: 29187579
Conc: 11.23 ng/ml

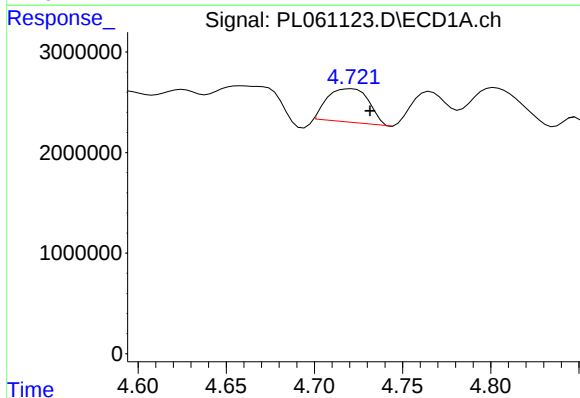


#5 Aldrin

R.T.: 4.721 min
Delta R.T.: -0.010 min
Response: 5437361
Conc: 2.61 ng/ml

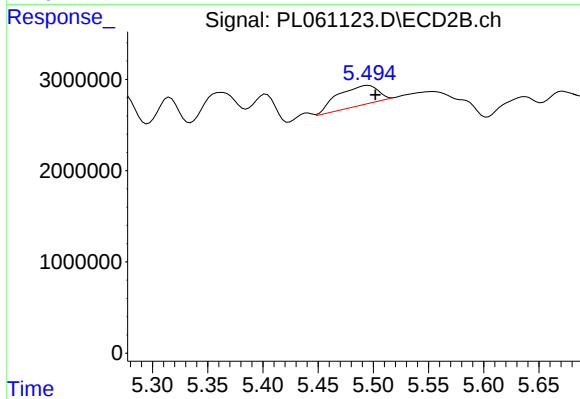

#5 Aldrin


R.T.: 5.496 min
Delta R.T.: -0.006 min
Response: 5447049
Conc: 1.62 ng/ml

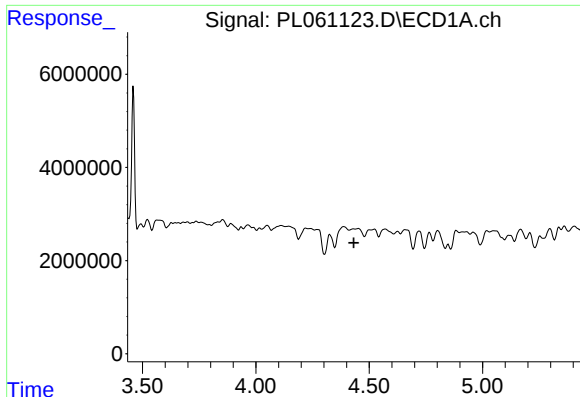

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.432 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

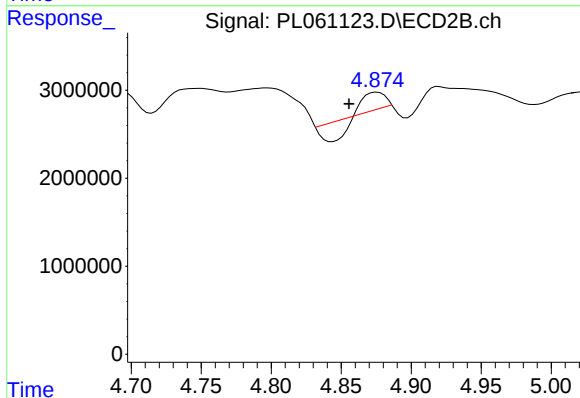


#6 beta-BHC

R.T.: 4.876 min
Delta R.T.: 0.020 min
Response: 313508
Conc: 0.21 ng/ml

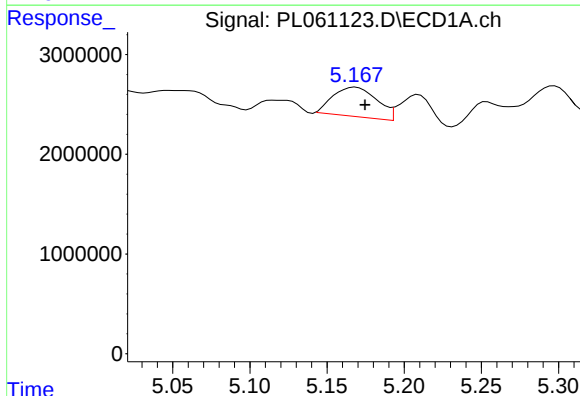


#8 Heptachlor epoxide

R.T.: 5.168 min
Delta R.T.: -0.006 min
Response: 5842092
Conc: 2.96 ng/ml

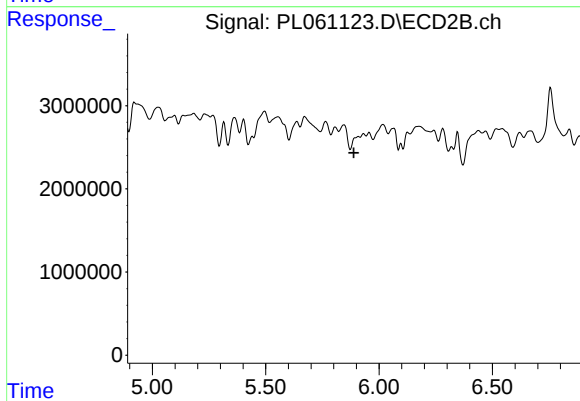

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.889 min
Response: 0
Conc: N.D.

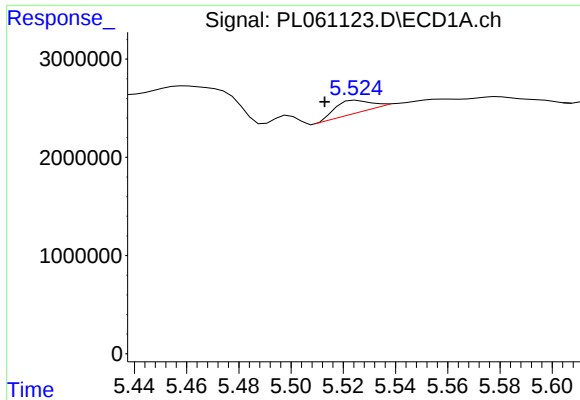

#9 Endosulfan I


R.T.: 5.526 min
Delta R.T.: 0.013 min
Response: 1142732
Conc: 0.63 ng/ml

Instrument :
ECD_L
ClientSampleId :

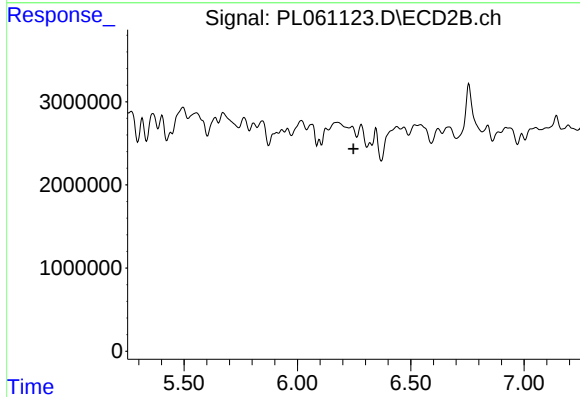


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.248 min
Response: 0
Conc: N.D.

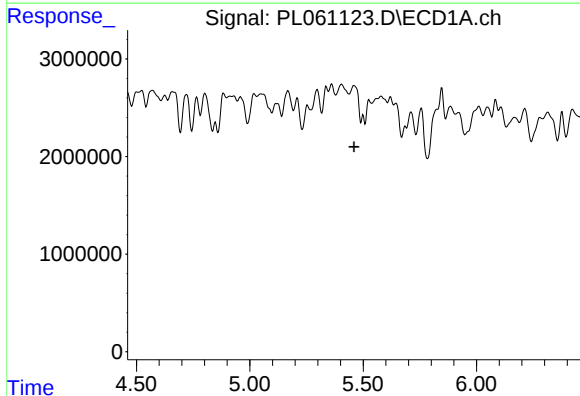


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.460 min
Response: 0
Conc: N.D.

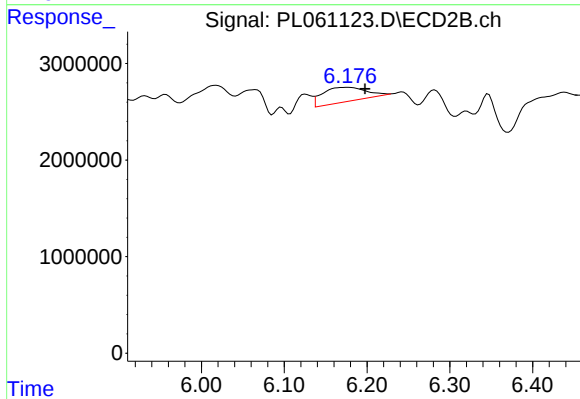

#11 alpha-Chlordane


R.T.: 6.178 min
Delta R.T.: -0.020 min
Response: 5462497
Conc: 1.76 ng/ml

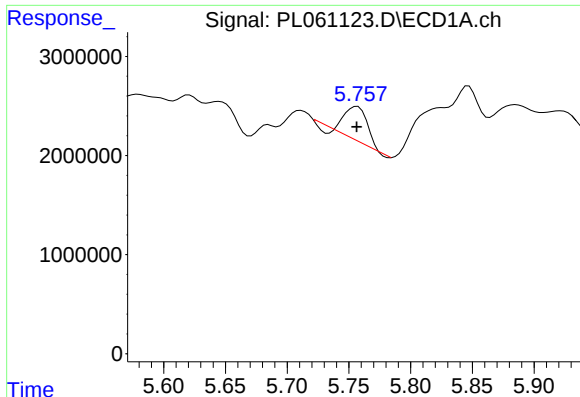

#13 Dieldrin


R.T.: 5.757 min
Delta R.T.: 0.000 min
Response: 3982897
Conc: 2.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

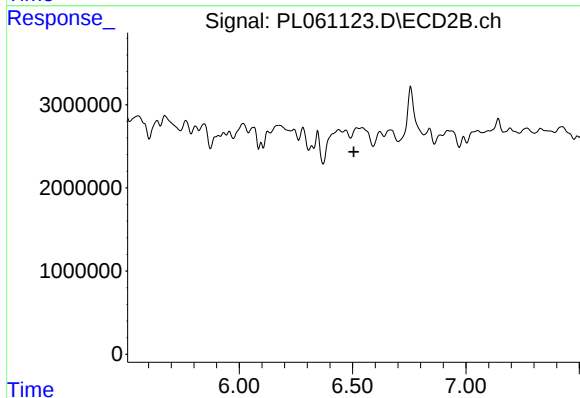


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.506 min
Response: 0
Conc: N.D.

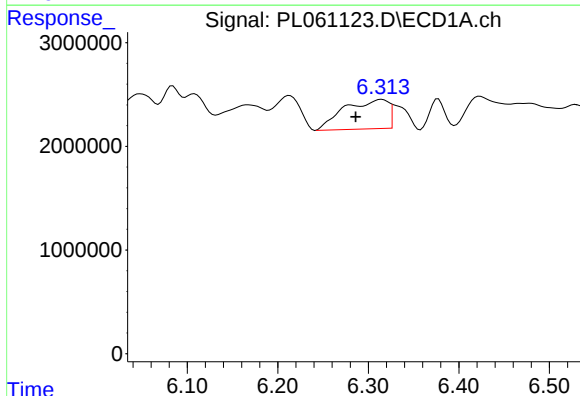


#15 Endosulfan II

R.T.: 6.315 min
Delta R.T.: 0.028 min
Response: 9596956
Conc: 5.38 ng/ml

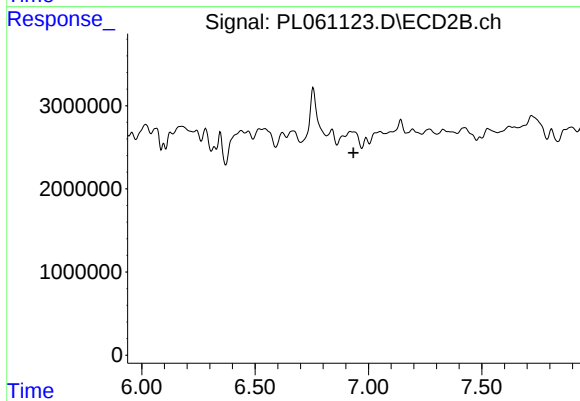

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.934 min
Response: 0
Conc: N.D.

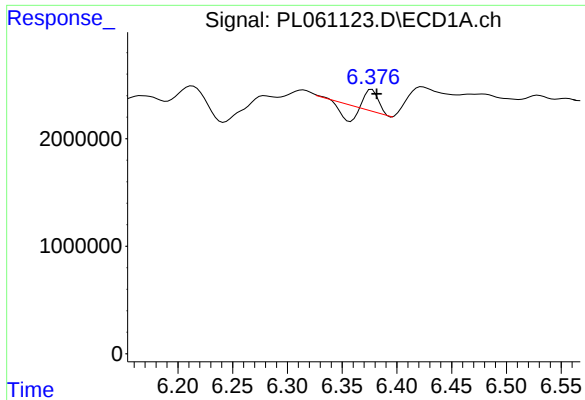

#17 4,4'-DDT


R.T.: 6.377 min
Delta R.T.: -0.004 min
Response: 598142
Conc: 0.40 ng/ml

Instrument :
ECD_L
ClientSampleId :

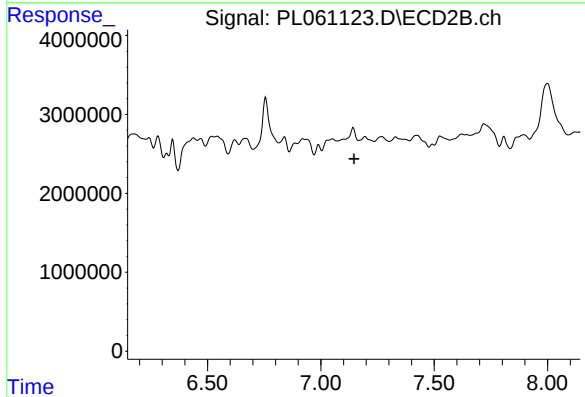


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.147 min
Response: 0
Conc: N.D.

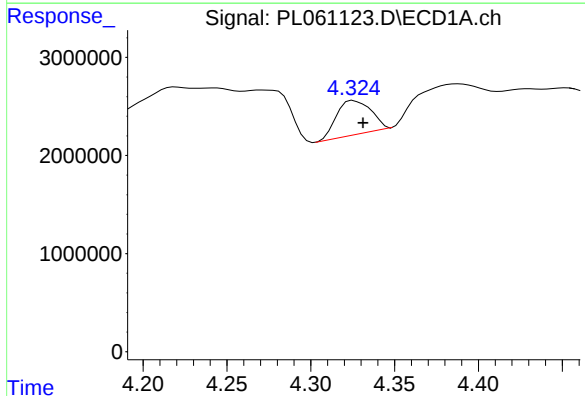


#23 Chlordane-1

R.T.: 4.326 min
Delta R.T.: -0.006 min
Response: 4913267
Conc: 80.47 ng/ml

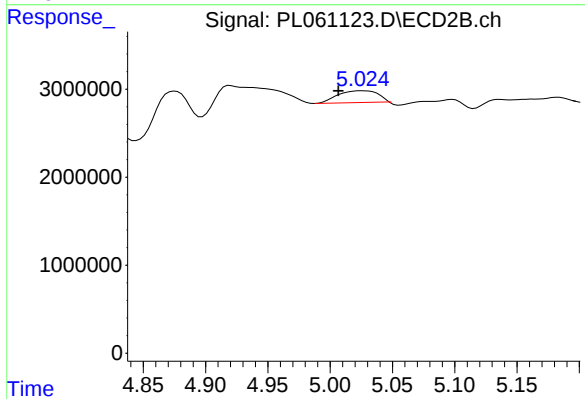

#23 Chlordane-1


R.T.: 5.026 min
Delta R.T.: 0.019 min
Response: 3059409
Conc: 25.16 ng/ml

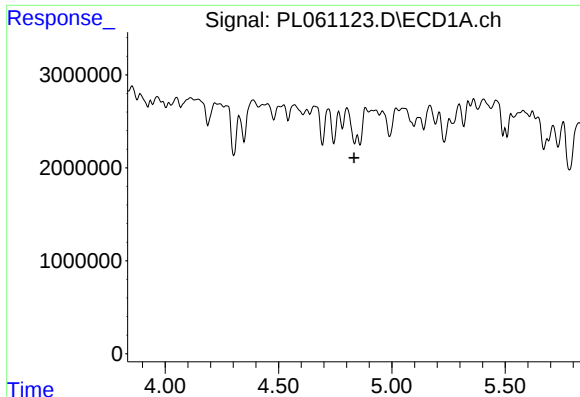

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.833 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

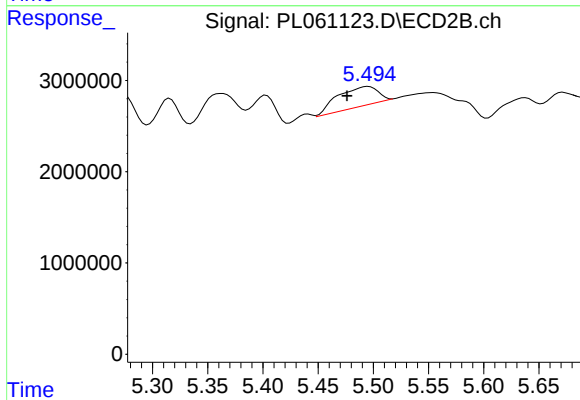


#24 Chlordane-2

R.T.: 5.496 min
Delta R.T.: 0.019 min
Response: 5447049
Conc: 52.93 ng/ml

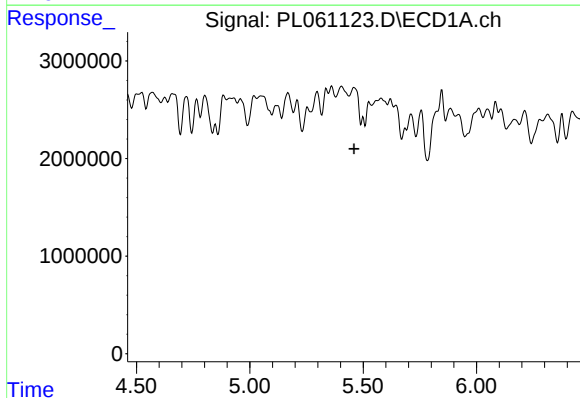


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.460 min
Response: 0
Conc: N.D.

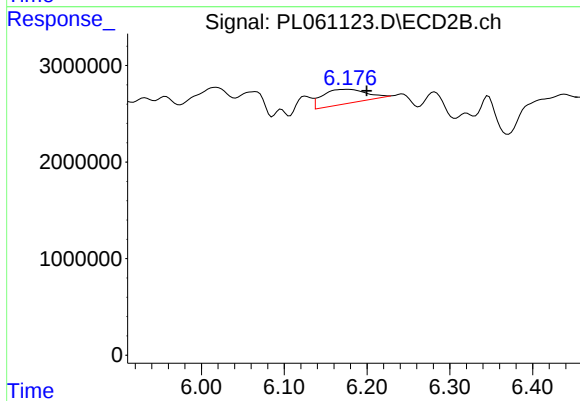

#26 Chlordane-4


R.T.: 6.178 min
Delta R.T.: -0.022 min
Response: 5462497
Conc: 11.36 ng/ml

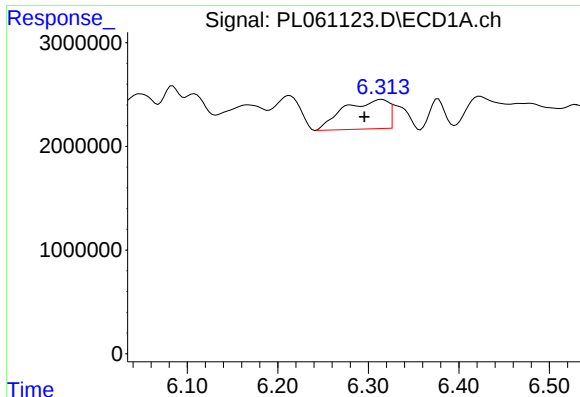

#27 Chlordane-5


R.T.: 6.315 min
Delta R.T.: 0.019 min
Response: 9596956
Conc: 153.37 ng/ml

Instrument :
ECD_L
ClientSampleId :

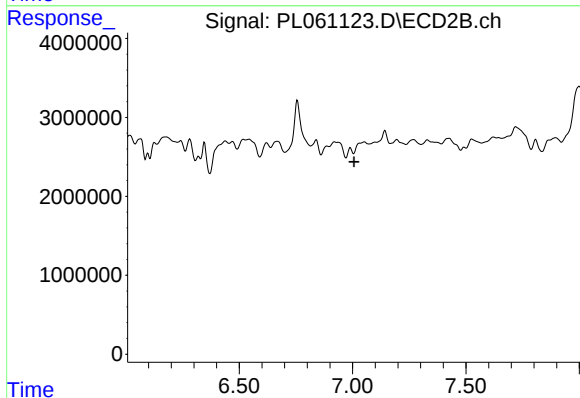


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 7.007 min
Response: 0
Conc: N.D.

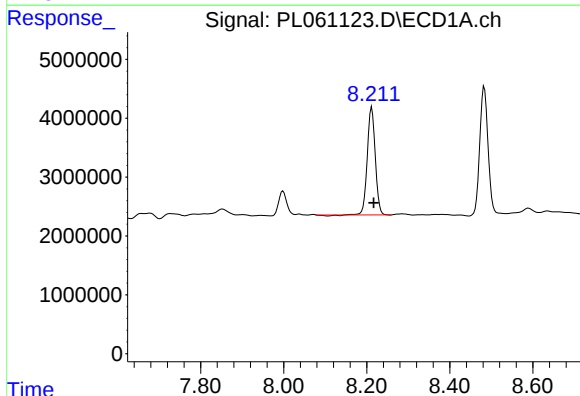

#28 Decachlorobiphenyl

R.T.: 8.212 min
Delta R.T.: -0.005 min
Response: 24240060
Conc: 14.39 ng/ml

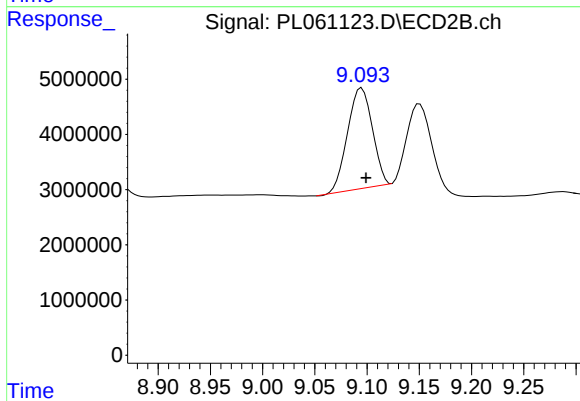

#28 Decachlorobiphenyl

R.T.: 9.095 min
Delta R.T.: -0.004 min
Response: 30016792
Conc: 14.23 ng/ml