

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090120\
 Data File : PL061125.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Sep 2020 10:40
 Operator : DD\AJ
 Sample : L3847-19
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 14:50:23 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 25 16:59:57 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.460	4.008	25548659	34202626	13.845	13.160
28)	SA Decachlor...	8.212	9.095	20669014	29197266	12.269	13.837
Target Compounds							
12)	B 4,4'-DDE	5.622	6.351	10727302	14740165	5.830	5.100
17)	MA 4,4'-DDT	6.378	7.143	7099027	10998351	4.696	4.776



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090120\
Data File : PL061125.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Sep 2020 10:40
Operator : DD\AJ
Sample : L3847-19
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 14:50:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
Quant Title : GC Extractables
QLast Update : Tue Aug 25 16:59:57 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

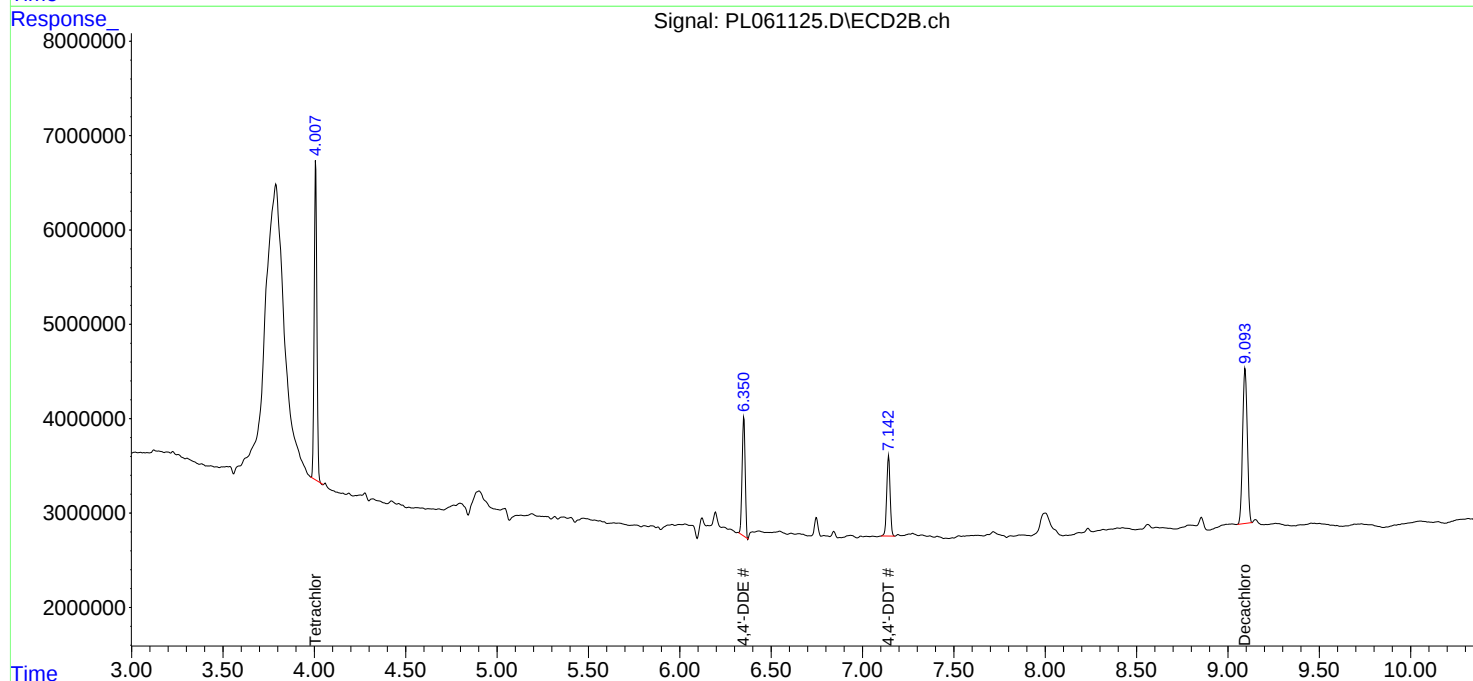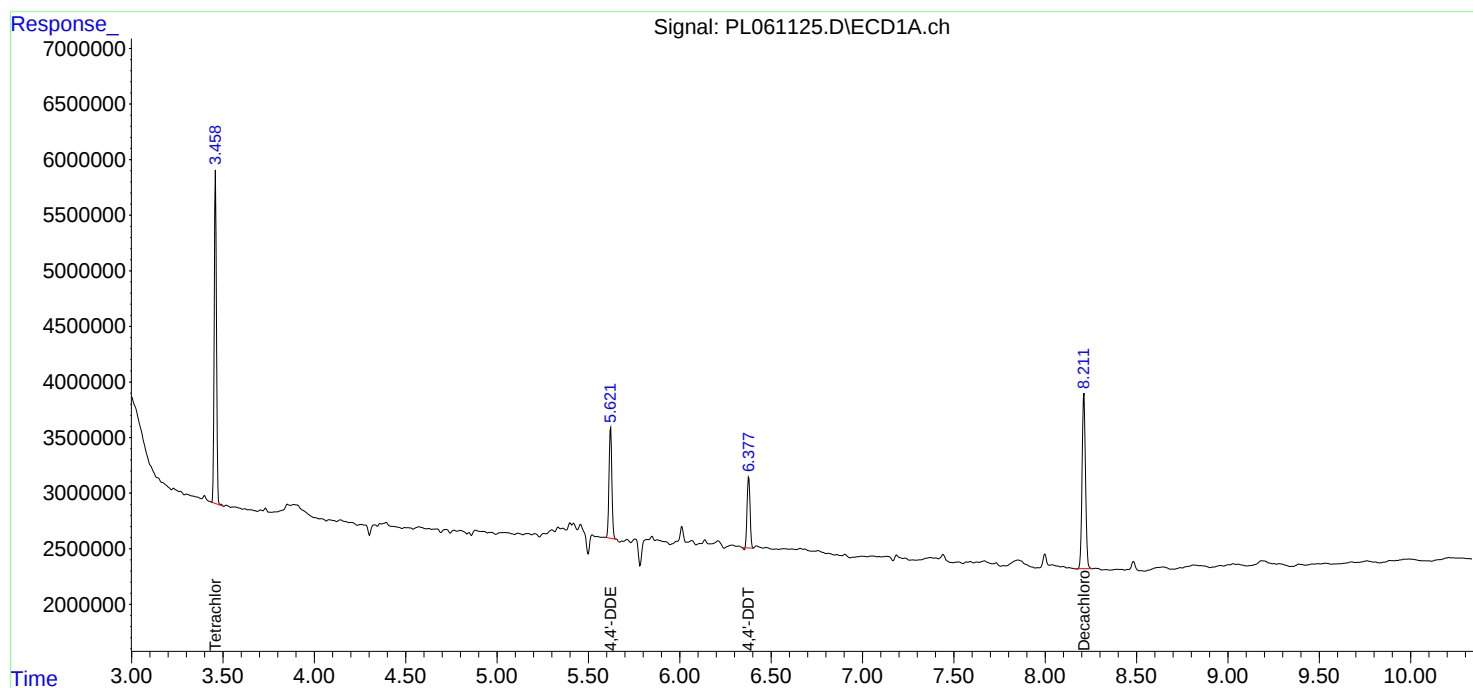


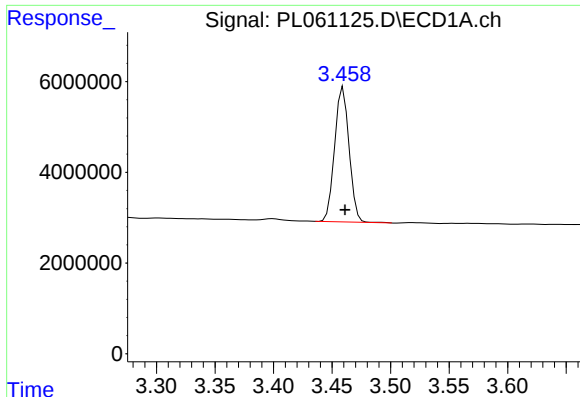

#1 Tetrachloro-m-xylene


R.T.: 3.460 min
Delta R.T.: -0.001 min
Response: 25548659
Conc: 13.84 ng/ml

Instrument :
ECD_L
ClientSampleId :

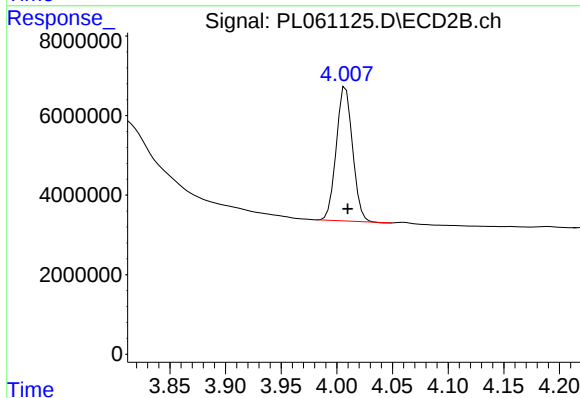


#1 Tetrachloro-m-xylene

R.T.: 4.008 min
Delta R.T.: -0.002 min
Response: 34202626
Conc: 13.16 ng/ml

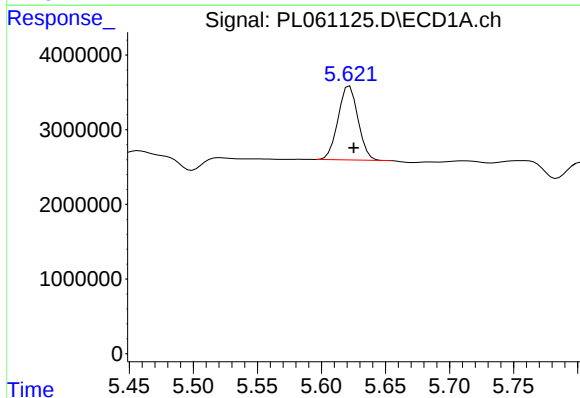


#12 4,4'-DDE

R.T.: 5.622 min
Delta R.T.: -0.003 min
Response: 10727302
Conc: 5.83 ng/ml

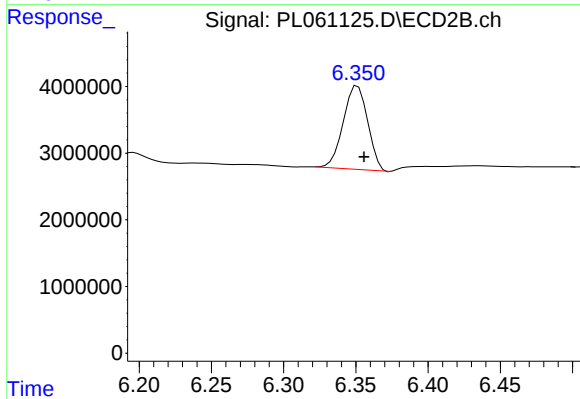

#12 4,4'-DDE


R.T.: 6.351 min
Delta R.T.: -0.004 min
Response: 14740165
Conc: 5.10 ng/ml

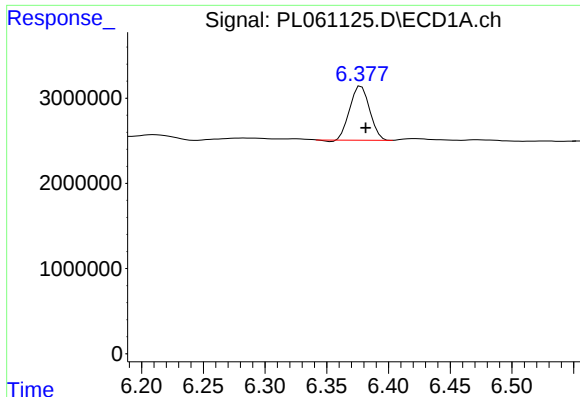

#17 4,4'-DDT


R.T.: 6.378 min
Delta R.T.: -0.004 min
Response: 7099027
Conc: 4.70 ng/ml

Instrument :
ECD_L
ClientSampleId :

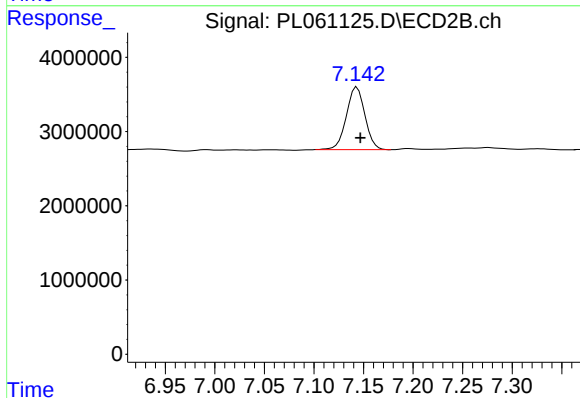


#17 4,4'-DDT

R.T.: 7.143 min
Delta R.T.: -0.003 min
Response: 10998351
Conc: 4.78 ng/ml

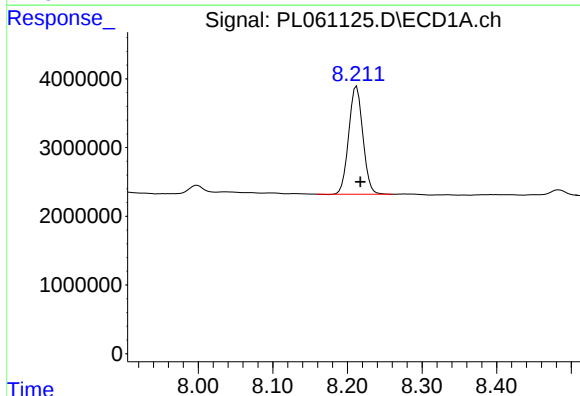

#28 Decachlorobiphenyl

R.T.: 8.212 min
Delta R.T.: -0.005 min
Response: 20669014
Conc: 12.27 ng/ml

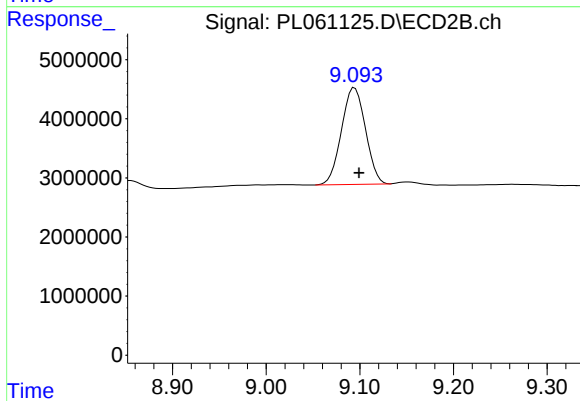

#28 Decachlorobiphenyl

R.T.: 9.095 min
Delta R.T.: -0.005 min
Response: 29197266
Conc: 13.84 ng/ml