

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090120\
 Data File : PL061126.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Sep 2020 10:54
 Operator : DD\AJ
 Sample : L3847-25
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 14:50:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 25 16:59:57 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.460	4.008	26058069	35239636	14.121	13.559
28)	SA Decachlor...	8.213	9.095	21297253	29555773	12.642	14.007
Target Compounds							
6)	B beta-BHC	0.000	4.882f	0	67514	N.D.	0.045 #
23)	Chlordane-1	4.326	0.000	4129140	0	67.627	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090120\
Data File : PL061126.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Sep 2020 10:54
Operator : DD\AJ
Sample : L3847-25
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 14:50:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
Quant Title : GC Extractables
QLast Update : Tue Aug 25 16:59:57 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

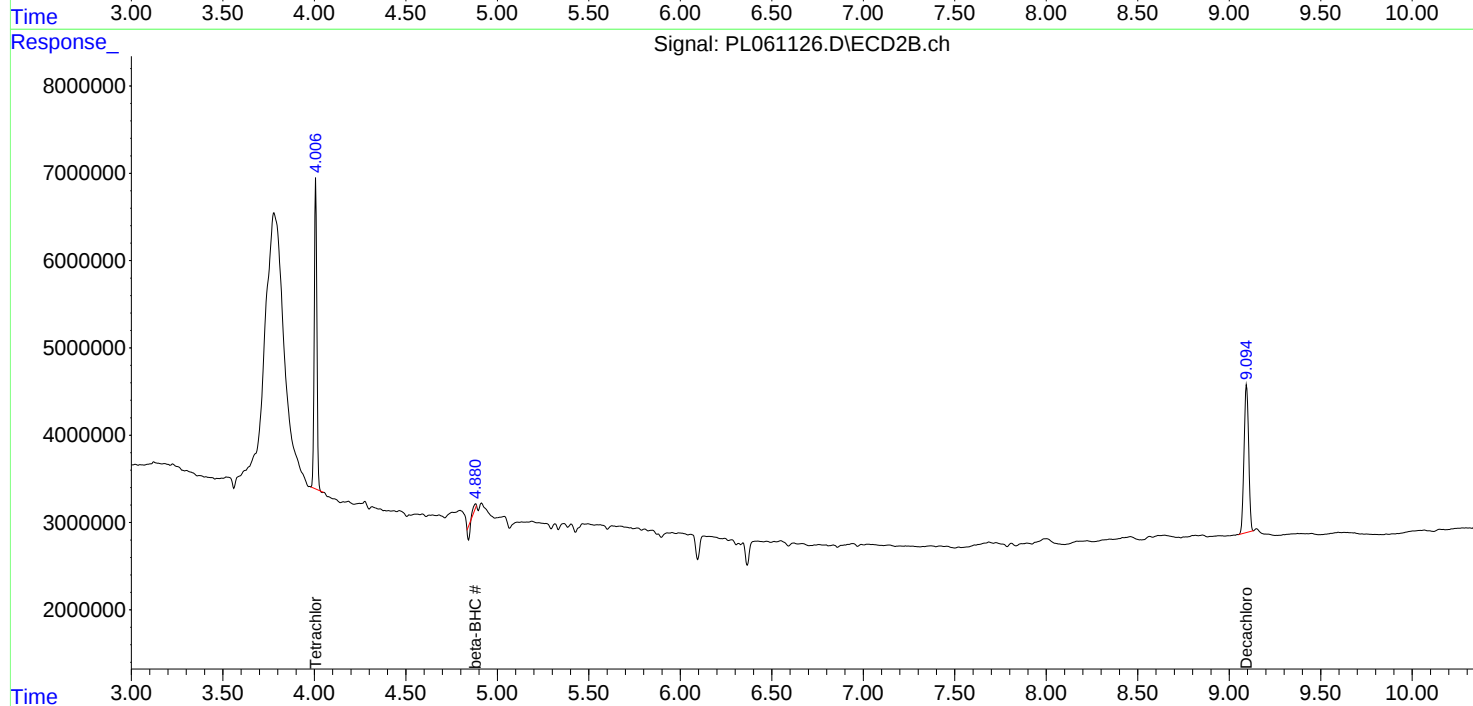


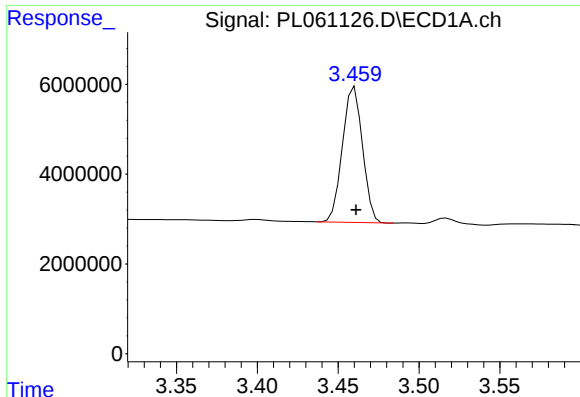

#1 Tetrachloro-m-xylene


R.T.: 3.460 min
Delta R.T.: 0.000 min
Response: 26058069
Conc: 14.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

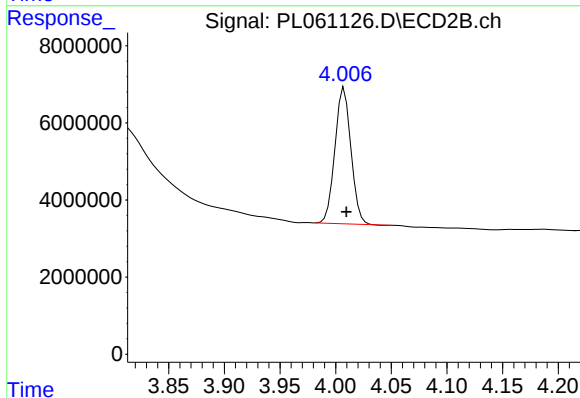


#1 Tetrachloro-m-xylene

R.T.: 4.008 min
Delta R.T.: -0.002 min
Response: 35239636
Conc: 13.56 ng/ml

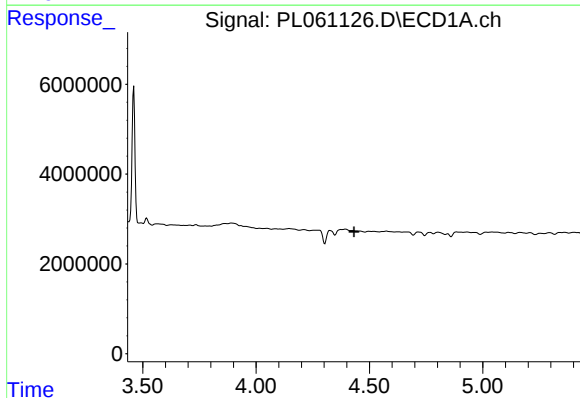


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.432 min
Response: 0
Conc: N.D.

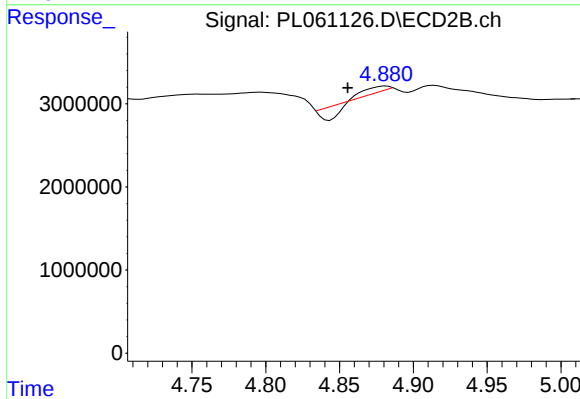

#6 beta-BHC


R.T.: 4.882 min
Delta R.T.: 0.026 min
Response: 67514
Conc: 0.05 ng/ml

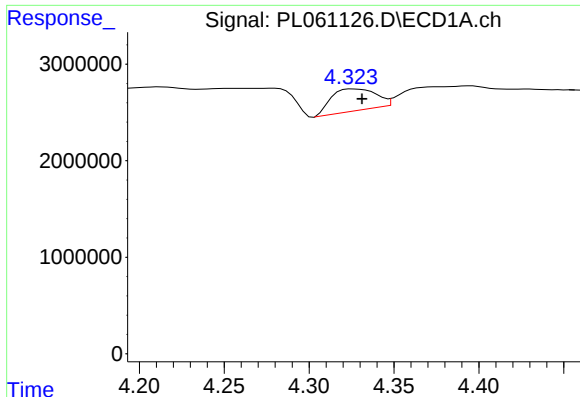

#23 Chlordane-1


R.T.: 4.326 min
Delta R.T.: -0.006 min
Response: 4129140
Conc: 67.63 ng/ml

Instrument :
ECD_L
ClientSampleId :

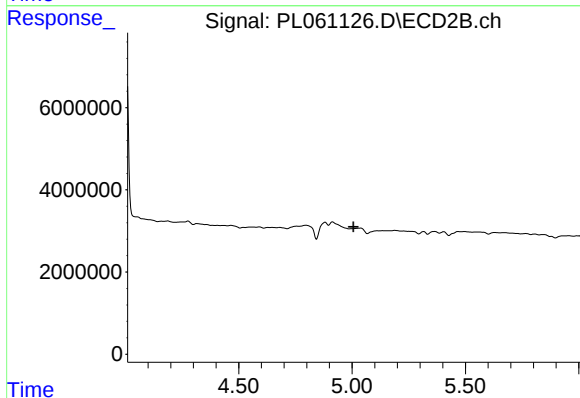


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.007 min
Response: 0
Conc: N.D.

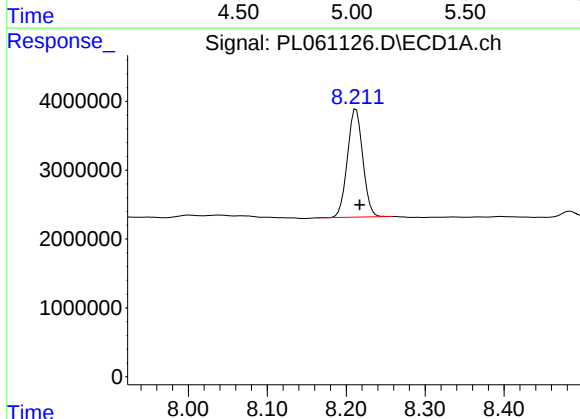

#28 Decachlorobiphenyl

R.T.: 8.213 min
Delta R.T.: -0.005 min
Response: 21297253
Conc: 12.64 ng/ml

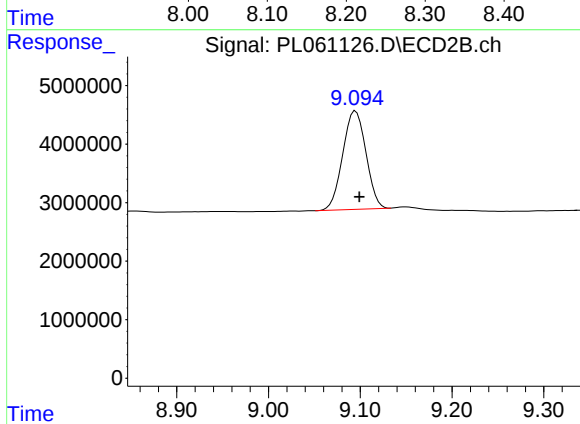

#28 Decachlorobiphenyl

R.T.: 9.095 min
Delta R.T.: -0.004 min
Response: 29555773
Conc: 14.01 ng/ml