

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090120\
 Data File : PL061134.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Sep 2020 12:46
 Operator : DD\AJ
 Sample : L3837-20
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 14:52:04 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 25 16:59:57 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.460	4.008	41925374	58020725	22.719	22.324
28)	SA Decachlor...	8.211	9.094	31820875	42947595	18.889	20.354
Target Compounds							
2)	A alpha-BHC	0.000	4.403	0	6381911	N.D.	1.571 #
3)	MA gamma-BHC...	4.201f	0.000	6155118	0	2.411	N.D. #
9)	A Endosulfan I	5.531f	0.000	12386608	0	6.817	N.D. #
11)	B alpha-Chl...	0.000	6.171f	0	5417667	N.D.	1.743 #
13)	MA Dieldrin	5.752	0.000	7528993	0	3.912	N.D. #
23)	Chlordane-1	4.318	0.000	2638371	0	43.211	N.D. #
24)	Chlordane-2	4.844	0.000	3420136	0	53.180	N.D. #
26)	Chlordane-4	0.000	6.171f	0	5417667	N.D.	11.270 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090120\
Data File : PL061134.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Sep 2020 12:46
Operator : DD\AJ
Sample : L3837-20
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 14:52:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
Quant Title : GC Extractables
QLast Update : Tue Aug 25 16:59:57 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

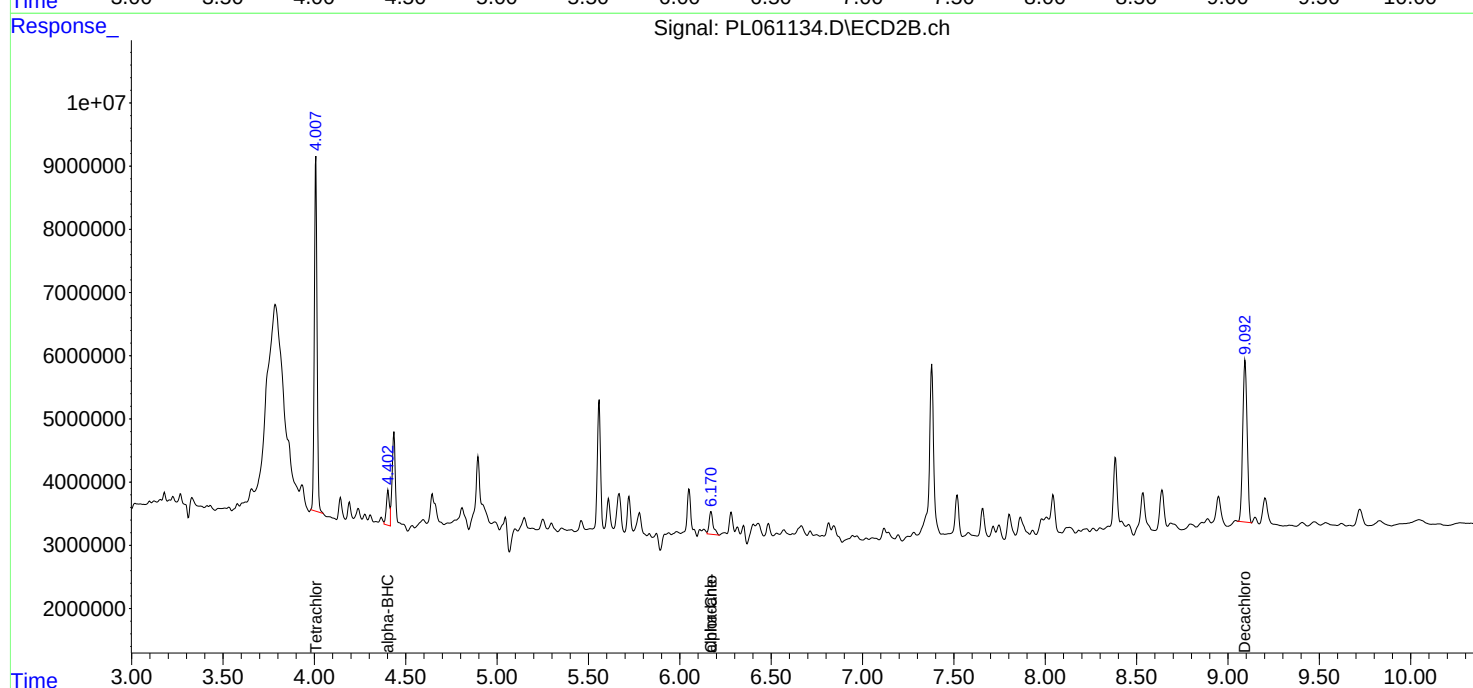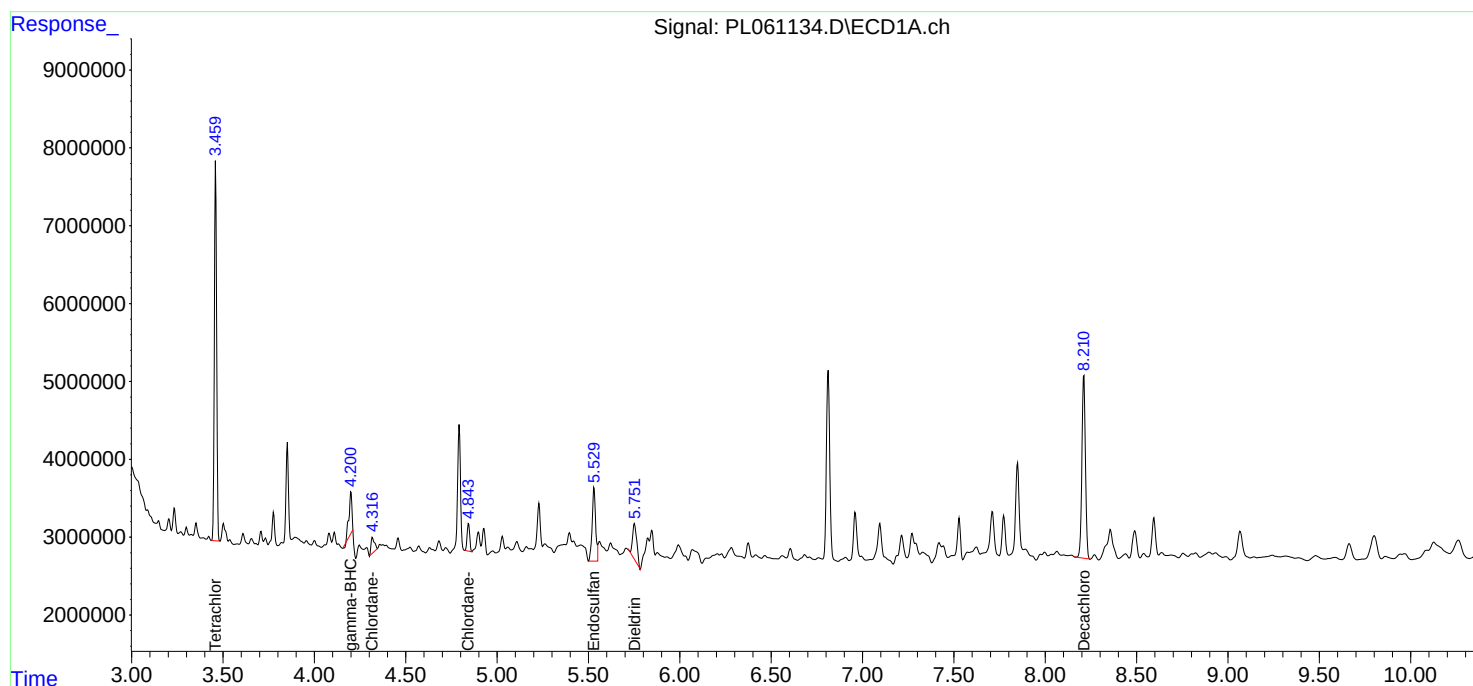


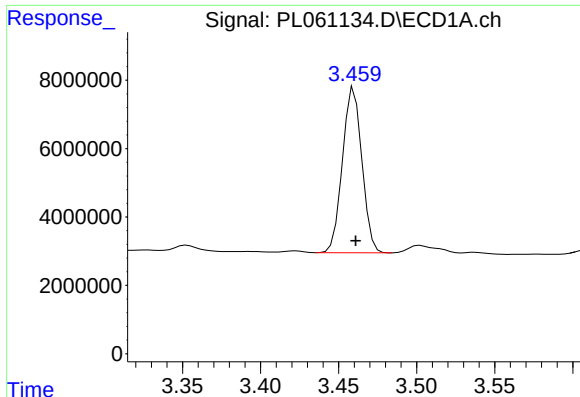

#1 Tetrachloro-m-xylene


R.T.: 3.460 min
Delta R.T.: 0.000 min
Response: 41925374
Conc: 22.72 ng/ml

Instrument :
ECD_L
ClientSampleId :

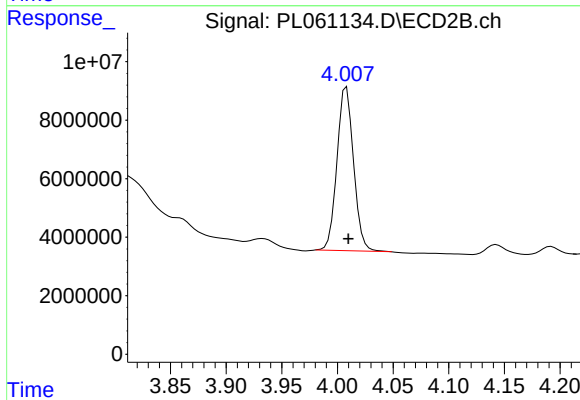


#1 Tetrachloro-m-xylene

R.T.: 4.008 min
Delta R.T.: -0.002 min
Response: 58020725
Conc: 22.32 ng/ml

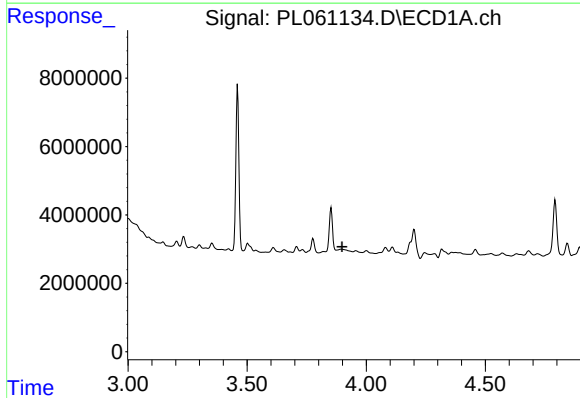


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.898 min
Response: 0
Conc: N.D.

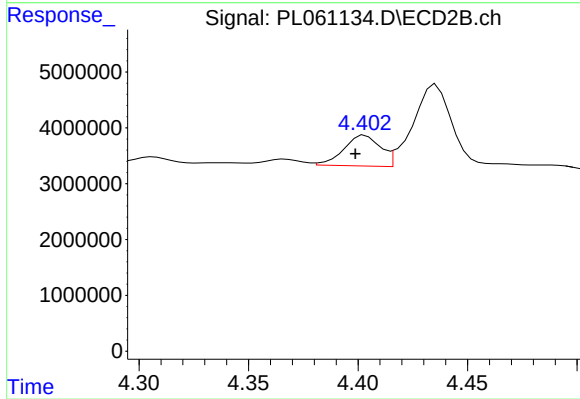

#2 alpha-BHC


R.T.: 4.403 min
Delta R.T.: 0.005 min
Response: 6381911
Conc: 1.57 ng/ml

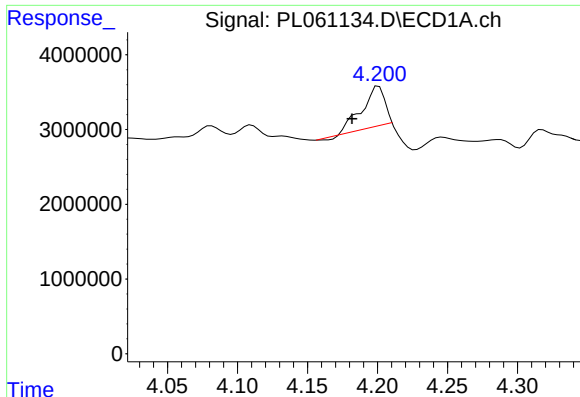

#3 gamma-BHC (Lindane)


R.T.: 4.201 min
Delta R.T.: 0.019 min
Response: 6155118
Conc: 2.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

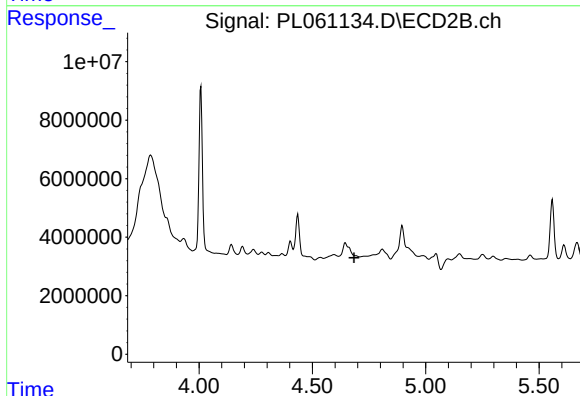


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.685 min
Response: 0
Conc: N.D.

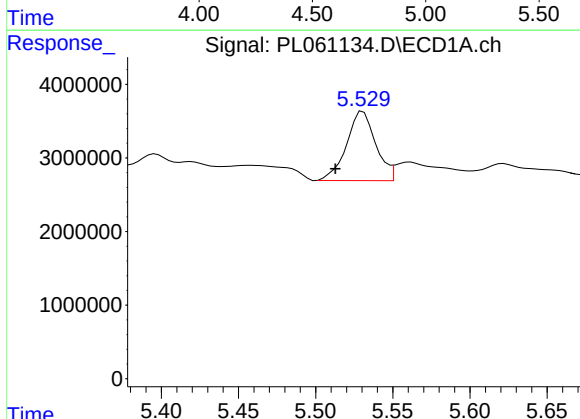


#9 Endosulfan I

R.T.: 5.531 min
Delta R.T.: 0.018 min
Response: 12386608
Conc: 6.82 ng/ml

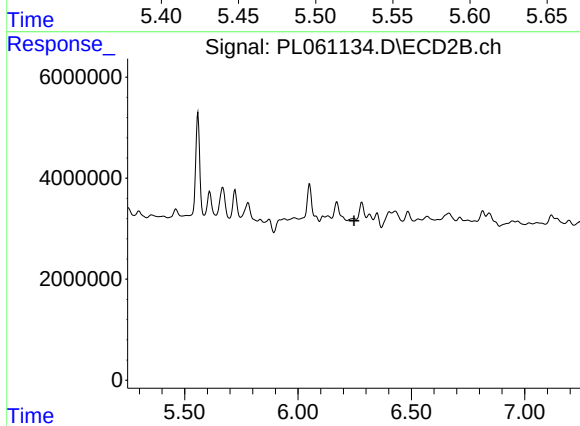

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.248 min
Response: 0
Conc: N.D.

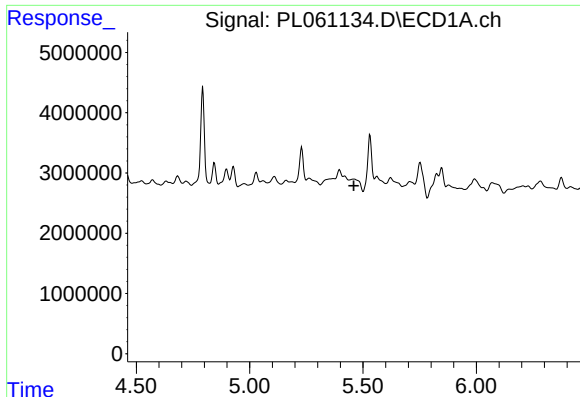

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.460 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

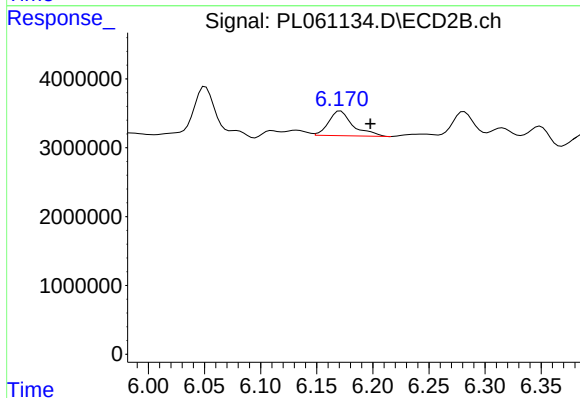


#11 alpha-Chlordane

R.T.: 6.171 min
Delta R.T.: -0.027 min
Response: 5417667
Conc: 1.74 ng/ml

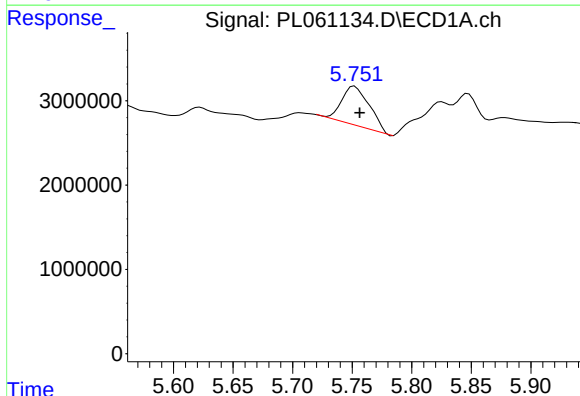


#13 Dieldrin

R.T.: 5.752 min
Delta R.T.: -0.004 min
Response: 7528993
Conc: 3.91 ng/ml

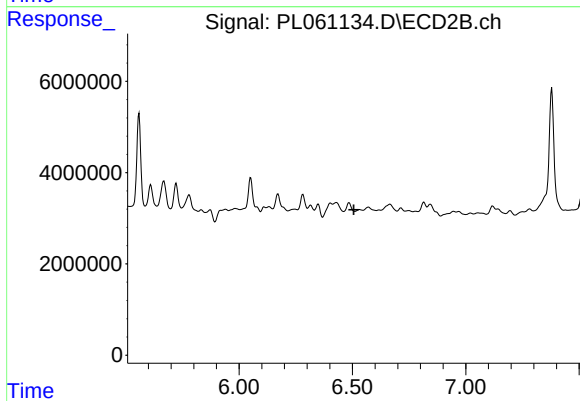

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.506 min
Response: 0
Conc: N.D.

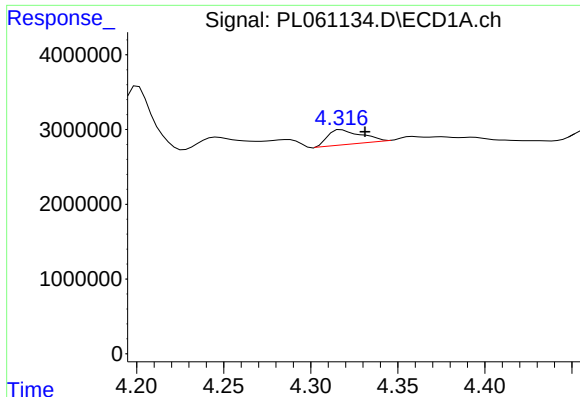

#23 Chlordane-1


R.T.: 4.318 min
Delta R.T.: -0.013 min
Response: 2638371
Conc: 43.21 ng/ml

Instrument :
ECD_L
ClientSampleId :

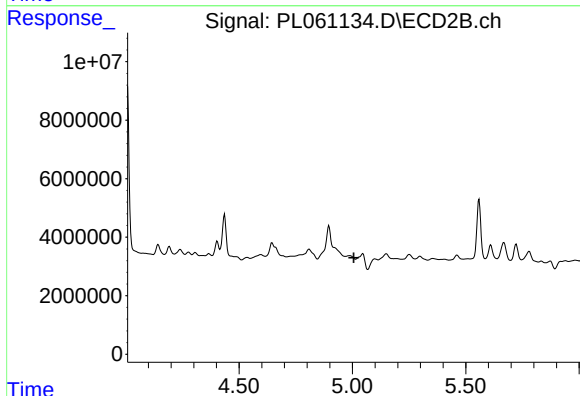


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.007 min
Response: 0
Conc: N.D.

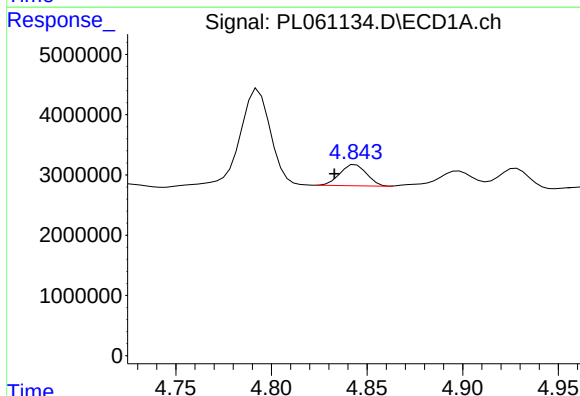


#24 Chlordane-2

R.T.: 4.844 min
Delta R.T.: 0.011 min
Response: 3420136
Conc: 53.18 ng/ml

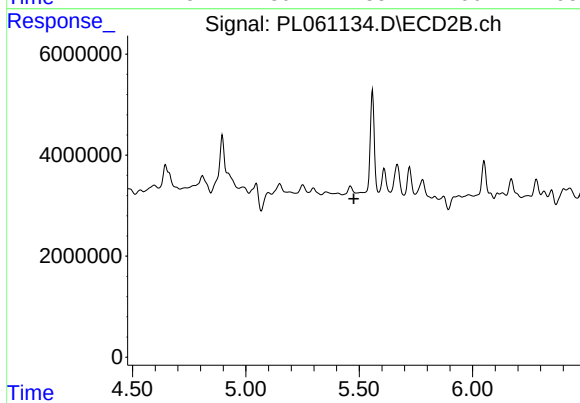

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.476 min
Response: 0
Conc: N.D.

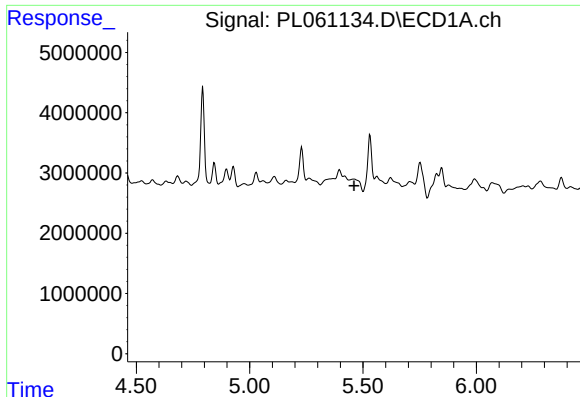

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.460 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

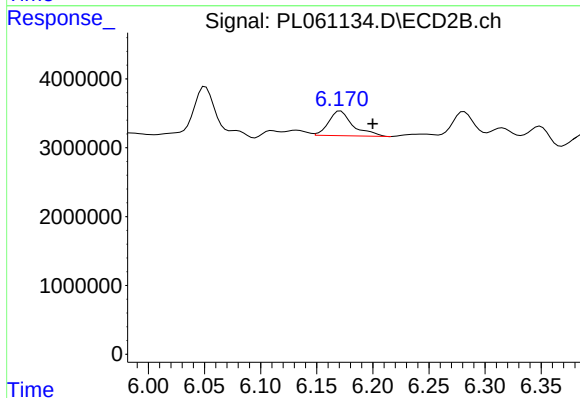


#26 Chlordane-4

R.T.: 6.171 min
Delta R.T.: -0.029 min
Response: 5417667
Conc: 11.27 ng/ml

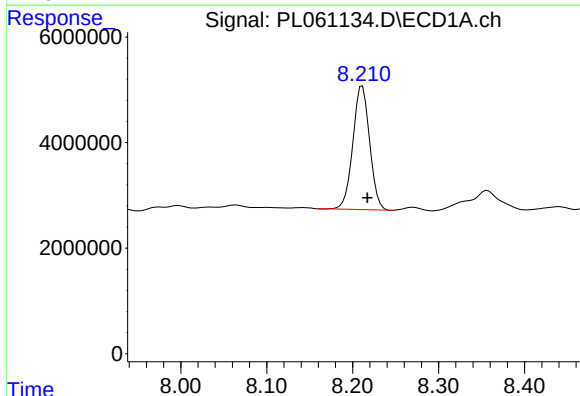

#28 Decachlorobiphenyl

R.T.: 8.211 min
Delta R.T.: -0.006 min
Response: 31820875
Conc: 18.89 ng/ml

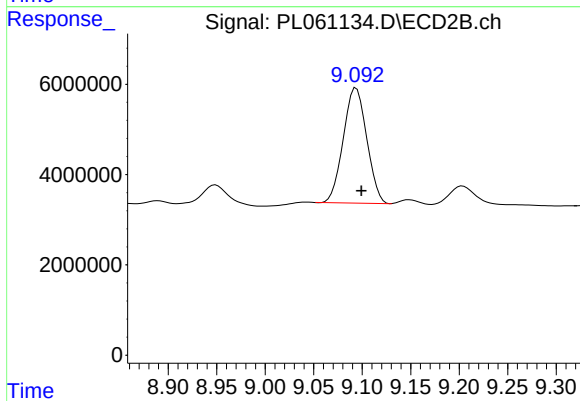

#28 Decachlorobiphenyl

R.T.: 9.094 min
Delta R.T.: -0.005 min
Response: 42947595
Conc: 20.35 ng/ml