

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090120\
 Data File : PL061150.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Sep 2020 18:29
 Operator : DD\AJ
 Sample : L3827-18
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 789UMR-TP11-2430-01

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 02 07:25:05 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 25 16:59:57 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.461	4.009	37790354	52254538	20.478	20.105
28)	SA Decachlor...	8.213	0.000	77559610	0	46.040	N.D. #
Target Compounds							
2)	A alpha-BHC	0.000	4.404	0	3380871	N.D.	0.832 #
3)	MA gamma-BHC...	4.202f	4.664f	3123635	2735607	1.224	0.727 #
9)	A Endosulfan I	5.533f	0.000	4730847	0	2.603	N.D. #
10)	B gamma-Chl...	5.396	0.000	7511924	0	3.823	N.D. #
11)	B alpha-Chl...	0.000	6.173f	0	11132262	N.D.	3.581 #
12)	B 4,4'-DDE	5.623	6.353	23531573	33581687	12.789	11.619
13)	MA Dieldrin	0.000	6.487f	0	2995202	N.D.	1.003 #
17)	MA 4,4'-DDT	6.378	7.146	11319551	16941047	7.488	7.356
19)	B Endosulfa...	0.000	7.277	0	3091091	N.D.	1.275 #
25)	Chlordane-3	5.396	0.000	7511924	0	41.621	N.D. #
26)	Chlordane-4	0.000	6.173f	0	11132262	N.D.	23.157 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090120\
Data File : PL061150.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Sep 2020 18:29
Operator : DD\AJ
Sample : L3827-18
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
789UMR-TP11-2430-01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 02 07:25:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
Quant Title : GC Extractables
QLast Update : Tue Aug 25 16:59:57 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

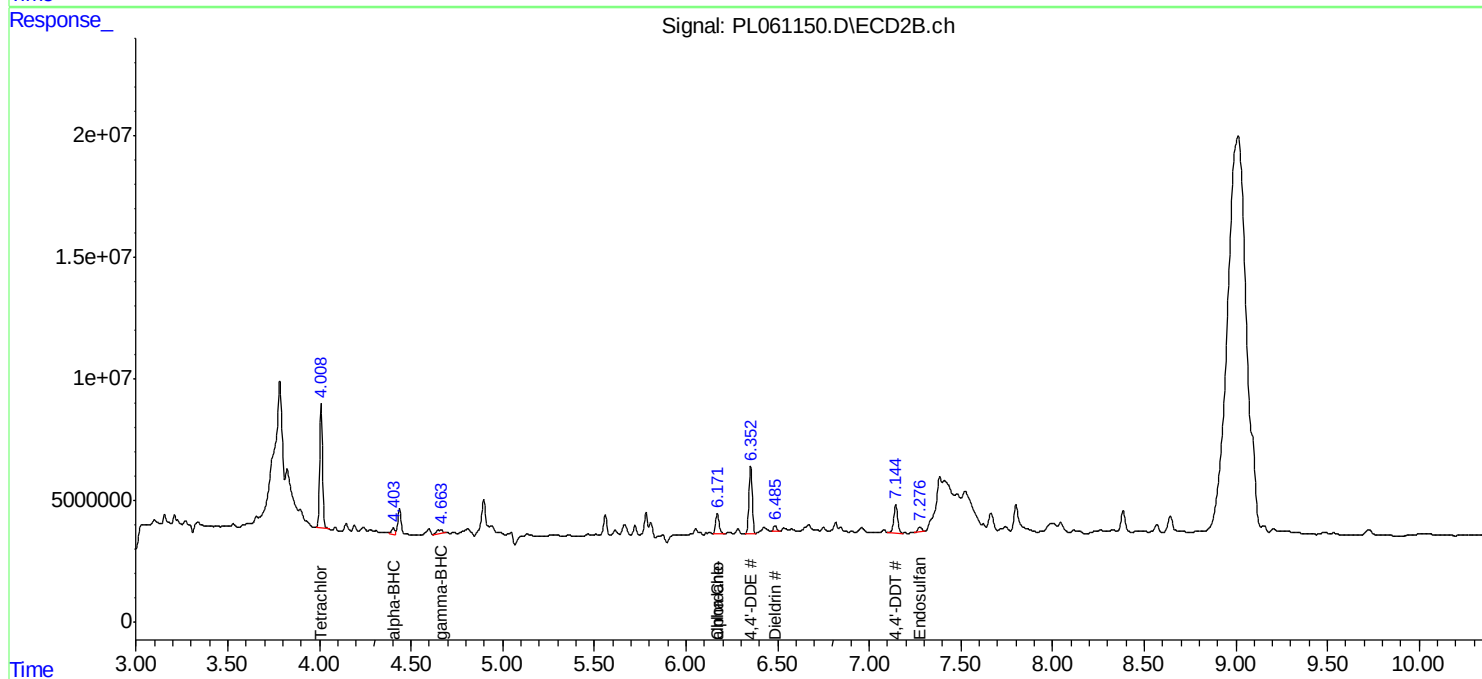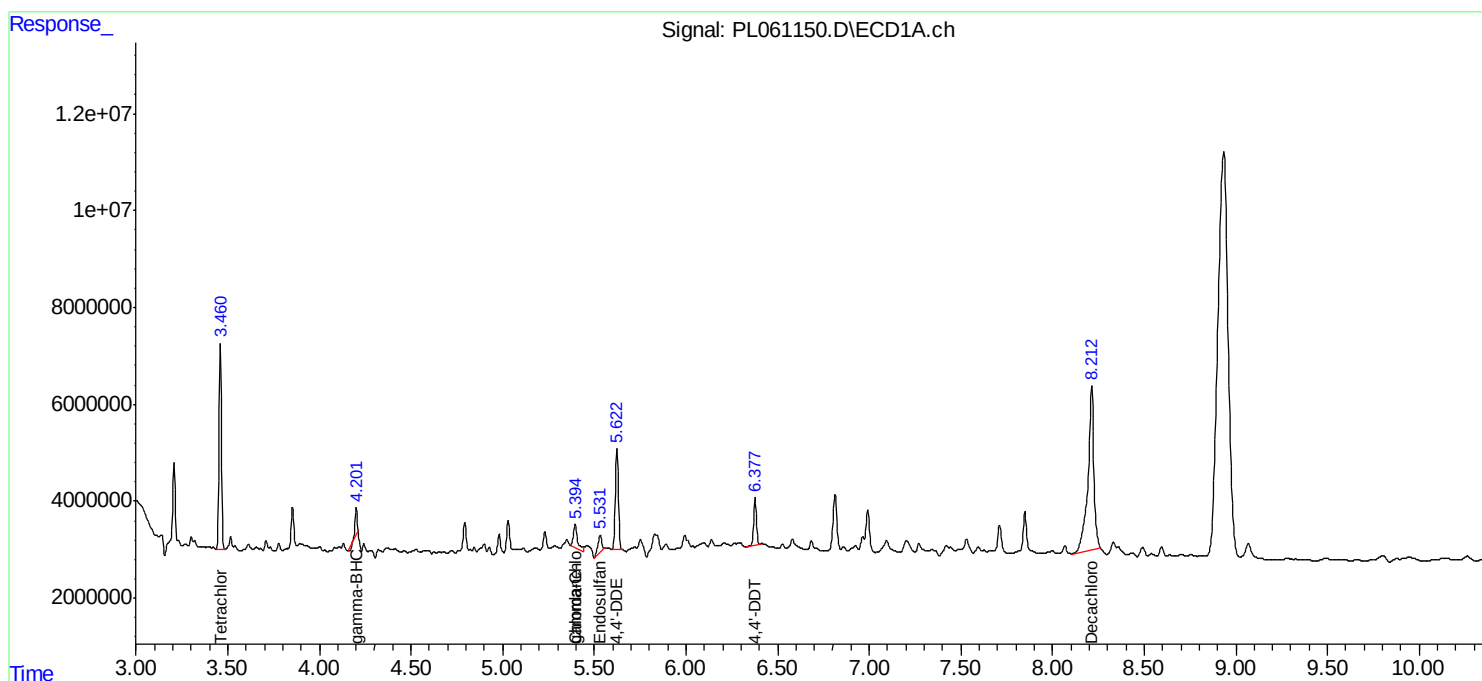


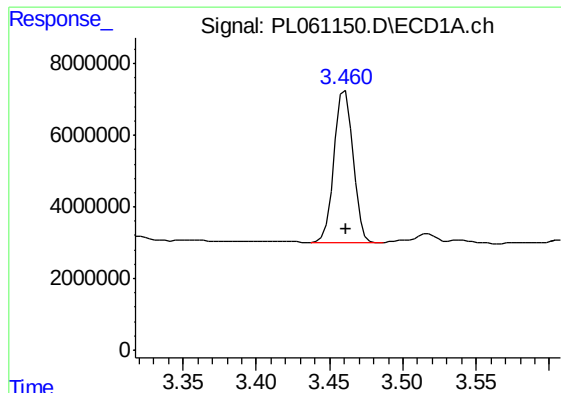

#1 Tetrachloro-m-xylene


R.T.: 3.461 min
Delta R.T.: 0.000 min
Response: 37790354
Conc: 20.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
789UMR-TP11-2430-01

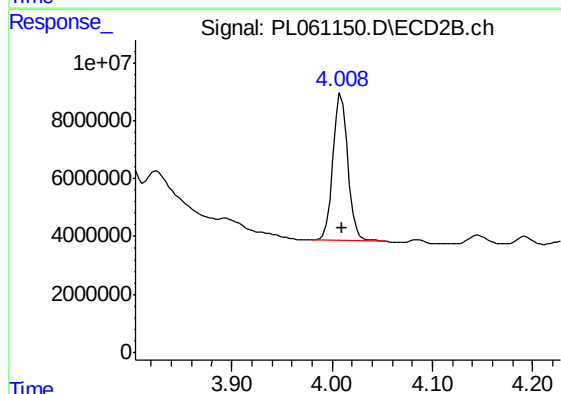


#1 Tetrachloro-m-xylene

R.T.: 4.009 min
Delta R.T.: 0.000 min
Response: 52254538
Conc: 20.11 ng/ml

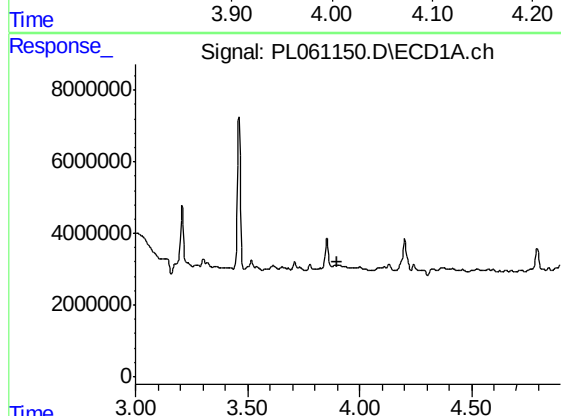


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.898 min
Response: 0
Conc: N.D.

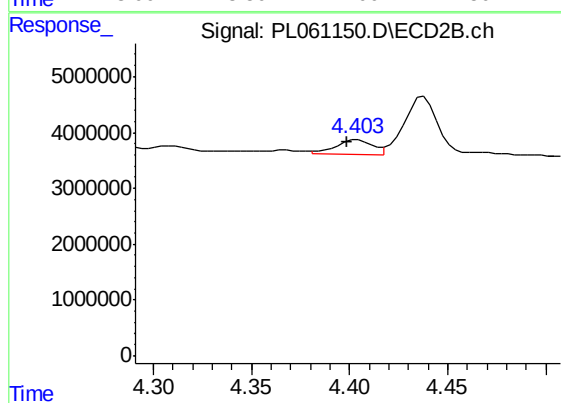

#2 alpha-BHC


R.T.: 4.404 min
Delta R.T.: 0.006 min
Response: 3380871
Conc: 0.83 ng/ml

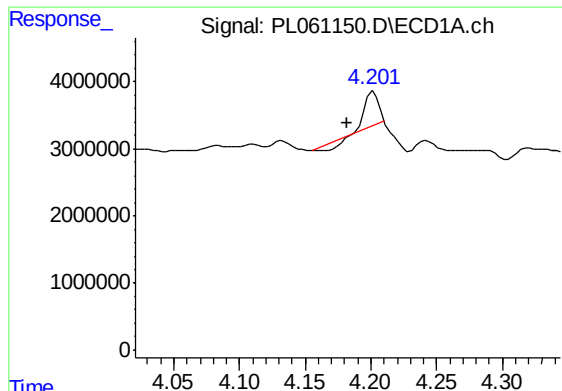

#3 gamma-BHC (Lindane)


R.T.: 4.202 min
Delta R.T.: 0.021 min
Response: 3123635
Conc: 1.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
789UMR-TP11-2430-01

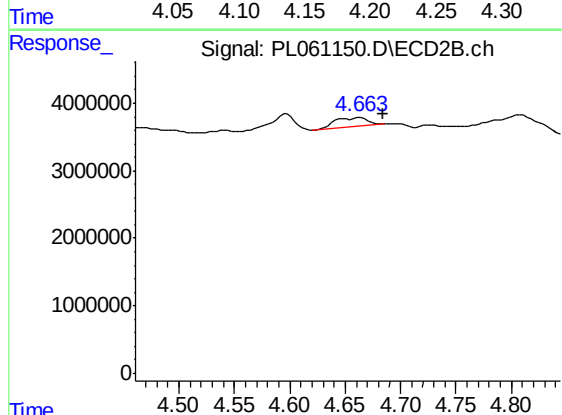


#3 gamma-BHC (Lindane)

R.T.: 4.664 min
Delta R.T.: -0.021 min
Response: 2735607
Conc: 0.73 ng/ml

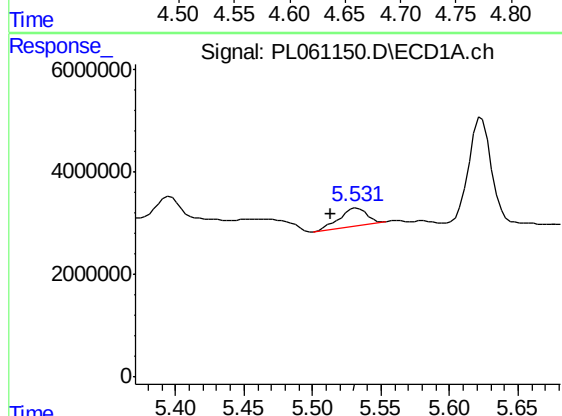


#9 Endosulfan I

R.T.: 5.533 min
Delta R.T.: 0.020 min
Response: 4730847
Conc: 2.60 ng/ml

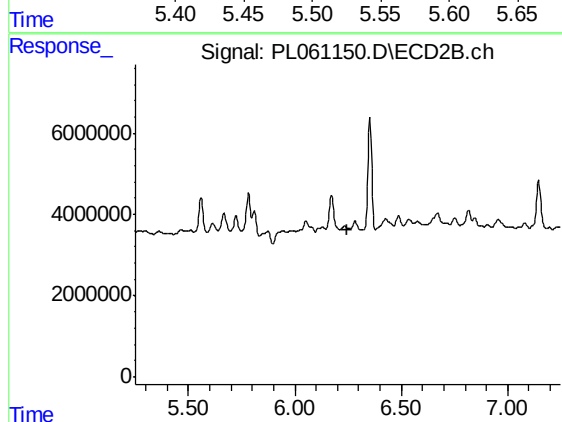

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.248 min
Response: 0
Conc: N.D.

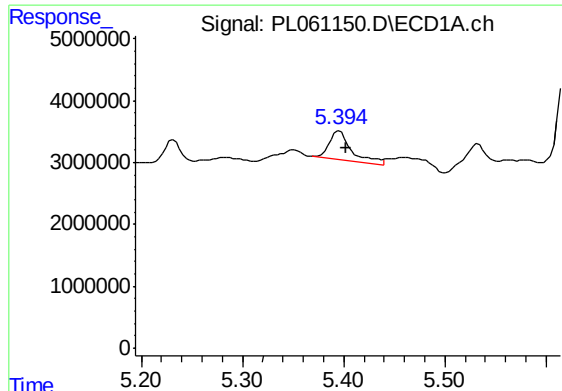

#10 gamma-Chlordane


R.T.: 5.396 min
Delta R.T.: -0.006 min
Response: 7511924
Conc: 3.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
789UMR-TP11-2430-01

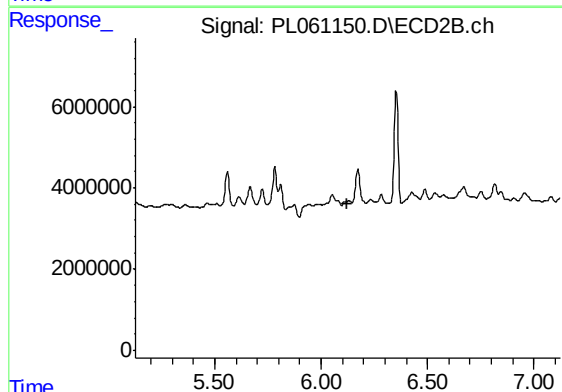


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.125 min
Response: 0
Conc: N.D.

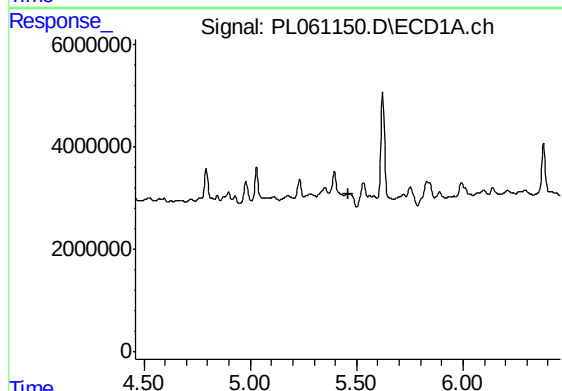


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.460 min
Response: 0
Conc: N.D.

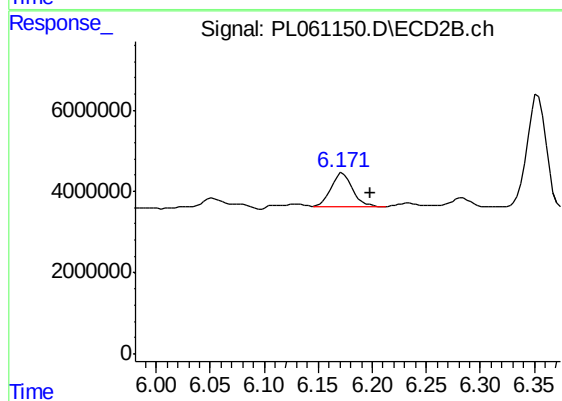

#11 alpha-Chlordane


R.T.: 6.173 min
Delta R.T.: -0.025 min
Response: 11132262
Conc: 3.58 ng/ml

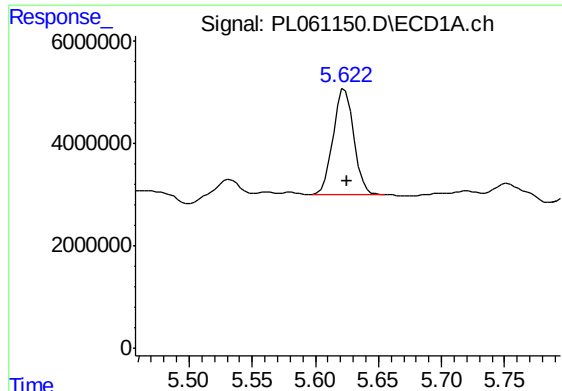

#12 4,4'-DDE


R.T.: 5.623 min
Delta R.T.: -0.002 min
Response: 23531573
Conc: 12.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
789UMR-TP11-2430-01

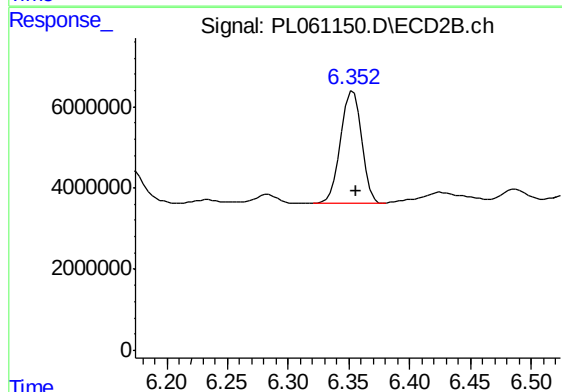


#12 4,4'-DDE

R.T.: 6.353 min
Delta R.T.: -0.002 min
Response: 33581687
Conc: 11.62 ng/ml

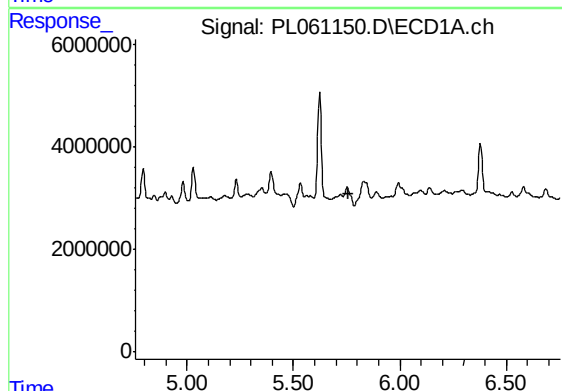


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 5.756 min
Response: 0
Conc: N.D.

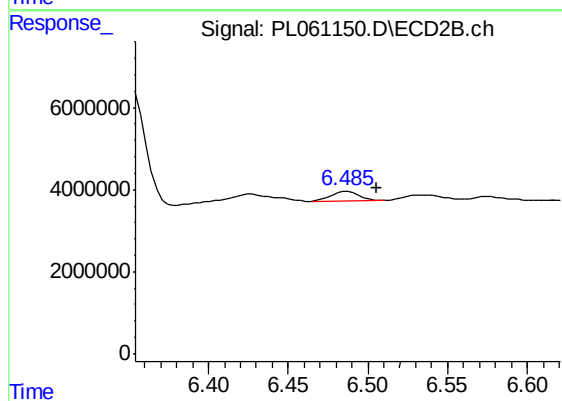

#13 Dieldrin


R.T.: 6.487 min
Delta R.T.: -0.019 min
Response: 2995202
Conc: 1.00 ng/ml

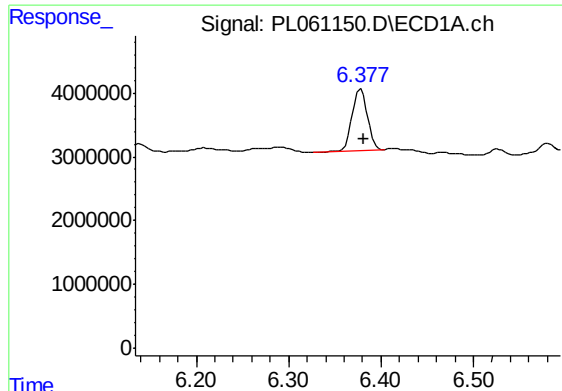

#17 4,4'-DDT


R.T.: 6.378 min
Delta R.T.: -0.003 min
Response: 11319551
Conc: 7.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
789UMR-TP11-2430-01

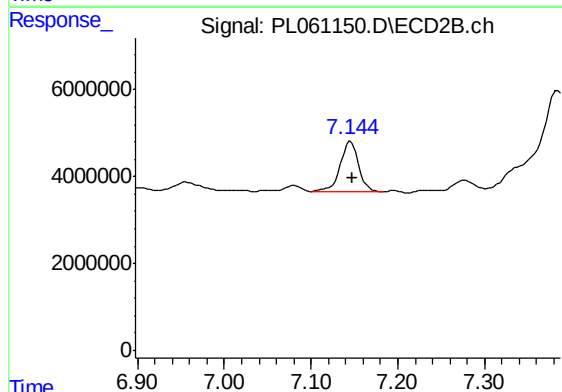


#17 4,4'-DDT

R.T.: 7.146 min
Delta R.T.: -0.001 min
Response: 16941047
Conc: 7.36 ng/ml

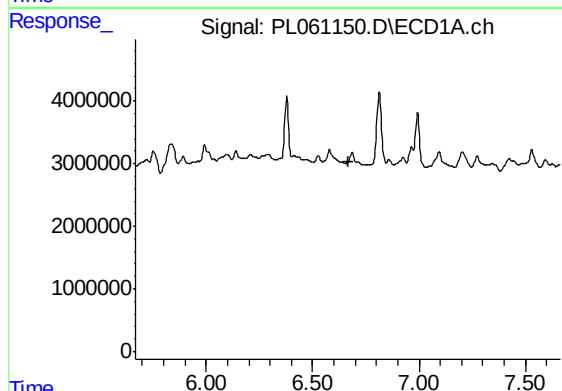


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 6.667 min
Response: 0
Conc: N.D.

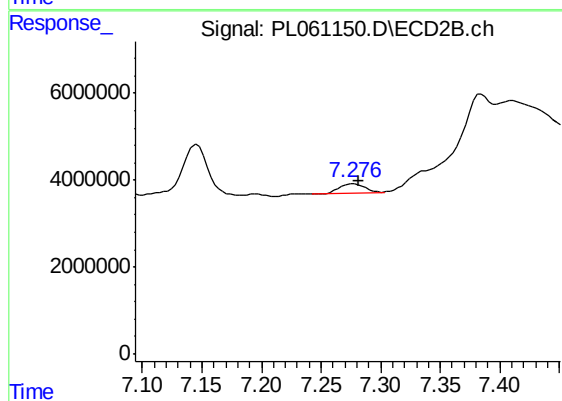

#19 Endosulfan Sulfate


R.T.: 7.277 min
Delta R.T.: -0.004 min
Response: 3091091
Conc: 1.28 ng/ml

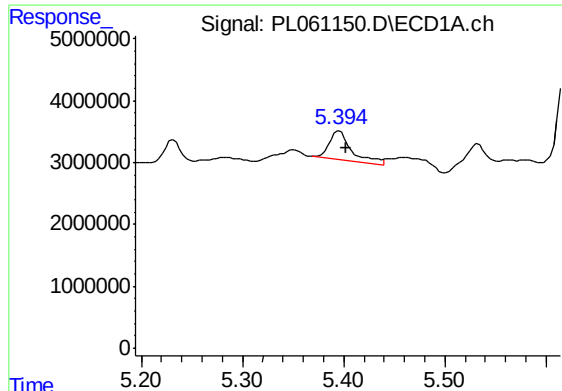

#25 Chlordane-3


R.T.: 5.396 min
Delta R.T.: -0.006 min
Response: 7511924
Conc: 41.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
789UMR-TP11-2430-01

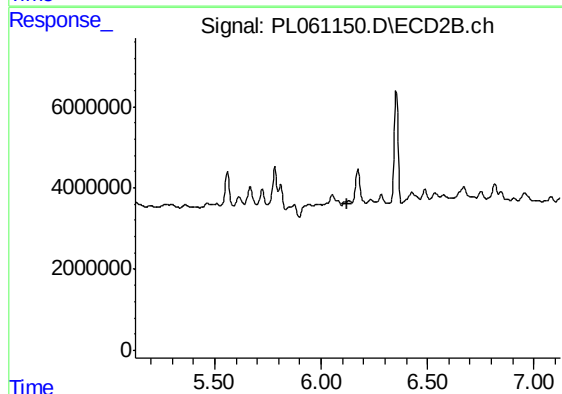


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.125 min
Response: 0
Conc: N.D.

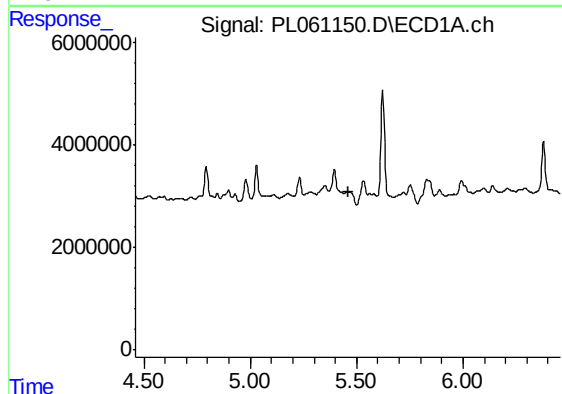


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.460 min
Response: 0
Conc: N.D.

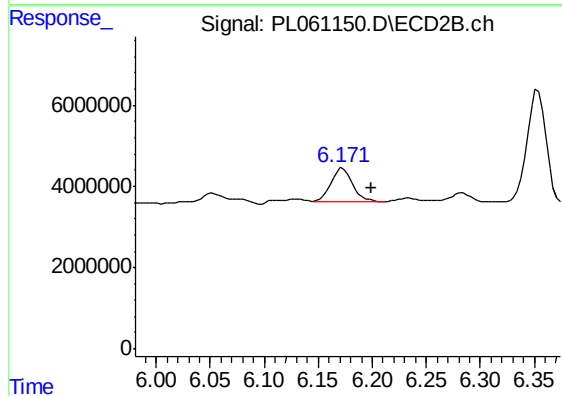

#26 Chlordane-4


R.T.: 6.173 min
Delta R.T.: -0.027 min
Response: 11132262
Conc: 23.16 ng/ml

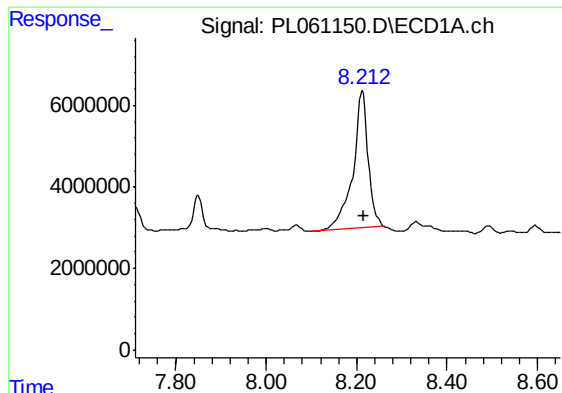

#28 Decachlorobiphenyl

R.T.: 8.213 min
Delta R.T.: -0.004 min
Response: 77559610
Conc: 46.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
789UMR-TP11-2430-01

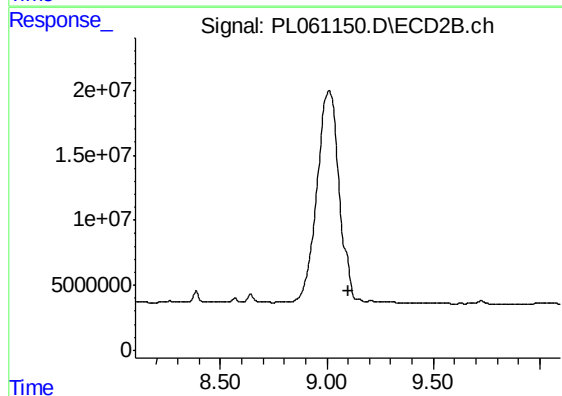

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.099 min
Response: 0
Conc: N.D.