

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090120\
 Data File : PL061159.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Sep 2020 20:36
 Operator : DD\AJ
 Sample : L3849-06
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 232

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 02 07:27:45 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 25 16:59:57 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.460	4.010	30824737	26360319	16.704	10.142 #
28)	SA Decachlor...	8.214	9.096	27049591	38212143	16.057	18.110
Target Compounds							
5)	MB Aldrin	0.000	5.484f	0	3615901	N.D.	1.073 #
13)	MA Dieldrin	0.000	6.531f	0	4404624	N.D.	1.475 #
14)	MA Endrin	0.000	6.750f	0	1980695	N.D.	0.780 #
15)	B Endosulfa...	0.000	6.919f	0	4443353	N.D.	1.727 #
16)	A 4,4'-DDD	6.140	6.841	2011511	8265604	1.272	3.539 #
19)	B Endosulfa...	0.000	7.253f	0	3362037	N.D.	1.387 #
20)	A Methoxychlor	6.925	7.594	4795019	5137569	5.342	3.974 #
24)	Chlordane-2	0.000	5.484	0	3615901	N.D.	35.136 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090120\
Data File : PL061159.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Sep 2020 20:36
Operator : DD\AJ
Sample : L3849-06
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
232

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 02 07:27:45 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
Quant Title : GC Extractables
QLast Update : Tue Aug 25 16:59:57 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

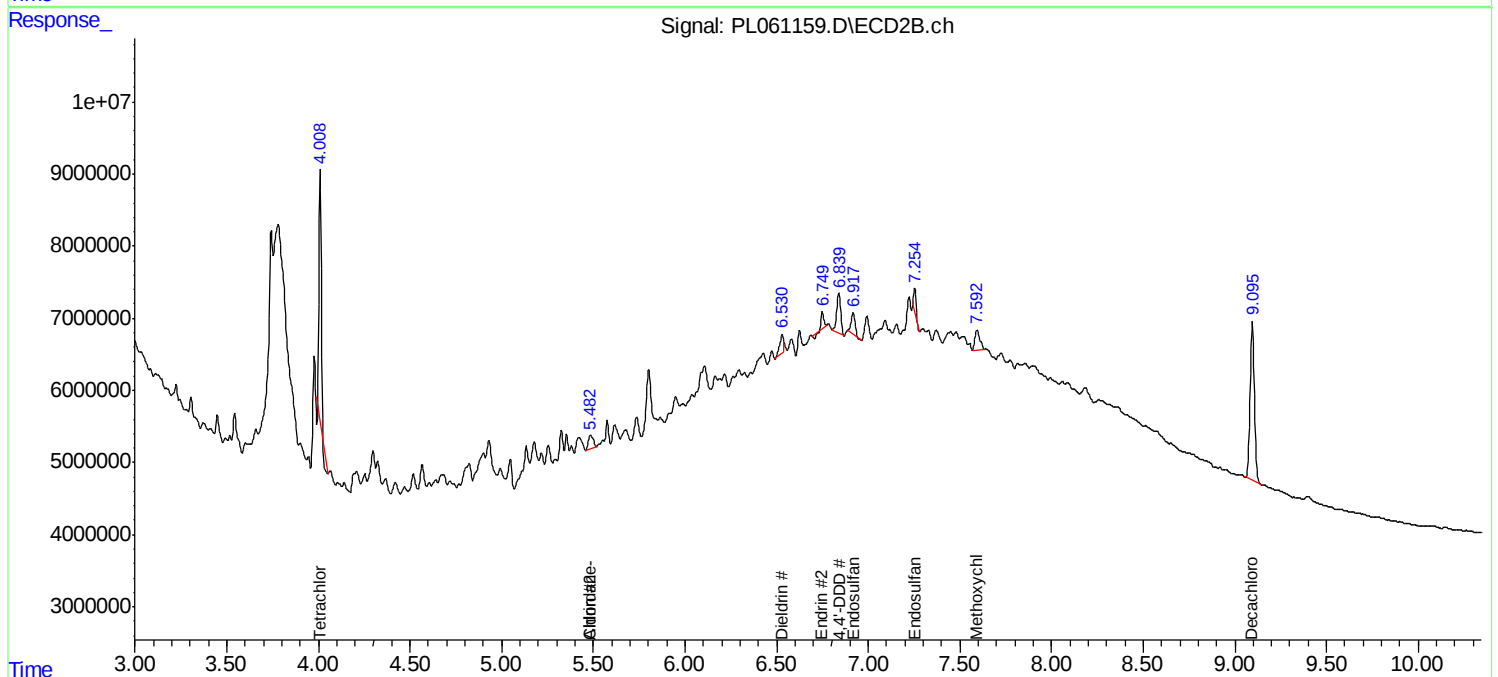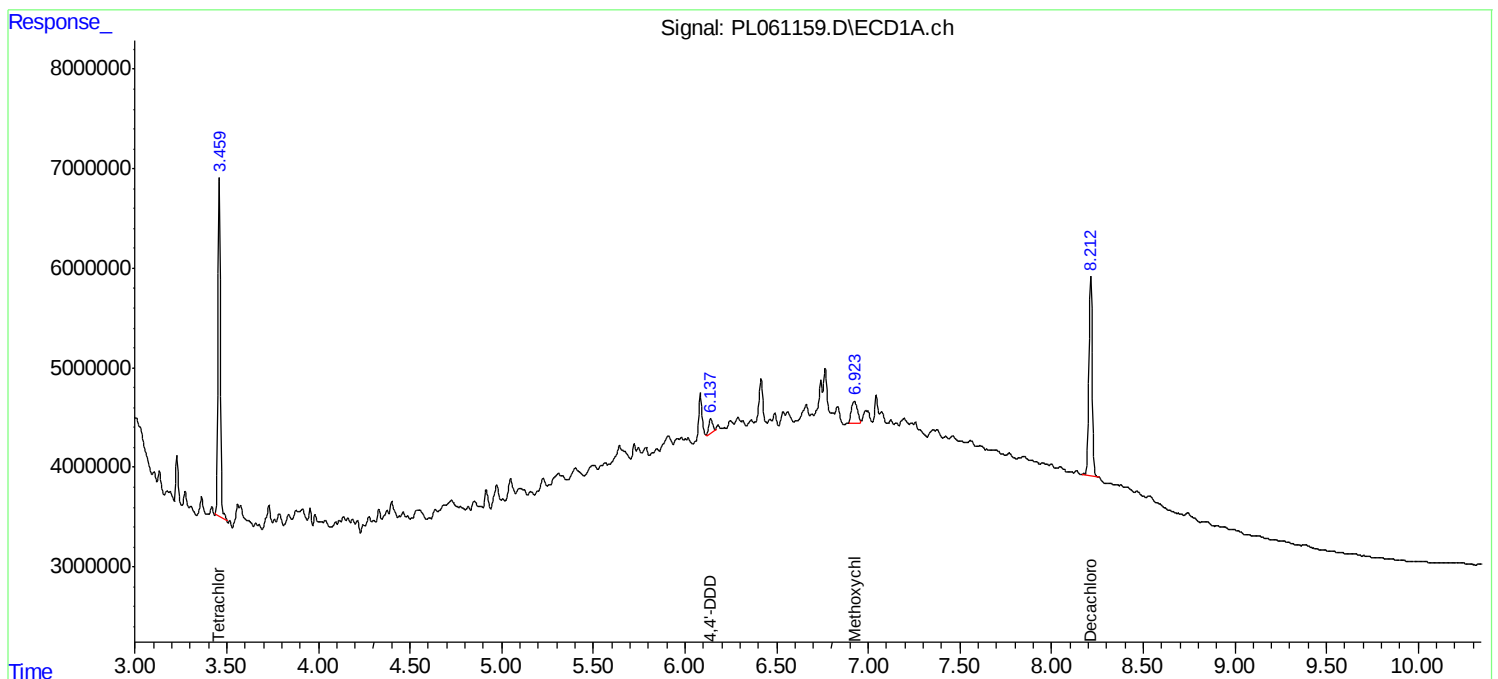


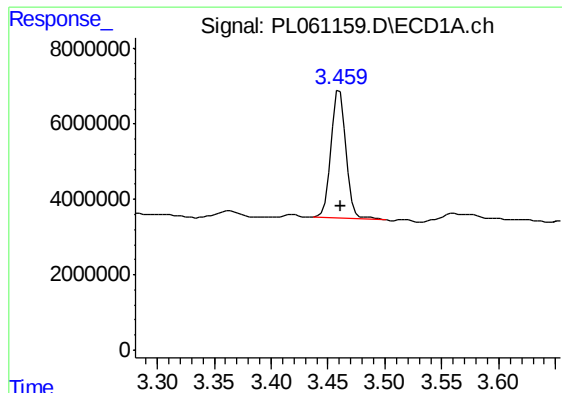

#1 Tetrachloro-m-xylene


R.T.: 3.460 min
Delta R.T.: 0.000 min
Response: 30824737
Conc: 16.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
232

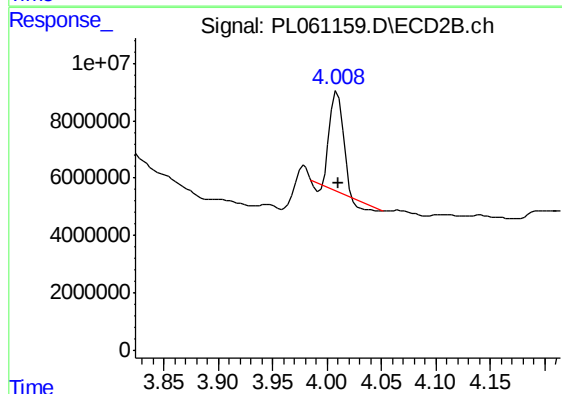


#1 Tetrachloro-m-xylene

R.T.: 4.010 min
Delta R.T.: 0.000 min
Response: 26360319
Conc: 10.14 ng/ml

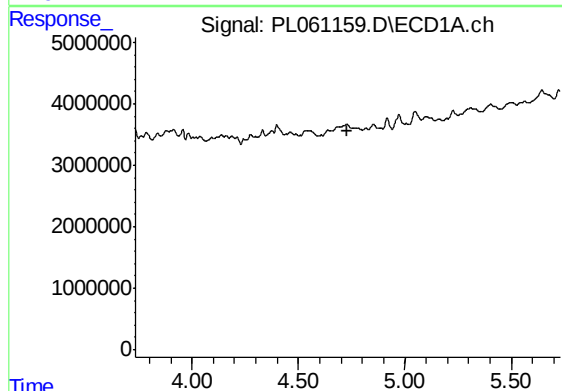


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.732 min
Response: 0
Conc: N.D.

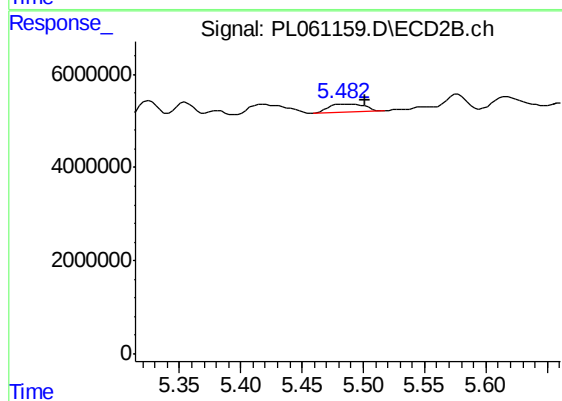

#5 Aldrin


R.T.: 5.484 min
Delta R.T.: -0.018 min
Response: 3615901
Conc: 1.07 ng/ml

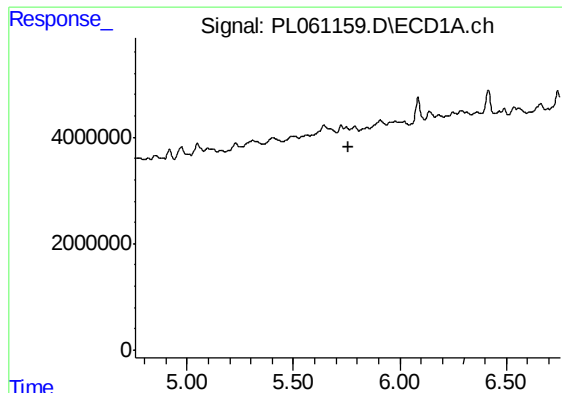

#13 Dielddrin


R.T.: 0.000 min
Exp R.T. : 5.756 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
232

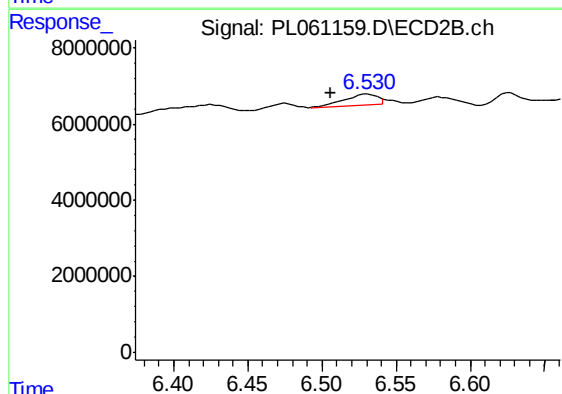


#13 Dielddrin

R.T.: 6.531 min
Delta R.T.: 0.025 min
Response: 4404624
Conc: 1.47 ng/ml

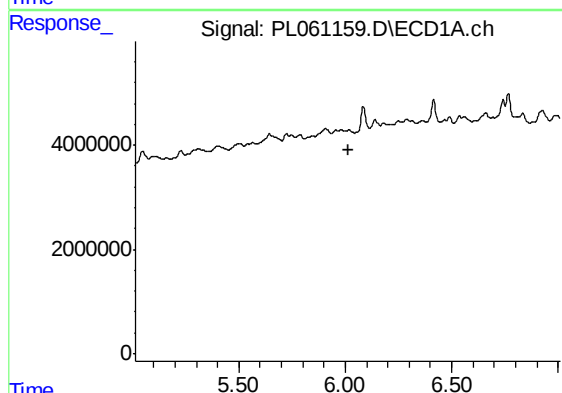


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.013 min
Response: 0
Conc: N.D.

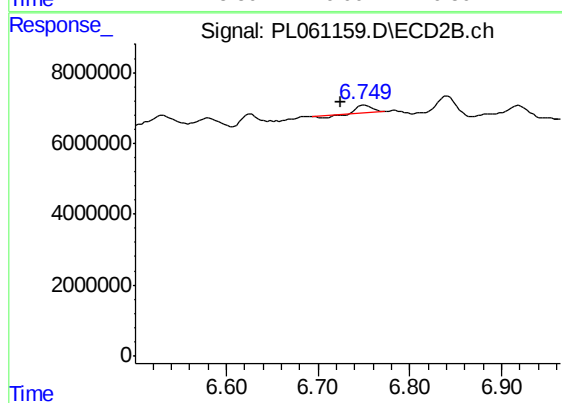

#14 Endrin


R.T.: 6.750 min
Delta R.T.: 0.026 min
Response: 1980695
Conc: 0.78 ng/ml

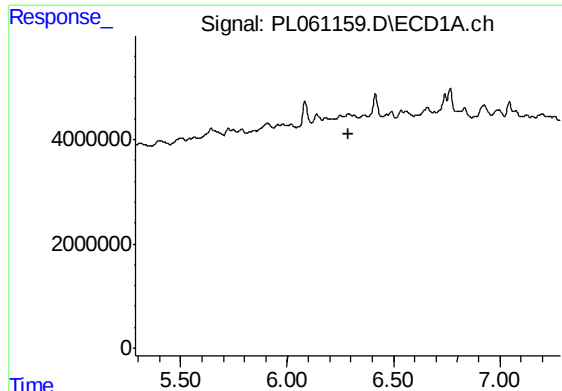

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.286 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
232

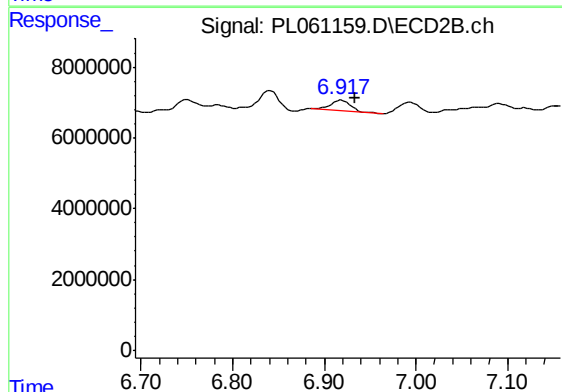


#15 Endosulfan II

R.T.: 6.919 min
Delta R.T.: -0.016 min
Response: 4443353
Conc: 1.73 ng/ml

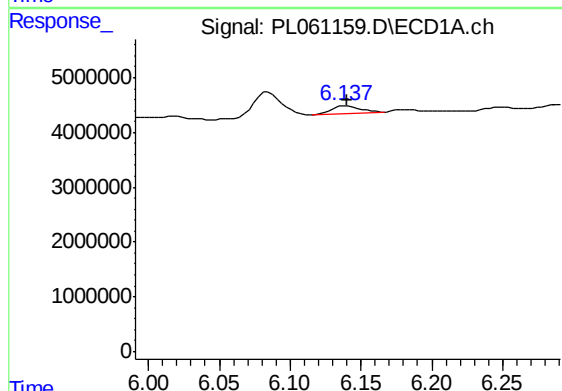


#16 4,4'-DDD

R.T.: 6.140 min
Delta R.T.: -0.001 min
Response: 2011511
Conc: 1.27 ng/ml

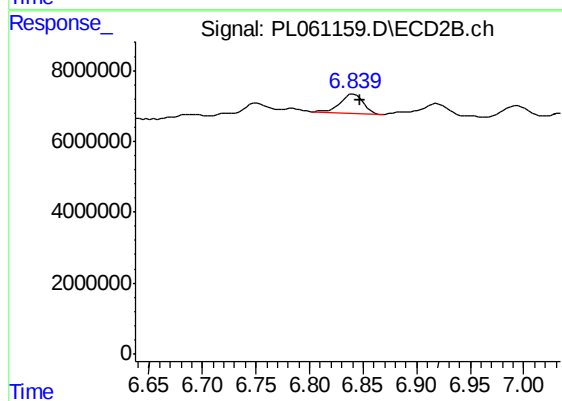

#16 4,4'-DDD


R.T.: 6.841 min
Delta R.T.: -0.007 min
Response: 8265604
Conc: 3.54 ng/ml

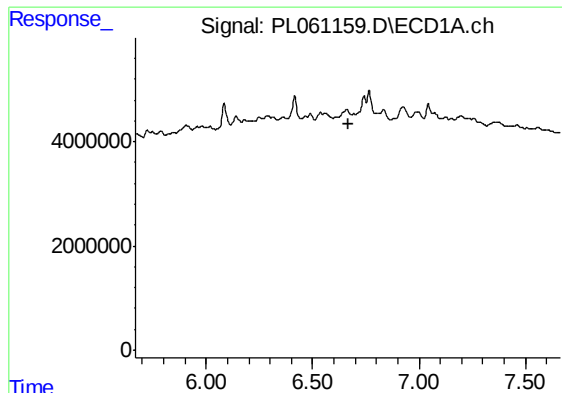

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 6.667 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
232

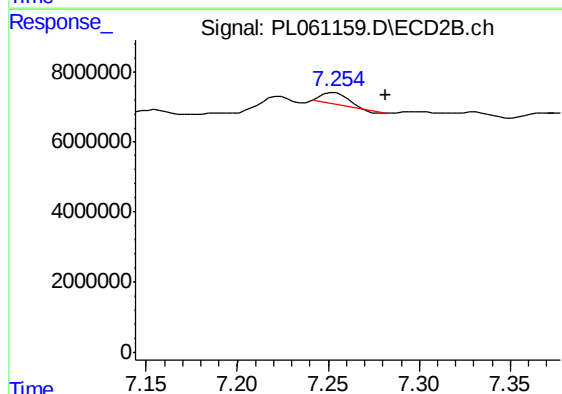


#19 Endosulfan Sulfate

R.T.: 7.253 min
Delta R.T.: -0.028 min
Response: 3362037
Conc: 1.39 ng/ml

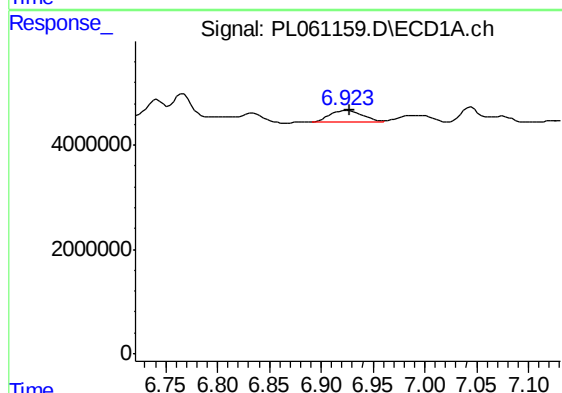


#20 Methoxychlor

R.T.: 6.925 min
Delta R.T.: -0.003 min
Response: 4795019
Conc: 5.34 ng/ml

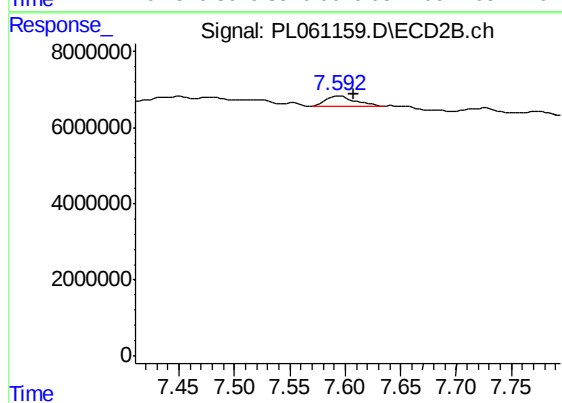

#20 Methoxychlor


R.T.: 7.594 min
Delta R.T.: -0.013 min
Response: 5137569
Conc: 3.97 ng/ml

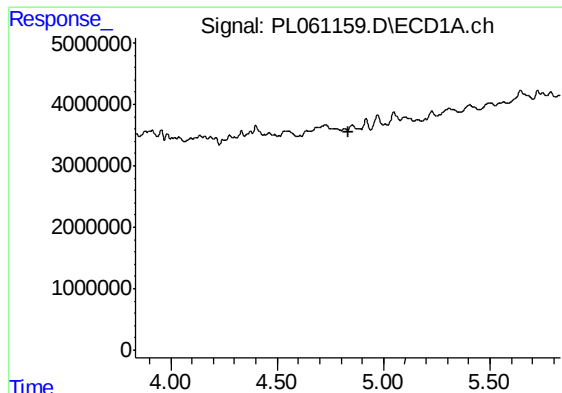

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.833 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
232

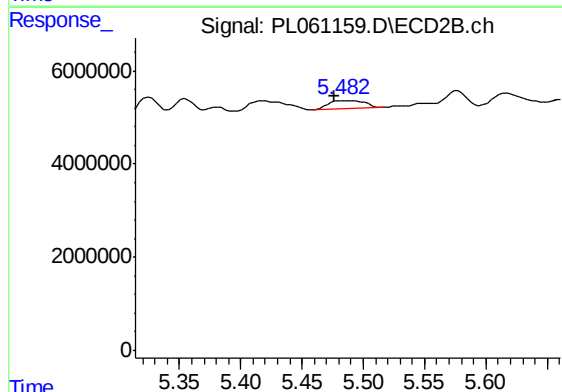


#24 Chlordane-2

R.T.: 5.484 min
Delta R.T.: 0.007 min
Response: 3615901
Conc: 35.14 ng/ml

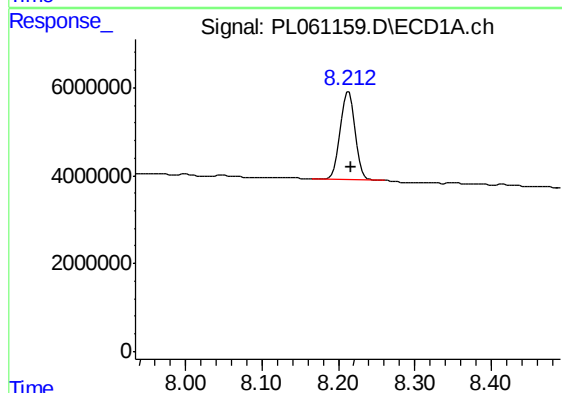

#28 Decachlorobiphenyl

R.T.: 8.214 min
Delta R.T.: -0.004 min
Response: 27049591
Conc: 16.06 ng/ml

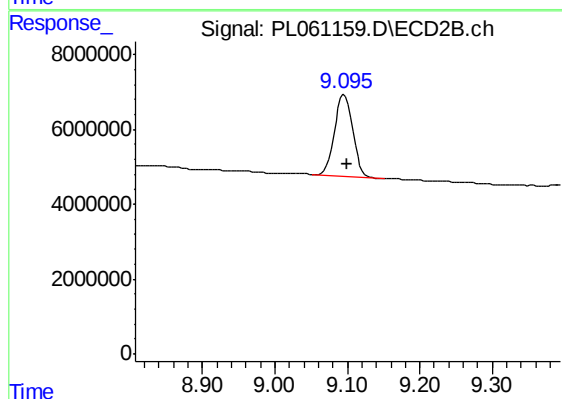

#28 Decachlorobiphenyl

R.T.: 9.096 min
Delta R.T.: -0.003 min
Response: 38212143
Conc: 18.11 ng/ml