

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL090120\  
 Data File : PL061179.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 02 Sep 2020 01:33  
 Operator : DD\AJ  
 Sample : L3506-15  
 Misc :  
 ALS Vial : 58 Sample Multiplier: 1

Instrument :  
 ECD\_L  
 ClientSampleId :  
 OR-02-083120

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Sep 02 07:33:00 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL082520.M  
 Quant Title : GC Extractables  
 QLast Update : Tue Aug 25 16:59:57 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

|                             | Compound        | RT#1  | RT#2   | Resp#1   | Resp#2   | ng/ml  | ng/ml    |
|-----------------------------|-----------------|-------|--------|----------|----------|--------|----------|
| -----                       |                 |       |        |          |          |        |          |
| System Monitoring Compounds |                 |       |        |          |          |        |          |
| 1)                          | SA Tetrachlo... | 3.460 | 4.009  | 33460945 | 45554096 | 18.132 | 17.527   |
| 28)                         | SA Decachlor... | 8.213 | 9.097  | 28449100 | 37886330 | 16.888 | 17.955   |
| Target Compounds            |                 |       |        |          |          |        |          |
| 3)                          | MA gamma-BHC... | 4.185 | 4.665f | 5612220  | 6942344  | 2.198  | 1.846    |
| 10)                         | B gamma-Chl...  | 0.000 | 6.107f | 0        | 14131401 | N.D.   | 4.550 #  |
| 13)                         | MA Dieldrin     | 0.000 | 6.531f | 0        | 191244   | N.D.   | 0.064 #  |
| 25)                         | Chlordane-3     | 0.000 | 6.107f | 0        | 14131401 | N.D.   | 35.357 # |
| -----                       |                 |       |        |          |          |        |          |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL090120\  
Data File : PL061179.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 02 Sep 2020 01:33  
Operator : DD\AJ  
Sample : L3506-15  
Misc :  
ALS Vial : 58 Sample Multiplier: 1

Instrument :  
ECD\_L  
ClientSampleId :  
OR-02-083120

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 02 07:33:00 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL082520.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 25 16:59:57 2020  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

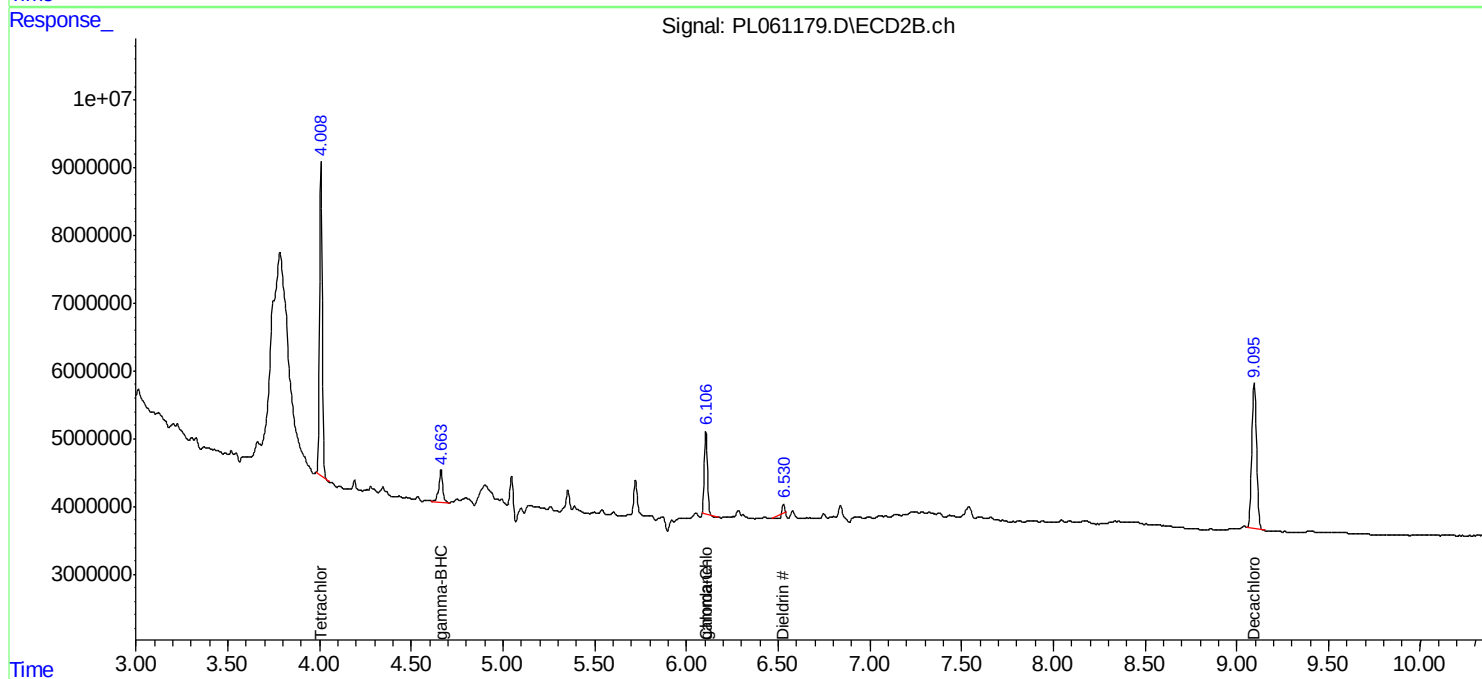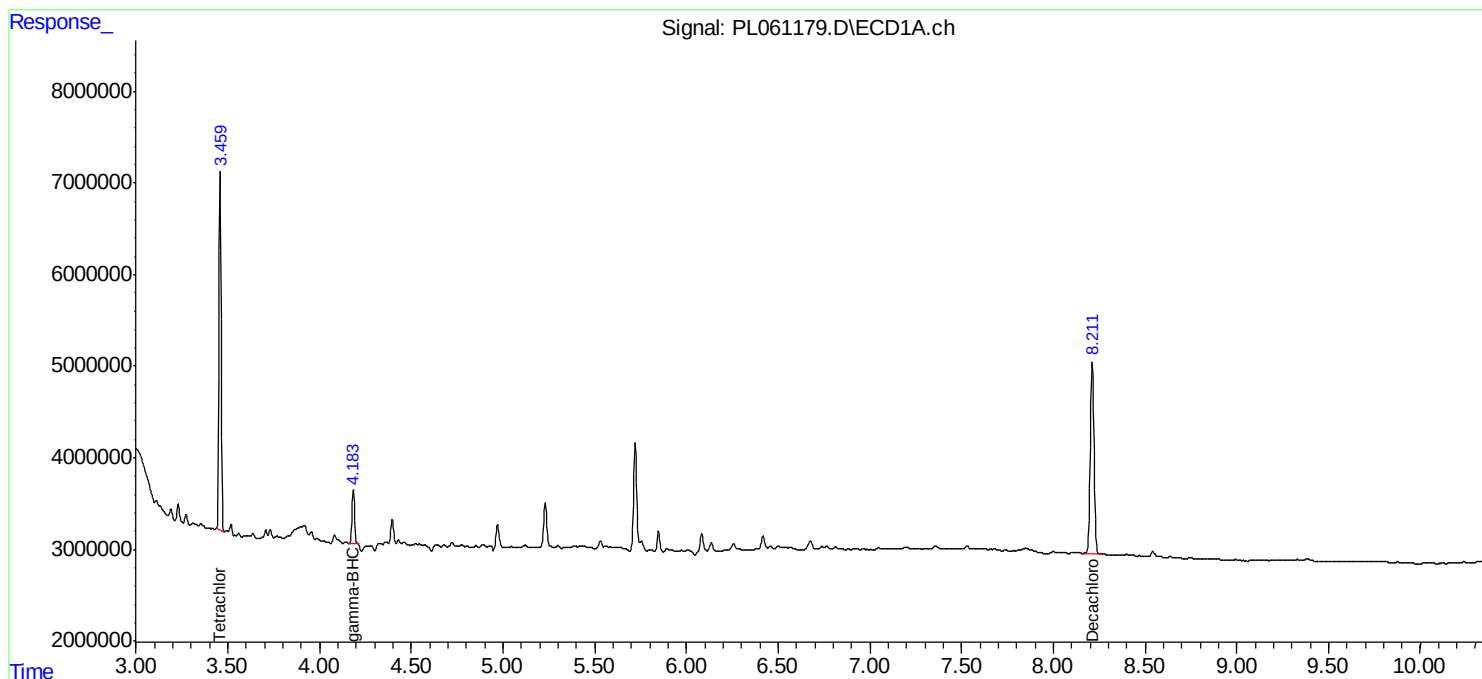


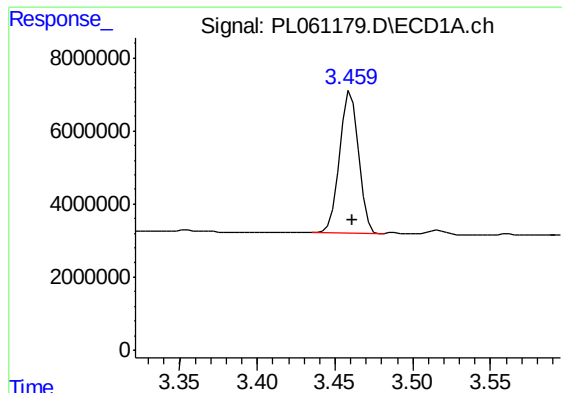

#1 Tetrachloro-m-xylene


R.T.: 3.460 min  
Delta R.T.: 0.000 min  
Response: 33460945  
Conc: 18.13 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :  
OR-02-083120

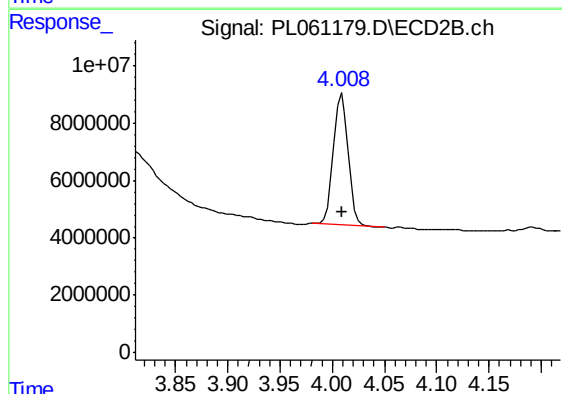


#1 Tetrachloro-m-xylene

R.T.: 4.009 min  
Delta R.T.: 0.000 min  
Response: 45554096  
Conc: 17.53 ng/ml

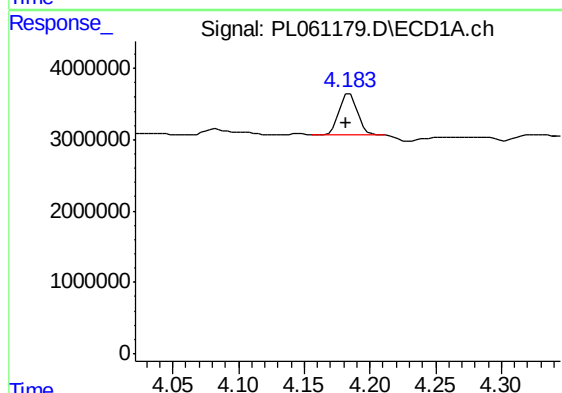


#3 gamma-BHC (Lindane)

R.T.: 4.185 min  
Delta R.T.: 0.003 min  
Response: 5612220  
Conc: 2.20 ng/ml

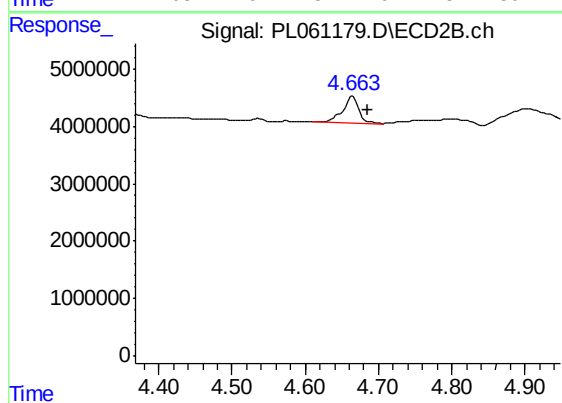

#3 gamma-BHC (Lindane)


R.T.: 4.665 min  
Delta R.T.: -0.020 min  
Response: 6942344  
Conc: 1.85 ng/ml

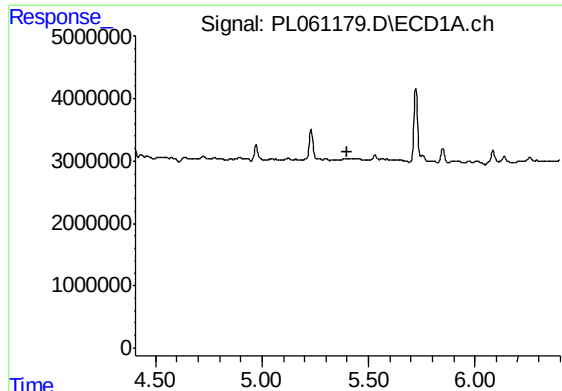

#10 gamma-Chlordane


R.T.: 0.000 min  
Exp R.T. : 5.402 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_L  
ClientSampleId :  
OR-02-083120

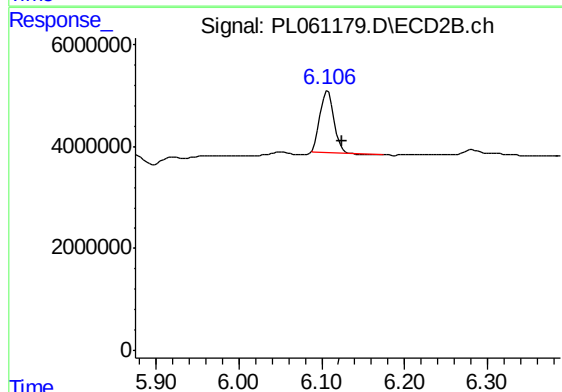


#10 gamma-Chlordane

R.T.: 6.107 min  
Delta R.T.: -0.017 min  
Response: 14131401  
Conc: 4.55 ng/ml

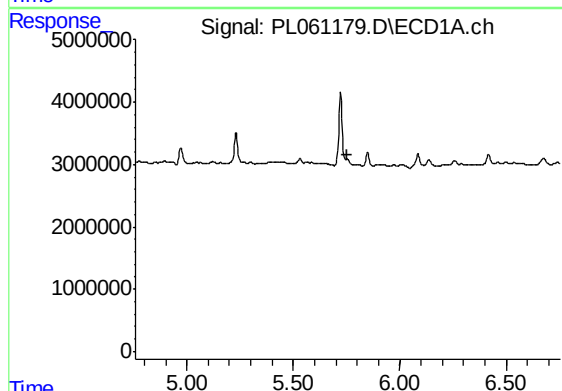


#13 Dieldrin

R.T.: 0.000 min  
Exp R.T. : 5.756 min  
Response: 0  
Conc: N.D.

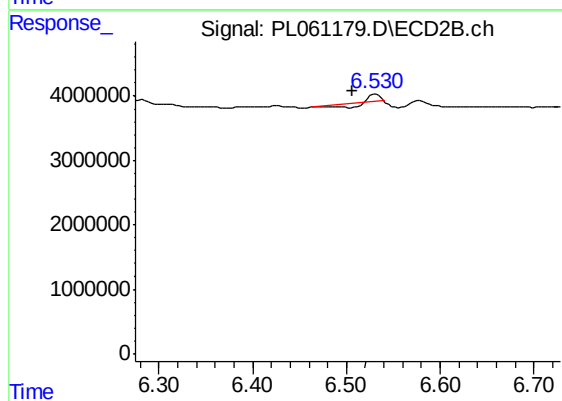

#13 Dieldrin


R.T.: 6.531 min  
Delta R.T.: 0.026 min  
Response: 191244  
Conc: 0.06 ng/ml

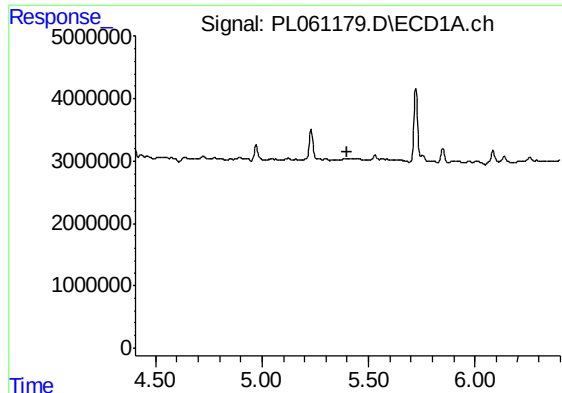

#25 Chlordane-3


R.T.: 0.000 min  
Exp R.T.: 5.402 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_L  
ClientSampleId :  
OR-02-083120

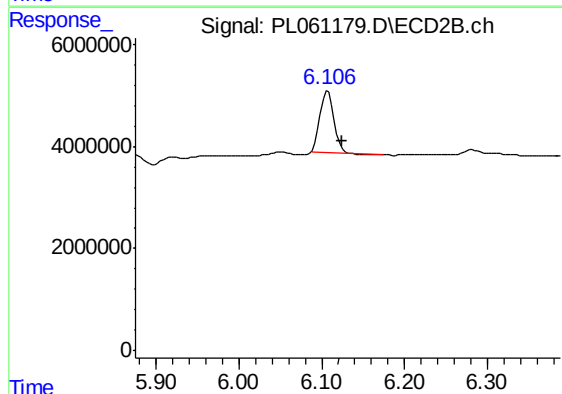


#25 Chlordane-3

R.T.: 6.107 min  
Delta R.T.: -0.017 min  
Response: 14131401  
Conc: 35.36 ng/ml

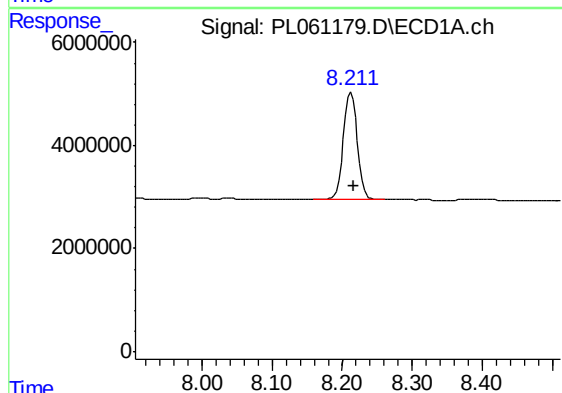

#28 Decachlorobiphenyl

R.T.: 8.213 min  
Delta R.T.: -0.004 min  
Response: 28449100  
Conc: 16.89 ng/ml

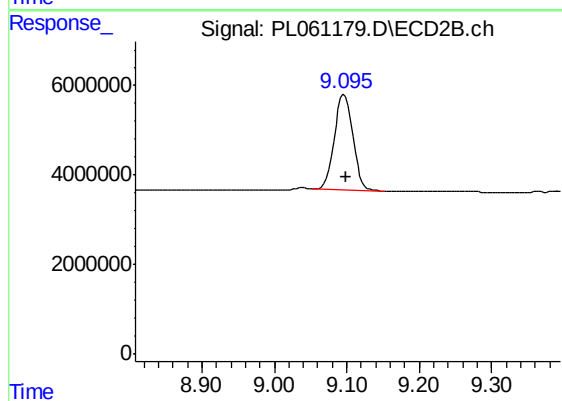

#28 Decachlorobiphenyl

R.T.: 9.097 min  
Delta R.T.: -0.002 min  
Response: 37886330  
Conc: 17.96 ng/ml