

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090120\
 Data File : PL061123.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Sep 2020 10:11
 Operator : DD\AJ
 Sample : L3847-07
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 LINDEN-JOP-BH-09-A

Manual Integrations
 APPROVED

Ankita
 9/2/2020 1:26:12 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 14:49:59 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 25 16:59:57 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.460	4.008	24666498	29187579	13.367	11.230
28)	SA Decachlor...	8.211	9.093	24451611	34433897	14.515m	16.319m
Target Compounds							
17)	MA 4,4'-DDT	6.376	7.141	3041856	2010099	2.012m	0.873m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090120\
Data File : PL061123.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Sep 2020 10:11
Operator : DD\AJ
Sample : L3847-07
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
LINDEN-JOP-BH-09-A


Manual Integrations
APPROVED

Ankita
9/2/2020 1:26:12 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 14:49:59 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
Quant Title : GC Extractables
QLast Update : Tue Aug 25 16:59:57 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

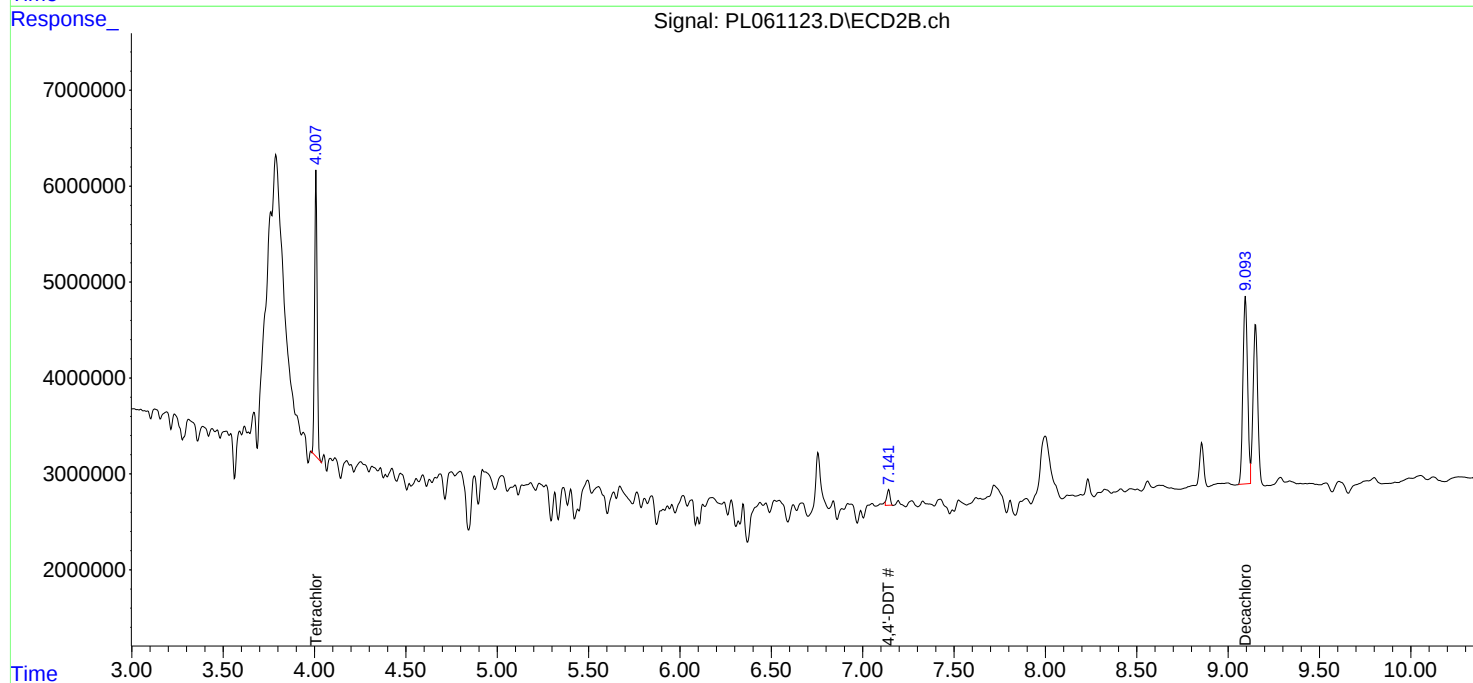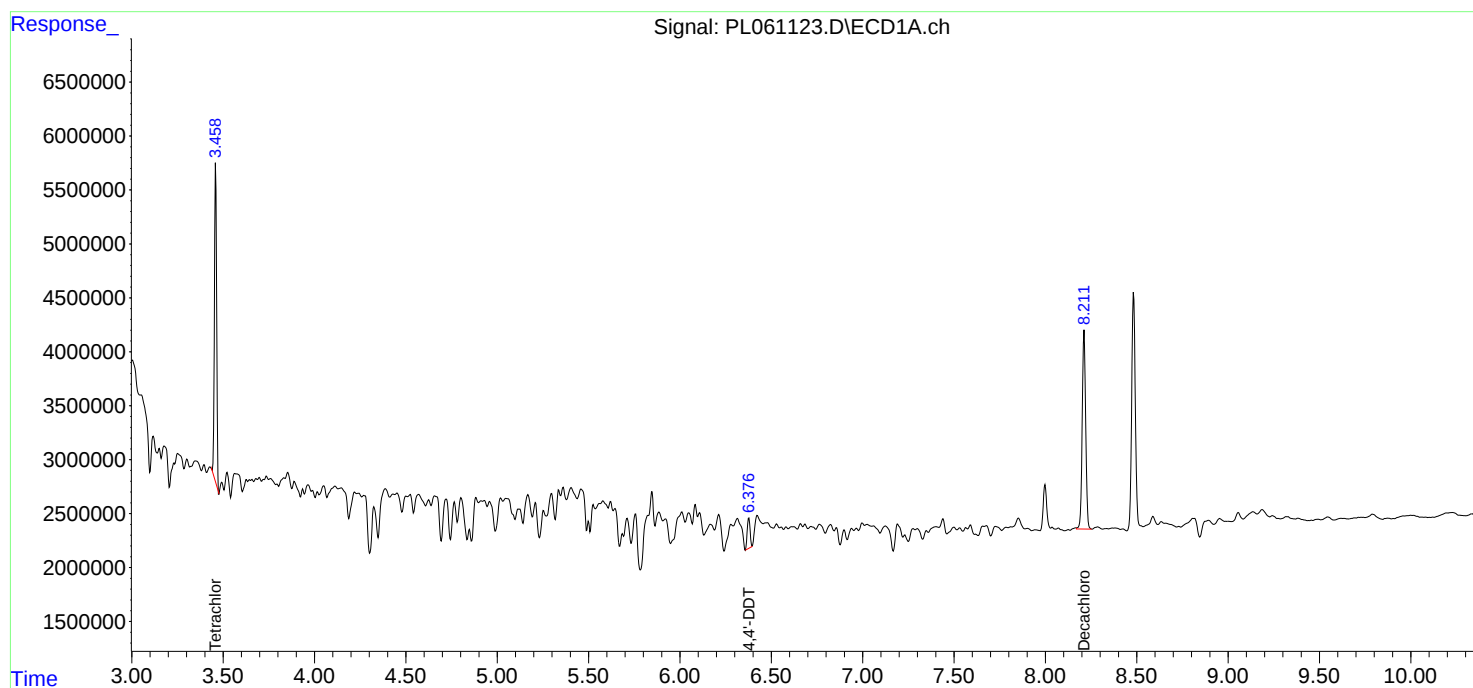

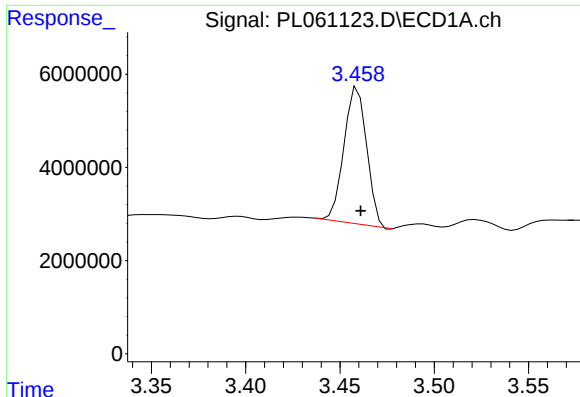


#1 Tetrachloro-m-xylene

R.T.: 3.460 min
Delta R.T.: -0.001 min
Response: 24666498
Conc: 13.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
LINDEN-JOP-BH-09-A


Manual Integrations
APPROVED

Ankita
9/2/2020 1:26:12 PM

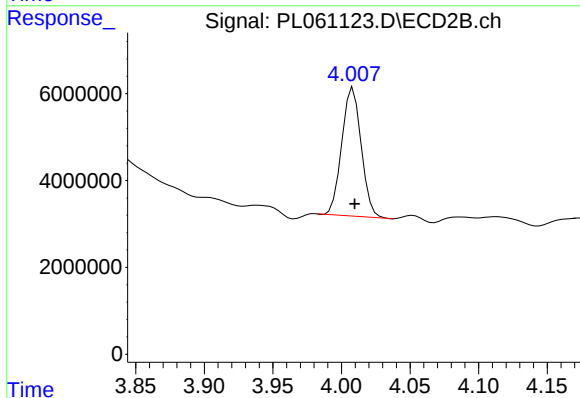


#1 Tetrachloro-m-xylene

R.T.: 4.008 min
Delta R.T.: -0.001 min
Response: 29187579
Conc: 11.23 ng/ml

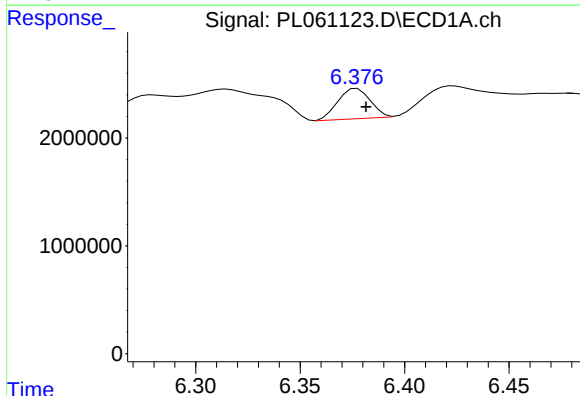


#17 4,4'-DDT

R.T.: 6.376 min
Delta R.T.: -0.006 min
Response: 3041856
Conc: 2.01 ng/ml m

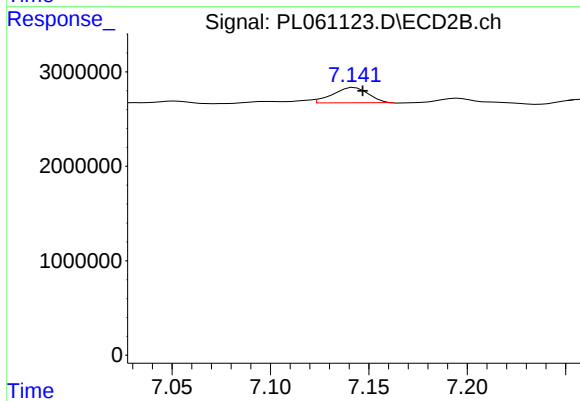

#17 4,4'-DDT

R.T.: 7.141 min
Delta R.T.: -0.006 min
Response: 2010099
Conc: 0.87 ng/ml m

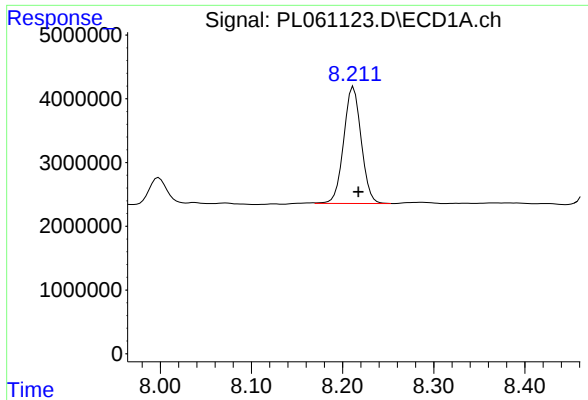


#28 Decachlorobiphenyl

R.T.: 8.211 min
Delta R.T.: -0.007 min
Response: 24451611
Conc: 14.51 ng/ml m

Instrument :
ECD_L
ClientSampleId :
LINDEN-JOP-BH-09-A

Manual Integrations
APPROVED

Ankita
9/2/2020 1:26:12 PM

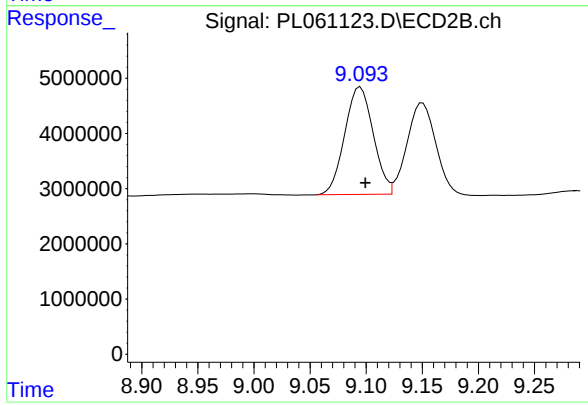

#28 Decachlorobiphenyl

R.T.: 9.093 min
Delta R.T.: -0.006 min
Response: 34433897
Conc: 16.32 ng/ml m