

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090120\
 Data File : PL061124.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Sep 2020 10:26
 Operator : DD\AJ
 Sample : L3847-13
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 LINDEN-JOP-BH-10-A

Manual Integrations
 APPROVED

Ankita
 9/2/2020 1:26:14 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 14:50:11 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 25 16:59:57 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.460	4.008	25036668	31372752	13.567	12.071
28)	SA Decachlor...	8.212	9.093	22605698	31188005	13.419m	14.781m
Target Compounds							
11)	B alpha-Chl...	5.455	6.196	3732660	3913378	1.913m	1.259 #
12)	B 4,4'-DDE	5.622	6.350	7785308	10704627	4.231	3.704
16)	A 4,4'-DDD	6.137	6.844	2637534	6386442	1.668m	2.735 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090120\
Data File : PL061124.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Sep 2020 10:26
Operator : DD\AJ
Sample : L3847-13
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
LINDEN-JOP-BH-10-A


Manual Integrations
APPROVED

Ankita
9/2/2020 1:26:14 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 14:50:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
Quant Title : GC Extractables
QLast Update : Tue Aug 25 16:59:57 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

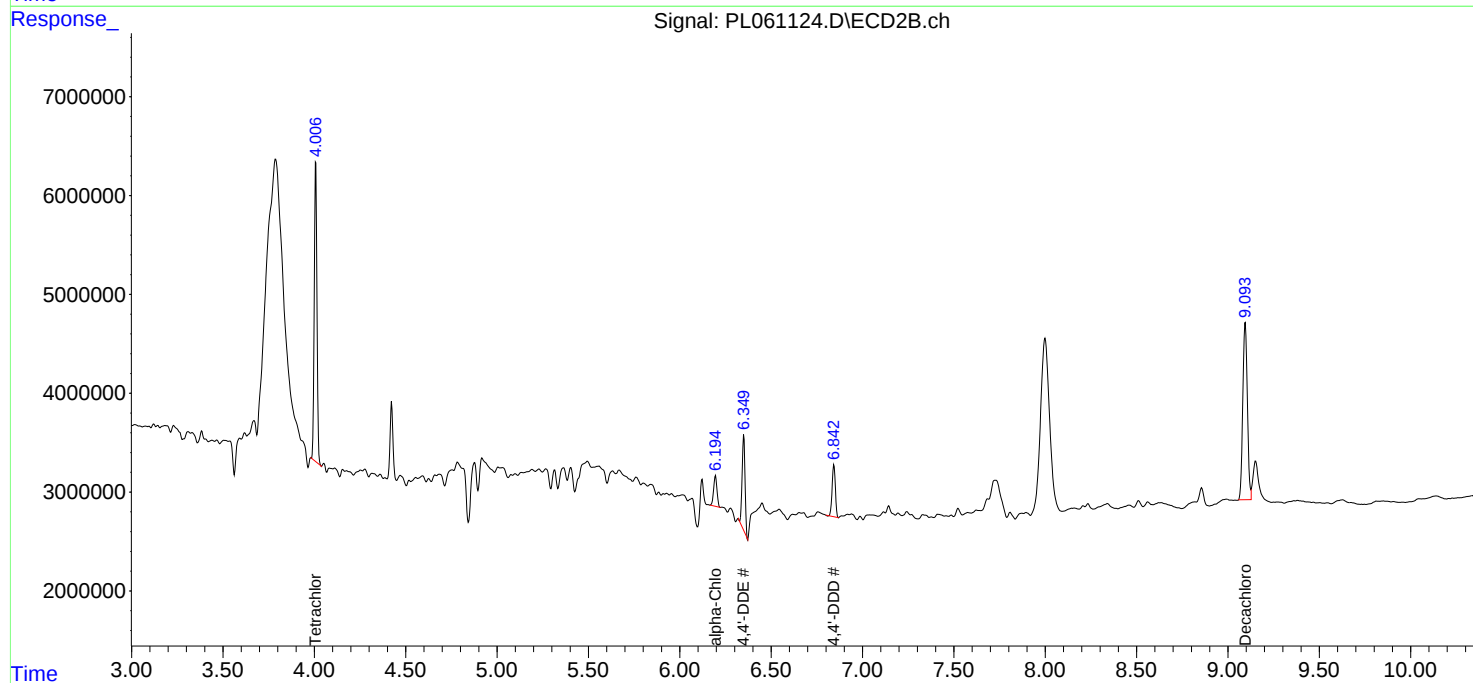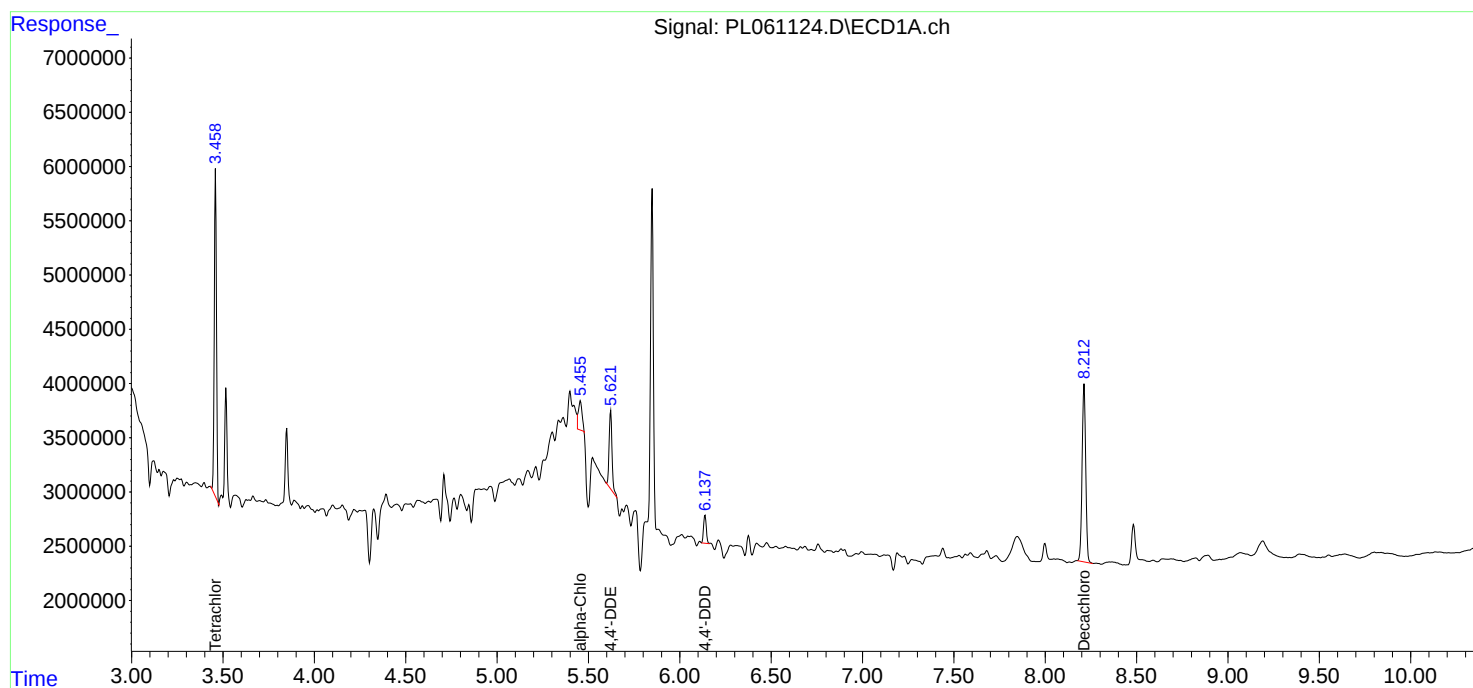

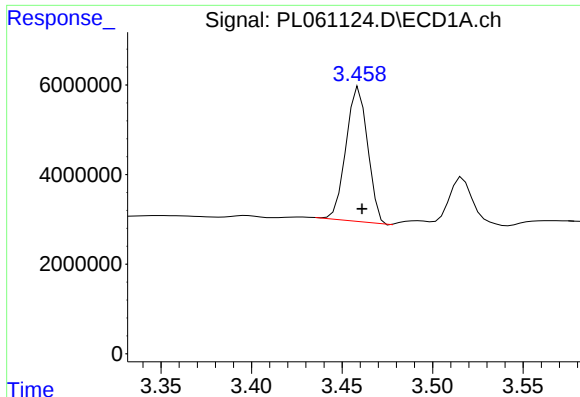


#1 Tetrachloro-m-xylene

R.T.: 3.460 min
Delta R.T.: -0.001 min
Response: 25036668
Conc: 13.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
LINDEN-JOP-BH-10-A


Manual Integrations
APPROVED

Ankita
9/2/2020 1:26:14 PM

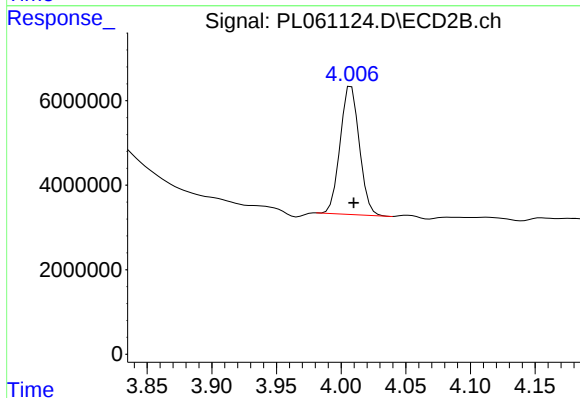


#1 Tetrachloro-m-xylene

R.T.: 4.008 min
Delta R.T.: -0.002 min
Response: 31372752
Conc: 12.07 ng/ml

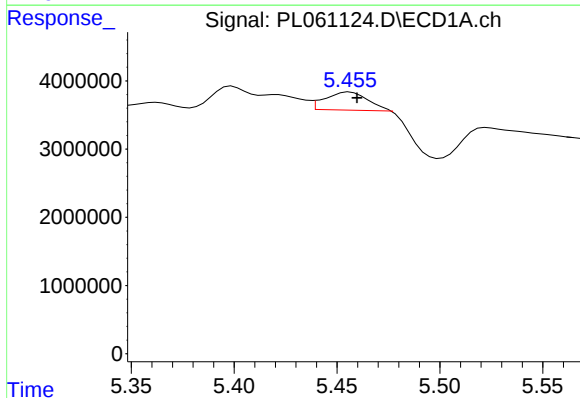


#11 alpha-Chlordane

R.T.: 5.455 min
Delta R.T.: -0.005 min
Response: 3732660
Conc: 1.91 ng/ml m

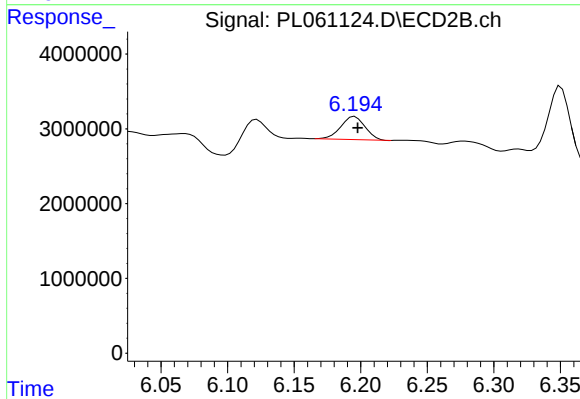

#11 alpha-Chlordane

R.T.: 6.196 min
Delta R.T.: -0.002 min
Response: 3913378
Conc: 1.26 ng/ml

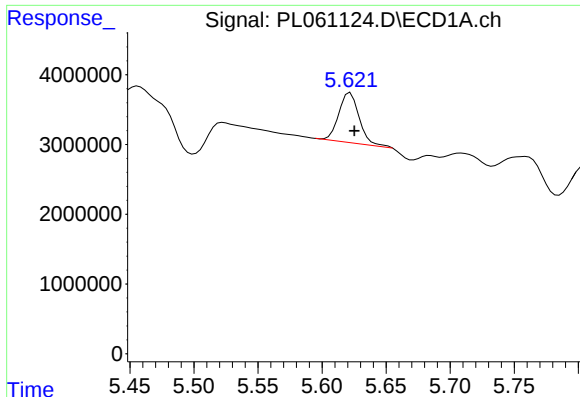


#12 4,4'-DDE

R.T.: 5.622 min
Delta R.T.: -0.003 min
Response: 7785308
Conc: 4.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
LINDEN-JOP-BH-10-A


Manual Integrations
APPROVED

Ankita
9/2/2020 1:26:14 PM

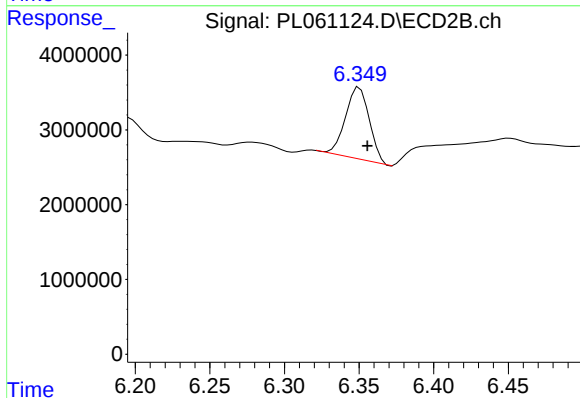


#12 4,4'-DDE

R.T.: 6.350 min
Delta R.T.: -0.005 min
Response: 10704627
Conc: 3.70 ng/ml

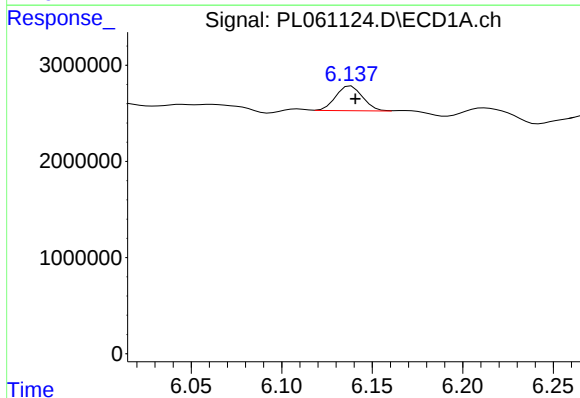


#16 4,4'-DDD

R.T.: 6.137 min
Delta R.T.: -0.004 min
Response: 2637534
Conc: 1.67 ng/ml m

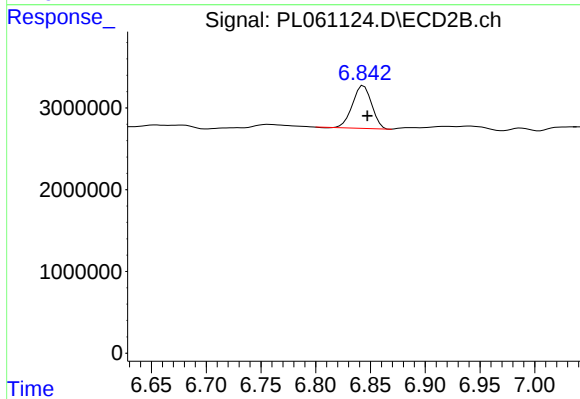

#16 4,4'-DDD

R.T.: 6.844 min
Delta R.T.: -0.004 min
Response: 6386442
Conc: 2.73 ng/ml

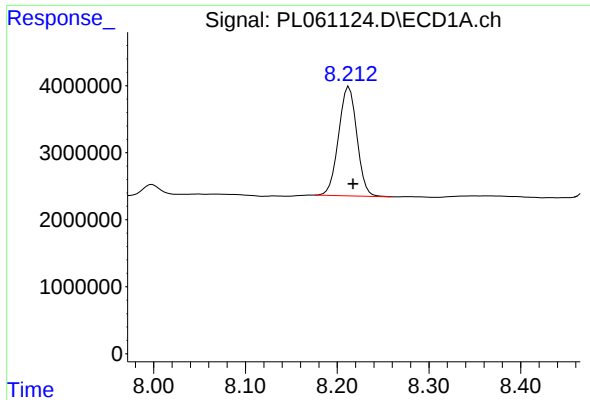


#28 Decachlorobiphenyl

R.T.: 8.212 min
Delta R.T.: -0.006 min
Response: 22605698
Conc: 13.42 ng/ml m

Instrument :
ECD_L
ClientSampleId :
LINDEN-JOP-BH-10-A

Manual Integrations
APPROVED

Ankita
9/2/2020 1:26:14 PM

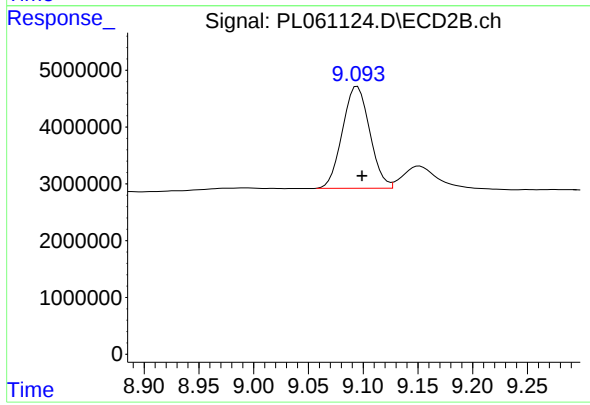

#28 Decachlorobiphenyl

R.T.: 9.093 min
Delta R.T.: -0.006 min
Response: 31188005
Conc: 14.78 ng/ml m