

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090120\
 Data File : PL061127.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Sep 2020 11:08
 Operator : DD\AJ
 Sample : L3848-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 LINDEN-BH-02-A

Manual Integrations
 APPROVED

Ankita
 9/2/2020 1:26:38 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 14:50:47 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 25 16:59:57 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.460	4.008	22748577	30047691	12.327	11.561
28)	SA Decachlor...	8.213	9.095	17499498	24798663	10.388	11.753
Target Compounds							
12)	B 4,4'-DDE	5.622	6.352	7201759	10491882	3.914	3.630
16)	A 4,4'-DDD	6.137	6.845	3139246	5159818	1.986	2.209
17)	MA 4,4'-DDT	6.375	7.142	2170574	2517939	1.436m	1.093m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090120\
Data File : PL061127.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Sep 2020 11:08
Operator : DD\AJ
Sample : L3848-03
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
LINDEN-BH-02-A


Manual Integrations
APPROVED

Ankita
9/2/2020 1:26:38 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 14:50:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
Quant Title : GC Extractables
QLast Update : Tue Aug 25 16:59:57 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

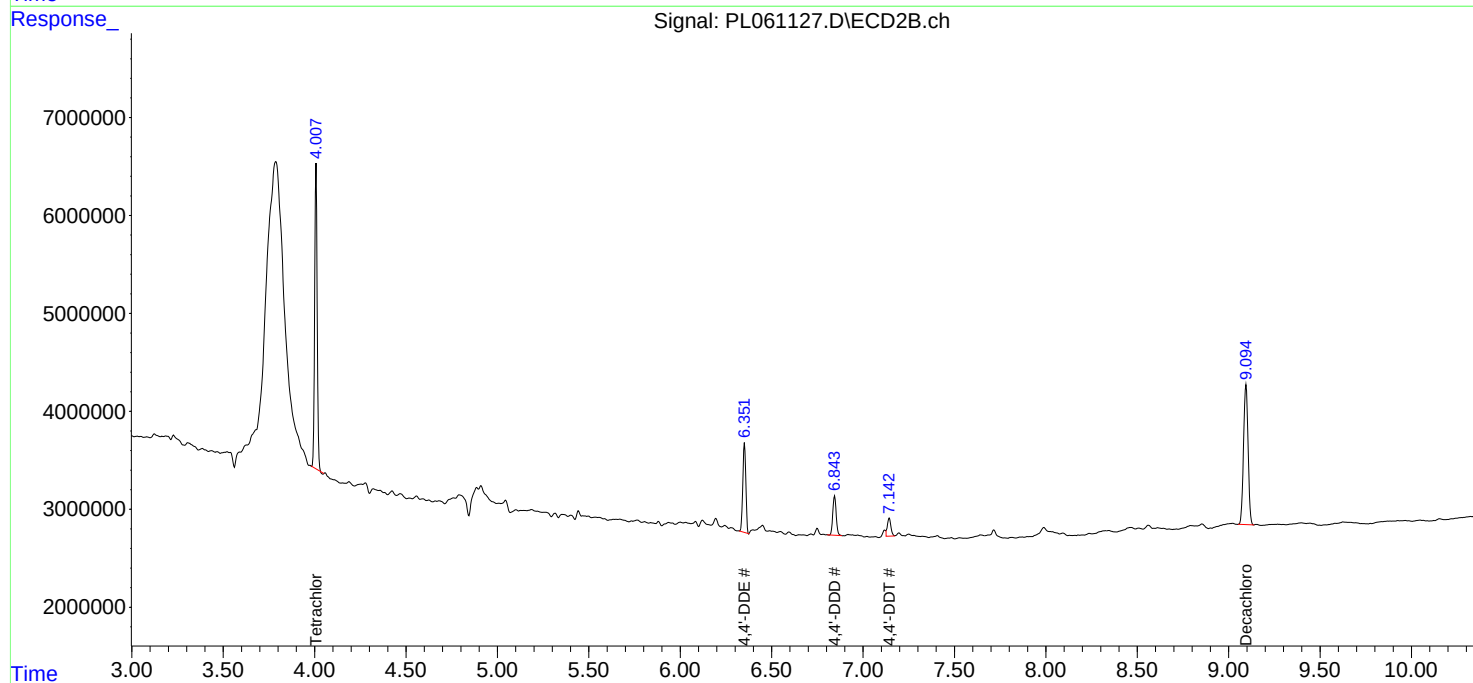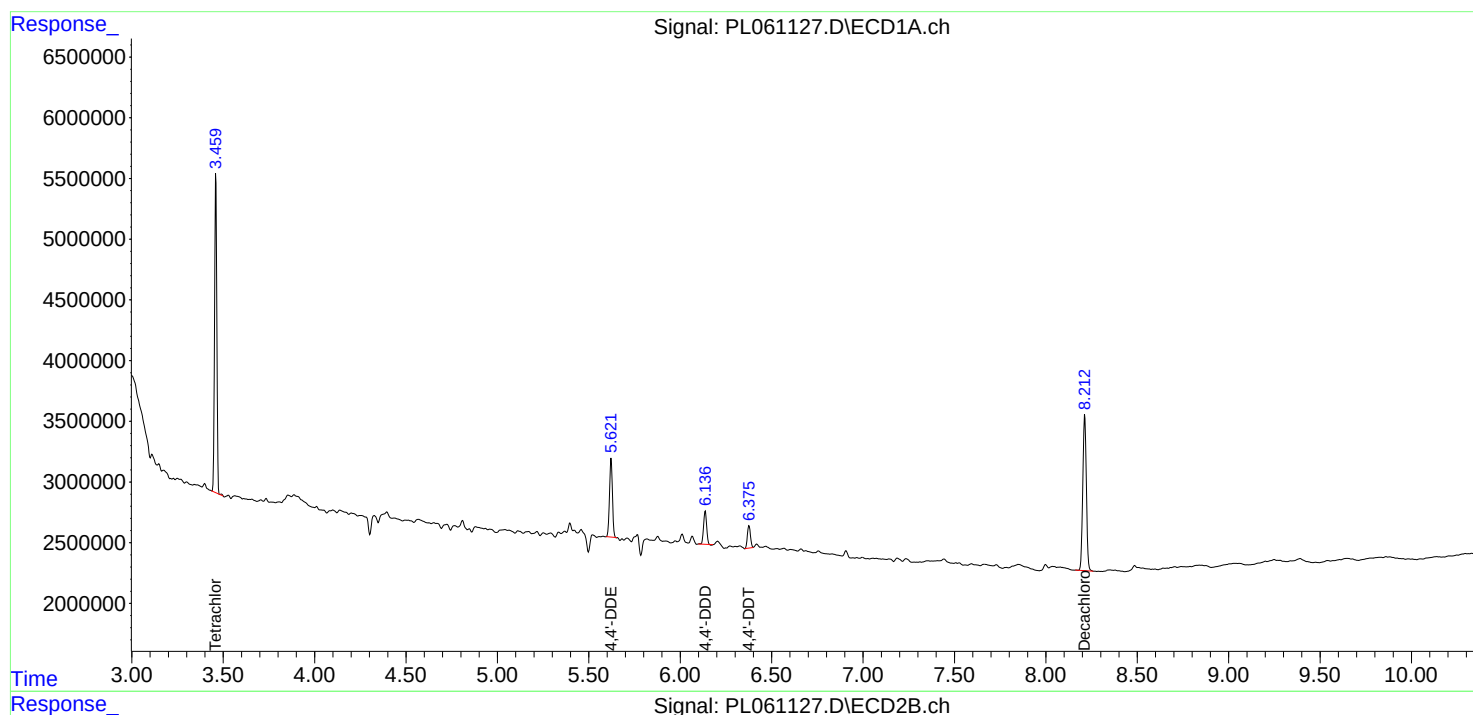

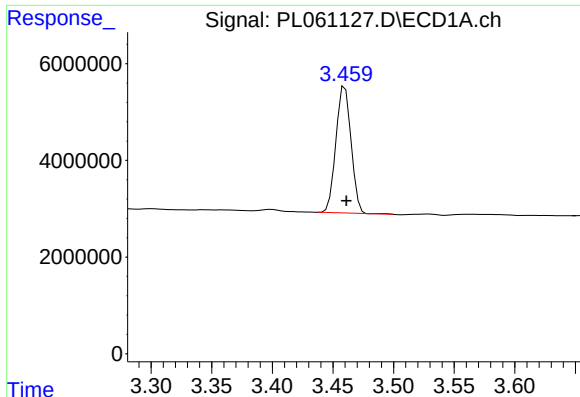


#1 Tetrachloro-m-xylene

R.T.: 3.460 min
Delta R.T.: 0.000 min
Response: 22748577
Conc: 12.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
LINDEN-BH-02-A


Manual Integrations
APPROVED

Ankita
9/2/2020 1:26:38 PM

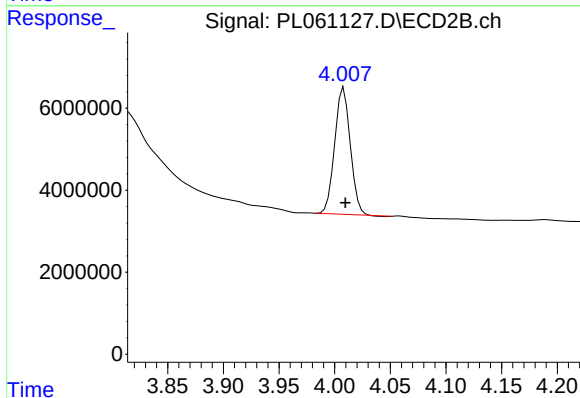


#1 Tetrachloro-m-xylene

R.T.: 4.008 min
Delta R.T.: -0.002 min
Response: 30047691
Conc: 11.56 ng/ml

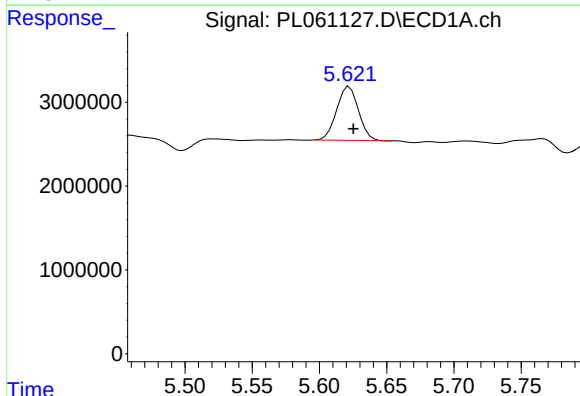


#12 4,4'-DDE

R.T.: 5.622 min
Delta R.T.: -0.003 min
Response: 7201759
Conc: 3.91 ng/ml

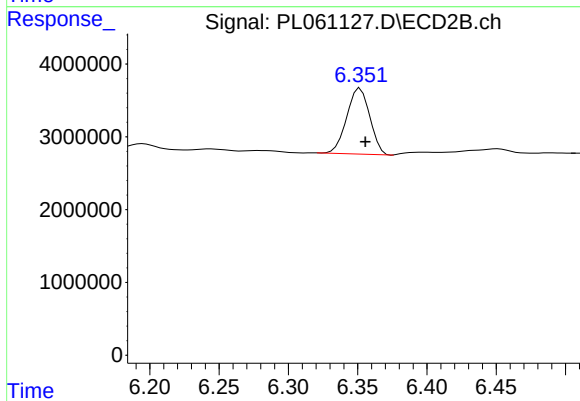

#12 4,4'-DDE

R.T.: 6.352 min
Delta R.T.: -0.004 min
Response: 10491882
Conc: 3.63 ng/ml

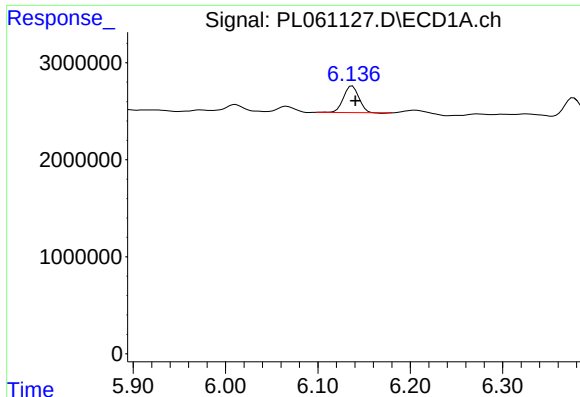


#16 4,4'-DDD

R.T.: 6.137 min
Delta R.T.: -0.003 min
Response: 3139246
Conc: 1.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
LINDEN-BH-02-A


Manual Integrations
APPROVED

Ankita
9/2/2020 1:26:38 PM

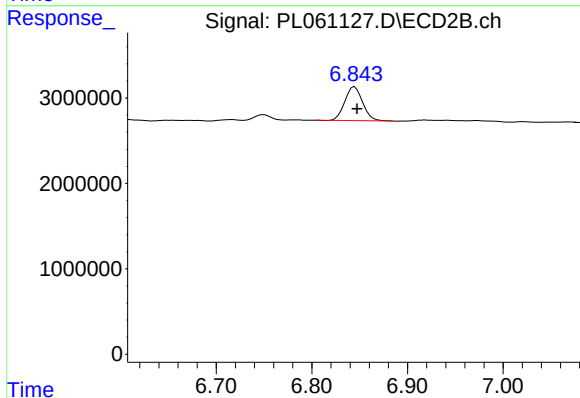


#16 4,4'-DDD

R.T.: 6.845 min
Delta R.T.: -0.003 min
Response: 5159818
Conc: 2.21 ng/ml

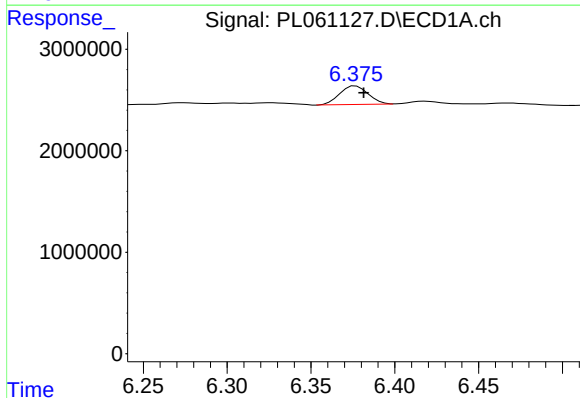


#17 4,4'-DDT

R.T.: 6.375 min
Delta R.T.: -0.006 min
Response: 2170574
Conc: 1.44 ng/ml m

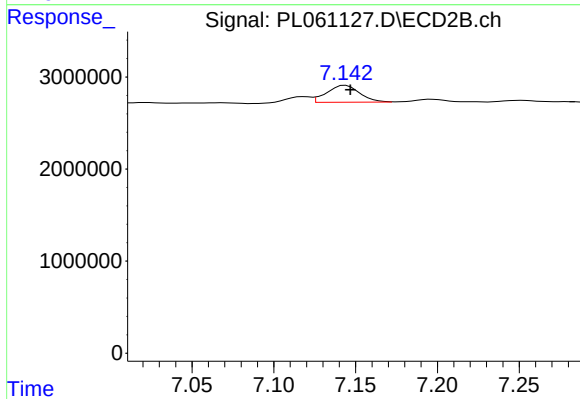

#17 4,4'-DDT

R.T.: 7.142 min
Delta R.T.: -0.004 min
Response: 2517939
Conc: 1.09 ng/ml m

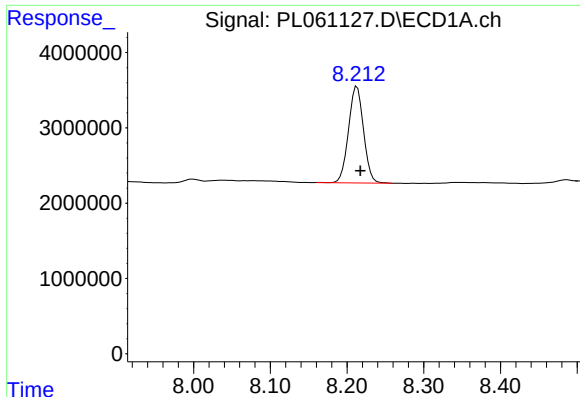


#28 Decachlorobiphenyl

R.T.: 8.213 min
Delta R.T.: -0.004 min
Response: 17499498
Conc: 10.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
LINDEN-BH-02-A

Manual Integrations
APPROVED

Ankita
9/2/2020 1:26:38 PM

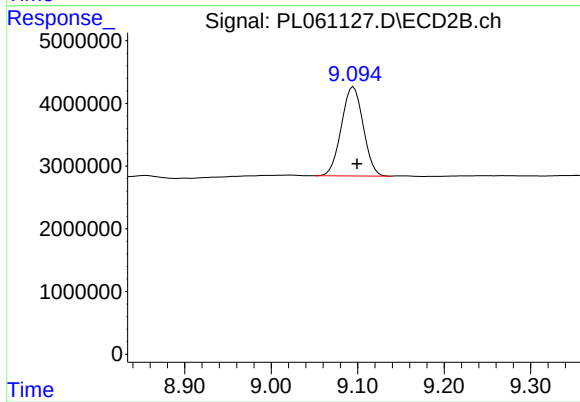

#28 Decachlorobiphenyl

R.T.: 9.095 min
Delta R.T.: -0.004 min
Response: 24798663
Conc: 11.75 ng/ml