

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090120\
 Data File : PL061129.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Sep 2020 11:36
 Operator : DD\AJ
 Sample : L3848-11
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 LINDEN-BH-04-A

Manual Integrations
 APPROVED

Ankita
 9/2/2020 1:26:40 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 14:51:05 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 25 16:59:57 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.460	4.008	24122780	31969192	13.072	12.300
28)	SA Decachlor...	8.212	9.095	20155776	28062086	11.965	13.299
Target Compounds							
12)	B 4,4'-DDE	5.622	6.351	3718278	5189520	2.021	1.796
17)	MA 4,4'-DDT	6.375	7.142	1373601	1489226	0.909m	0.647m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090120\
Data File : PL061129.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Sep 2020 11:36
Operator : DD\AJ
Sample : L3848-11
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
LINDEN-BH-04-A


Manual Integrations
APPROVED

Ankita
9/2/2020 1:26:40 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 14:51:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
Quant Title : GC Extractables
QLast Update : Tue Aug 25 16:59:57 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

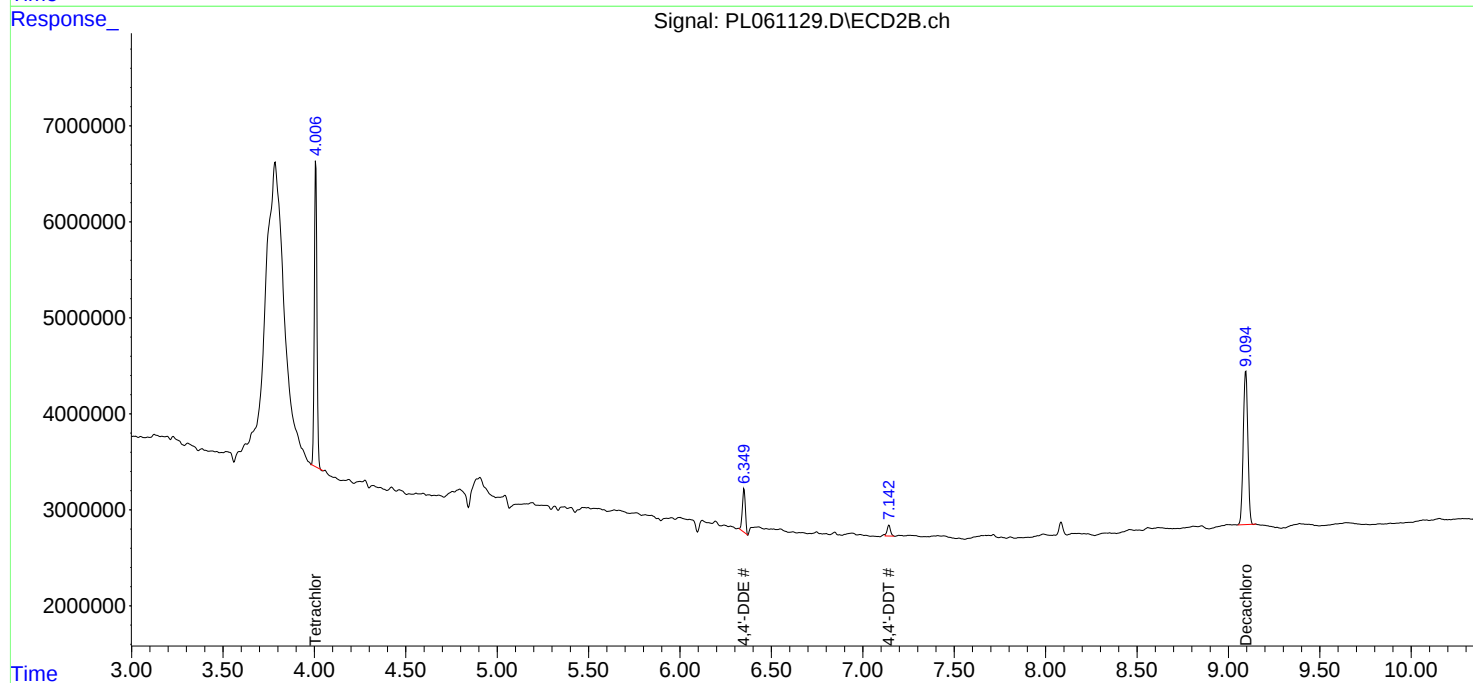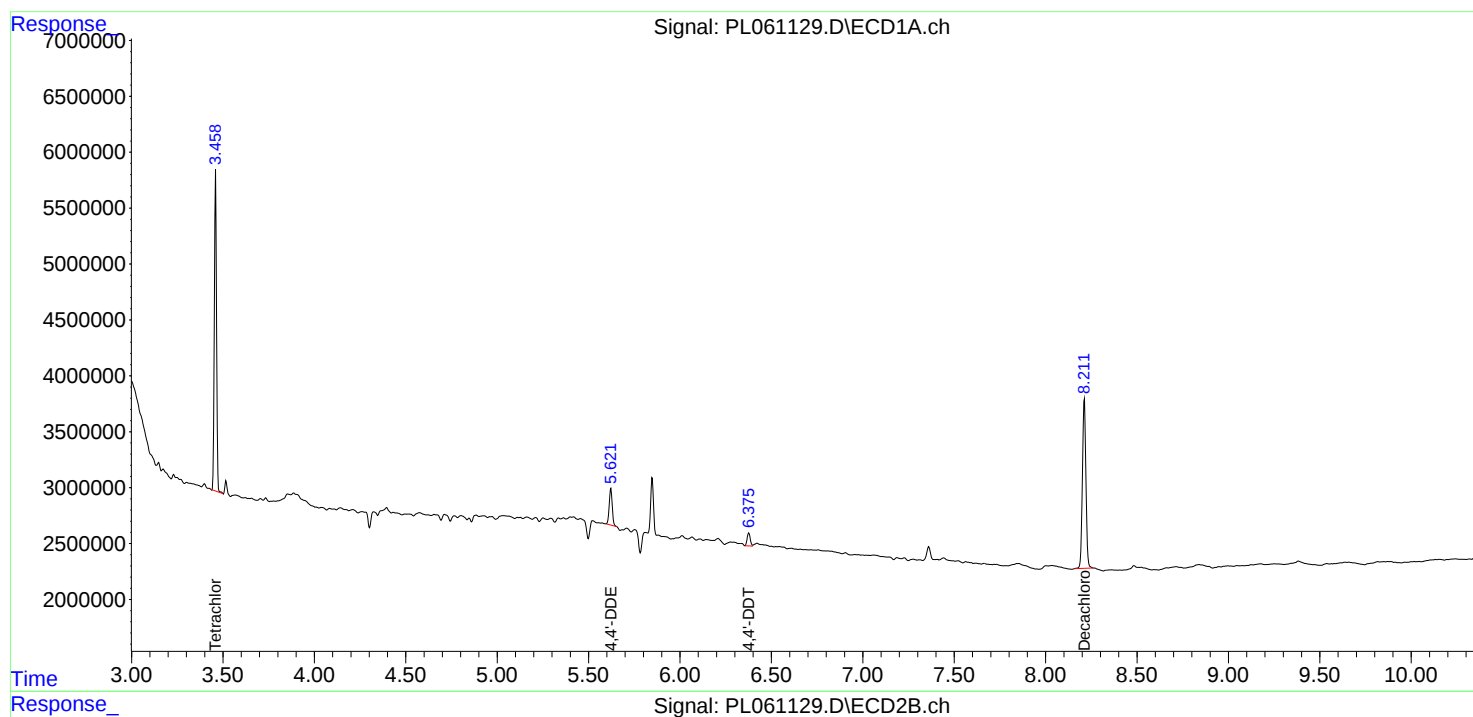

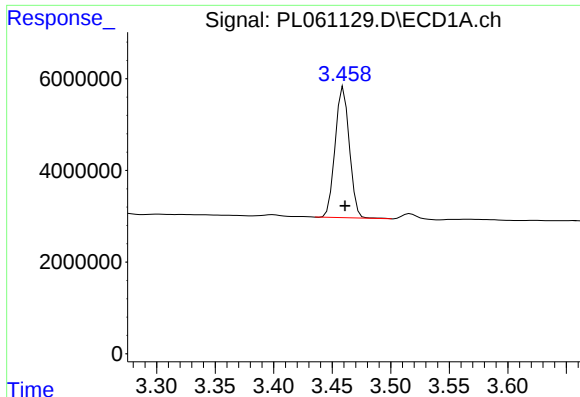


#1 Tetrachloro-m-xylene

R.T.: 3.460 min
Delta R.T.: -0.001 min
Response: 24122780
Conc: 13.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
LINDEN-BH-04-A


Manual Integrations
APPROVED

Ankita
9/2/2020 1:26:40 PM

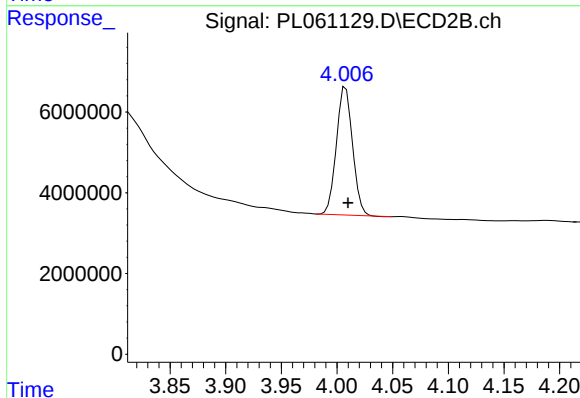


#1 Tetrachloro-m-xylene

R.T.: 4.008 min
Delta R.T.: -0.002 min
Response: 31969192
Conc: 12.30 ng/ml

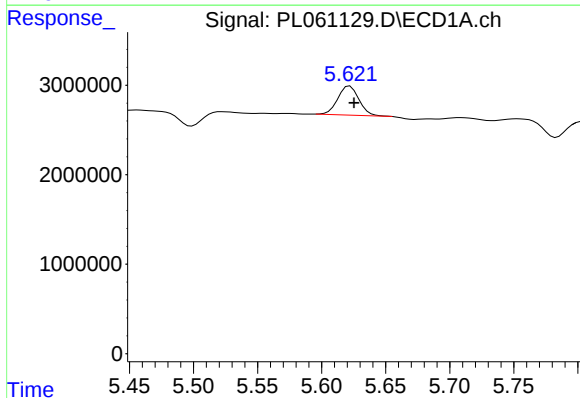


#12 4,4'-DDE

R.T.: 5.622 min
Delta R.T.: -0.003 min
Response: 3718278
Conc: 2.02 ng/ml

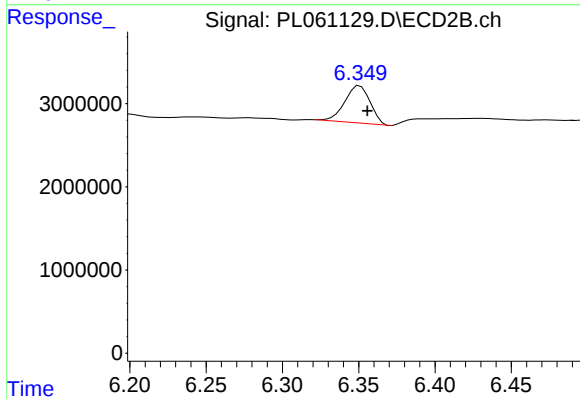

#12 4,4'-DDE

R.T.: 6.351 min
Delta R.T.: -0.005 min
Response: 5189520
Conc: 1.80 ng/ml

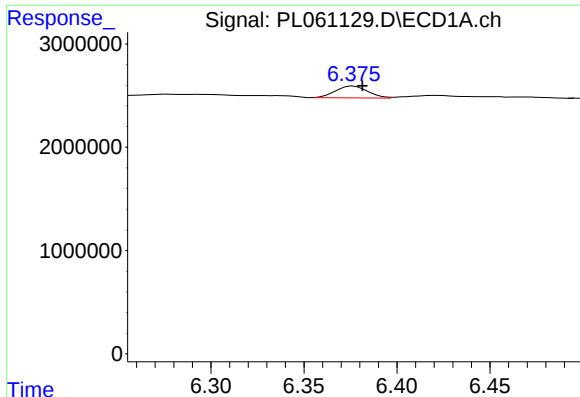


#17 4,4'-DDT

R.T.: 6.375 min
Delta R.T.: -0.006 min
Response: 1373601
Conc: 0.91 ng/ml m

Instrument :
ECD_L
ClientSampleId :
LINDEN-BH-04-A


Manual Integrations
APPROVED

Ankita
9/2/2020 1:26:40 PM

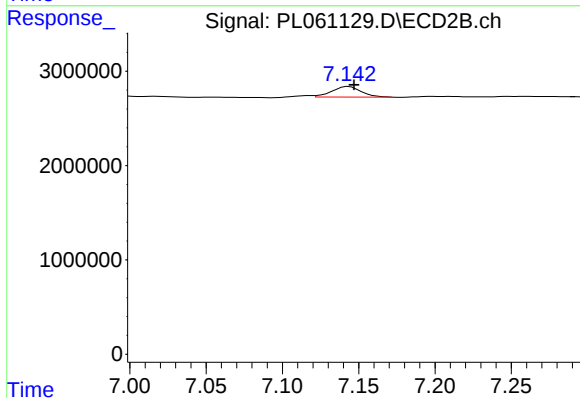


#17 4,4'-DDT

R.T.: 7.142 min
Delta R.T.: -0.005 min
Response: 1489226
Conc: 0.65 ng/ml m

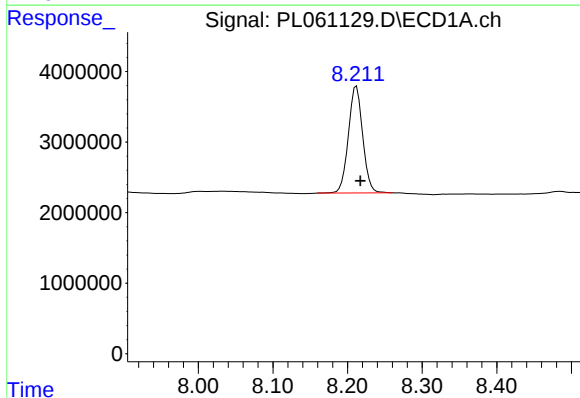

#28 Decachlorobiphenyl

R.T.: 8.212 min
Delta R.T.: -0.005 min
Response: 20155776
Conc: 11.96 ng/ml

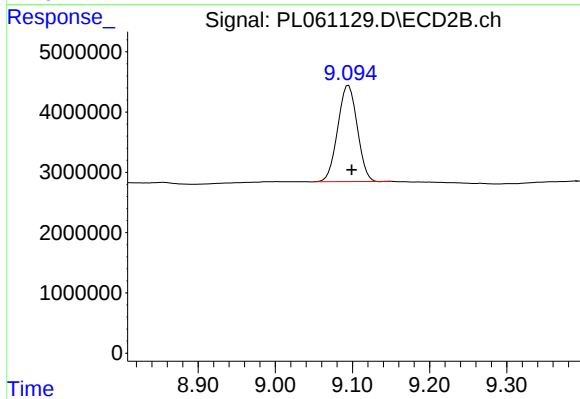

#28 Decachlorobiphenyl

R.T.: 9.095 min
Delta R.T.: -0.004 min
Response: 28062086
Conc: 13.30 ng/ml