

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090120\
 Data File : PL061171.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Sep 2020 23:40
 Operator : DD\AJ
 Sample : L3851-12
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 24743

Manual Integrations
 APPROVED

Ankita
 9/2/2020 1:27:00 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 02 07:31:07 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 25 16:59:57 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.461	4.008	35022987	49199876	18.979	18.930m
28)	SA Decachlor...	8.214	9.096	30568287	41962893	18.146	19.887

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090120\
Data File : PL061171.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Sep 2020 23:40
Operator : DD\AJ
Sample : L3851-12
Misc :
ALS Vial : 50 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
24743


Manual Integrations
APPROVED

Ankita
9/2/2020 1:27:00 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 02 07:31:07 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
Quant Title : GC Extractables
QLast Update : Tue Aug 25 16:59:57 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

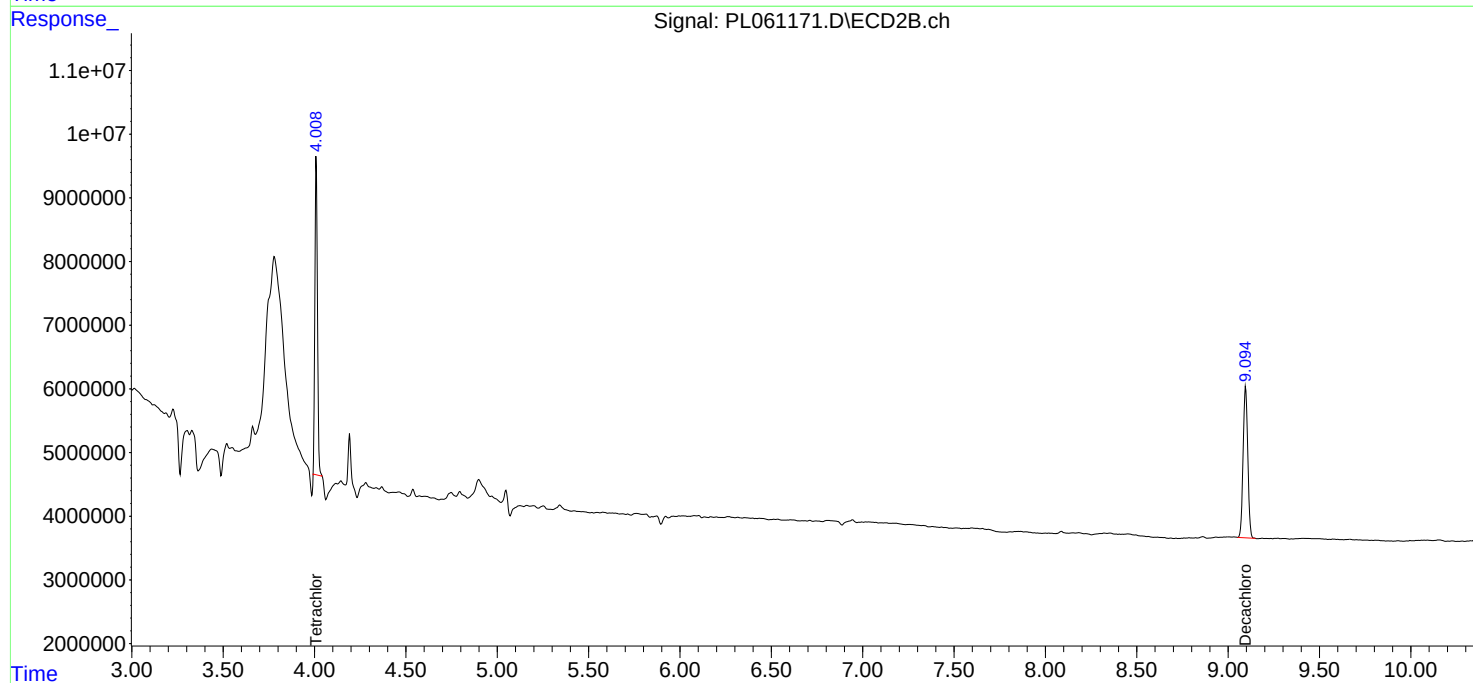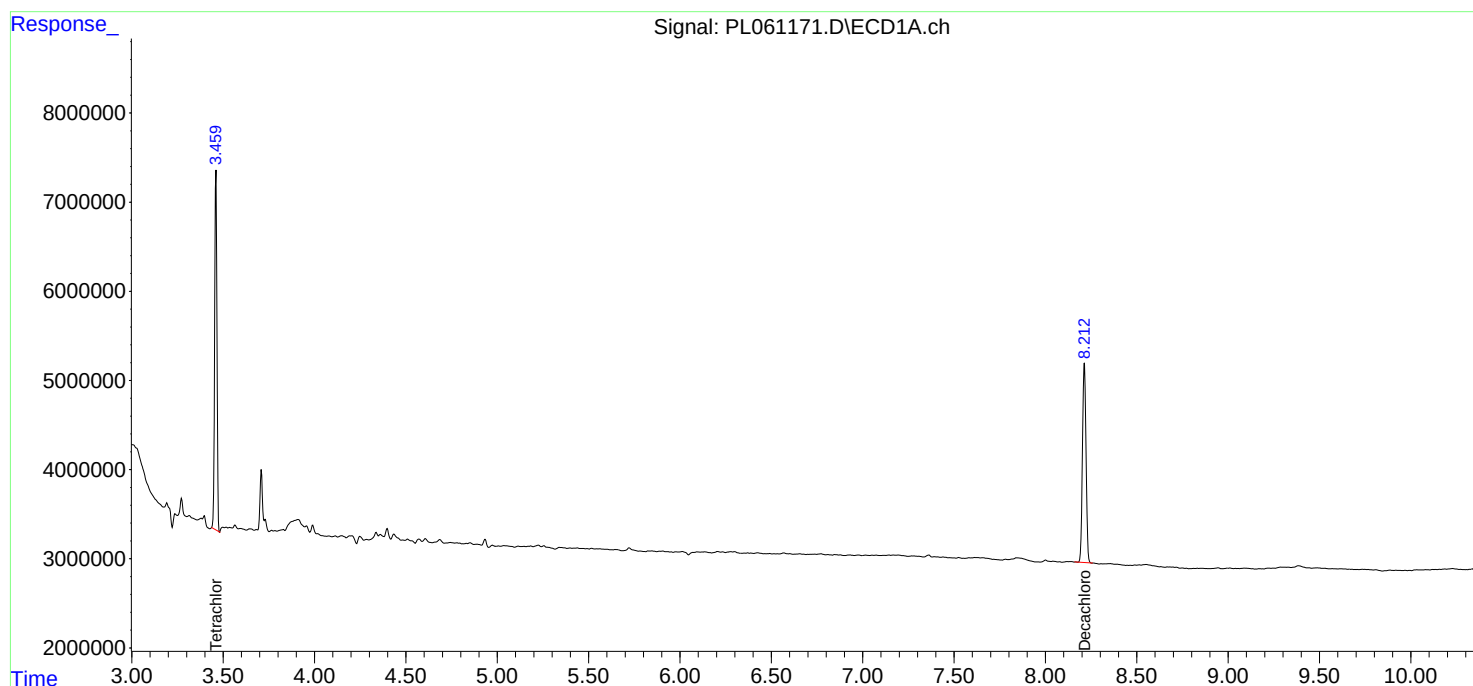

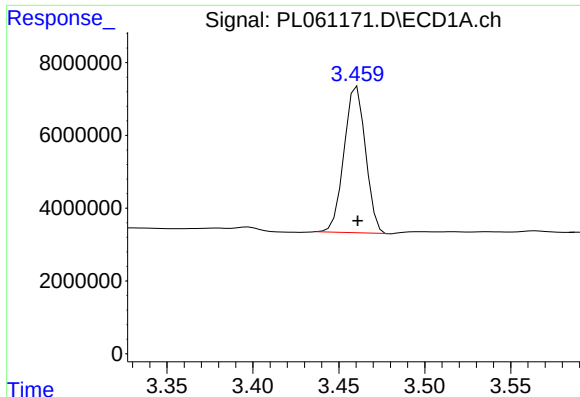


#1 Tetrachloro-m-xylene

R.T.: 3.461 min
Delta R.T.: 0.000 min
Response: 35022987
Conc: 18.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
24743


Manual Integrations
APPROVED

Ankita
9/2/2020 1:27:00 PM

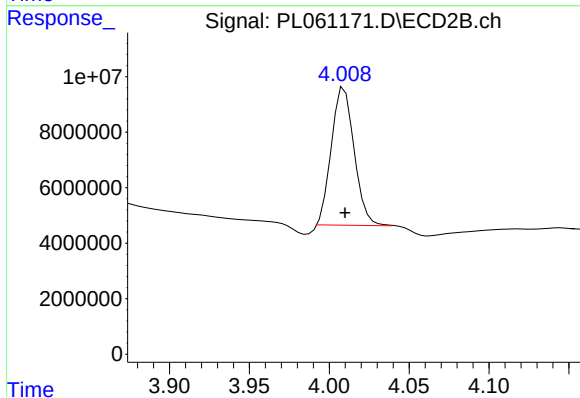


#1 Tetrachloro-m-xylene

R.T.: 4.008 min
Delta R.T.: -0.002 min
Response: 49199876
Conc: 18.93 ng/ml m

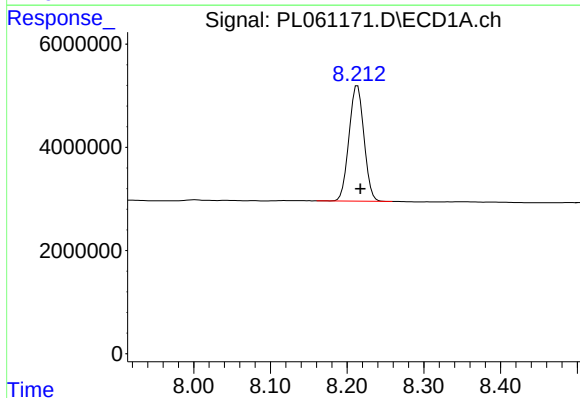

#28 Decachlorobiphenyl

R.T.: 8.214 min
Delta R.T.: -0.004 min
Response: 30568287
Conc: 18.15 ng/ml

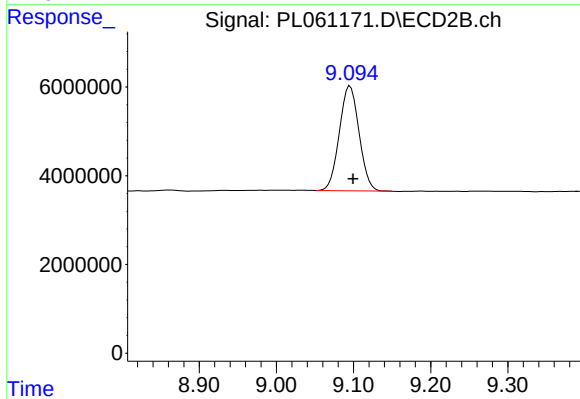

#28 Decachlorobiphenyl

R.T.: 9.096 min
Delta R.T.: -0.004 min
Response: 41962893
Conc: 19.89 ng/ml