

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090120\
 Data File : PL061174.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Sep 2020 00:22
 Operator : DD\AJ
 Sample : L3852-03
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 251378

Manual Integrations
 APPROVED

Ankita
 9/2/2020 1:27:02 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 02 07:31:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 25 16:59:57 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.461	4.010	31752941	43351858	17.207	16.680
28) SA Decachlor...	8.213	9.096	28430371	38703694	16.876	18.343
Target Compounds						
8) B Heptachlo...	5.173	5.884	2540353	2231152	1.288	0.853m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090120\
Data File : PL061174.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Sep 2020 00:22
Operator : DD\AJ
Sample : L3852-03
Misc :
ALS Vial : 53 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
251378


Manual Integrations
APPROVED

Ankita
9/2/2020 1:27:02 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 02 07:31:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
Quant Title : GC Extractables
QLast Update : Tue Aug 25 16:59:57 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

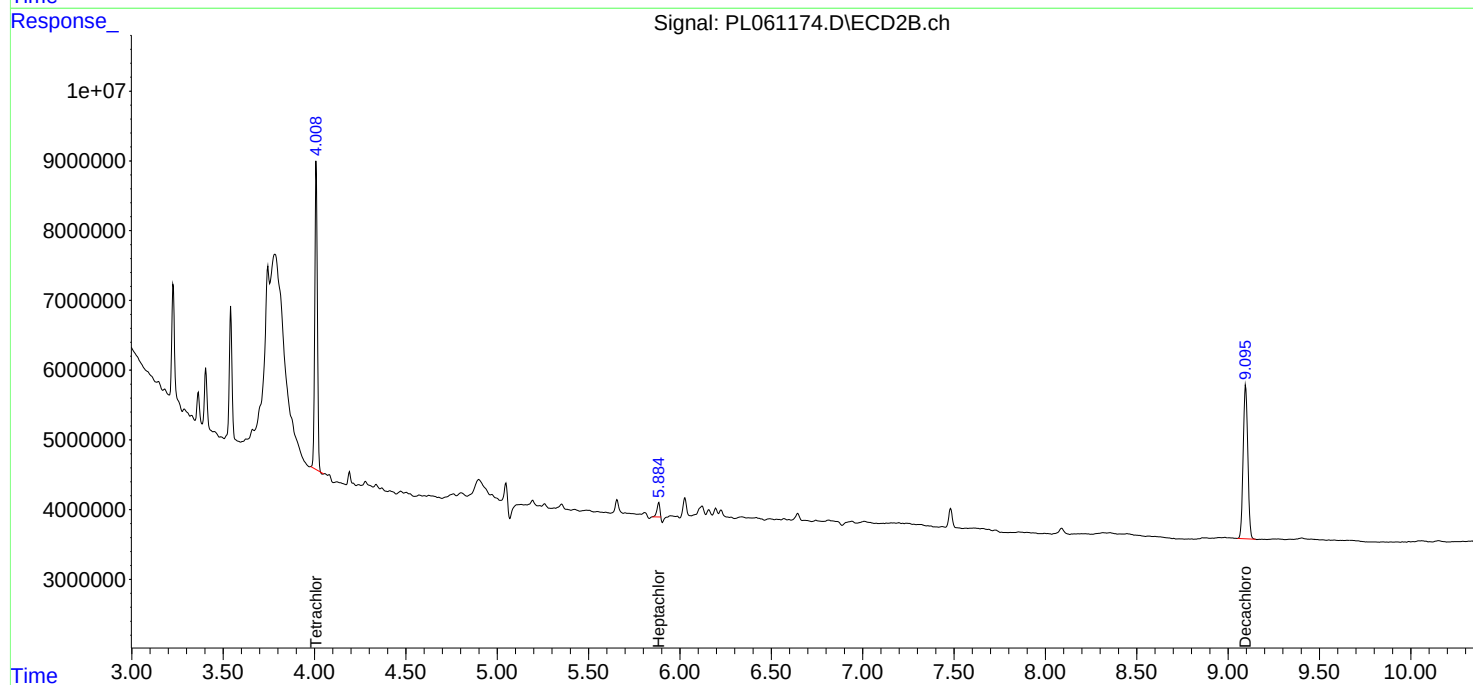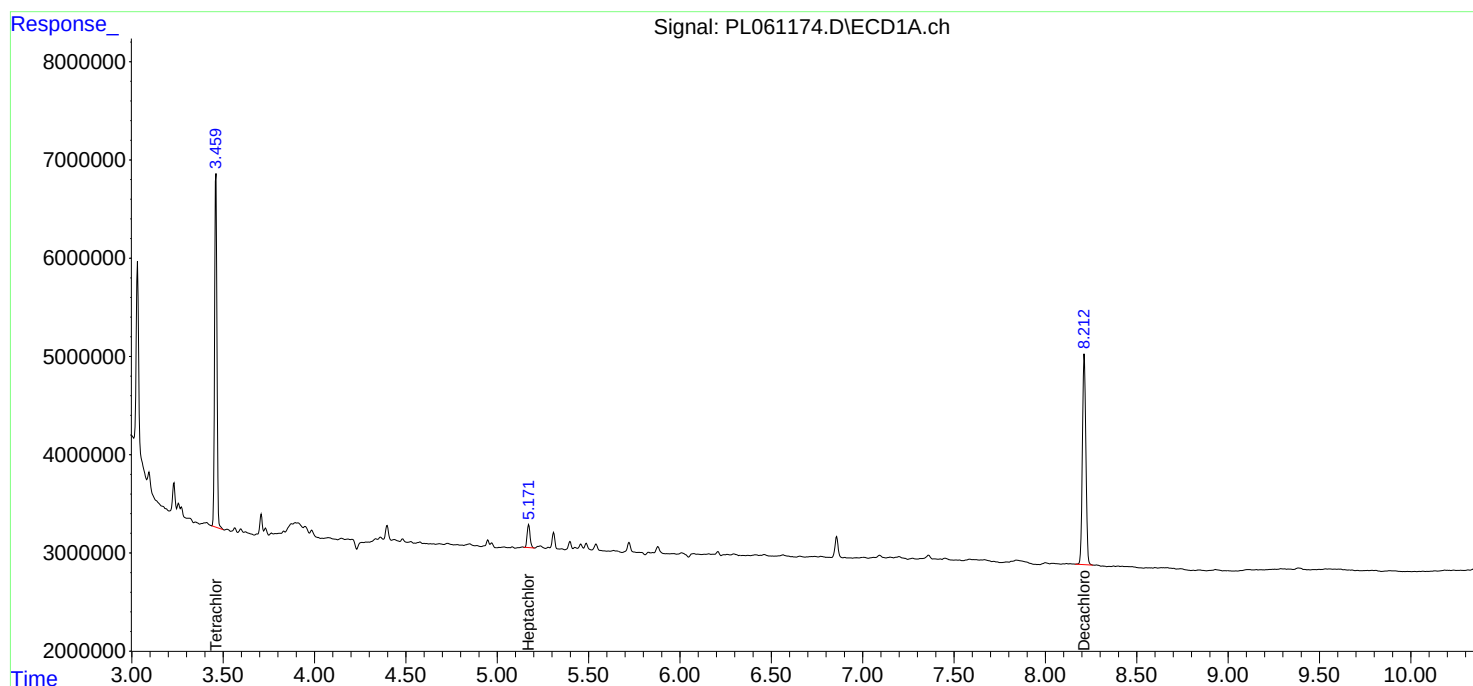

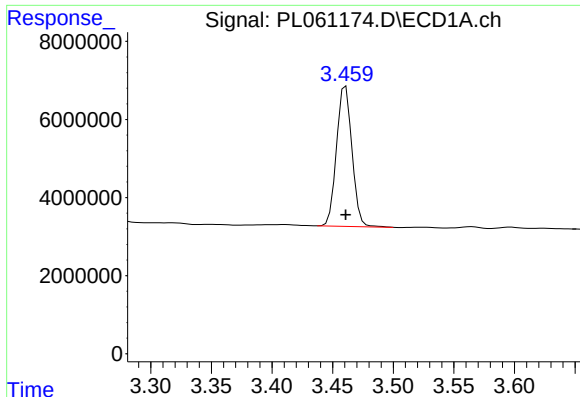


#1 Tetrachloro-m-xylene

R.T.: 3.461 min
Delta R.T.: 0.000 min
Response: 31752941
Conc: 17.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
251378


Manual Integrations
APPROVED

Ankita
9/2/2020 1:27:02 PM

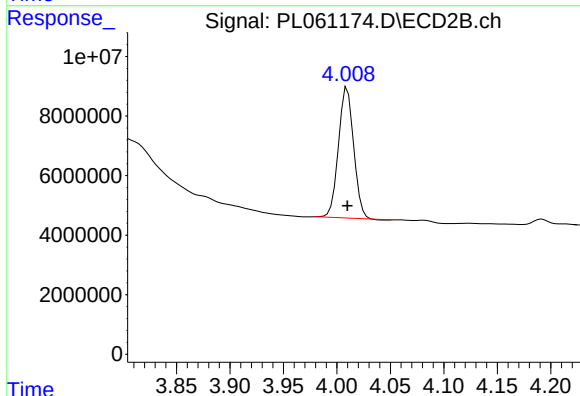


#1 Tetrachloro-m-xylene

R.T.: 4.010 min
Delta R.T.: 0.000 min
Response: 43351858
Conc: 16.68 ng/ml

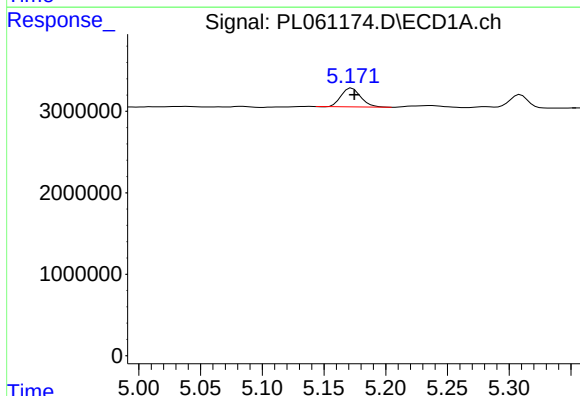


#8 Heptachlor epoxide

R.T.: 5.173 min
Delta R.T.: -0.002 min
Response: 2540353
Conc: 1.29 ng/ml

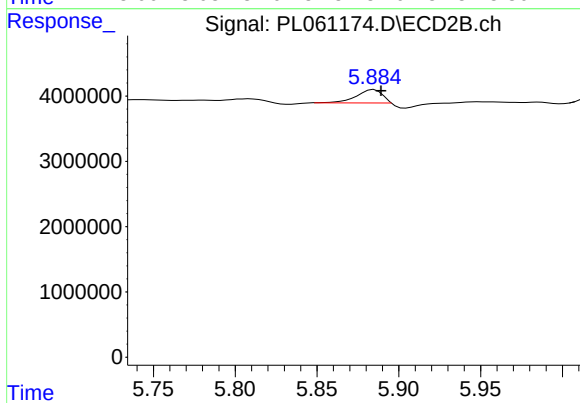

#8 Heptachlor epoxide

R.T.: 5.884 min
Delta R.T.: -0.006 min
Response: 2231152
Conc: 0.85 ng/ml m

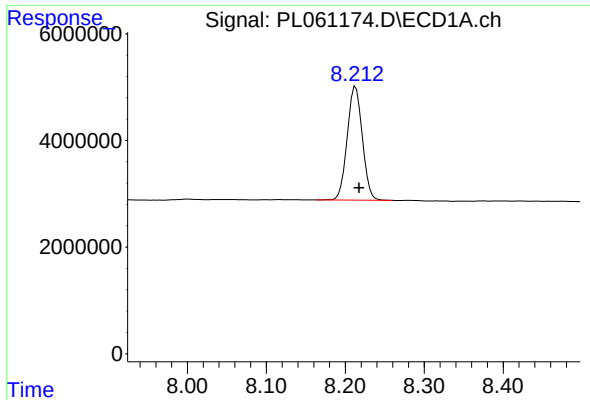


#28 Decachlorobiphenyl

R.T.: 8.213 min
Delta R.T.: -0.004 min
Response: 28430371
Conc: 16.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
251378

Manual Integrations
APPROVED

Ankita
9/2/2020 1:27:02 PM

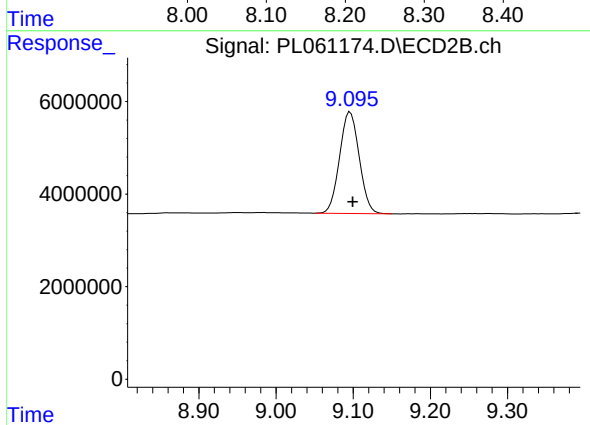

#28 Decachlorobiphenyl

R.T.: 9.096 min
Delta R.T.: -0.003 min
Response: 38703694
Conc: 18.34 ng/ml