

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090122\
 Data File : PL077456.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Sep 2022 18:23
 Operator : AR\AJ
 Sample : N4455-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 KTS2-WC-L-MH-02

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/02/2022
 Supervised By : Ankita Jodhani 09/02/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 02 01:16:25 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082222.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 23 05:36:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.417	2.629	15445426	29802905	11.351	9.697m
2) SA Decachlor...	8.907	7.731	6565895	11363896	5.603	4.073 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090122\
Data File : PL077456.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Sep 2022 18:23
Operator : AR\AJ
Sample : N4455-01
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
KTS2-WC-L-MH-02


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 09/02/2022
Supervised By : Ankita Jodhani 09/02/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 02 01:16:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082222.M
Quant Title : GC Extractables
QLast Update : Tue Aug 23 05:36:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

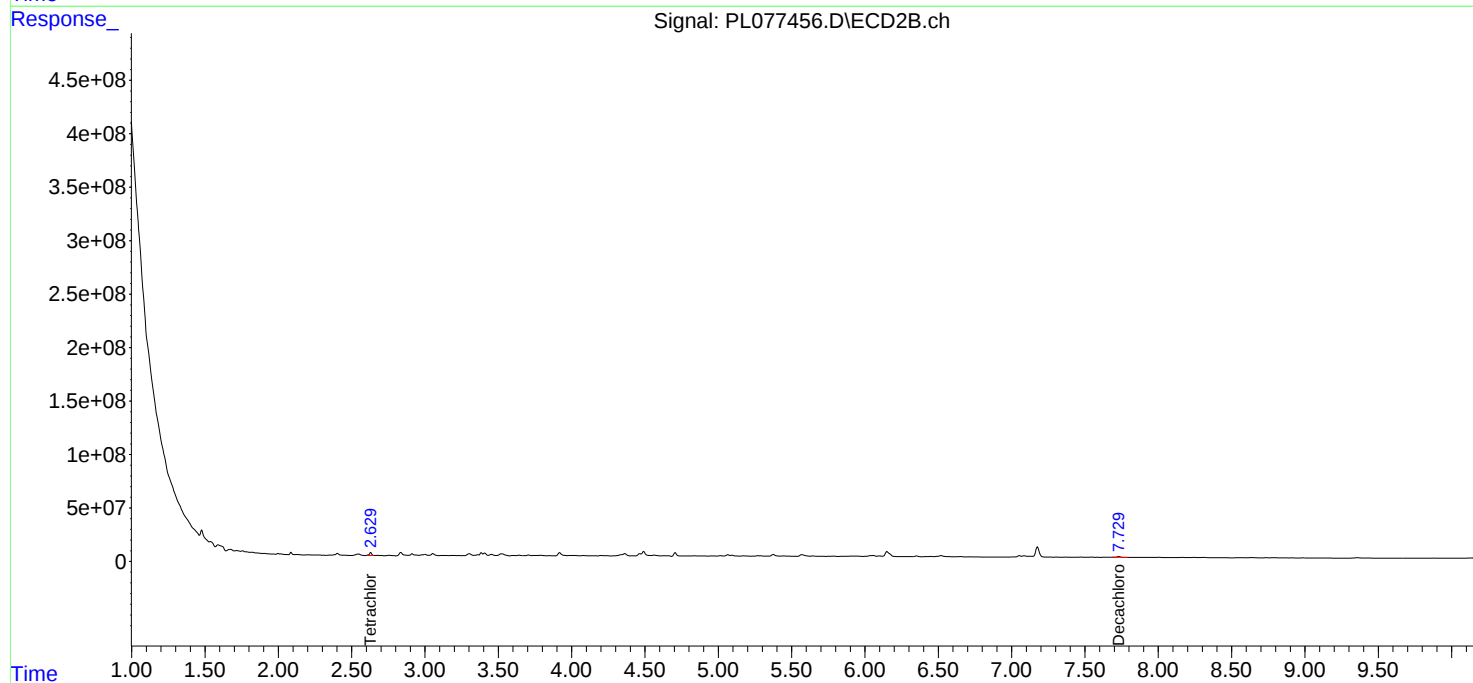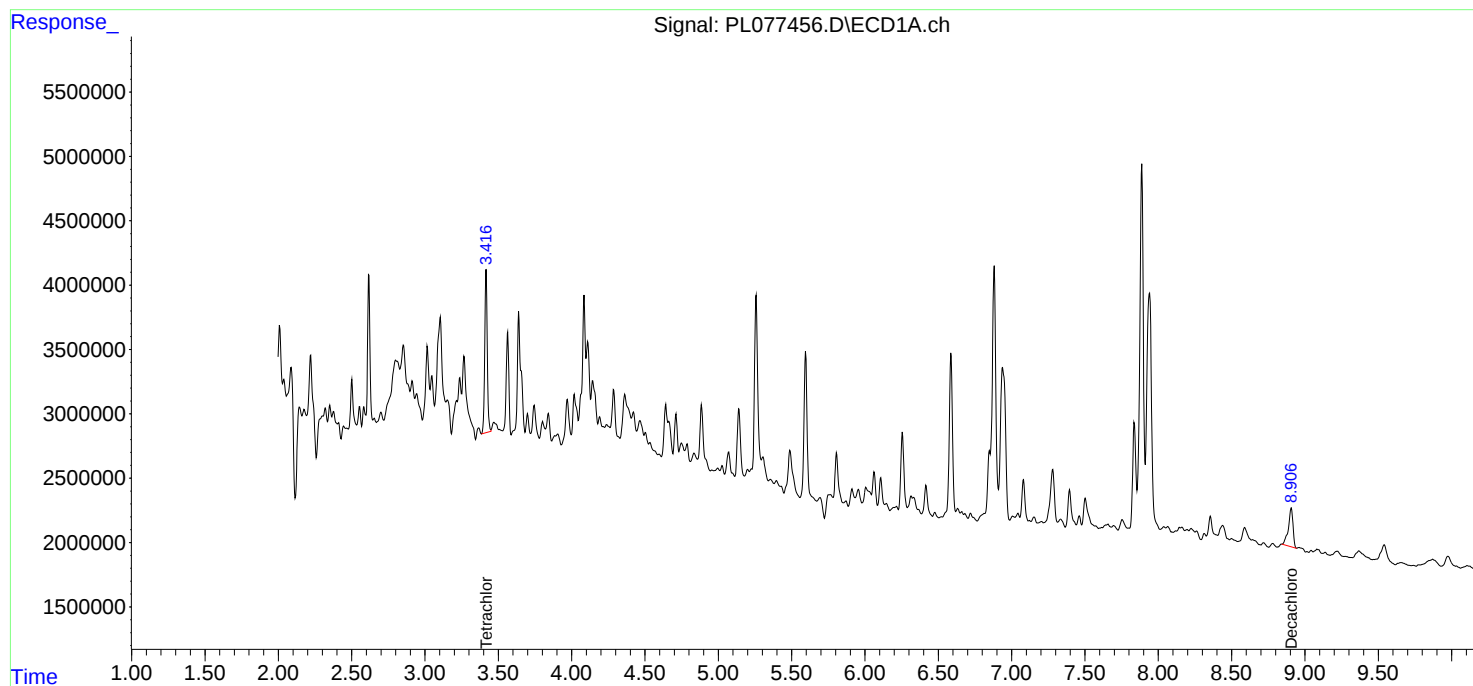

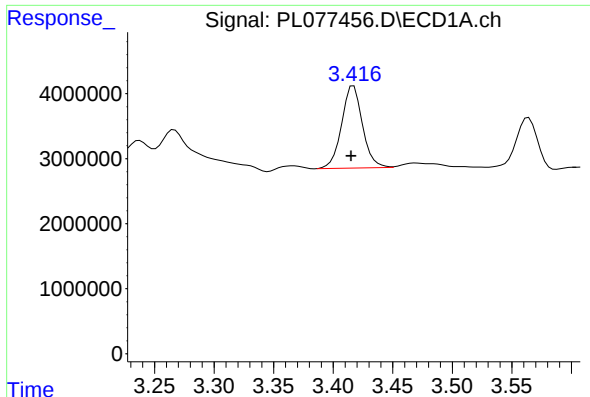


#1 Tetrachloro-m-xylene

R.T.: 3.417 min
Delta R.T.: 0.002 min
Response: 15445426
Conc: 11.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
KTS2-WC-L-MH-02


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/02/2022
Supervised By :Ankita Jodhani 09/02/2022

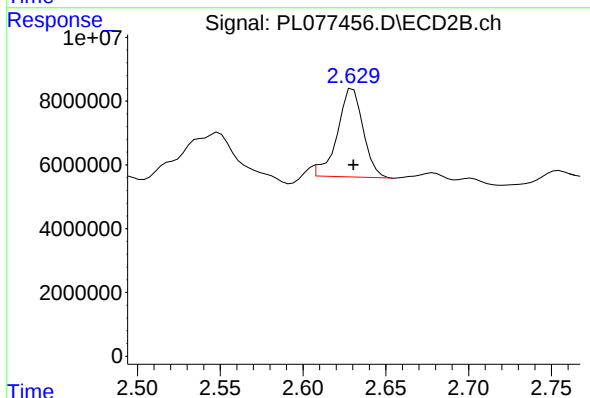


#1 Tetrachloro-m-xylene

R.T.: 2.629 min
Delta R.T.: -0.002 min
Response: 29802905
Conc: 9.70 ng/ml m

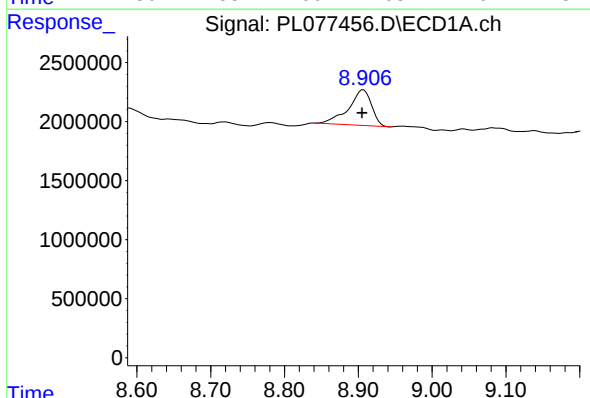

#28 Decachlorobiphenyl

R.T.: 8.907 min
Delta R.T.: 0.002 min
Response: 6565895
Conc: 5.60 ng/ml

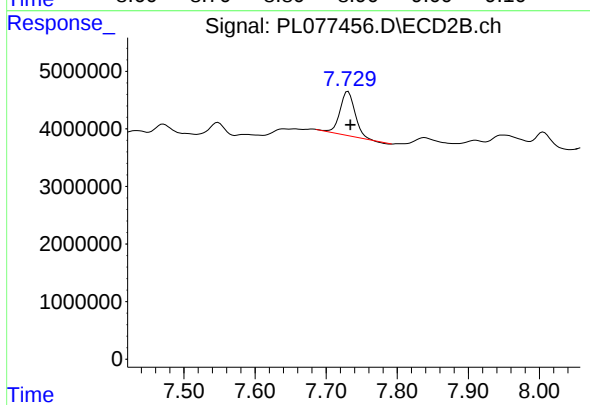

#28 Decachlorobiphenyl

R.T.: 7.731 min
Delta R.T.: -0.003 min
Response: 11363896
Conc: 4.07 ng/ml