

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090124\
 Data File : PL091458.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Aug 2024 17:28
 Operator : AR\AJ
 Sample : P3795-03
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 239

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 03:39:36 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081324.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 14 13:09:19 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	2.784	23695771	25100464	11.036m	12.859
28)	SA Decachlor...	9.052	7.921	22940770	27473345	15.048	14.505
Target Compounds							
11)	B alpha-Chl...	6.021	5.046	1403902	721975	0.583m	0.307m#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090124\
Data File : PL091458.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Aug 2024 17:28
Operator : AR\AJ
Sample : P3795-03
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
239

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 03:39:36 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081324.M
Quant Title : GC Extractables
QLast Update : Wed Aug 14 13:09:19 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

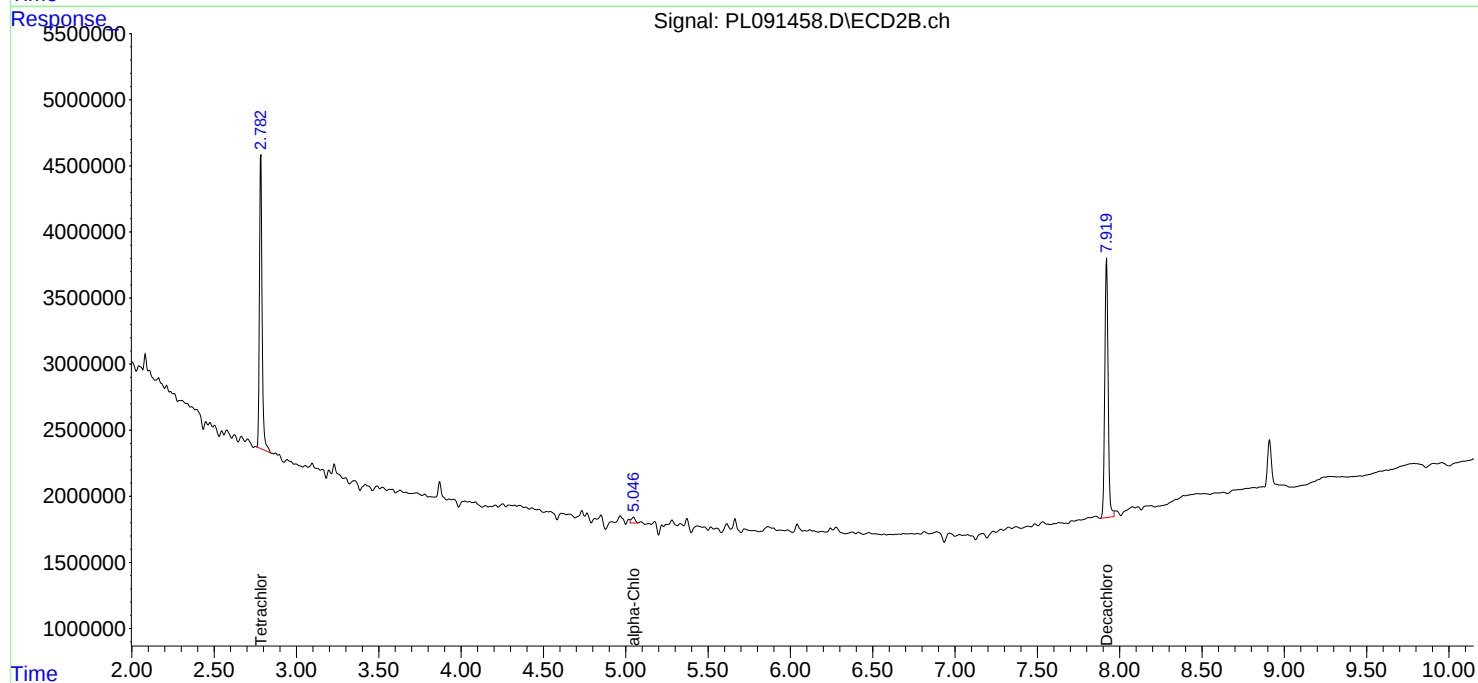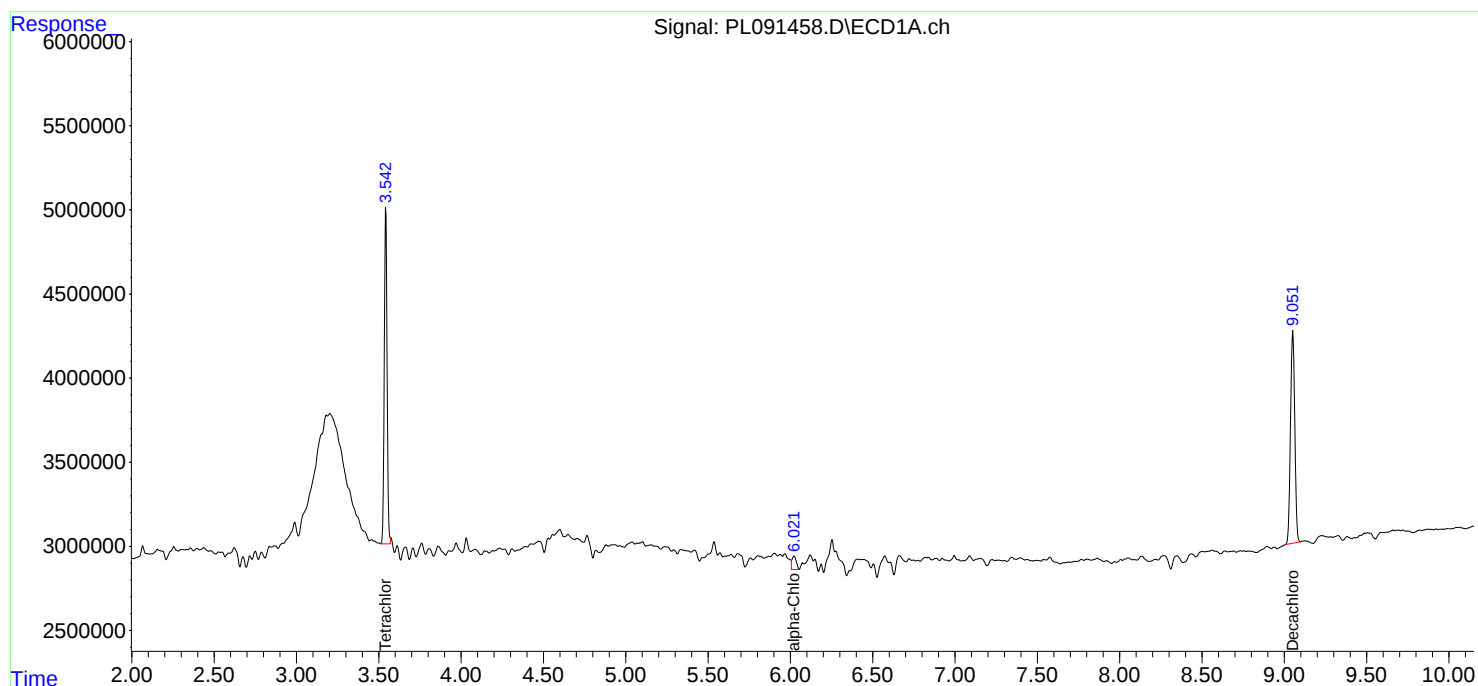


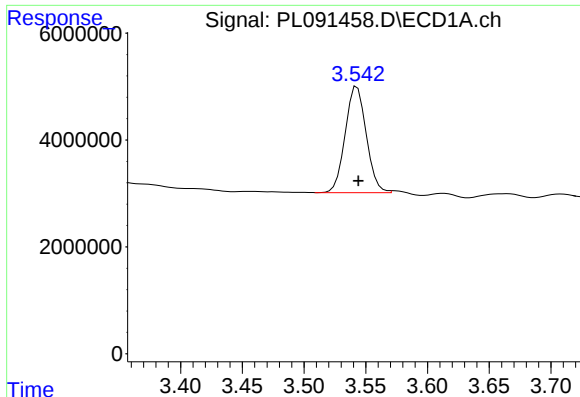

#1 Tetrachloro-m-xylene


R.T.: 3.542 min
Delta R.T.: -0.002 min
Response: 23695771
Conc: 11.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
239

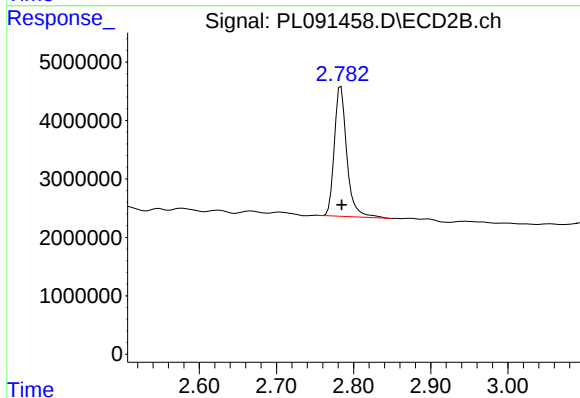


#1 Tetrachloro-m-xylene

R.T.: 2.784 min
Delta R.T.: -0.001 min
Response: 25100464
Conc: 12.86 ng/ml

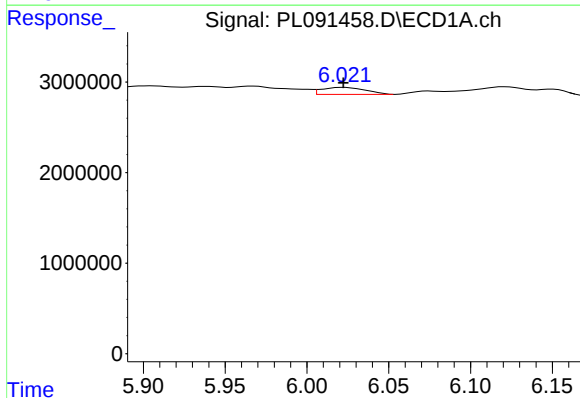


#11 alpha-Chlordane

R.T.: 6.021 min
Delta R.T.: 0.000 min
Response: 1403902
Conc: 0.58 ng/ml m

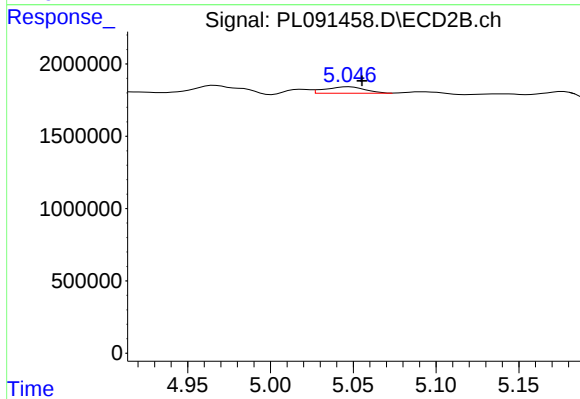

#11 alpha-Chlordane


R.T.: 5.046 min
Delta R.T.: -0.009 min
Response: 721975
Conc: 0.31 ng/ml m

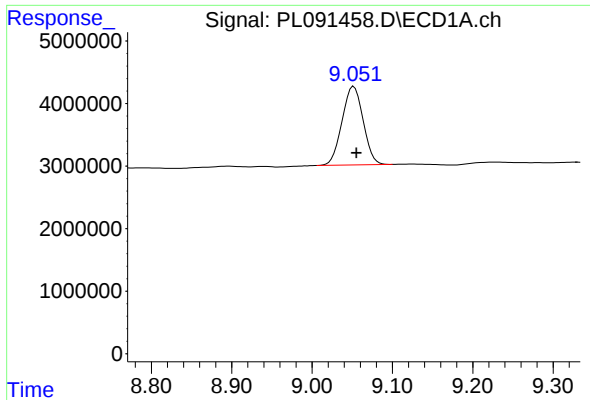

#28 Decachlorobiphenyl

R.T.: 9.052 min
Delta R.T.: -0.003 min
Response: 22940770
Conc: 15.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
239

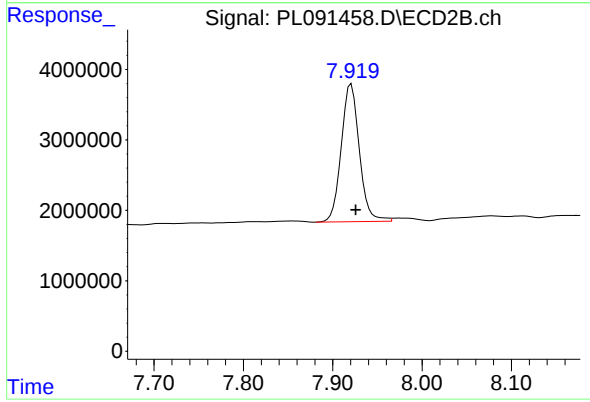

#28 Decachlorobiphenyl

R.T.: 7.921 min
Delta R.T.: -0.005 min
Response: 27473345
Conc: 14.50 ng/ml