

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090220\
 Data File : PL061186.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Sep 2020 09:49
 Operator : DD\AJ
 Sample : L3506-11
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 02 13:21:19 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 25 16:59:57 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.463	4.009	22287753	26454859	12.078	10.179
28)	SA Decachlor...	8.216	9.098	20383409	28228063	12.100	13.378
Target Compounds							
5)	MB Aldrin	0.000	5.474f	0	7303710	N.D.	2.167 #
8)	B Heptachlo...	0.000	5.886	0	1418032	N.D.	0.542 #
9)	A Endosulfan I	5.528f	0.000	1182122	0	0.651	N.D. #
10)	B gamma-Chl...	0.000	6.125	0	3407674	N.D.	1.097 #
11)	B alpha-Chl...	0.000	6.198	0	8285755	N.D.	2.665 #
14)	MA Endrin	6.015	0.000	7786074	0	4.281	N.D. #
23)	Chlordane-1	4.330	0.000	4218759	0	69.095	N.D. #
24)	Chlordane-2	0.000	5.474	0	7303710	N.D.	70.971 #
25)	Chlordane-3	0.000	6.125	0	3407674	N.D.	8.526 #
26)	Chlordane-4	0.000	6.198	0	8285755	N.D.	17.236 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090220\
Data File : PL061186.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Sep 2020 09:49
Operator : DD\AJ
Sample : L3506-11
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 02 13:21:19 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
Quant Title : GC Extractables
QLast Update : Tue Aug 25 16:59:57 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

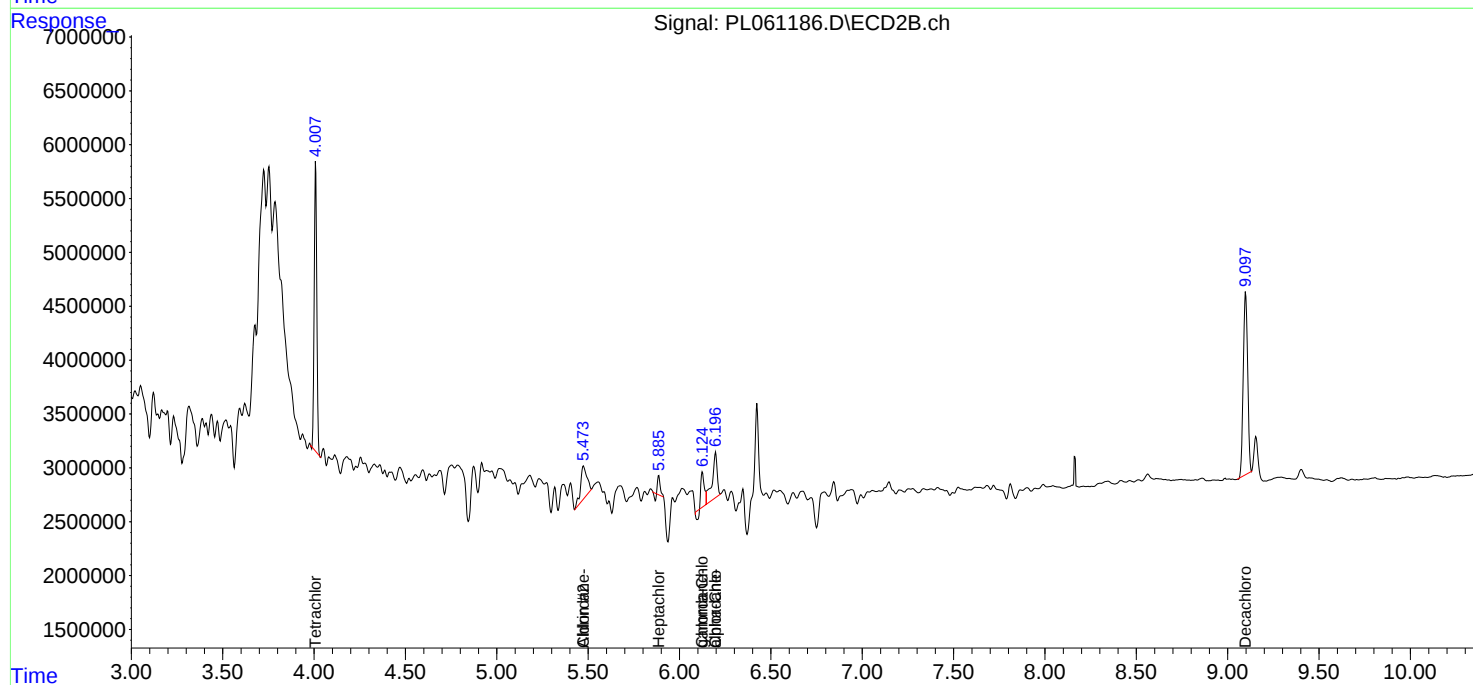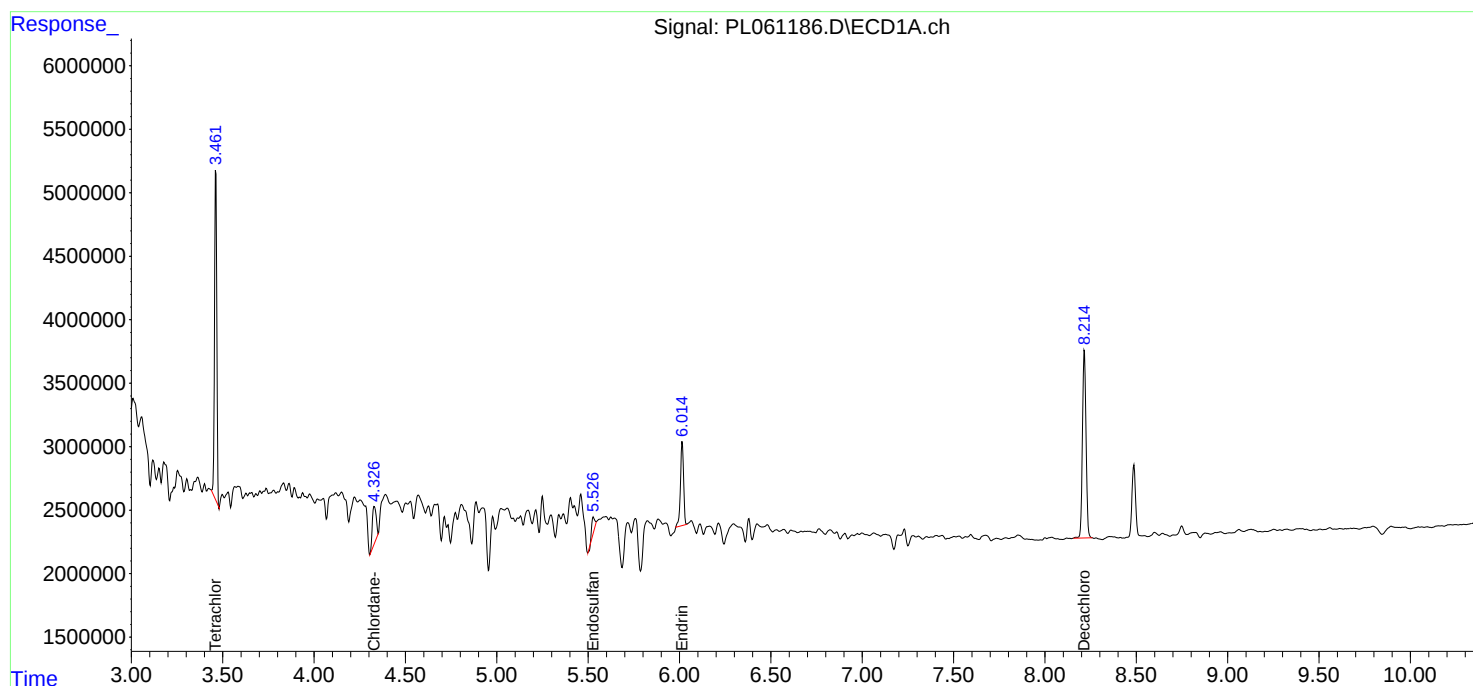


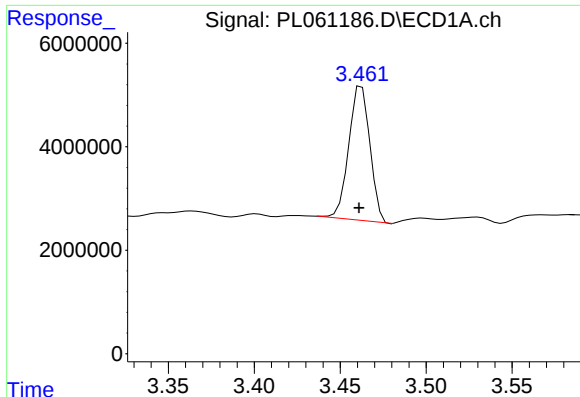

#1 Tetrachloro-m-xylene


R.T.: 3.463 min
Delta R.T.: 0.002 min
Response: 22287753
Conc: 12.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

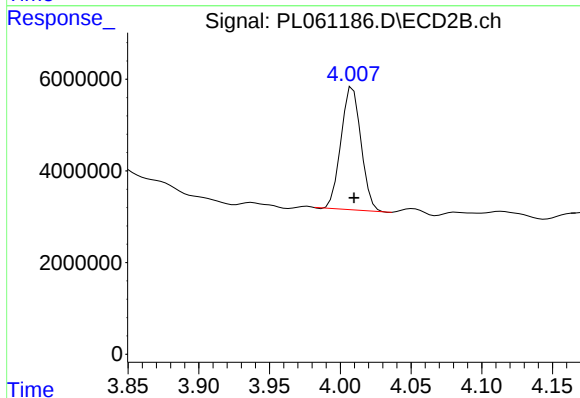


#1 Tetrachloro-m-xylene

R.T.: 4.009 min
Delta R.T.: -0.001 min
Response: 26454859
Conc: 10.18 ng/ml

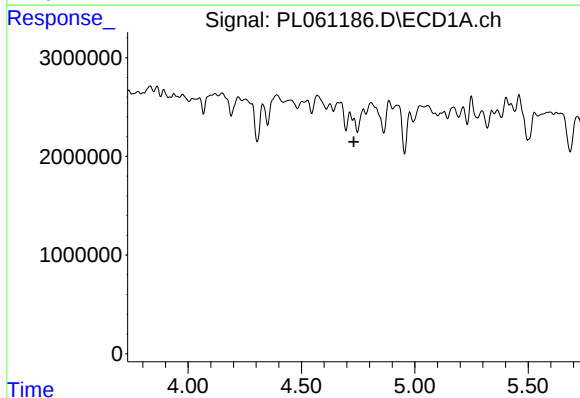


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.732 min
Response: 0
Conc: N.D.

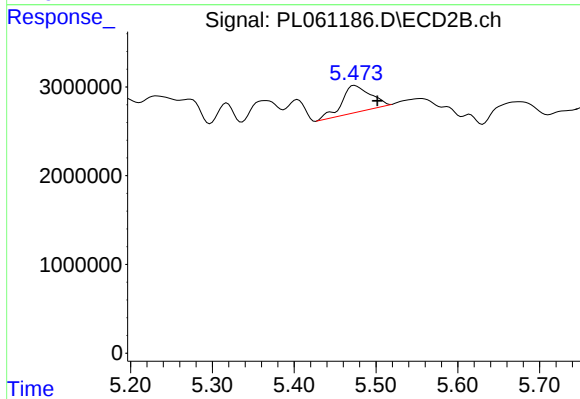

#5 Aldrin


R.T.: 5.474 min
Delta R.T.: -0.028 min
Response: 7303710
Conc: 2.17 ng/ml

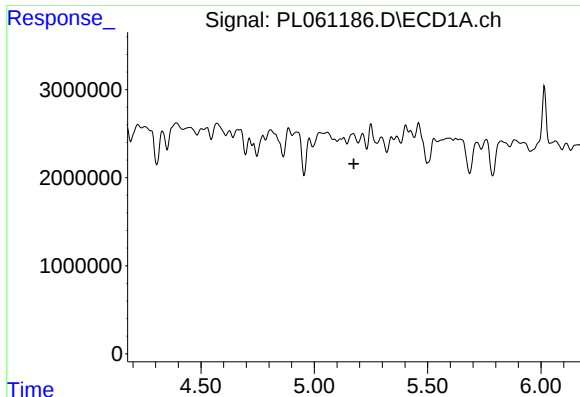

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.175 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

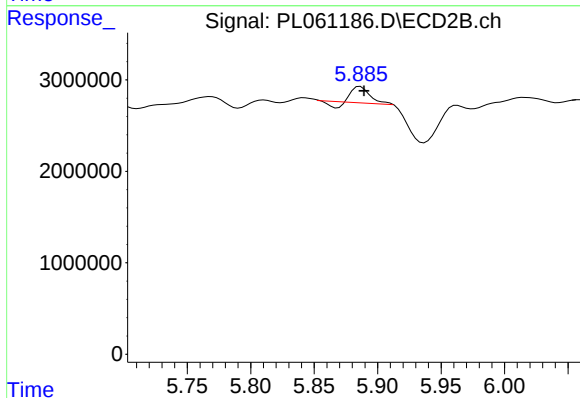


#8 Heptachlor epoxide

R.T.: 5.886 min
Delta R.T.: -0.003 min
Response: 1418032
Conc: 0.54 ng/ml

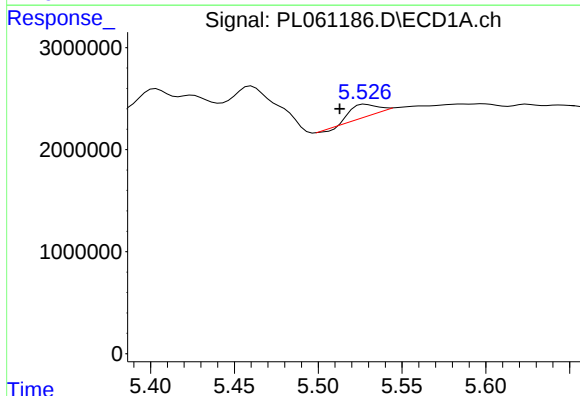


#9 Endosulfan I

R.T.: 5.528 min
Delta R.T.: 0.015 min
Response: 1182122
Conc: 0.65 ng/ml

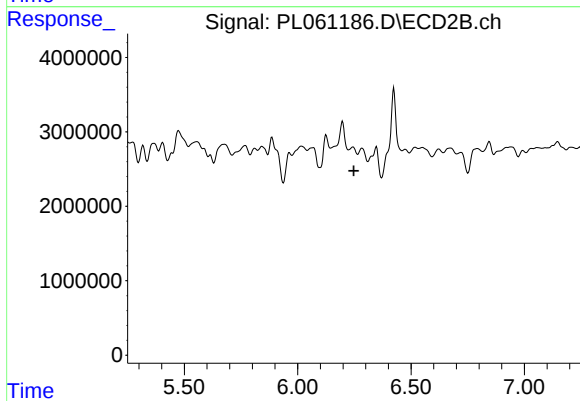

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.248 min
Response: 0
Conc: N.D.

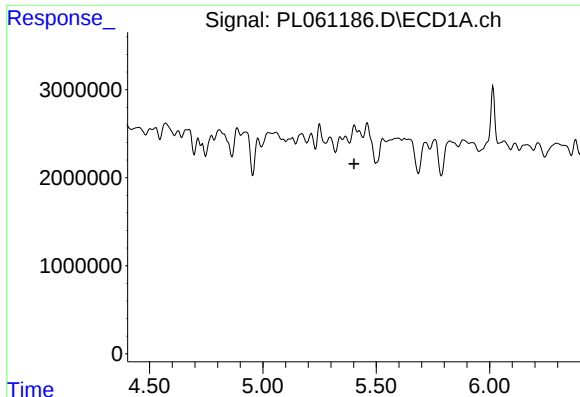

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.402 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

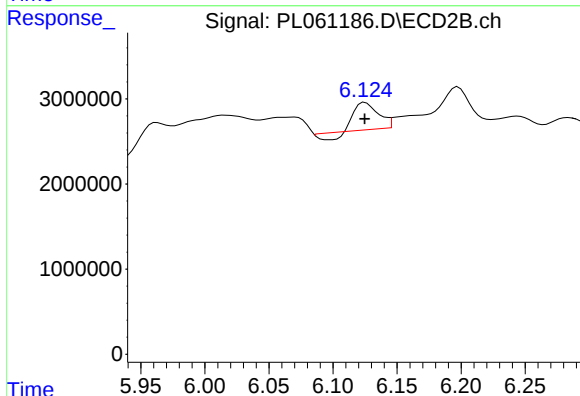


#10 gamma-Chlordane

R.T.: 6.125 min
Delta R.T.: 0.000 min
Response: 3407674
Conc: 1.10 ng/ml

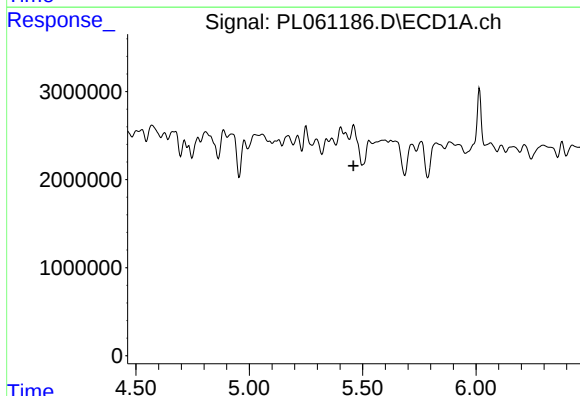


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.460 min
Response: 0
Conc: N.D.

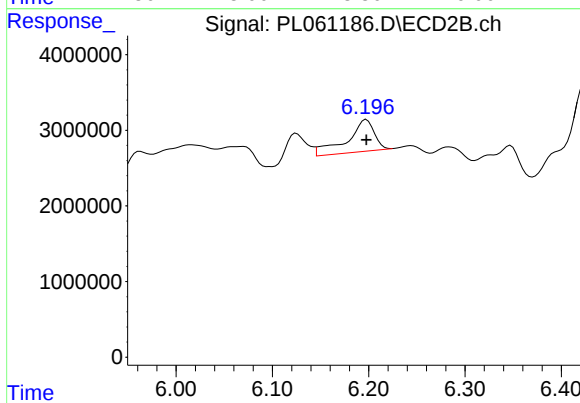

#11 alpha-Chlordane


R.T.: 6.198 min
Delta R.T.: 0.000 min
Response: 8285755
Conc: 2.67 ng/ml

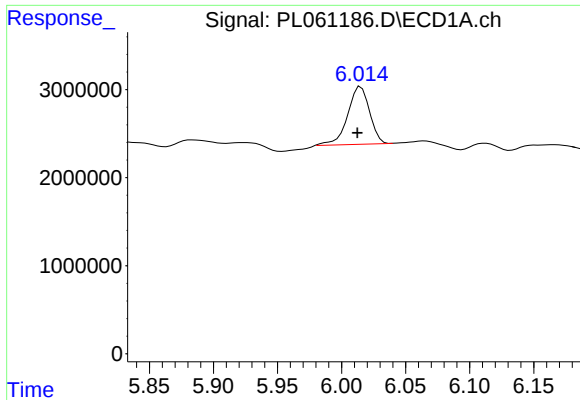

#14 Endrin


R.T.: 6.015 min
Delta R.T.: 0.002 min
Response: 7786074
Conc: 4.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

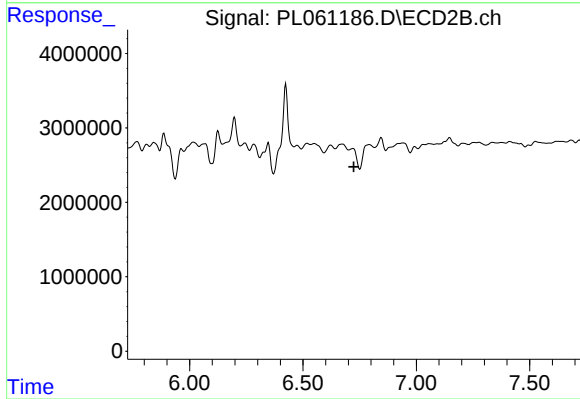


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.724 min
Response: 0
Conc: N.D.

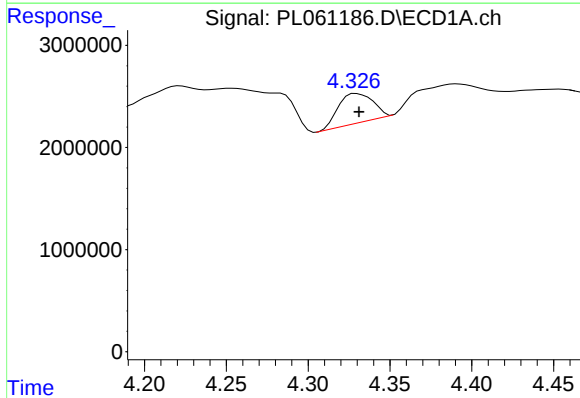


#23 Chlordane-1

R.T.: 4.330 min
Delta R.T.: -0.002 min
Response: 4218759
Conc: 69.09 ng/ml

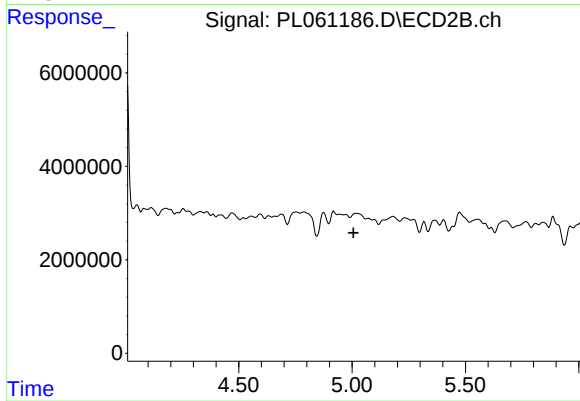

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.007 min
Response: 0
Conc: N.D.

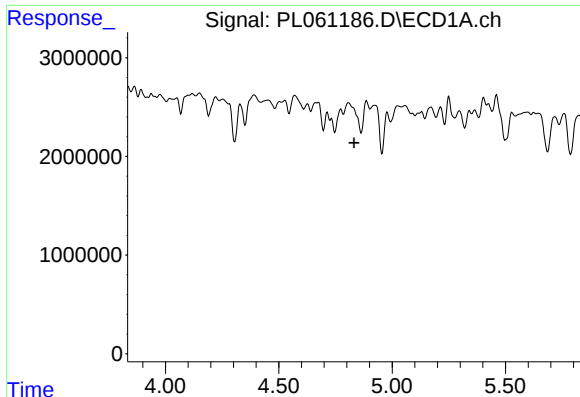

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.833 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

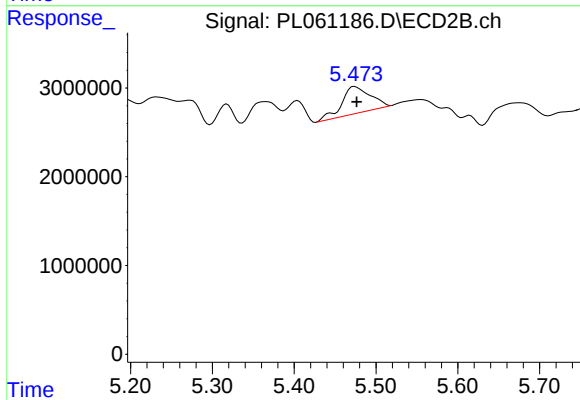


#24 Chlordane-2

R.T.: 5.474 min
Delta R.T.: -0.002 min
Response: 7303710
Conc: 70.97 ng/ml

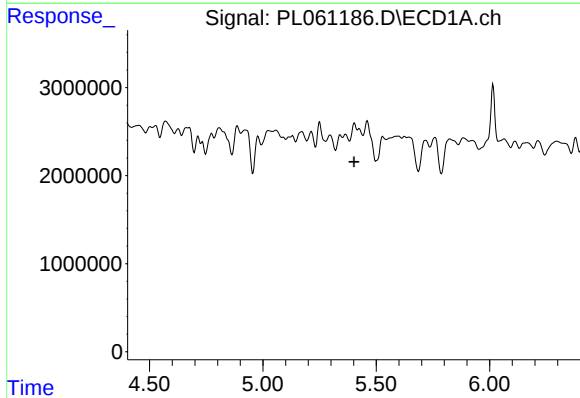


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.402 min
Response: 0
Conc: N.D.

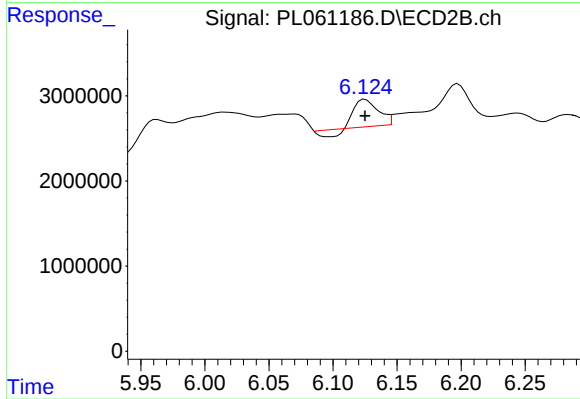

#25 Chlordane-3


R.T.: 6.125 min
Delta R.T.: 0.000 min
Response: 3407674
Conc: 8.53 ng/ml

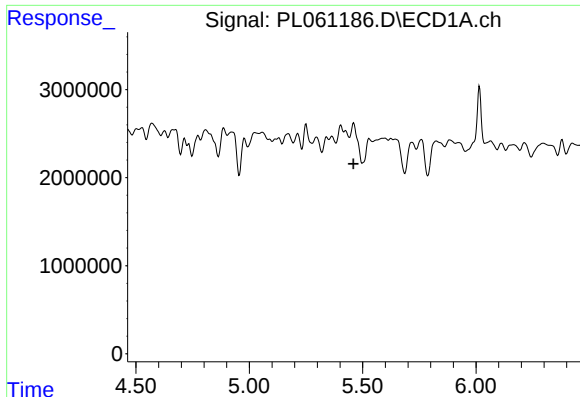

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.460 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

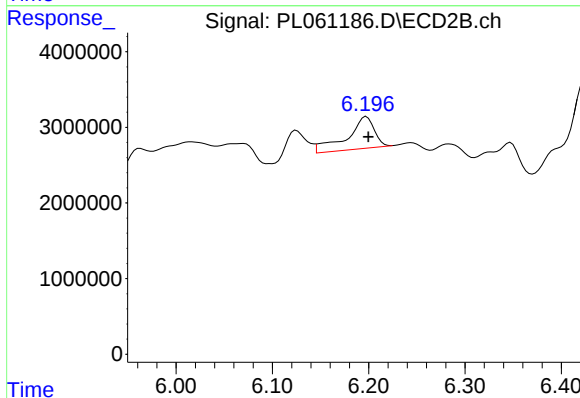


#26 Chlordane-4

R.T.: 6.198 min
Delta R.T.: -0.002 min
Response: 8285755
Conc: 17.24 ng/ml

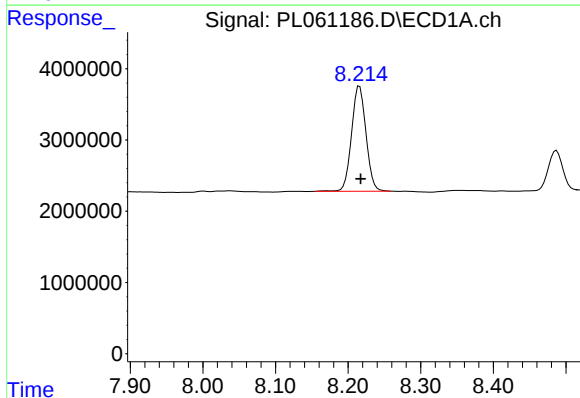

#28 Decachlorobiphenyl

R.T.: 8.216 min
Delta R.T.: -0.001 min
Response: 20383409
Conc: 12.10 ng/ml

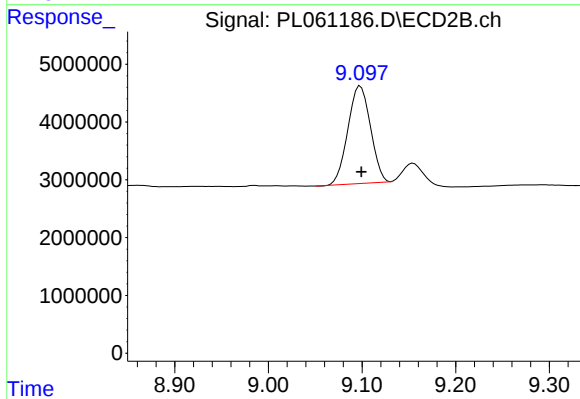

#28 Decachlorobiphenyl

R.T.: 9.098 min
Delta R.T.: 0.000 min
Response: 28228063
Conc: 13.38 ng/ml