

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090220\
 Data File : PL061195.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Sep 2020 15:11
 Operator : DD\AJ
 Sample : L3854-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 02 17:16:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 25 16:59:57 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.460	4.009	34410654	31434207	18.647	12.095 #
28)	SA Decachlor...	8.213	9.098	24991863	30450084	14.835	14.431
Target Compounds							
2)	A alpha-BHC	3.918f	4.373f	-1875880	8364422	N.D.	2.059
3)	MA gamma-BHC...	4.178	4.664f	59619262	1044903	23.353	0.278 #
8)	B Heptachlo...	0.000	5.880	0	5751612	N.D.	2.199 #
11)	B alpha-Chl...	5.444f	0.000	23756011	0	12.172	N.D. #
14)	MA Endrin	0.000	6.751f	0	4460091	N.D.	1.756 #
15)	B Endosulfa...	6.258f	0.000	4464980	0	2.501	N.D. #
17)	MA 4,4'-DDT	6.392	0.000	17389774	0	11.504	N.D. #
18)	B Endrin al...	0.000	7.044	0	17079026	N.D.	7.829 #
26)	Chlordane-4	5.444f	0.000	23756011	0	159.773	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090220\
Data File : PL061195.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Sep 2020 15:11
Operator : DD\AJ
Sample : L3854-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 02 17:16:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
Quant Title : GC Extractables
QLast Update : Tue Aug 25 16:59:57 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

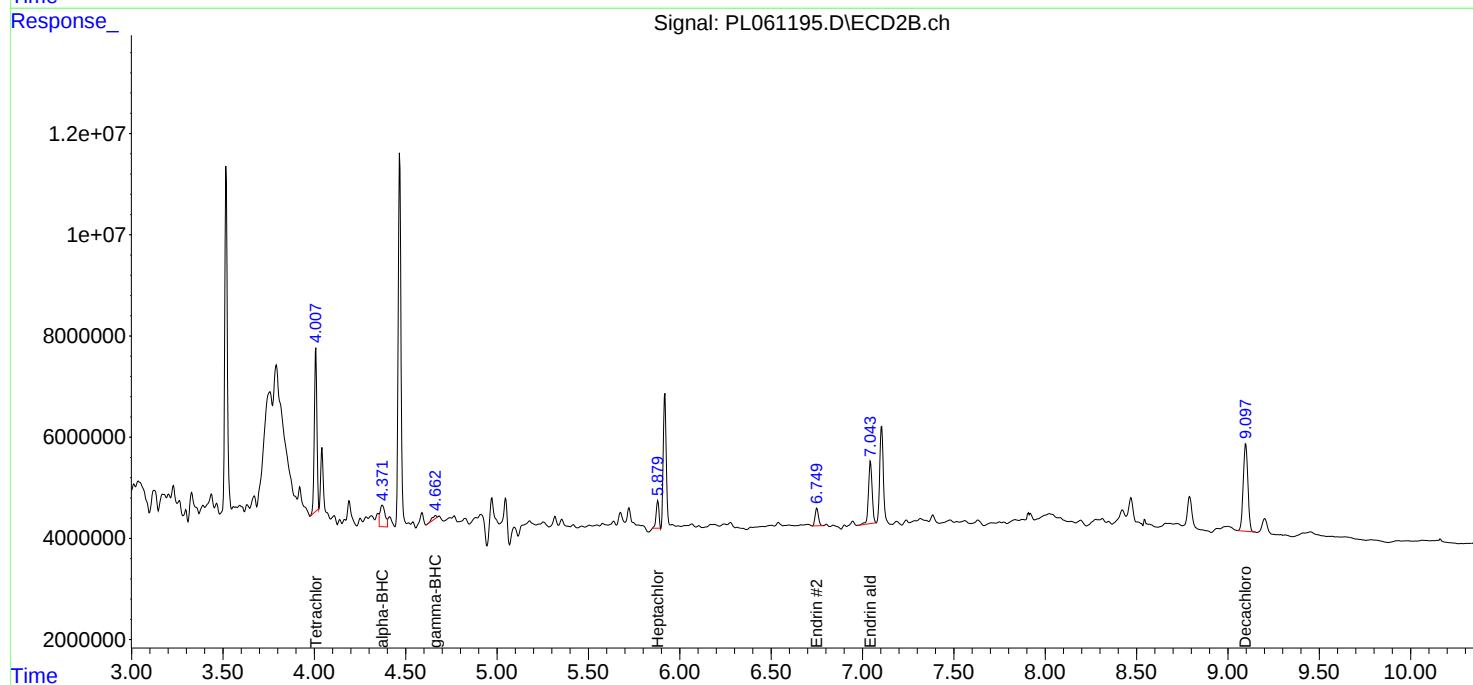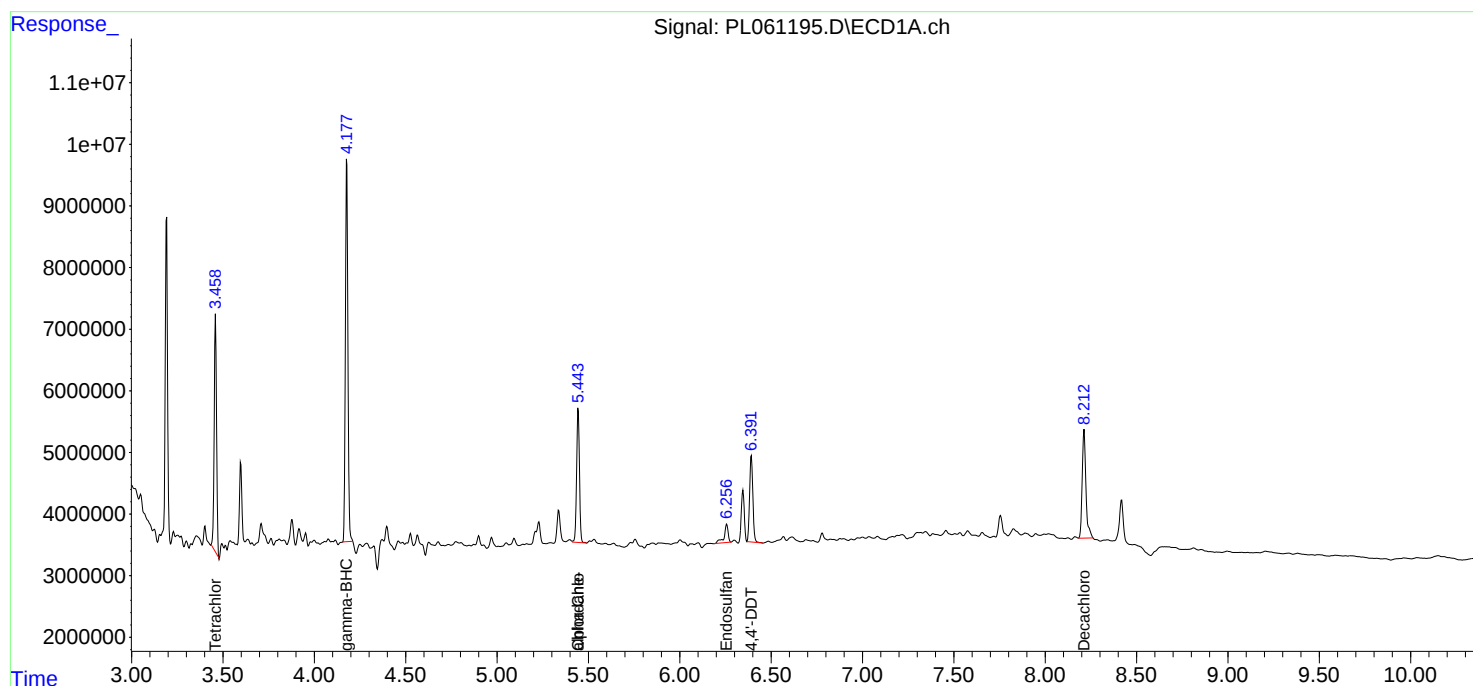


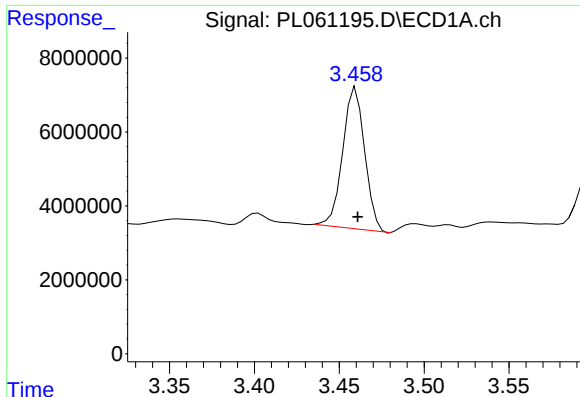

#1 Tetrachloro-m-xylene


R.T.: 3.460 min
Delta R.T.: -0.001 min
Response: 34410654
Conc: 18.65 ng/ml

Instrument :
ECD_L
ClientSampleId :

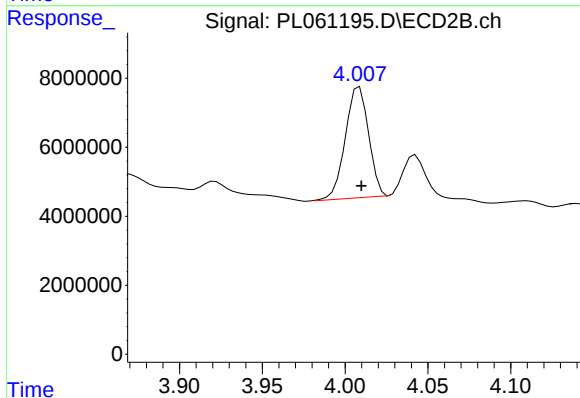


#1 Tetrachloro-m-xylene

R.T.: 4.009 min
Delta R.T.: -0.001 min
Response: 31434207
Conc: 12.09 ng/ml

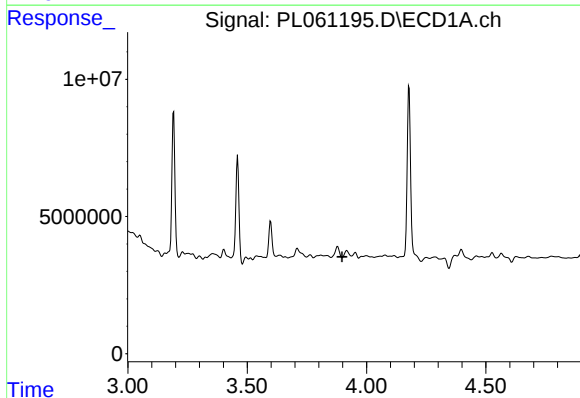


#2 alpha-BHC

R.T.: 3.918 min
Delta R.T.: 0.019 min
Response: -1875880
Conc: N.D.

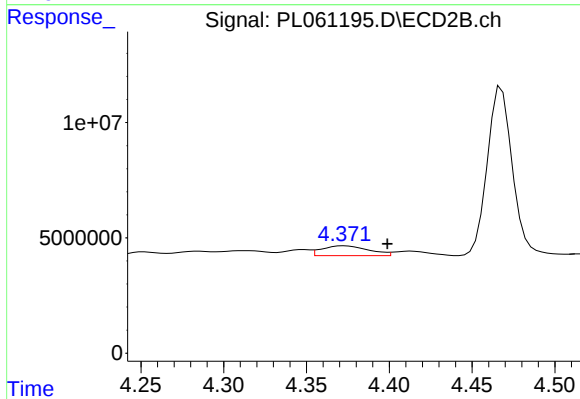

#2 alpha-BHC


R.T.: 4.373 min
Delta R.T.: -0.026 min
Response: 8364422
Conc: 2.06 ng/ml

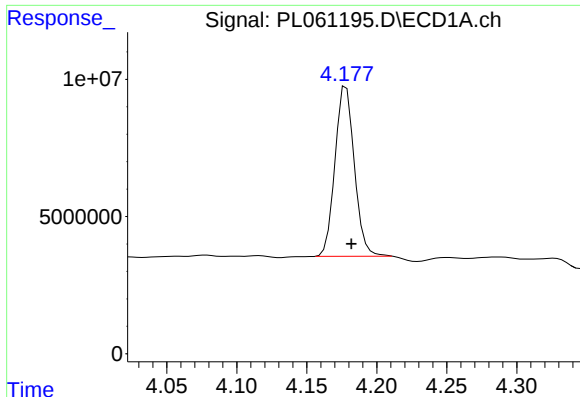

#3 gamma-BHC (Lindane)


R.T.: 4.178 min
Delta R.T.: -0.004 min
Response: 59619262
Conc: 23.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

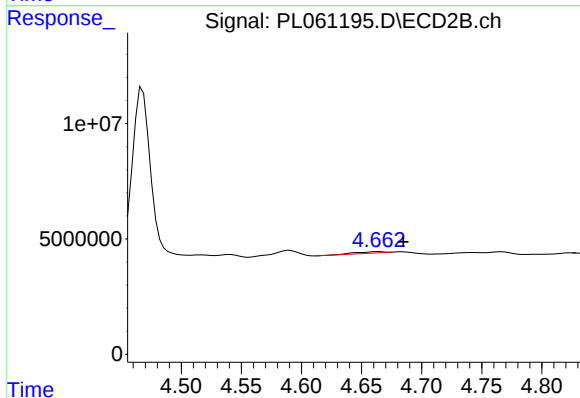


#3 gamma-BHC (Lindane)

R.T.: 4.664 min
Delta R.T.: -0.021 min
Response: 1044903
Conc: 0.28 ng/ml

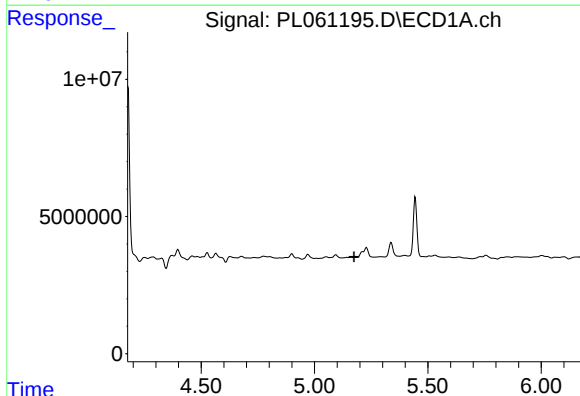


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.175 min
Response: 0
Conc: N.D.

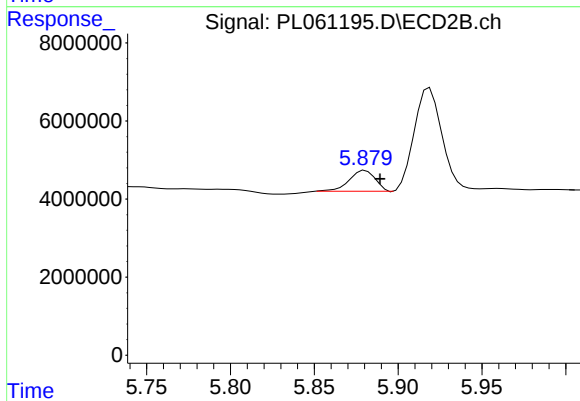

#8 Heptachlor epoxide


R.T.: 5.880 min
Delta R.T.: -0.009 min
Response: 5751612
Conc: 2.20 ng/ml

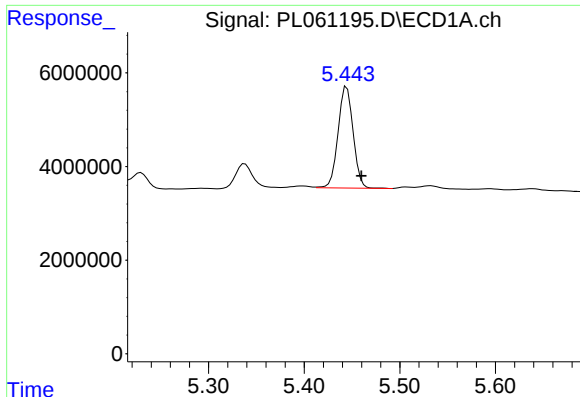

#11 alpha-Chlordane


R.T.: 5.444 min
Delta R.T.: -0.015 min
Response: 23756011
Conc: 12.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

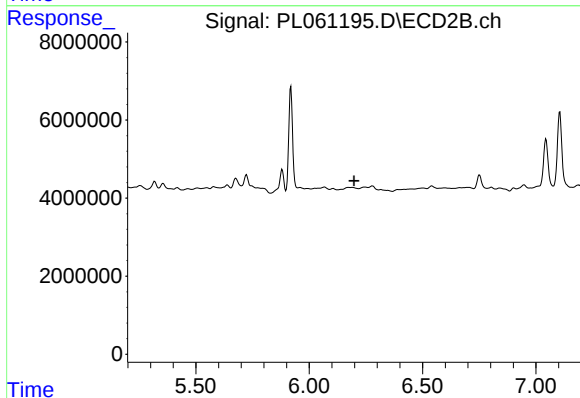


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.198 min
Response: 0
Conc: N.D.

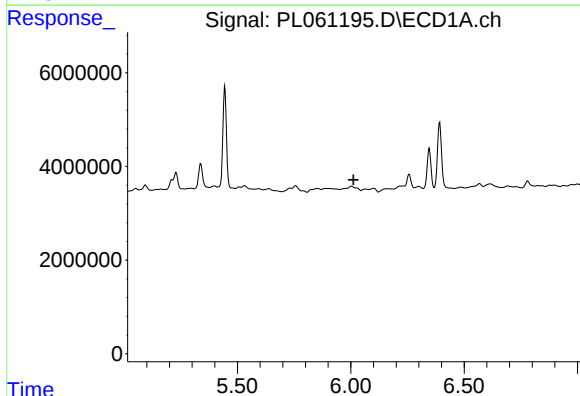


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.013 min
Response: 0
Conc: N.D.

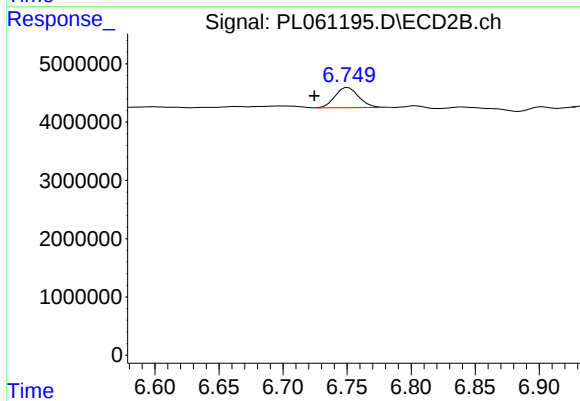

#14 Endrin


R.T.: 6.751 min
Delta R.T.: 0.026 min
Response: 4460091
Conc: 1.76 ng/ml

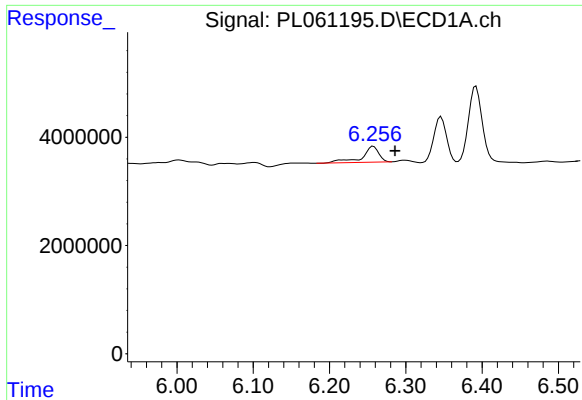

#15 Endosulfan II


R.T.: 6.258 min
Delta R.T.: -0.029 min
Response: 4464980
Conc: 2.50 ng/ml

Instrument :
ECD_L
ClientSampleId :

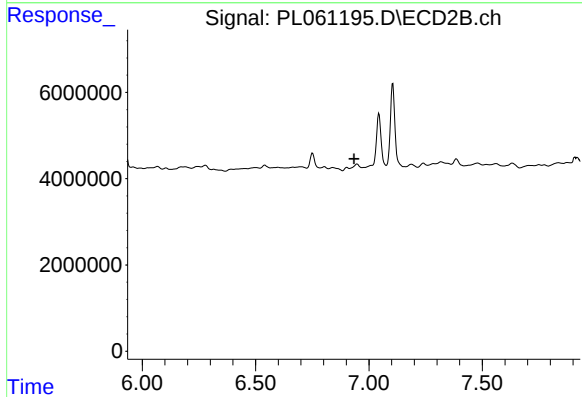


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.934 min
Response: 0
Conc: N.D.

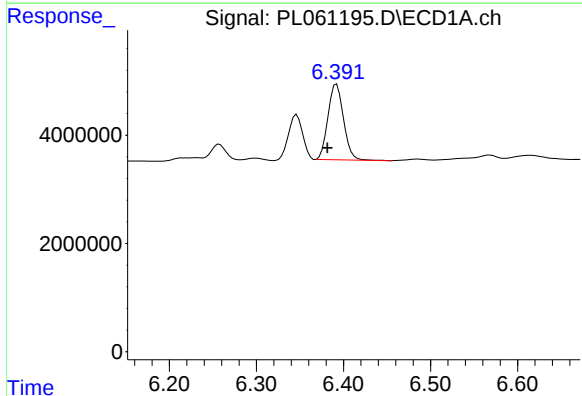


#17 4,4'-DDT

R.T.: 6.392 min
Delta R.T.: 0.011 min
Response: 17389774
Conc: 11.50 ng/ml

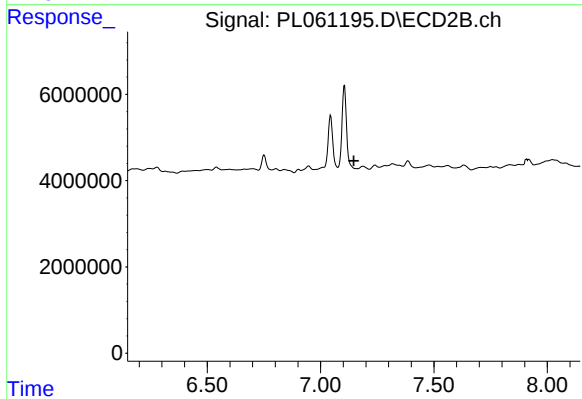

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 7.147 min
Response: 0
Conc: N.D.

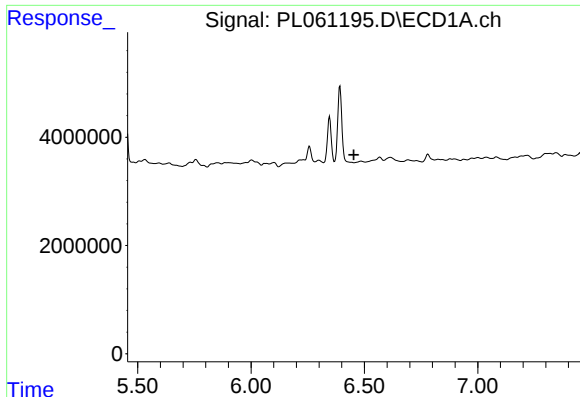

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.454 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

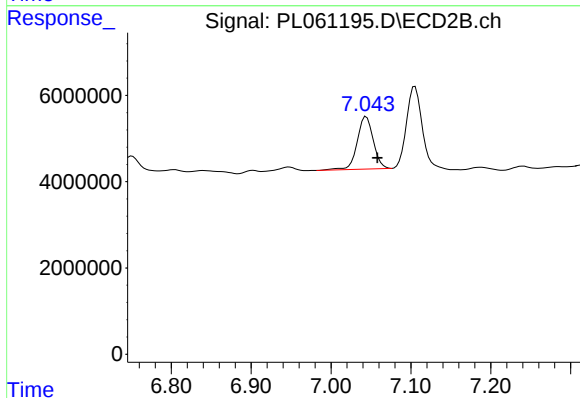


#18 Endrin aldehyde

R.T.: 7.044 min
Delta R.T.: -0.014 min
Response: 17079026
Conc: 7.83 ng/ml

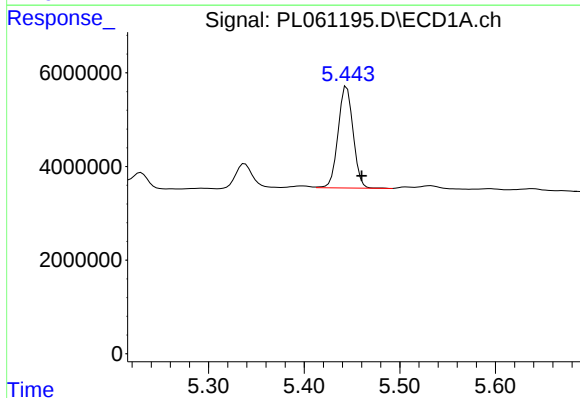


#26 Chlordane-4

R.T.: 5.444 min
Delta R.T.: -0.016 min
Response: 23756011
Conc: 159.77 ng/ml

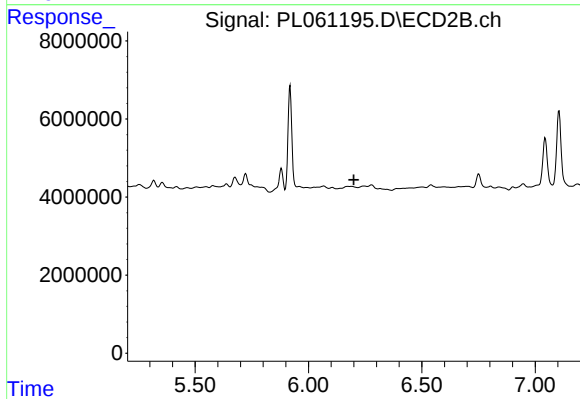

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 6.200 min
Response: 0
Conc: N.D.

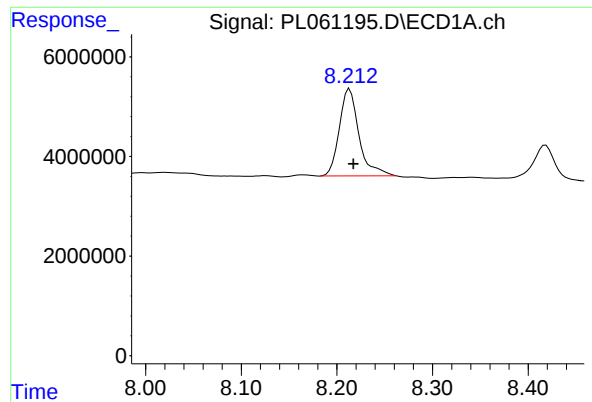

#28 Decachlorobiphenyl

R.T.: 8.213 min
Delta R.T.: -0.004 min
Response: 24991863
Conc: 14.84 ng/ml

Instrument :
ECD_L
ClientSampleId :

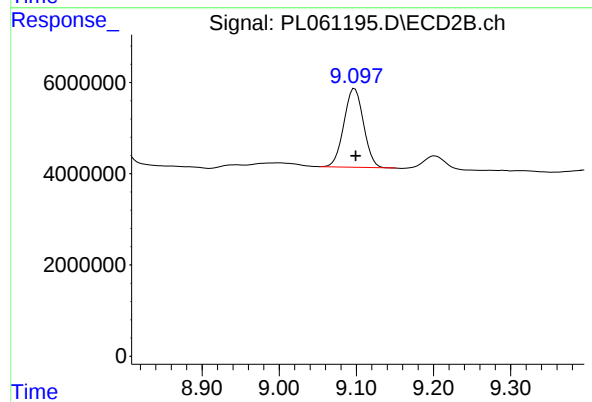

#28 Decachlorobiphenyl

R.T.: 9.098 min
Delta R.T.: -0.001 min
Response: 30450084
Conc: 14.43 ng/ml