

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090220\
 Data File : PL061186.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Sep 2020 09:49
 Operator : DD\AJ
 Sample : L3506-11
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OR-02-083120

Manual Integrations
 APPROVED

Ankita
 9/3/2020 10:46:09 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 02 13:21:19 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 25 16:59:57 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.463	4.009	22287753	26454859	12.078	10.179
28)	SA Decachlor...	8.216	9.097	20383409	30566278	12.100	14.486m
Target Compounds							
10)	B gamma-Chl...	5.402	6.124	2440511	1809638	1.242m	0.583m#
11)	B alpha-Chl...	5.459	6.196	2393314	5016098	1.226m	1.613m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090220\
Data File : PL061186.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Sep 2020 09:49
Operator : DD\AJ
Sample : L3506-11
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
OR-02-083120


Manual Integrations
APPROVED

Ankita
9/3/2020 10:46:09 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 02 13:21:19 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
Quant Title : GC Extractables
QLast Update : Tue Aug 25 16:59:57 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

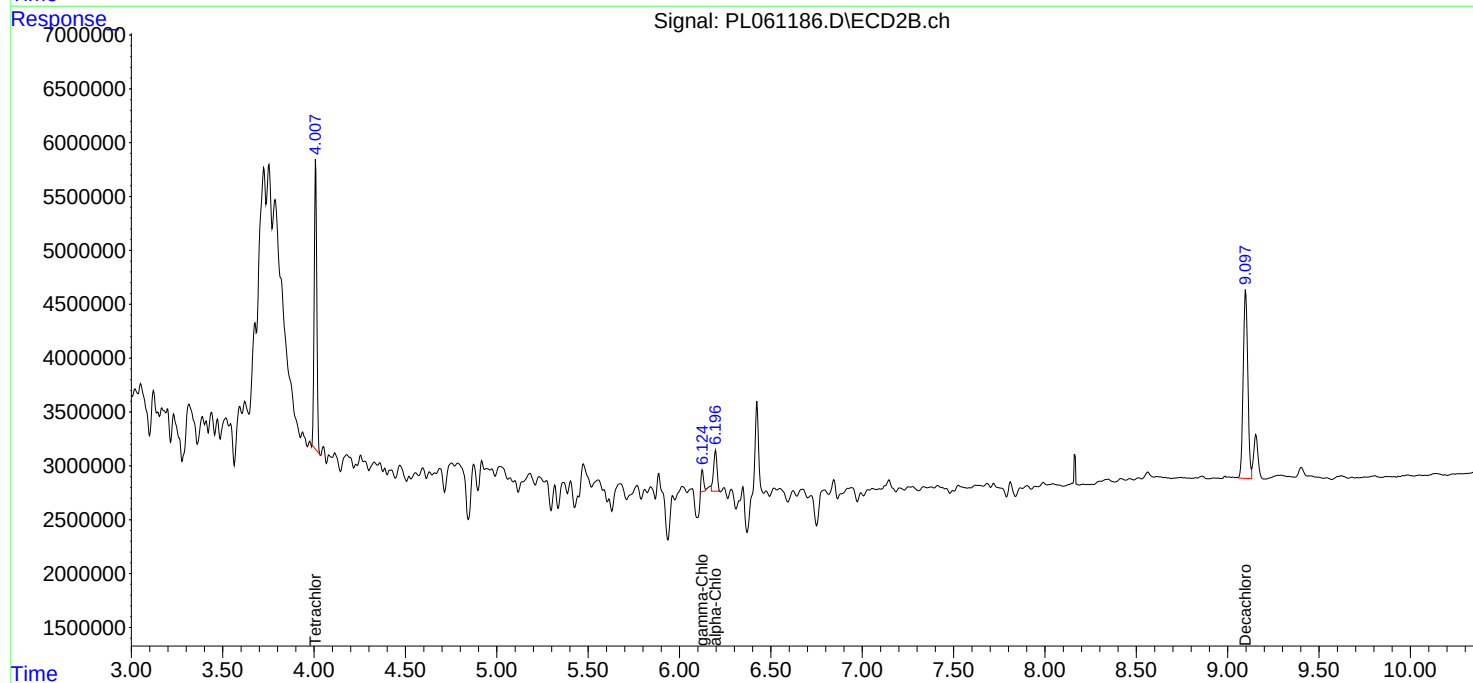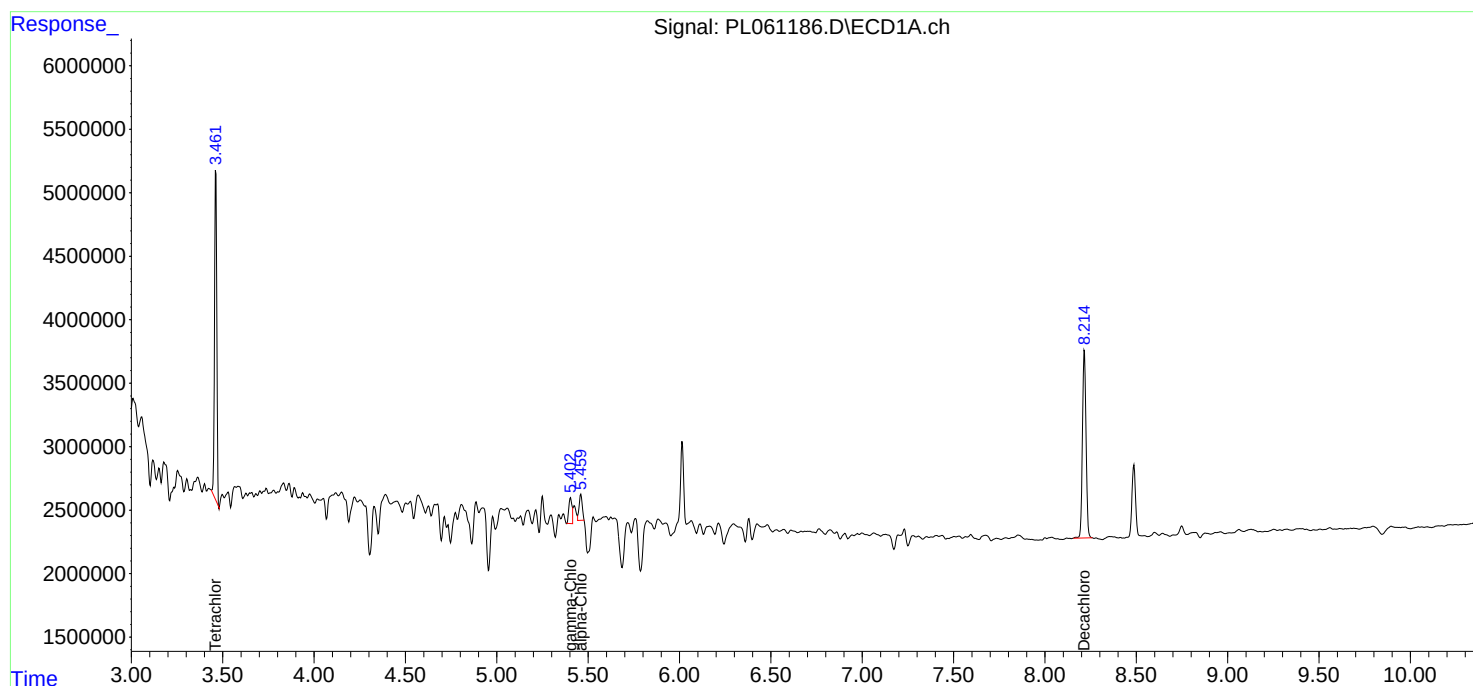

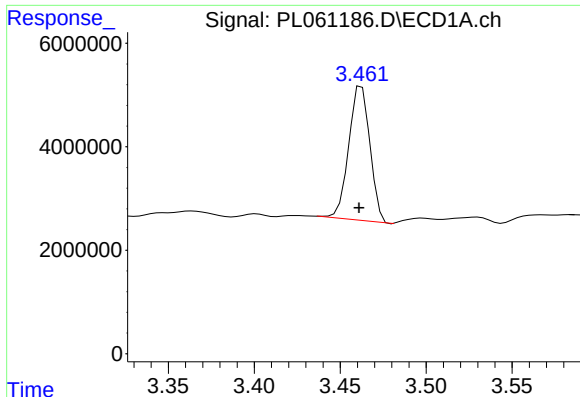


#1 Tetrachloro-m-xylene

R.T.: 3.463 min
Delta R.T.: 0.002 min
Response: 22287753
Conc: 12.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-02-083120


Manual Integrations
APPROVED

Ankita
9/3/2020 10:46:09 AM

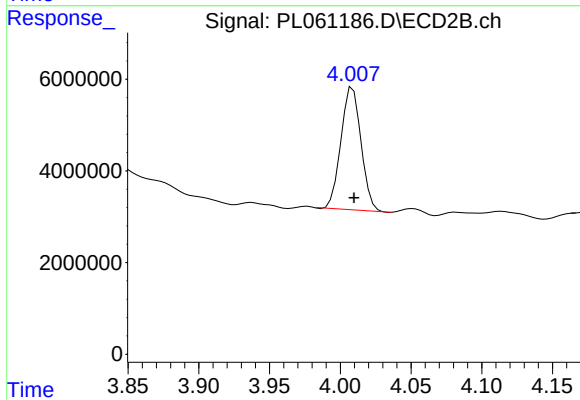


#1 Tetrachloro-m-xylene

R.T.: 4.009 min
Delta R.T.: -0.001 min
Response: 26454859
Conc: 10.18 ng/ml

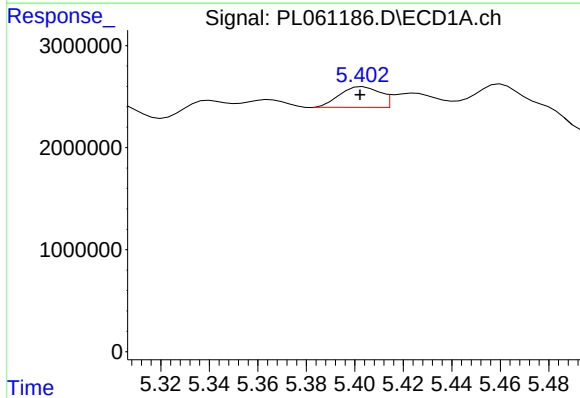


#10 gamma-Chlordane

R.T.: 5.402 min
Delta R.T.: 0.000 min
Response: 2440511
Conc: 1.24 ng/ml m

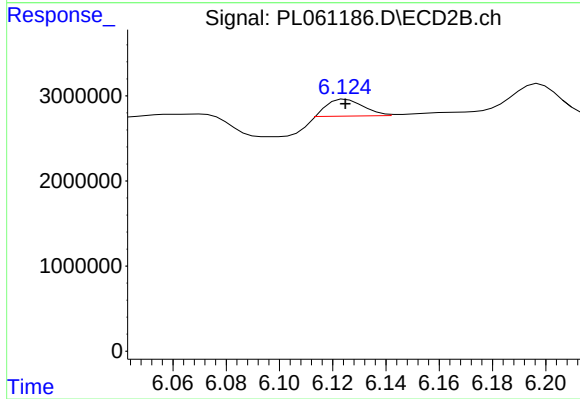

#10 gamma-Chlordane

R.T.: 6.124 min
Delta R.T.: -0.001 min
Response: 1809638
Conc: 0.58 ng/ml m

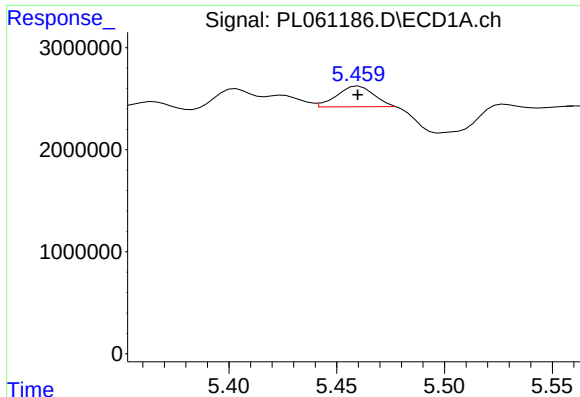


#11 alpha-Chlordane

R.T.: 5.459 min
Delta R.T.: 0.000 min
Response: 2393314
Conc: 1.23 ng/ml m

Instrument :
ECD_L
ClientSampleId :
OR-02-083120


Manual Integrations
APPROVED

Ankita
9/3/2020 10:46:09 AM

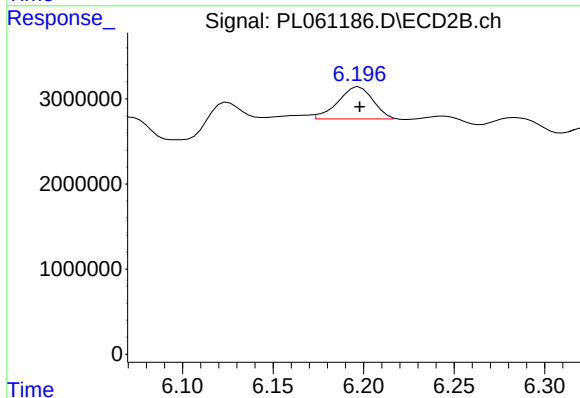


#11 alpha-Chlordane

R.T.: 6.196 min
Delta R.T.: -0.002 min
Response: 5016098
Conc: 1.61 ng/ml m

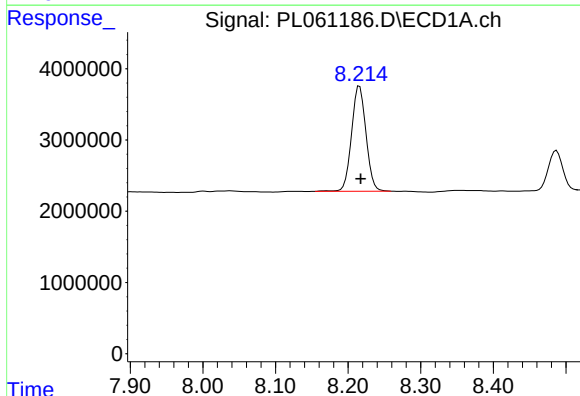

#28 Decachlorobiphenyl

R.T.: 8.216 min
Delta R.T.: -0.001 min
Response: 20383409
Conc: 12.10 ng/ml

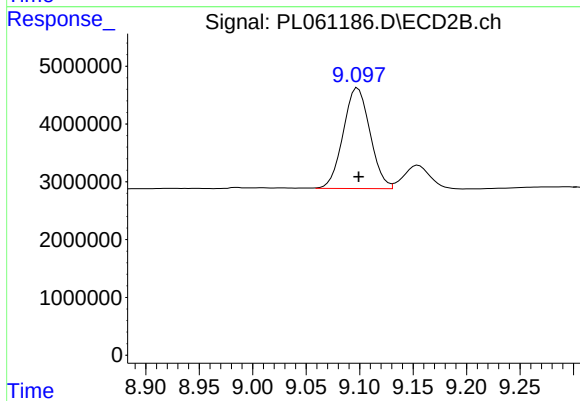

#28 Decachlorobiphenyl

R.T.: 9.097 min
Delta R.T.: -0.002 min
Response: 30566278
Conc: 14.49 ng/ml m