

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090221\
 Data File : PL069683.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Sep 2021 14:43
 Operator : AR\AJ
 Sample : PB138892BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 03 02:27:38 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL083021.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 31 01:49:30 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.639	5.567	7482748	25839025	24.036	20.538
28)	SA Decachlor...	10.407	11.496	10795798	19333250	18.306	17.133
Target Compounds							
3)	MA gamma-BHC...	0.000	6.560	0	1291080	N.D.	0.795 #
6)	B beta-BHC	0.000	6.779f	0	1323281	N.D.	1.523 #
8)	B Heptachlo...	0.000	8.057f	0	958479	N.D.	0.709 #
15)	B Endosulfa...	0.000	9.212	0	381535	N.D.	0.335 #
16)	A 4,4'-DDD	0.000	9.136f	0	39450	N.D.	0.036 #
17)	MA 4,4'-DDT	0.000	9.437	0	233209	N.D.	0.214 #
21)	B Endrin ke...	0.000	10.090f	0	1058171	N.D.	0.891 #
22)	Mirex	0.000	10.549	0	259659	N.D.	0.289 #
23)	Chlordane-1	0.000	6.926f	0	1366076	N.D.	24.723 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090221\
Data File : PL069683.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Sep 2021 14:43
Operator : AR\AJ
Sample : PB138892BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 03 02:27:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL083021.M
Quant Title : GC Extractables
QLast Update : Tue Aug 31 01:49:30 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

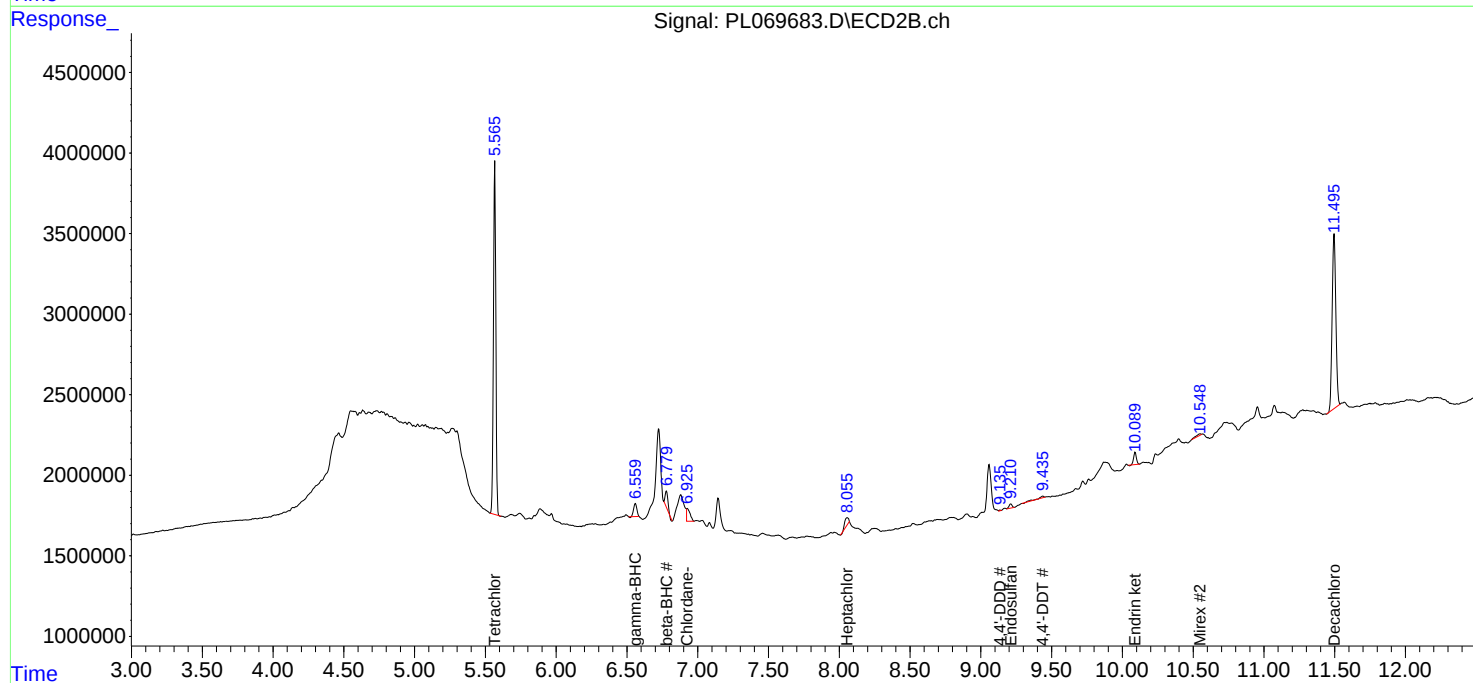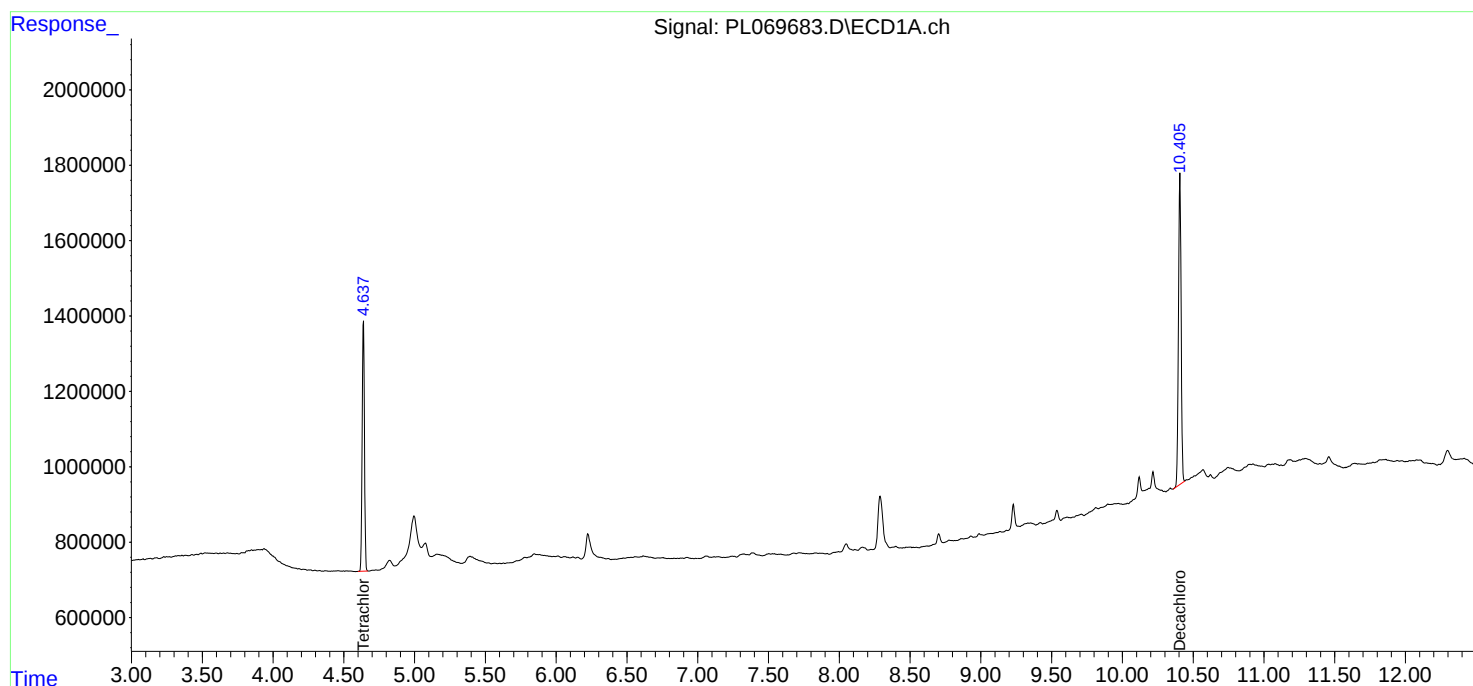


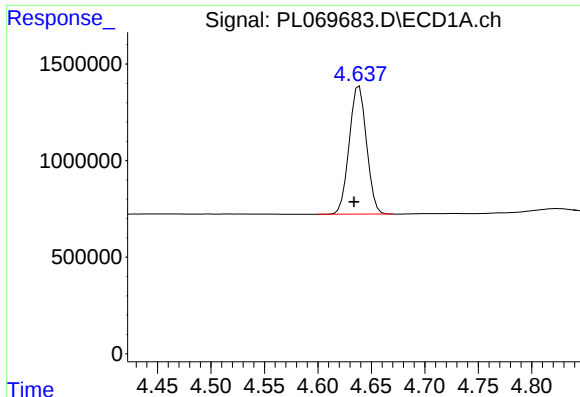

#1 Tetrachloro-m-xylene


R.T.: 4.639 min
Delta R.T.: 0.005 min
Response: 7482748
Conc: 24.04 ng/ml

Instrument :
ECD_L
ClientSampleId :

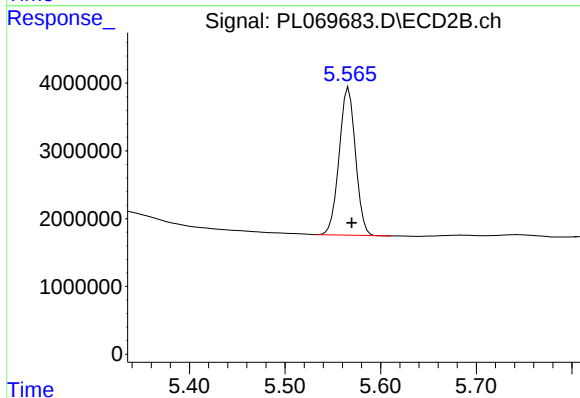


#1 Tetrachloro-m-xylene

R.T.: 5.567 min
Delta R.T.: -0.003 min
Response: 25839025
Conc: 20.54 ng/ml

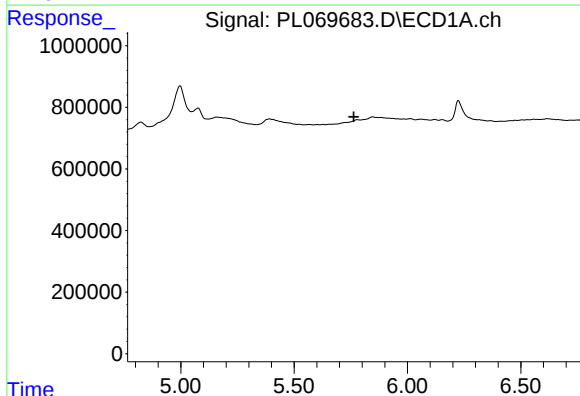


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 5.764 min
Response: 0
Conc: N.D.

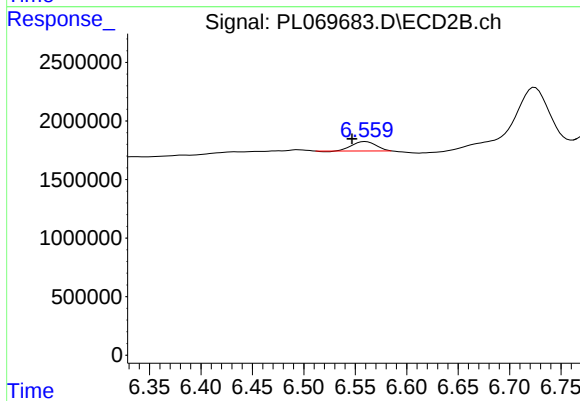

#3 gamma-BHC (Lindane)


R.T.: 6.560 min
Delta R.T.: 0.013 min
Response: 1291080
Conc: 0.79 ng/ml

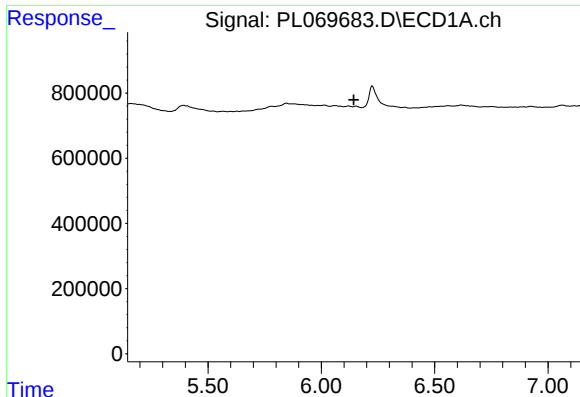

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.143 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

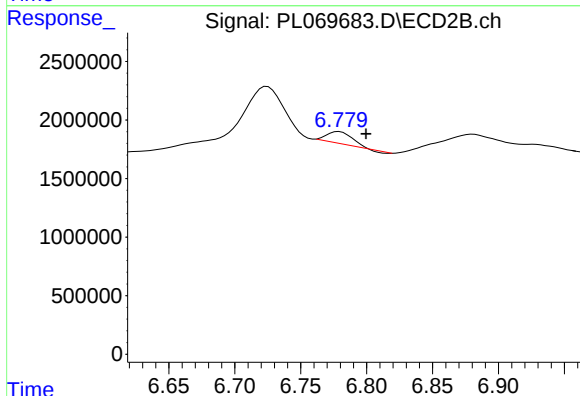


#6 beta-BHC

R.T.: 6.779 min
Delta R.T.: -0.020 min
Response: 1323281
Conc: 1.52 ng/ml

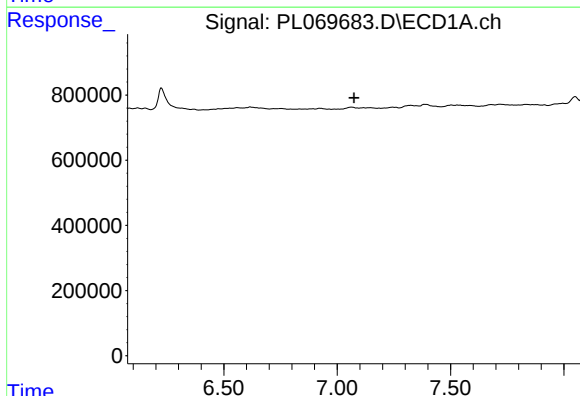


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 7.075 min
Response: 0
Conc: N.D.

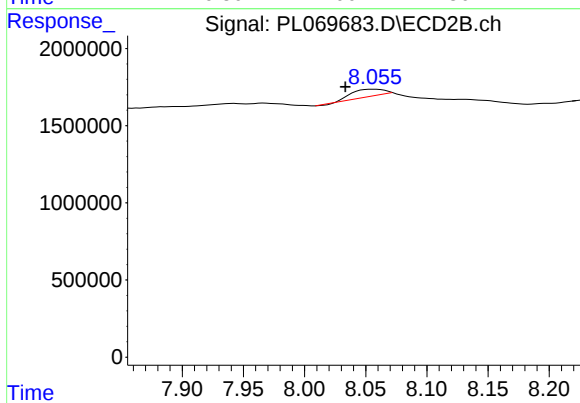

#8 Heptachlor epoxide


R.T.: 8.057 min
Delta R.T.: 0.024 min
Response: 958479
Conc: 0.71 ng/ml

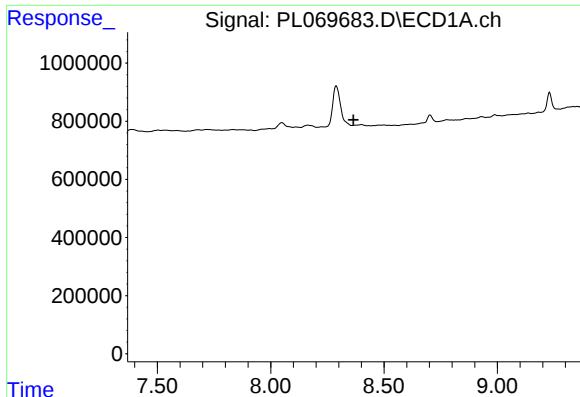

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.365 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

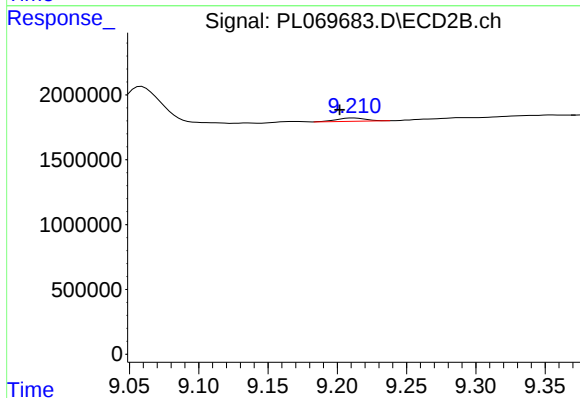


#15 Endosulfan II

R.T.: 9.212 min
Delta R.T.: 0.010 min
Response: 381535
Conc: 0.34 ng/ml

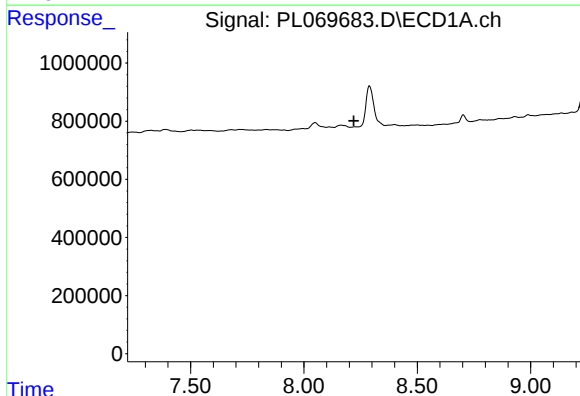


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 8.220 min
Response: 0
Conc: N.D.

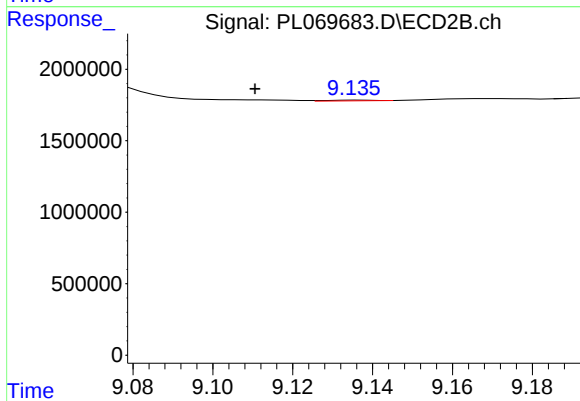

#16 4,4'-DDD


R.T.: 9.136 min
Delta R.T.: 0.025 min
Response: 39450
Conc: 0.04 ng/ml

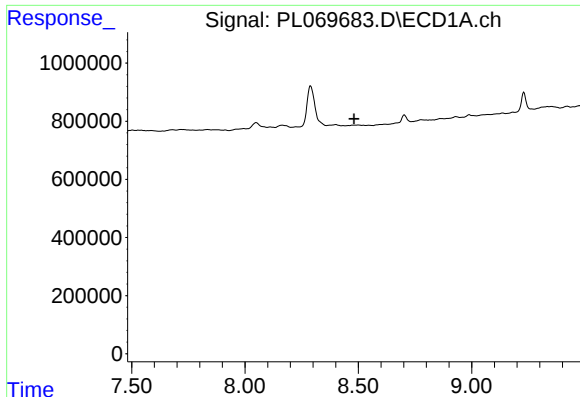

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 8.482 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

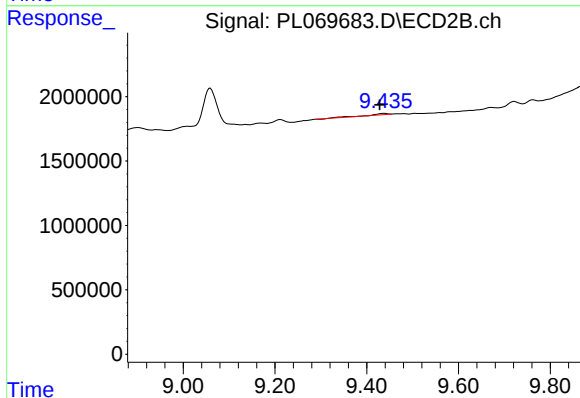


#17 4,4'-DDT

R.T.: 9.437 min
Delta R.T.: 0.009 min
Response: 233209
Conc: 0.21 ng/ml

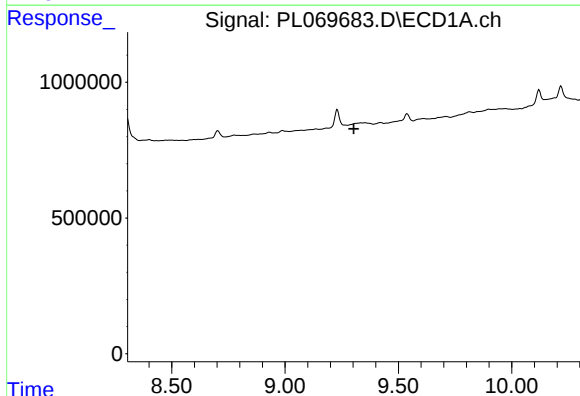


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 9.303 min
Response: 0
Conc: N.D.

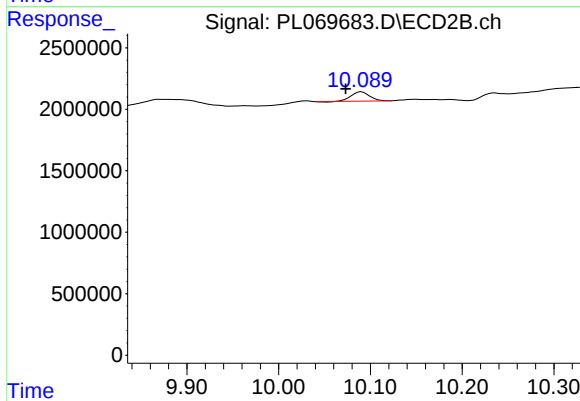

#21 Endrin ketone


R.T.: 10.090 min
Delta R.T.: 0.017 min
Response: 1058171
Conc: 0.89 ng/ml

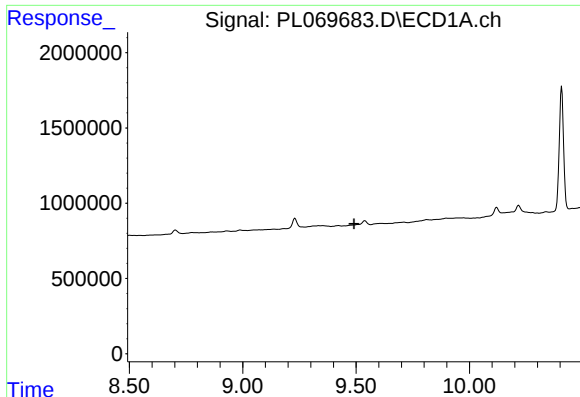

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 9.491 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

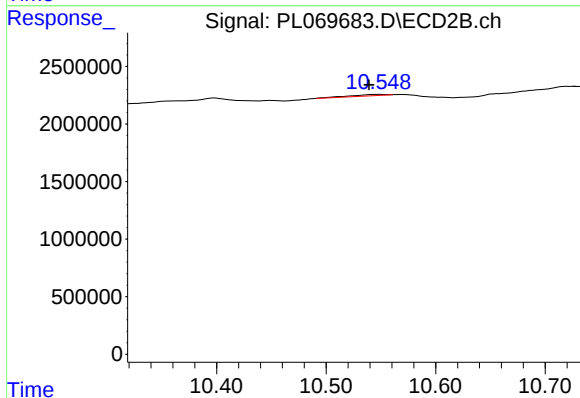


#22 Mirex

R.T.: 10.549 min
Delta R.T.: 0.010 min
Response: 259659
Conc: 0.29 ng/ml

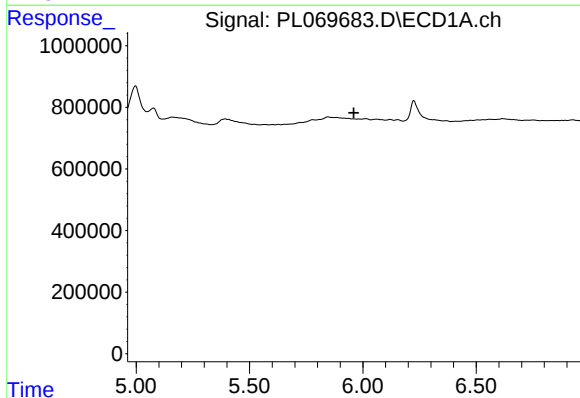


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.961 min
Response: 0
Conc: N.D.

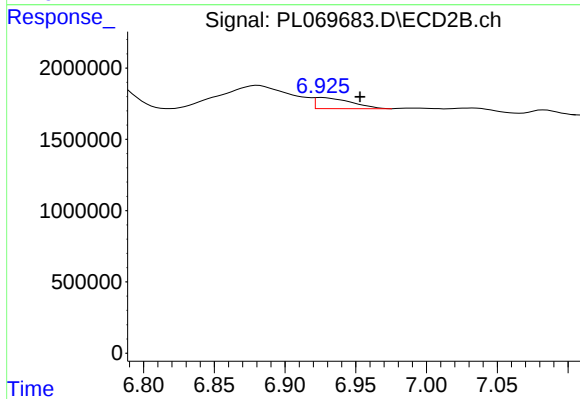

#23 Chlordane-1


R.T.: 6.926 min
Delta R.T.: -0.027 min
Response: 1366076
Conc: 24.72 ng/ml

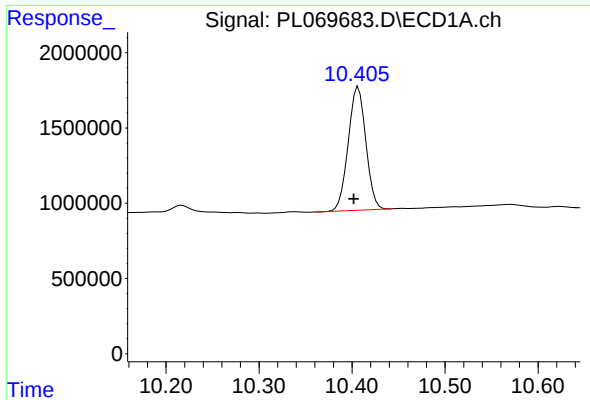

#28 Decachlorobiphenyl

R.T.: 10.407 min
Delta R.T.: 0.005 min
Response: 10795798
Conc: 18.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

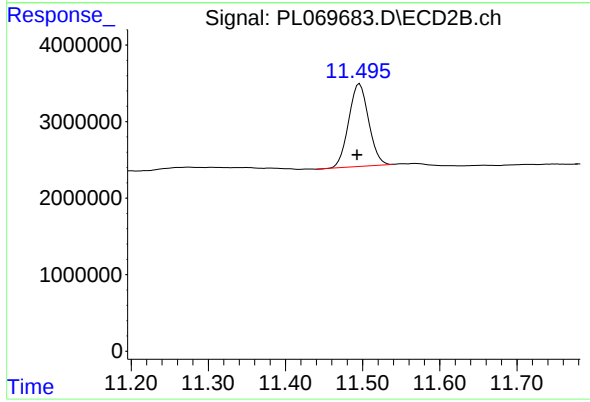

#28 Decachlorobiphenyl

R.T.: 11.496 min
Delta R.T.: 0.003 min
Response: 19333250
Conc: 17.13 ng/ml