

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090222\
 Data File : PL077473.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Sep 2022 16:43
 Operator : AR\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 02 16:55:45 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090222.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 02 16:29:56 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.416	2.629f	6328434	15878293	4.715	5.110
28)	SA Decachlor...	8.902	7.728f	6459563	13167922	5.772	5.627
Target Compounds							
23)	Chlordane-1	4.575	3.606f	2066721	4463024	40.291	50.109
24)	Chlordane-2	5.109	4.177f	4143081	5452829	66.841	52.974
25)	Chlordane-3	5.820	4.824	9981992	15894679	48.944	53.481
26)	Chlordane-4	5.899	4.861f	12085982	15453139	48.646	50.444
27)	Chlordane-5	6.755	5.526f	2056870	5083427	49.407	65.451 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090222\
Data File : PL077473.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Sep 2022 16:43
Operator : AR\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 02 16:55:45 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090222.M
Quant Title : GC Extractables
QLast Update : Fri Sep 02 16:29:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

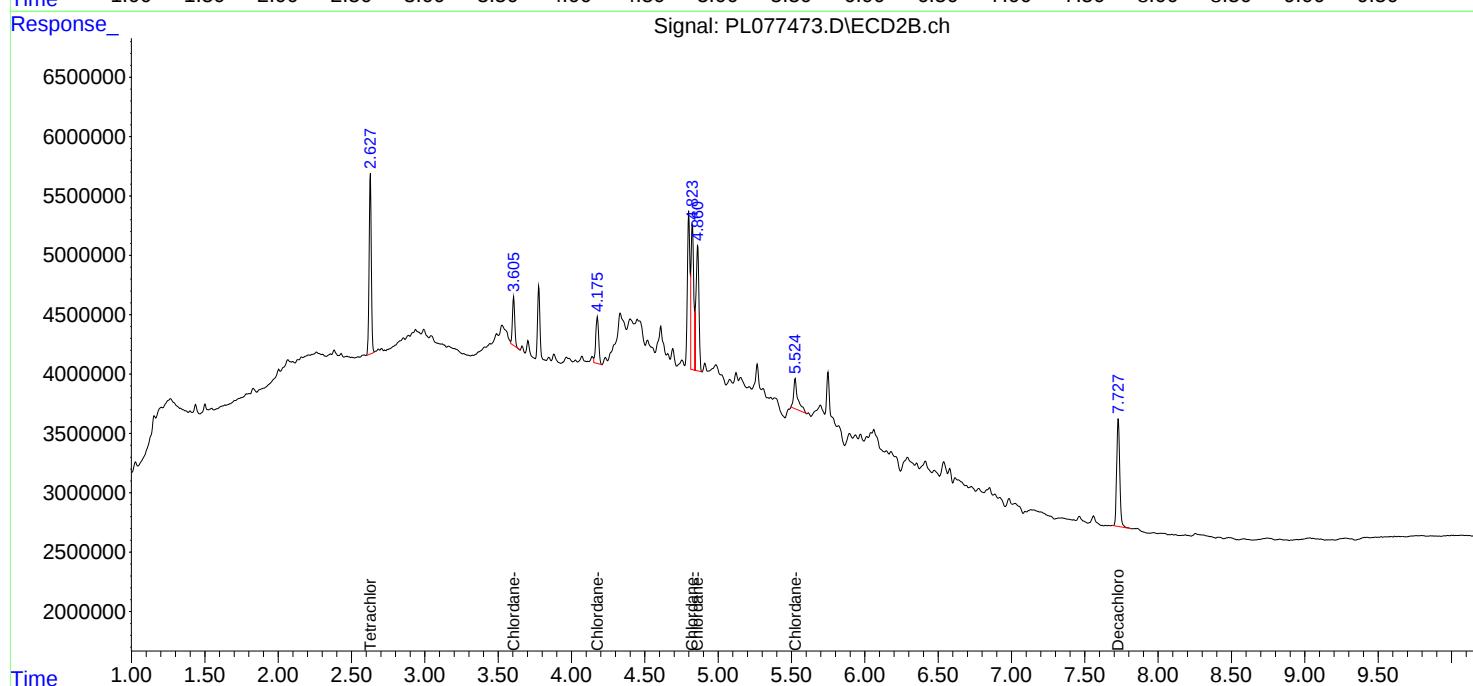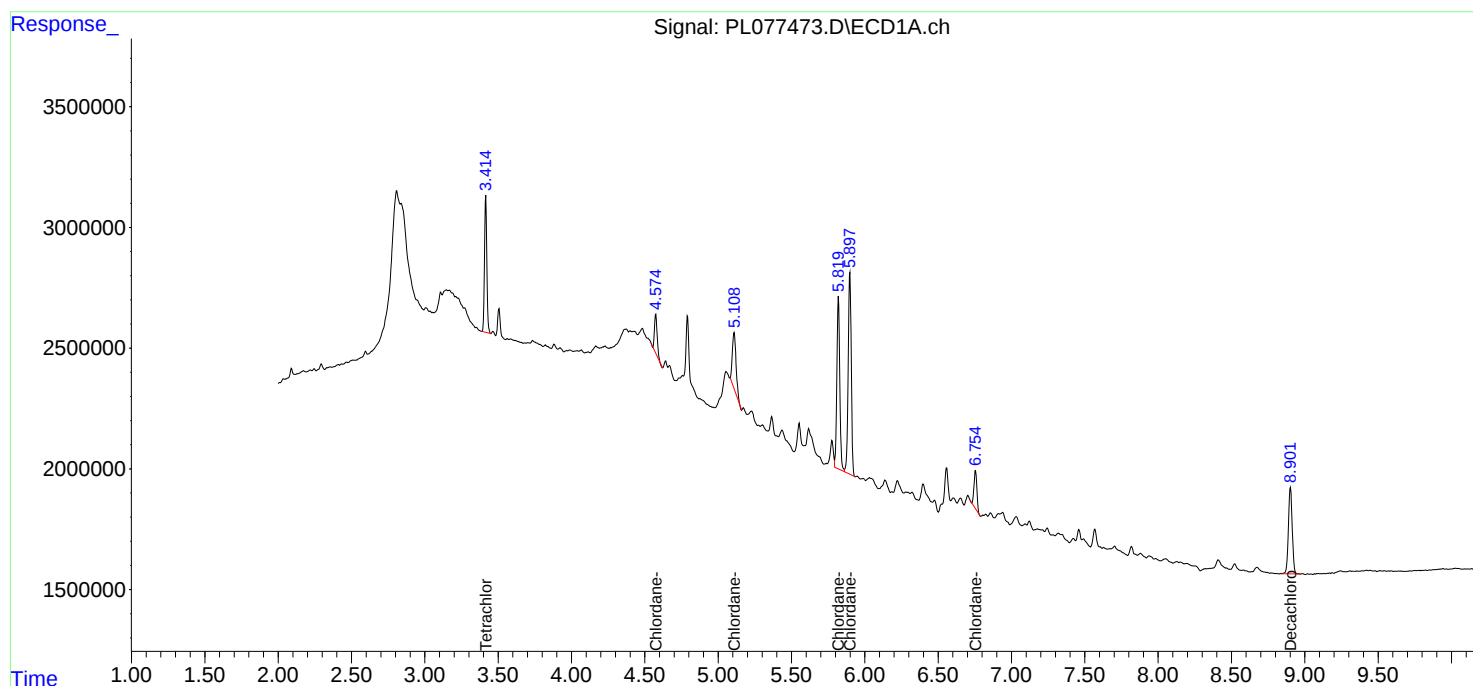


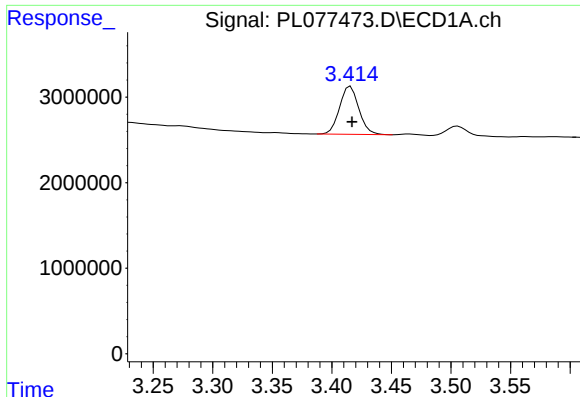

#1 Tetrachloro-m-xylene


R.T.: 3.416 min
Delta R.T.: -0.001 min
Response: 6328434
Conc: 4.71 ng/ml

Instrument :
ECD_L
ClientSampleId :

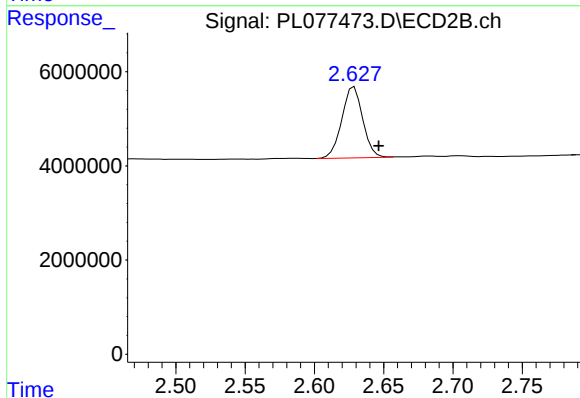


#1 Tetrachloro-m-xylene

R.T.: 2.629 min
Delta R.T.: -0.018 min
Response: 15878293
Conc: 5.11 ng/ml

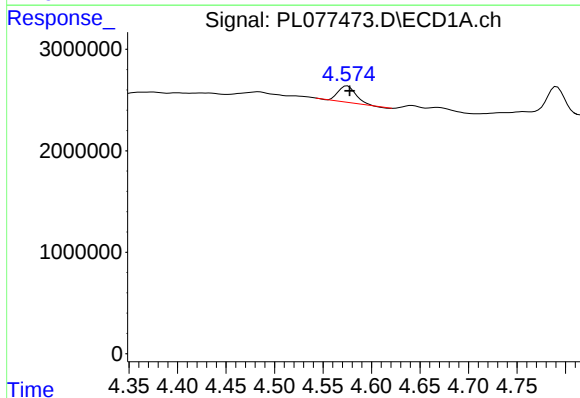


#23 Chlordane-1

R.T.: 4.575 min
Delta R.T.: -0.002 min
Response: 2066721
Conc: 40.29 ng/ml

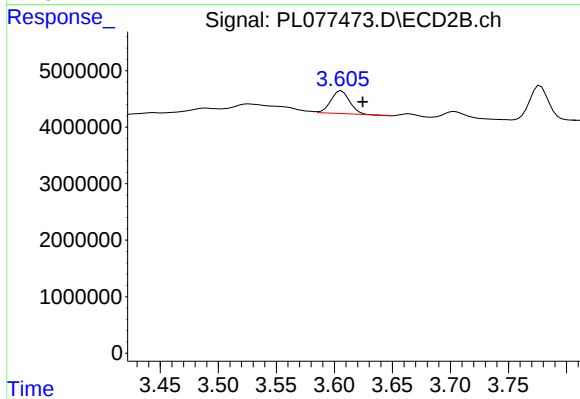

#23 Chlordane-1


R.T.: 3.606 min
Delta R.T.: -0.018 min
Response: 4463024
Conc: 50.11 ng/ml

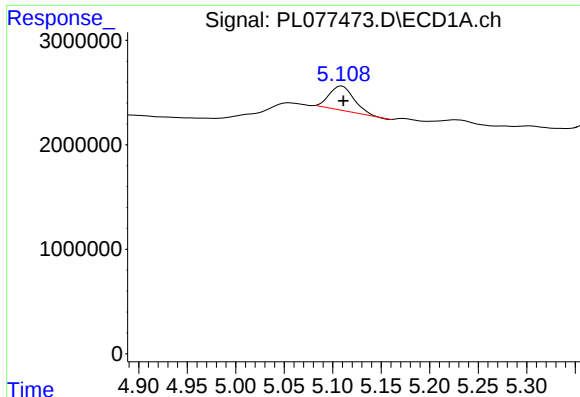

#24 Chlordane-2


R.T.: 5.109 min
Delta R.T.: -0.002 min
Response: 4143081
Conc: 66.84 ng/ml

Instrument :
ECD_L
ClientSampleId :

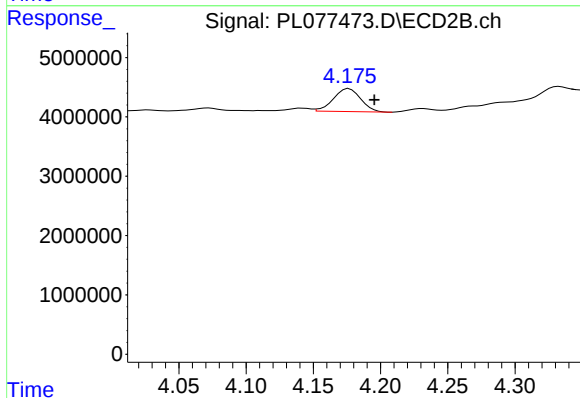


#24 Chlordane-2

R.T.: 4.177 min
Delta R.T.: -0.019 min
Response: 5452829
Conc: 52.97 ng/ml

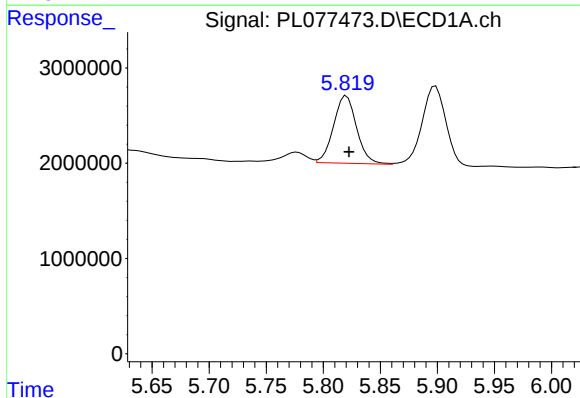


#25 Chlordane-3

R.T.: 5.820 min
Delta R.T.: -0.002 min
Response: 9981992
Conc: 48.94 ng/ml

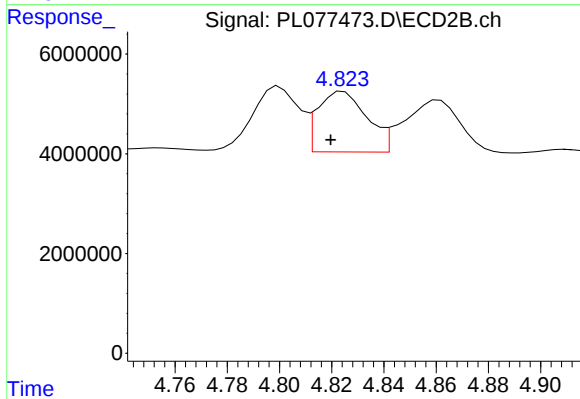

#25 Chlordane-3


R.T.: 4.824 min
Delta R.T.: 0.005 min
Response: 15894679
Conc: 53.48 ng/ml

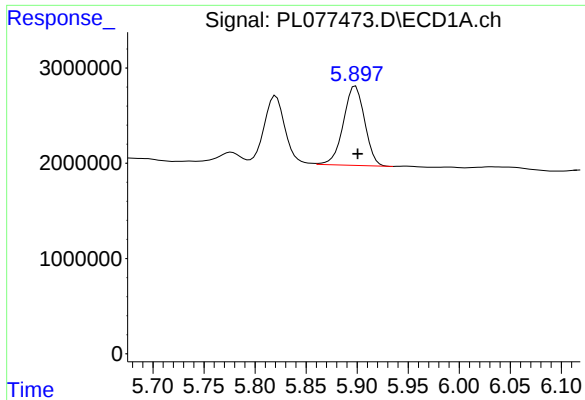

#26 Chlordane-4


R.T.: 5.899 min
Delta R.T.: -0.002 min
Response: 12085982
Conc: 48.65 ng/ml

Instrument :
ECD_L
ClientSampleId :

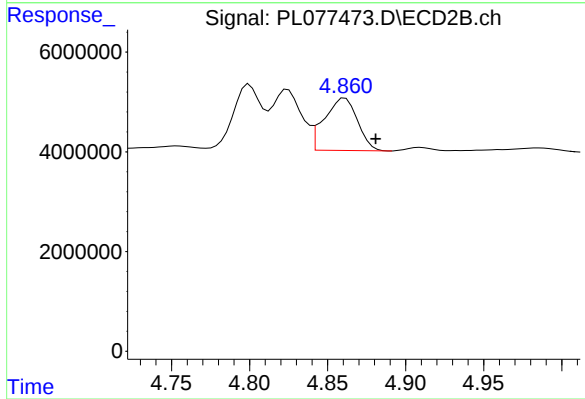


#26 Chlordane-4

R.T.: 4.861 min
Delta R.T.: -0.020 min
Response: 15453139
Conc: 50.44 ng/ml

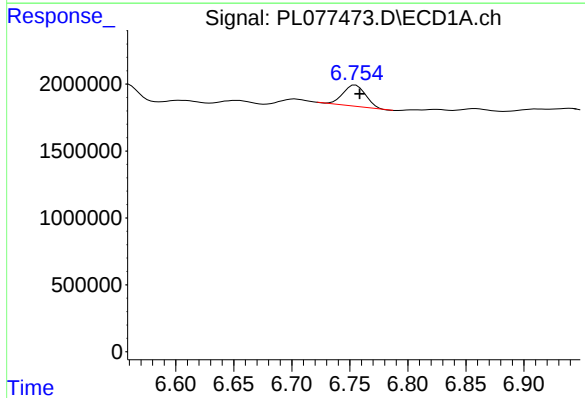


#27 Chlordane-5

R.T.: 6.755 min
Delta R.T.: -0.004 min
Response: 2056870
Conc: 49.41 ng/ml

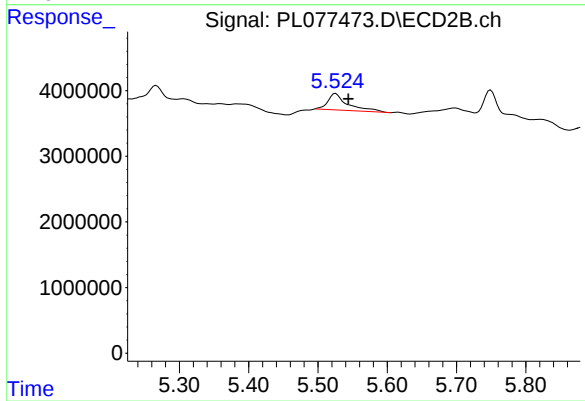

#27 Chlordane-5


R.T.: 5.526 min
Delta R.T.: -0.018 min
Response: 5083427
Conc: 65.45 ng/ml

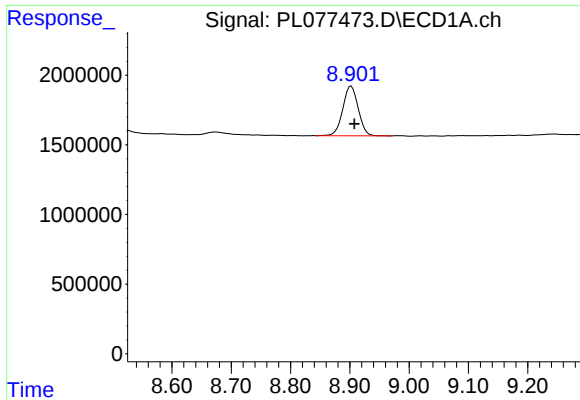

#28 Decachlorobiphenyl

R.T.: 8.902 min
Delta R.T.: -0.005 min
Response: 6459563
Conc: 5.77 ng/ml

Instrument :
ECD_L
ClientSampleId :

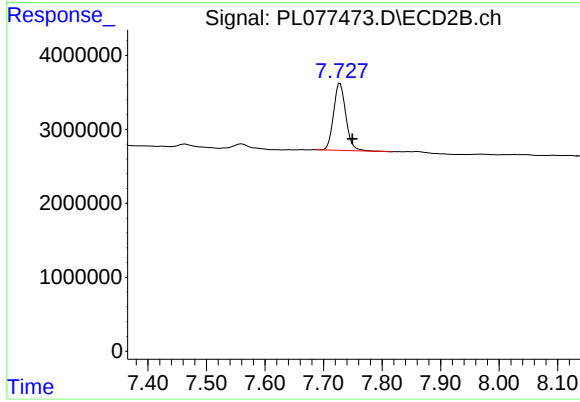

#28 Decachlorobiphenyl

R.T.: 7.728 min
Delta R.T.: -0.021 min
Response: 13167922
Conc: 5.63 ng/ml